


Instrument ID			IC-1	Analyst :	NF	Method: .00.0 / 9056A			date time	nlwt/Fin	Analyst
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name			
STD1	0	0	0	0	0	0	0	IC1-032125	3/21/2025 10:45	10	NF/IZ
STD2	0.421	0.619	0.631	2.075	0.523	1.052	3.247	IC1-032125	3/21/2025 11:07	10	NF/IZ
STD3	0.795	1.199	1.203	3.994	1.001	1.993	5.998	IC1-032125	3/21/2025 11:28	10	NF/IZ
STD4	0.977	1.475	1.468	4.904	1.226	2.407	7.216	IC1-032125	3/21/2025 11:50	10	NF/IZ
STD5	1.993	3.009	2.995	10.03	2.493	4.968	14.842	IC1-032125	3/21/2025 12:11	10	NF/IZ
STD6	4.034	5.988	5.986	19.975	5.011	10.256	30.502	IC1-032125	3/21/2025 12:32	10	NF/IZ
STD7	4.979	7.51	7.517	25.022	6.247	12.323	36.695	IC1-032125	3/21/2025 12:54	10	NF/IZ
ICV	2.031	3.038	3.08	10.364	2.568	5.199	15.269	IC1-032125	3/21/2025 13:37	10	NF/IZ
ICB	0	0.122	0.08	0	0	0	0	IC1-032125	3/21/2025 13:58	10	NF/IZ
CCV	2.107	3.167	3.17	10.669	2.647	5.399	15.534	IC1-032125	3/28/2025 9:47	10	NF/IZ
CCB	0	0	0	0	0	0	0	IC1-032125	3/28/2025 10:09	10	NF/IZ
LB135226BLW	0	0	0	0	0	0	0	IC1-032125	3/28/2025 10:30	10	NF/IZ
LB135226BSW	2.106	3.167	3.176	10.665	2.641	5.394	15.493	IC1-032125	3/28/2025 10:52	10	NF/IZ
Q1666-01	0.517	51.367	0.197	1.015	0.176	0	1147.725	IC1-032125	3/28/2025 11:13	10	NF/IZ
Q1666-01MS	2.432	52.503	3.104	12.405	2.618	5.138	1107.814	IC1-032125	3/28/2025 11:35	10	NF/IZ
Q1666-01MSD	2.436	52.625	3.114	12.343	2.621	5.16	1110.01	IC1-032125	3/28/2025 11:57	10	NF/IZ
Q1666-01DLX20	0.05	2.103	0	1.534	0	0	41.122	IC1-032125	3/28/2025 12:18	10	NF/IZ
CCV	2.101	3.166	3.187	10.748	2.647	5.445	15.57	IC1-032125	3/28/2025 12:40	10	NF/IZ
CCB	0	0	0	0	0	0	0	IC1-032125	3/28/2025 13:01	10	NF/IZ

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A									
ident	concentration F-	concentration CL-	concentration on NO2	concentration on BR-	concentration on NO3	concentration on HPO4	concentration on SO4	file name	date time
STD1	0	0	0	0	0	0	0	IC1-032125	3/21/2025 10:45
STD2	0.421	0.619	0.631	2.075	0.523	1.052	3.247	IC1-032125	3/21/2025 11:07
STD3	0.795	1.199	1.203	3.994	1.001	1.993	5.998	IC1-032125	3/21/2025 11:28
STD4	0.977	1.475	1.468	4.904	1.226	2.407	7.216	IC1-032125	3/21/2025 11:50
STD5	1.993	3.009	2.995	10.03	2.493	4.968	14.842	IC1-032125	3/21/2025 12:11
STD6	4.034	5.988	5.986	19.975	5.011	10.256	30.502	IC1-032125	3/21/2025 12:32
STD7	4.979	7.51	7.517	25.022	6.247	12.323	36.695	IC1-032125	3/21/2025 12:54
ident	True Value	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4		
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000		10 NF/IZ
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000		10 NF/IZ
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000		10 NF/IZ
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000		10 NF/IZ
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000		10 NF/IZ
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000		10 NF/IZ
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000		10 NF/IZ
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4		
STD1									
STD2	5.2500	3.1667	5.1667	3.7500	4.6000	5.2000	8.2333		
STD3	-0.6250	-0.0833	0.2500	-0.1500	0.1000	-0.3500	-0.0333		
STD4	-2.3000	-1.6667	-2.1333	-1.9200	-1.9200	-3.7200	-3.7867		
STD5	-0.3500	0.3000	-0.1667	0.3000	-0.2800	-0.6400	-1.0533		
STD6	0.8500	-0.2000	-0.2333	-0.1250	0.2200	2.5600	1.6733		
STD7	-0.4200	0.1333	0.2267	0.0880	-0.0480	-1.4160	-0.8243		

Initial wt/ Final Analyst

Fluoride (Anions)

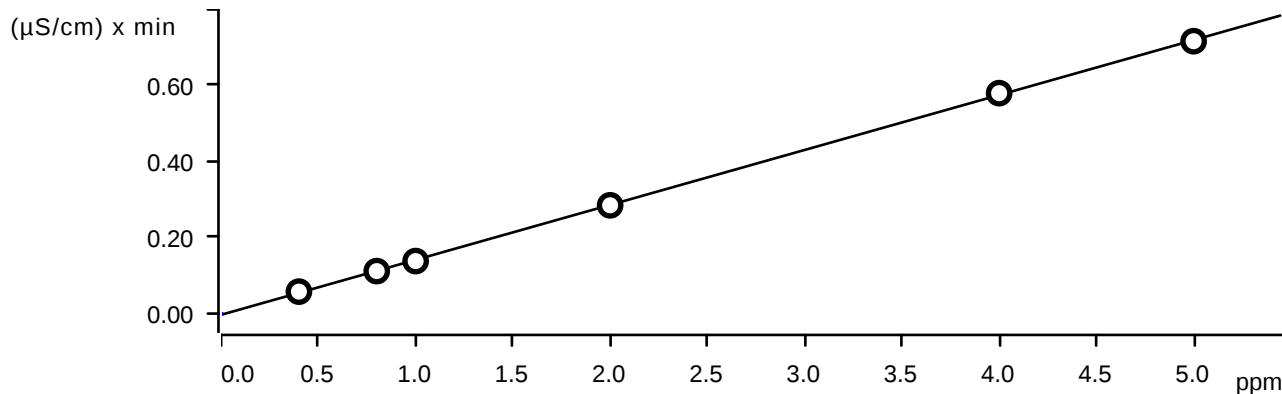


Function: $A = -4.00269E-3 + 0.0144679 \times Q$

Relative standard deviation 1.180947 %

Correlation coefficient 0.999926

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.111	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.137	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.284	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.580	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.716	STD7	2025-03-21 12:54:24 UTC-4	used


Chloride (Anions)

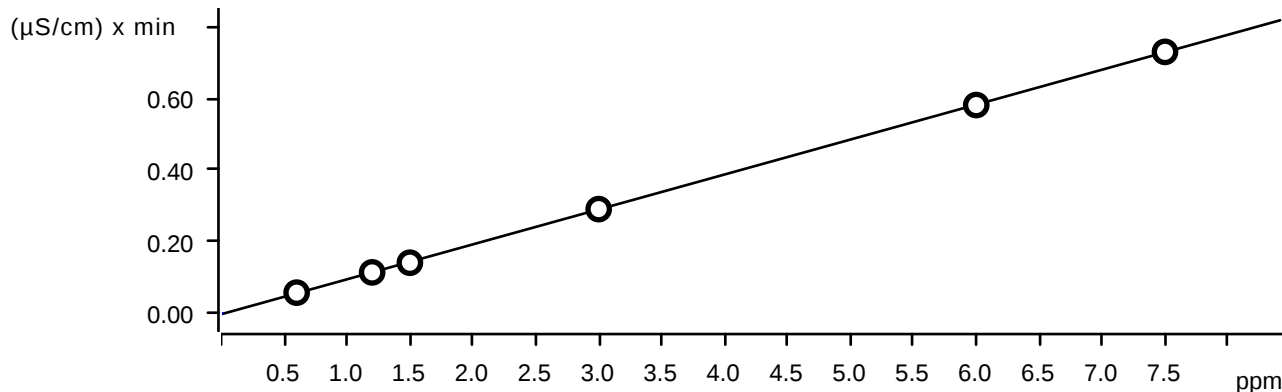

Function: $A = -2.25189E-3 + 9.74103E-3 \times Q$

Relative standard deviation 0.547466 %
Correlation coefficient 0.999984

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.058	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.115	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.141	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.291	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.581	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.729	STD7	2025-03-21 12:54:24 UTC-4	used

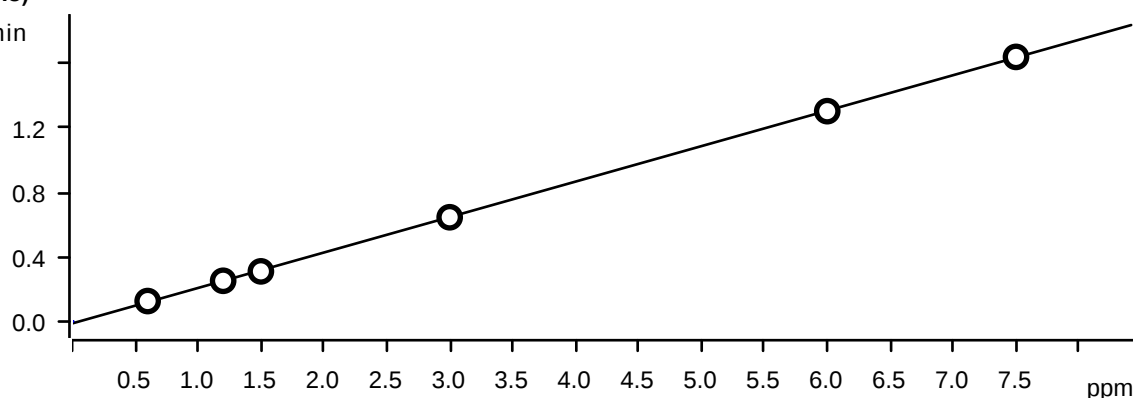
Nitrite (Anions) $(\mu\text{S/cm}) \times \text{min}$ 

Function: $A = -0.0127504 + 0.0219707 \times Q$
Relative standard deviation 0.767970 %
Correlation coefficient 0.999969

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.126	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.252	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.310	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.645	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.302	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.639	STD7	2025-03-21 12:54:24 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

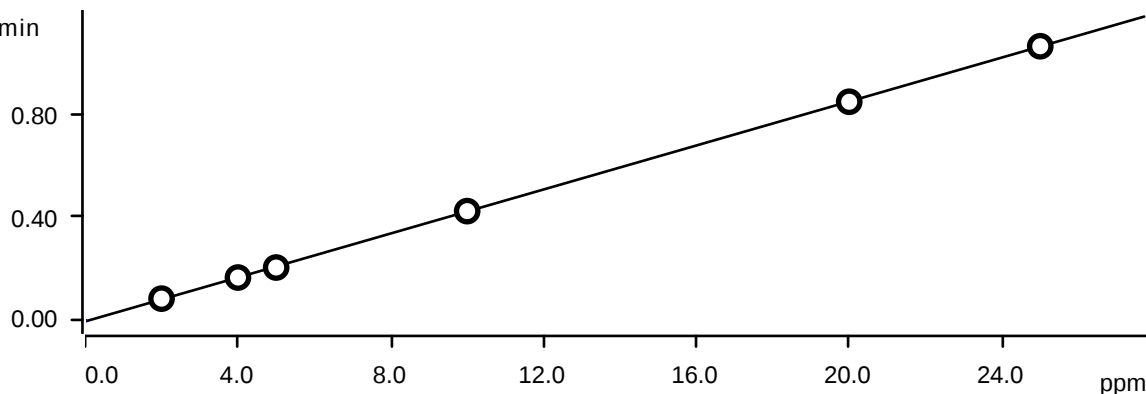

Function: $A = -4.26620E-3 + 4.25885E-3 \times Q$


Relative standard deviation: 0.597348 %

Correlation coefficient: 0.999981

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.084	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.166	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.205	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.423	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.846	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.061	STD7	2025-03-21 12:54:24 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

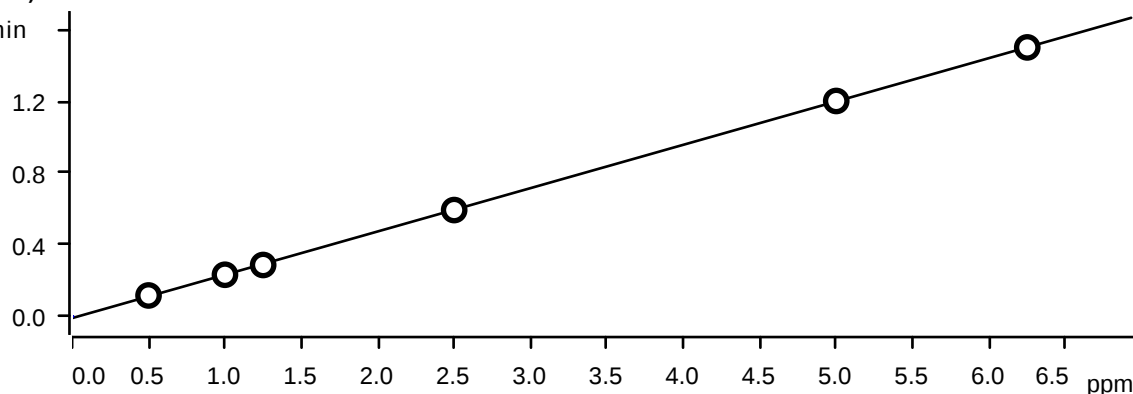


Function: $A = -9.20754E-3 + 0.0241631 \times Q$

Relative standard deviation: 0.659338 %

Correlation coefficient 0.999977


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.117	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.233	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.287	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.593	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.202	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.500	STD7	2025-03-21 12:54:24 UTC-4	used

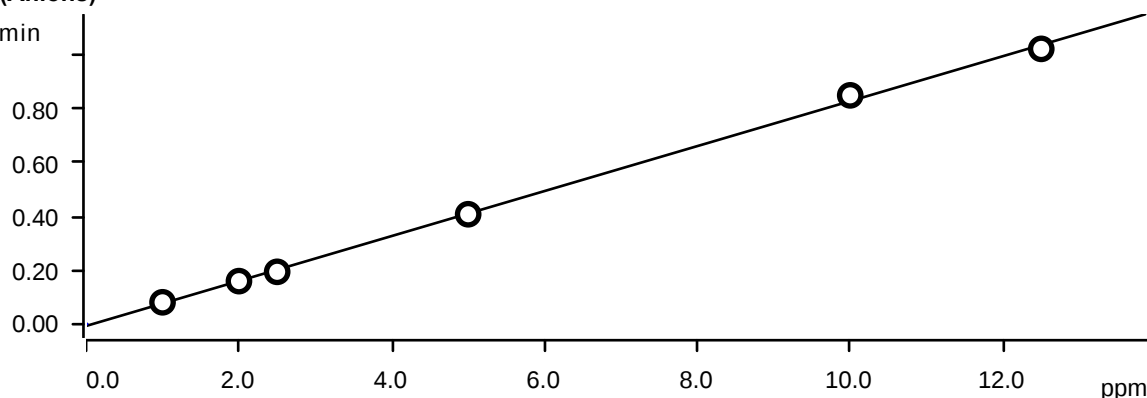Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -6.92112E-3 + 8.35786E-3 \times Q$

Relative standard deviation 3.051728 %

Correlation coefficient 0.999508

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.081	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.160	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.194	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.408	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.850	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.023	STD7	2025-03-21 12:54:24 UTC-4	used

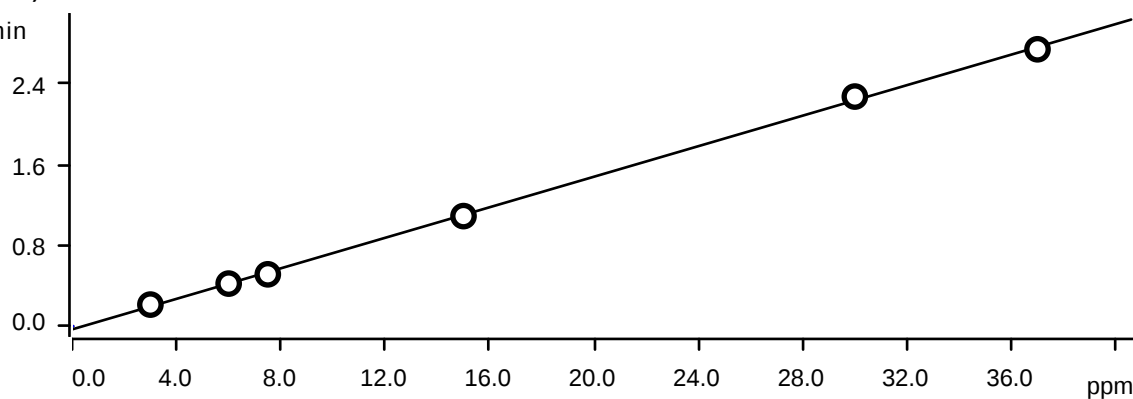Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0318458 + 7.56676E-3 \times Q$

Relative standard deviation 2.235653 %

Correlation coefficient 0.999739


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-03-21 10:45:52 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.214	STD2	2025-03-21 11:07:15 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.422	STD3	2025-03-21 11:28:39 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.514	STD4	2025-03-21 11:50:04 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.091	STD5	2025-03-21 12:11:30 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.276	STD6	2025-03-21 12:32:57 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.745	STD7	2025-03-21 12:54:24 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-03-21 10:45:52 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

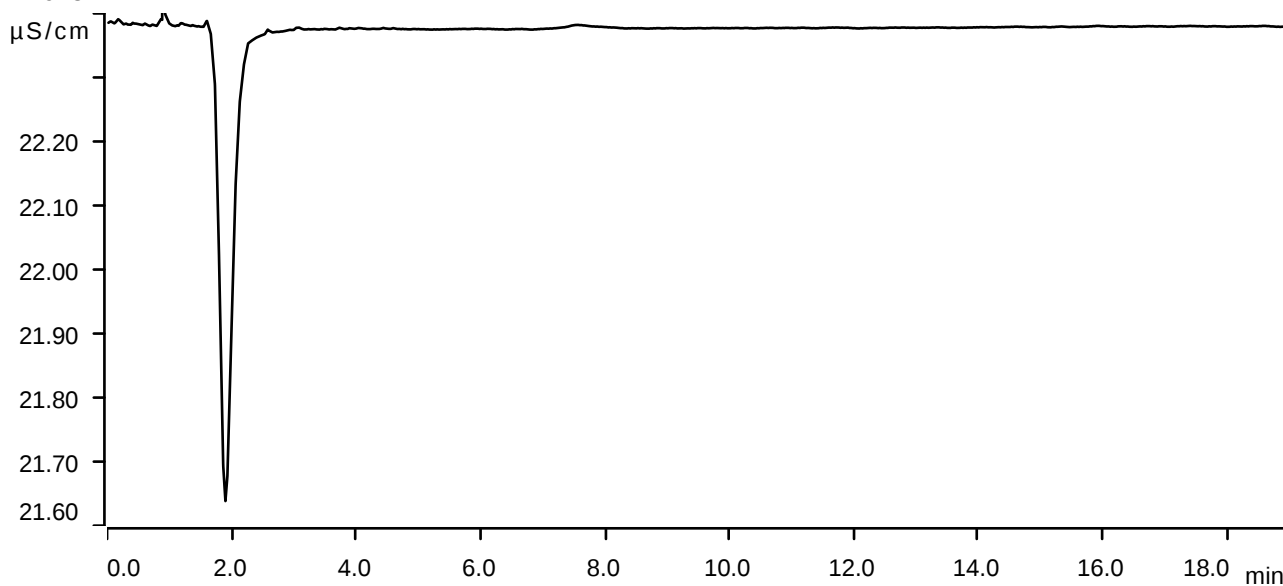Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-03-21 11:07:15 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

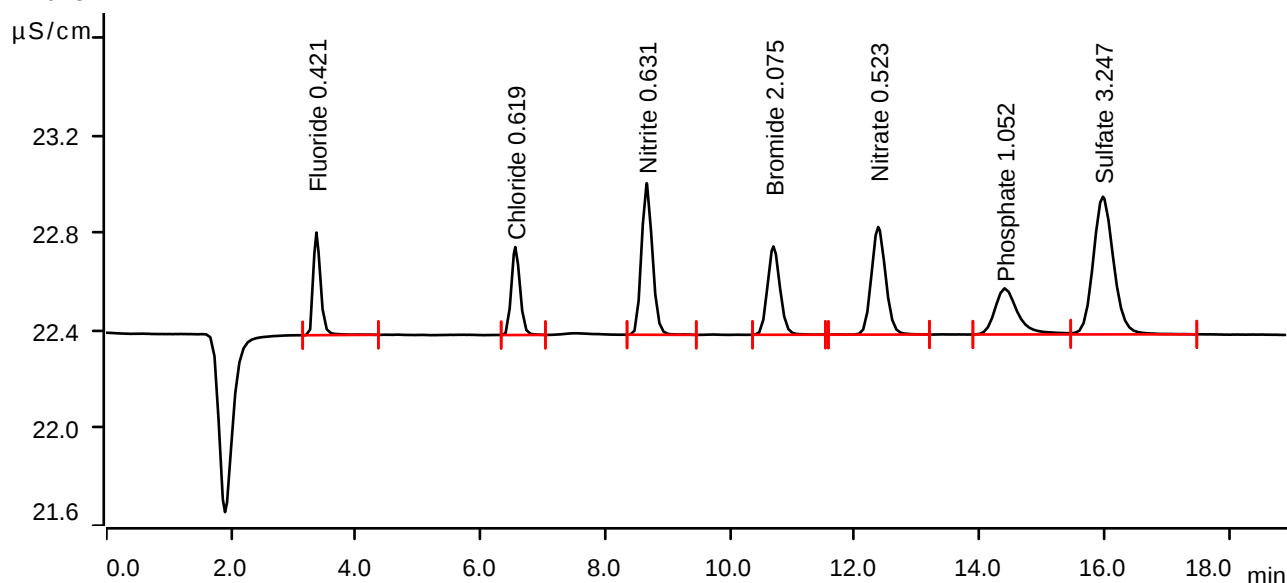

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.368	0.0570	0.420	0.421	Fluoride
2	6.557	0.0580	0.361	0.619	Chloride
3	8.662	0.1260	0.621	0.631	Nitrite
4	10.695	0.0841	0.362	2.075	Bromide
5	12.375	0.1171	0.441	0.523	Nitrate
6	14.403	0.0810	0.189	1.052	Phosphate
7	15.978	0.2139	0.564	3.247	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-03-21 11:28:39 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

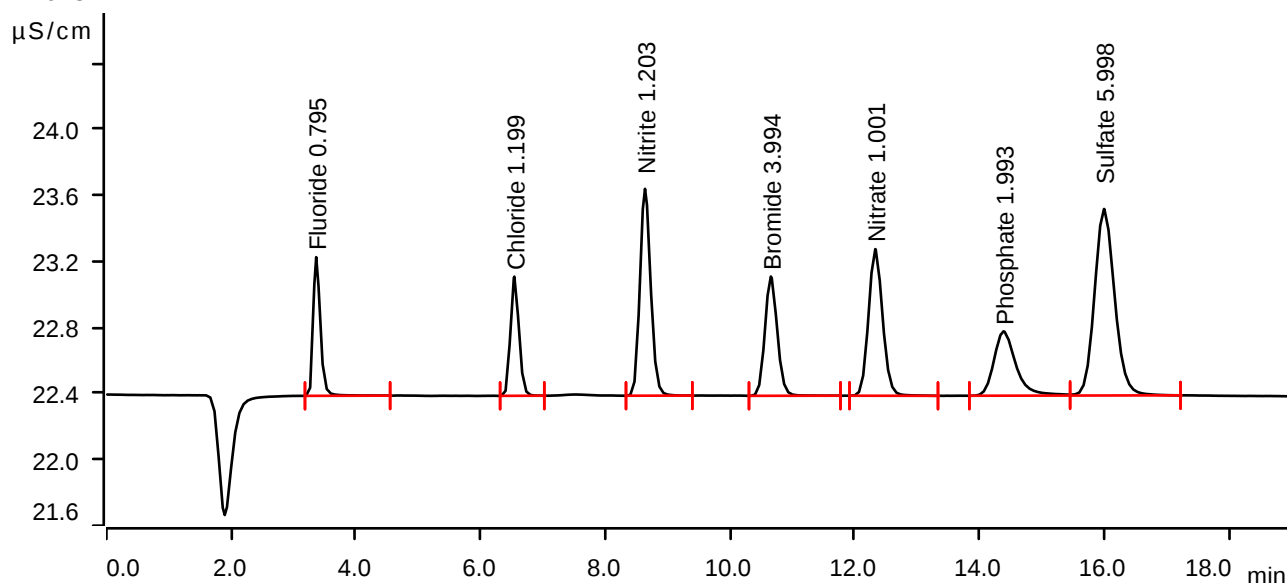

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.365	0.1110	0.839	0.795	Fluoride
2	6.542	0.1146	0.721	1.199	Chloride
3	8.637	0.2515	1.252	1.203	Nitrite
4	10.653	0.1658	0.722	3.994	Bromide
5	12.328	0.2325	0.888	1.001	Nitrate
6	14.383	0.1597	0.389	1.993	Phosphate
7	15.995	0.4220	1.129	5.998	Sulfate


Sample data

Ident STD4
 Sample type Standard 4
 Determination start 2025-03-21 11:50:04 UTC-4
 Method IC1-032125
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.49 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

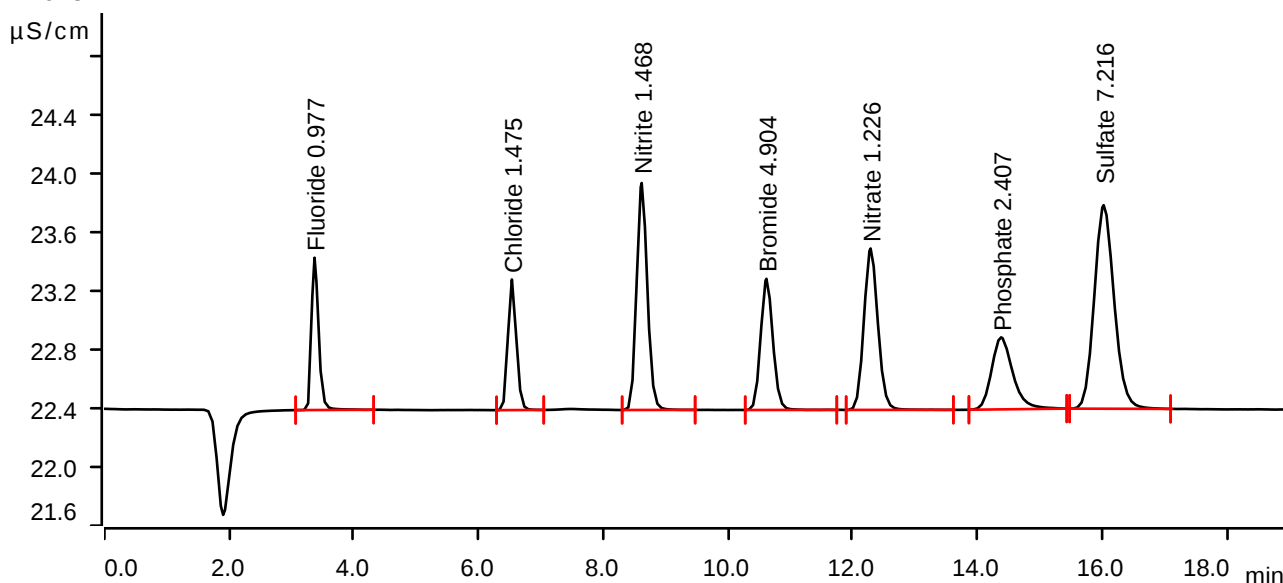

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.370	0.1374	1.040	0.977	Fluoride
2	6.533	0.1415	0.892	1.475	Chloride
3	8.615	0.3099	1.551	1.468	Nitrite
4	10.615	0.2046	0.896	4.904	Bromide
5	12.285	0.2869	1.103	1.226	Nitrate
6	14.378	0.1943	0.492	2.407	Phosphate
7	16.022	0.5142	1.391	7.216	Sulfate


Sample data

Ident STD5
 Sample type Standard 5
 Determination start 2025-03-21 12:11:30 UTC-4
 Method IC1-032125
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.20 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

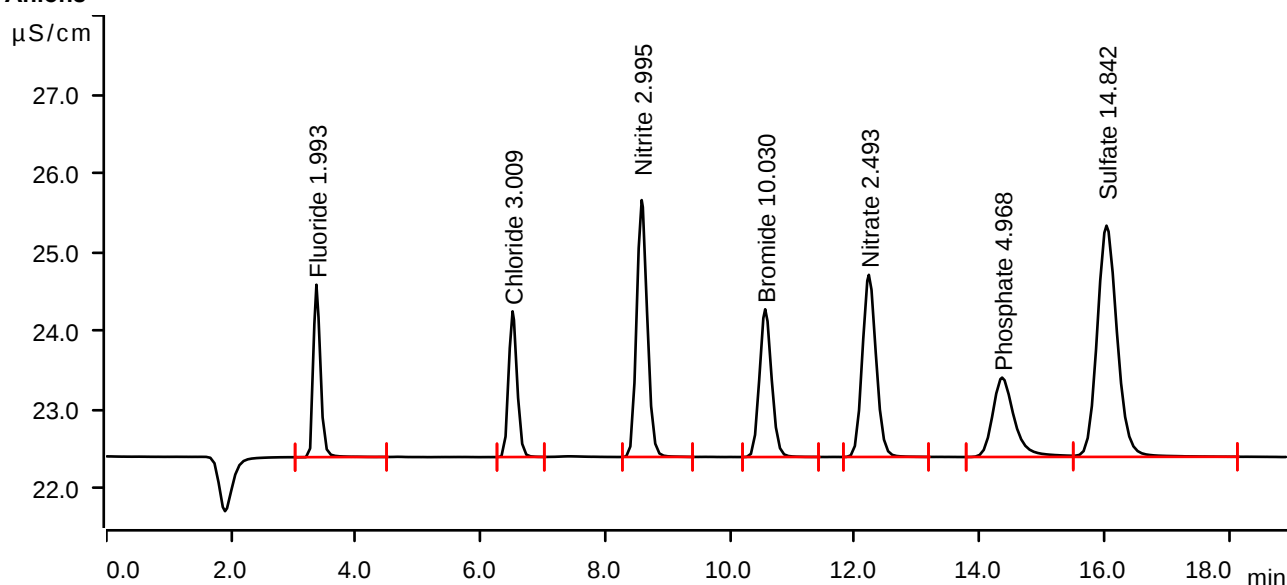

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.368	0.2843	2.188	1.993	Fluoride
2	6.513	0.2909	1.849	3.009	Chloride
3	8.583	0.6452	3.260	2.995	Nitrite
4	10.563	0.4229	1.875	10.030	Bromide
5	12.225	0.5933	2.311	2.493	Nitrate
6	14.362	0.4083	1.007	4.968	Phosphate
7	16.035	1.0913	2.934	14.842	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-03-21 12:32:57 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.09 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

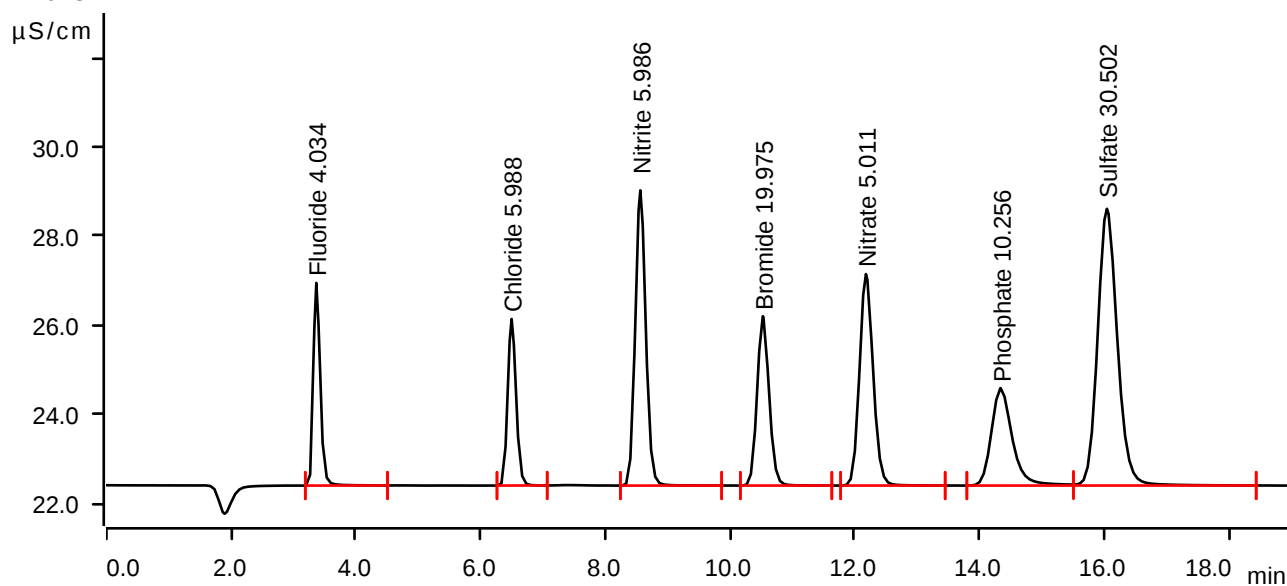

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.367	0.5796	4.549	4.034	Fluoride
2	6.498	0.5810	3.740	5.988	Chloride
3	8.562	1.3025	6.628	5.986	Nitrite
4	10.525	0.8465	3.803	19.975	Bromide
5	12.178	1.2015	4.749	5.011	Nitrate
6	14.338	0.8503	2.187	10.256	Phosphate
7	16.042	2.2762	6.214	30.502	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-03-21 12:54:24 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

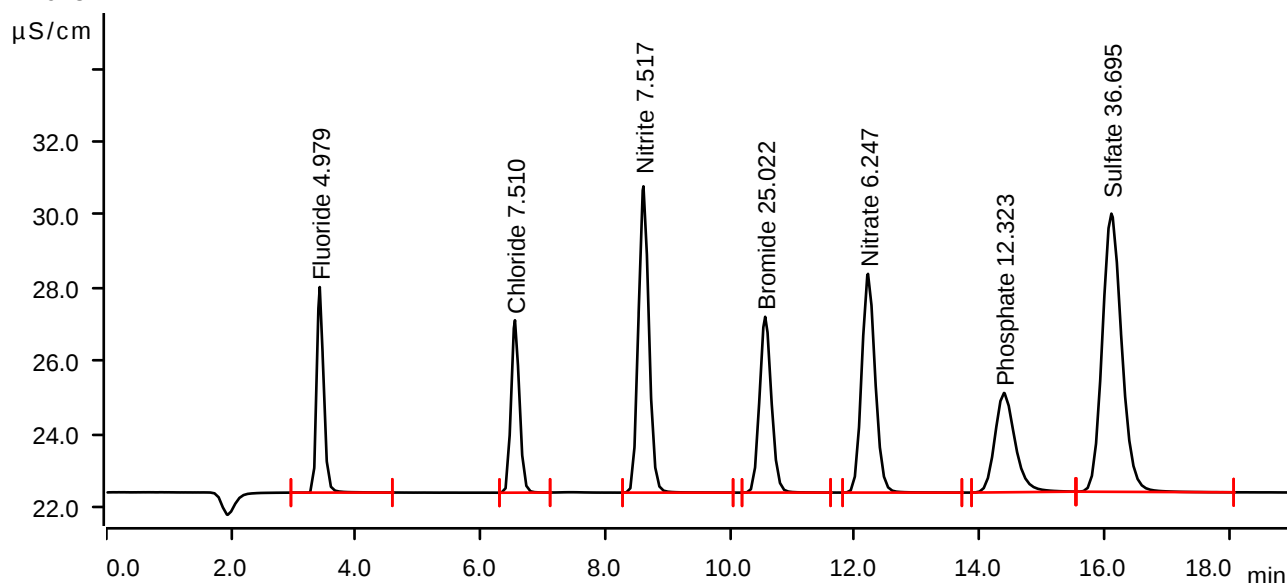

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.422	0.7164	5.617	4.979	Fluoride
2	6.552	0.7293	4.712	7.510	Chloride
3	8.612	1.6387	8.371	7.517	Nitrite
4	10.563	1.0614	4.806	25.022	Bromide
5	12.212	1.5003	5.978	6.247	Nitrate
6	14.392	1.0231	2.714	12.323	Phosphate
7	16.113	2.7448	7.604	36.695	Sulfate


Sample data

Ident CCV
 Sample type Check standard 1
 Determination start 2025-03-28 09:47:48 UTC-4
 Method IC1-032125
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.26 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

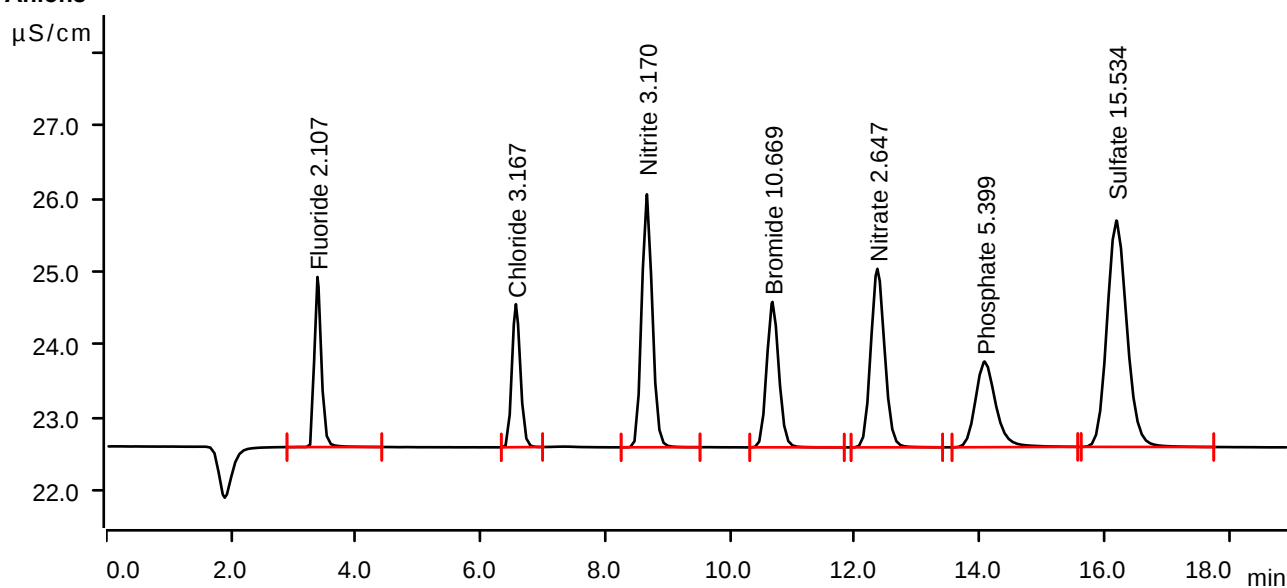


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.385	0.3009	2.325	2.107	Fluoride
2	6.567	0.3062	1.954	3.167	Chloride
3	8.665	0.6837	3.457	3.170	Nitrite
4	10.680	0.4501	1.988	10.669	Bromide
5	12.362	0.6305	2.441	2.647	Nitrate
6	14.082	0.4443	1.170	5.399	Phosphate
7	16.193	1.1436	3.093	15.534	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-03-28 10:09:19 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

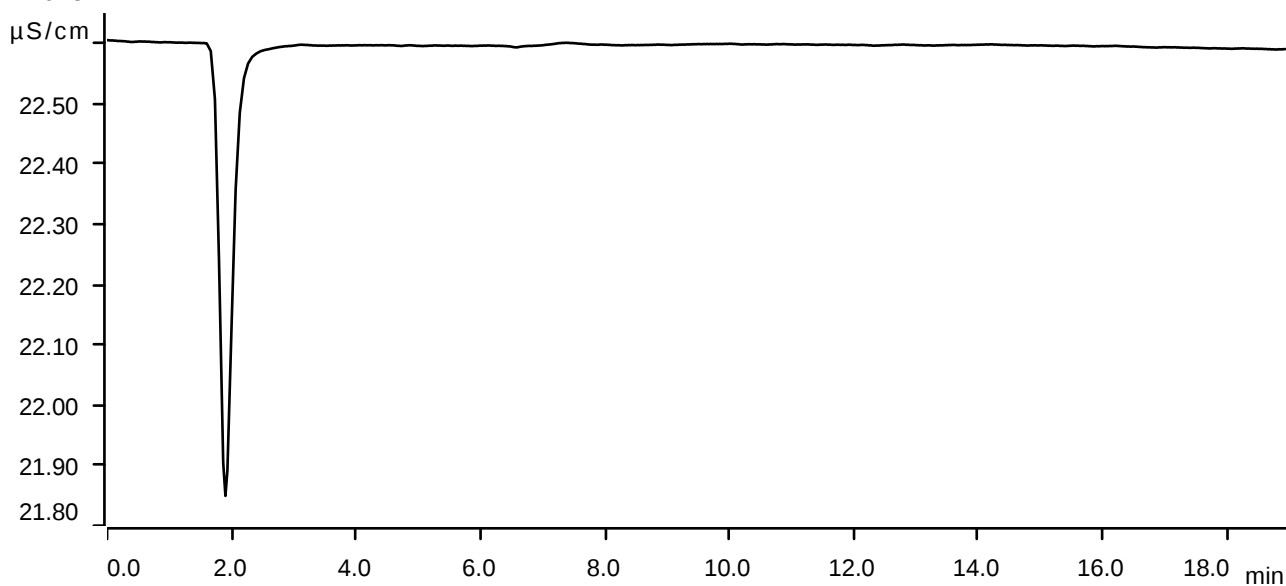
Anions

Sample data

Ident LB135226BLW
Sample type Sample
Determination start 2025-03-28 10:30:49 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

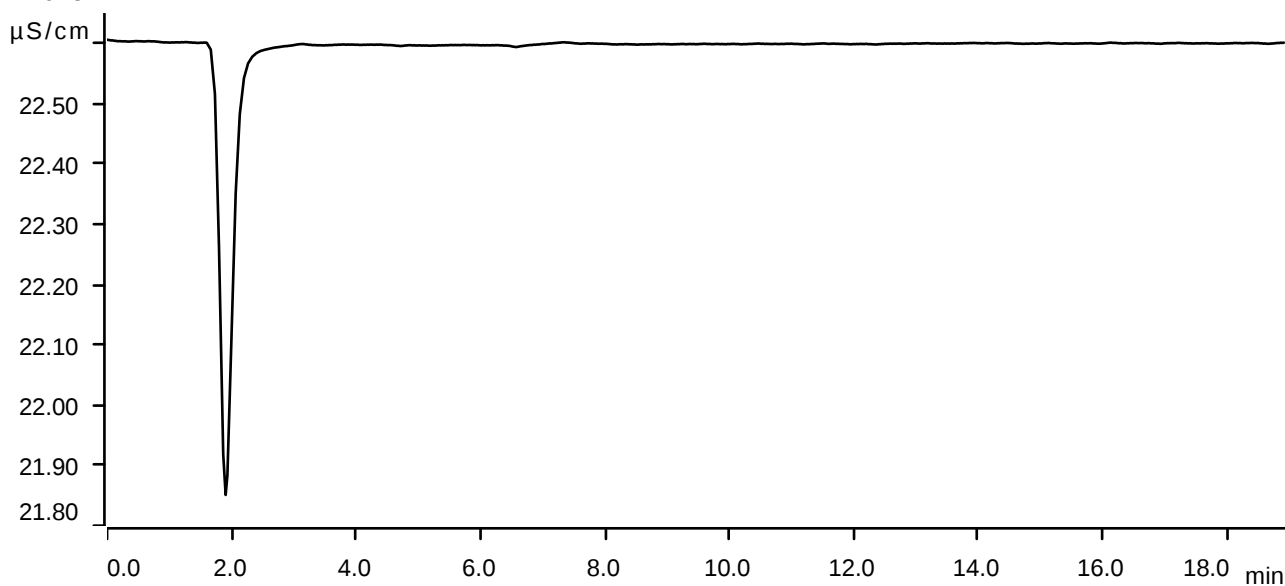Anions


Sample data

Ident LB135226BSW
Sample type Check standard 1
Determination start 2025-03-28 10:52:20 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

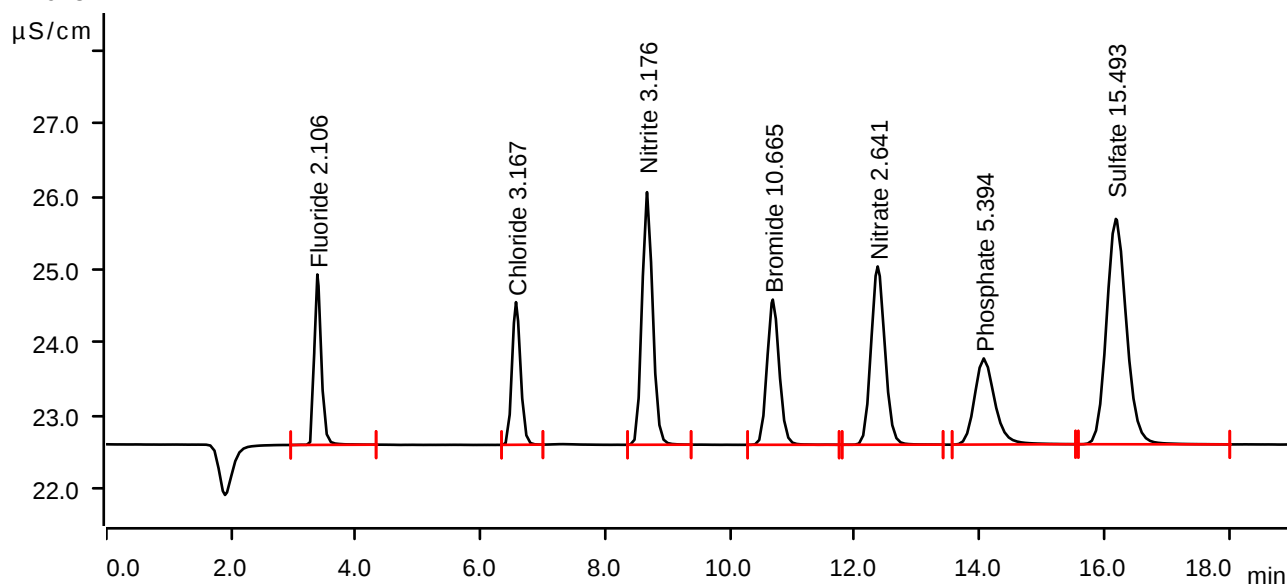

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.383	0.3007	2.328	2.106	Fluoride
2	6.568	0.3062	1.949	3.167	Chloride
3	8.670	0.6851	3.452	3.176	Nitrite
4	10.685	0.4499	1.984	10.665	Bromide
5	12.367	0.6289	2.436	2.641	Nitrate
6	14.067	0.4439	1.177	5.394	Phosphate
7	16.185	1.1405	3.080	15.493	Sulfate


Sample data

Ident Q1666-01
Sample type Sample
Determination start 2025-03-28 11:13:53 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

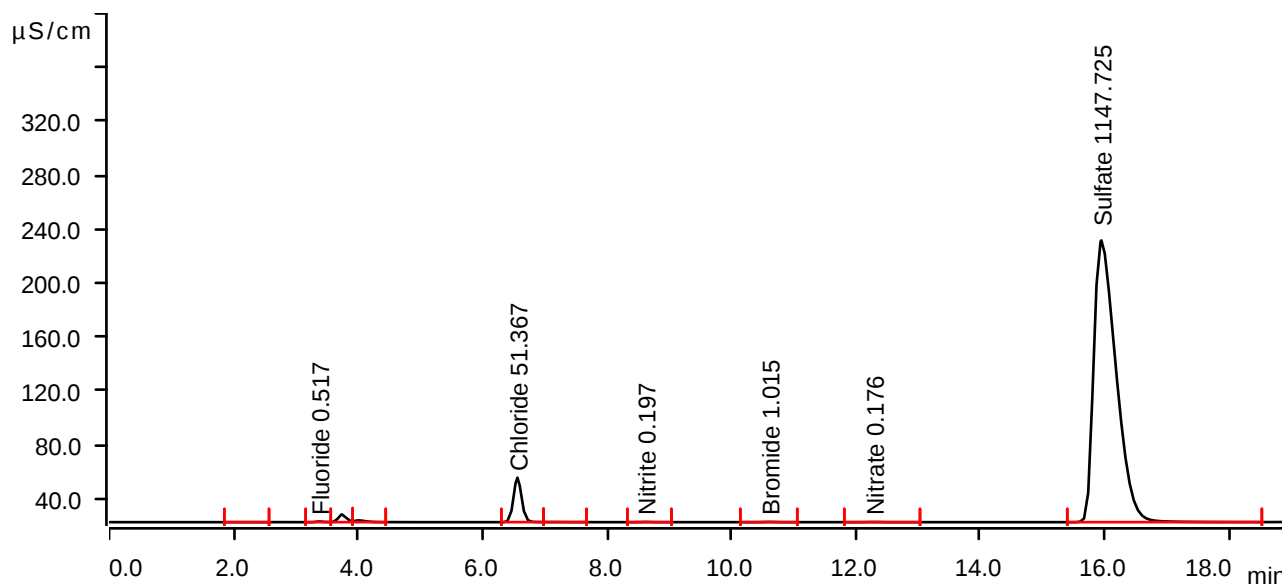

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	2.083	0.0106	0.032	invalid	
2	3.375	0.0708	0.475	0.517	Fluoride
3	3.742	0.8740	5.731	invalid	
4	4.015	0.2719	1.299	invalid	
5	6.563	5.0014	33.008	51.367	Chloride
6	7.182	0.0102	0.031	invalid	
7	8.622	0.0306	0.155	0.197	Nitrite
8	10.615	0.0390	0.173	1.015	Bromide
9	12.288	0.0334	0.129	0.176	Nitrate
10	15.947	86.8138	209.005	1147.725	Sulfate


Sample data

Ident Q1666-01MS
Sample type Sample
Determination start 2025-03-28 11:35:26 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.98 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

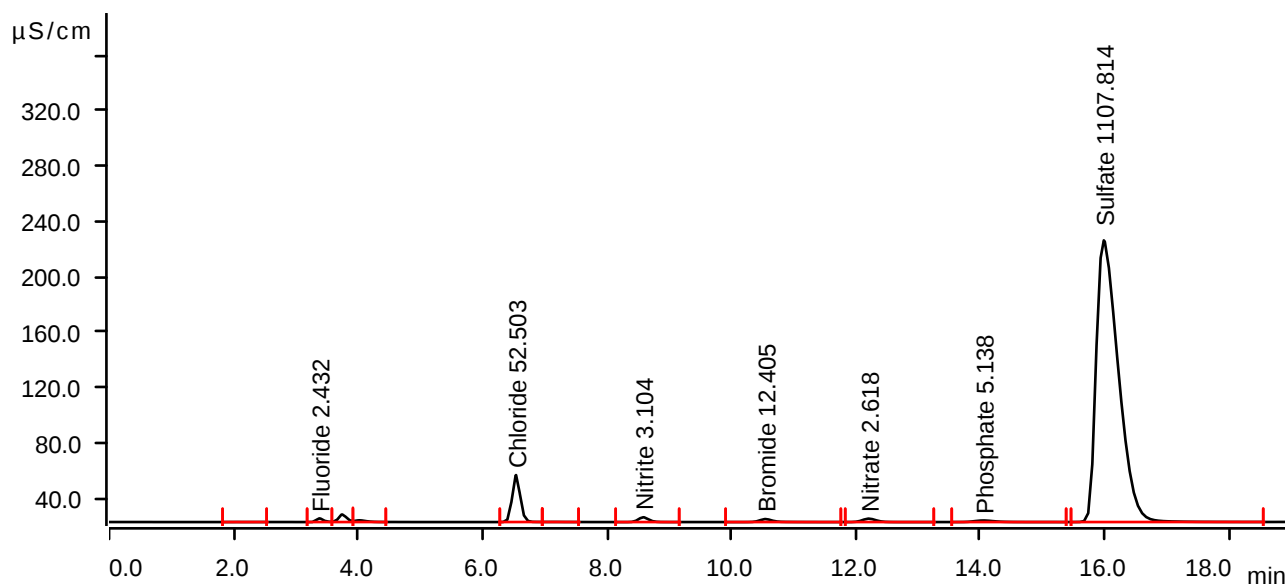

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	2.053	0.0083	0.028	invalid	
2	3.380	0.3478	2.656	2.432	Fluoride
3	3.748	0.8351	5.487	invalid	
4	4.025	0.2589	1.240	invalid	
5	6.542	5.1121	33.916	52.503	Chloride
6	7.147	0.0084	0.028	invalid	
7	8.585	0.6693	3.446	3.104	Nitrite
8	10.548	0.5240	2.152	12.405	Bromide
9	12.208	0.6234	2.472	2.618	Nitrate
10	14.050	0.4225	1.117	5.138	Phosphate
11	15.985	83.7938	203.476	1107.814	Sulfate


Sample data

Ident Q1666-01MSD
Sample type Sample
Determination start 2025-03-28 11:57:00 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.81 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

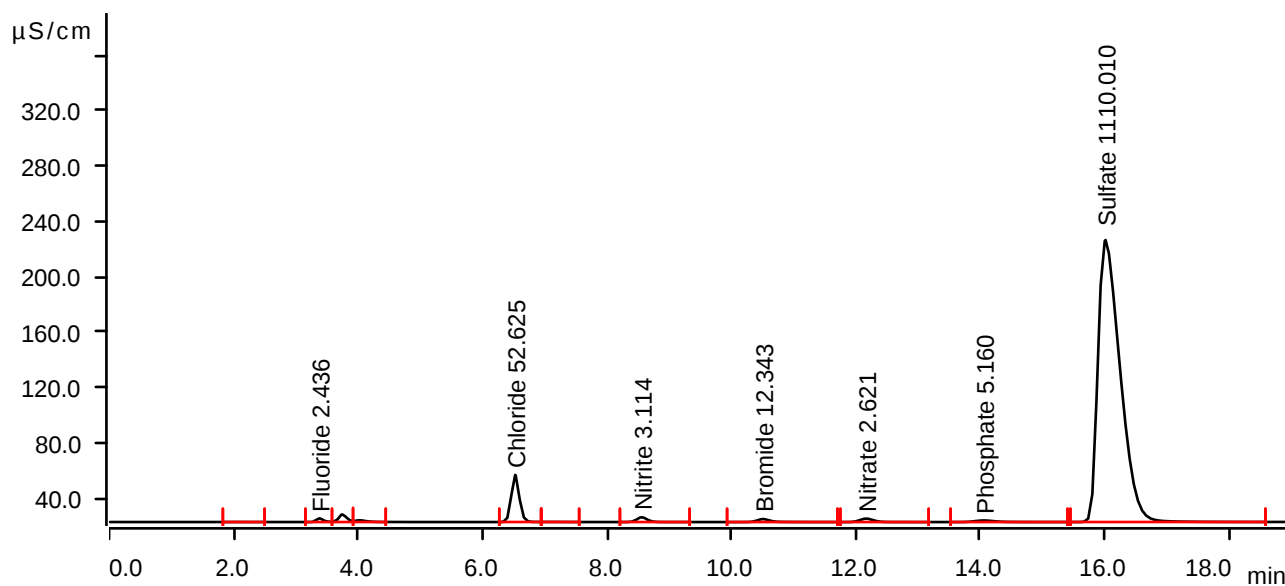

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	2.060	0.0080	0.028	invalid	
2	3.380	0.3485	2.659	2.436	Fluoride
3	3.750	0.8358	5.504	invalid	
4	4.027	0.2583	1.242	invalid	
5	6.527	5.1239	34.043	52.625	Chloride
6	7.118	0.0083	0.027	invalid	
7	8.560	0.6715	3.466	3.114	Nitrite
8	10.510	0.5214	2.157	12.343	Bromide
9	12.167	0.6241	2.486	2.621	Nitrate
10	14.055	0.4244	1.126	5.160	Phosphate
11	16.013	83.9600	203.702	1110.010	Sulfate


Sample data

Ident Q1666-01DLX20
Sample type Sample
Determination start 2025-03-28 12:18:35 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.70 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

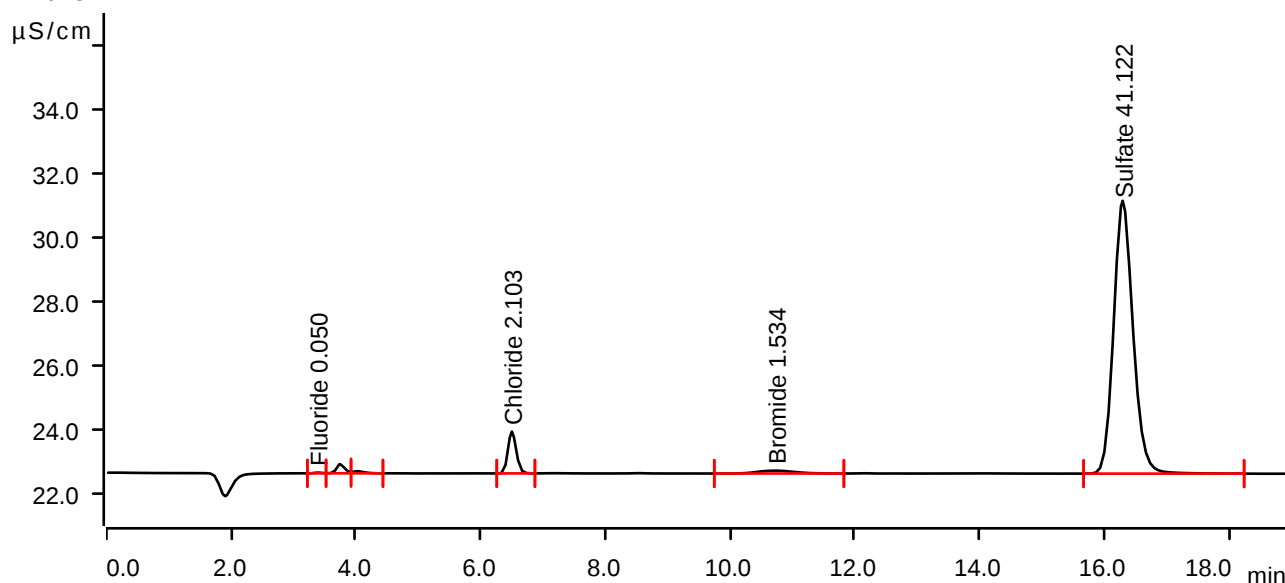

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.387	0.0032	0.023	0.050	Fluoride
2	3.747	0.0446	0.289	invalid	
3	4.023	0.0140	0.067	invalid	
4	6.502	0.2026	1.308	2.103	Chloride
5	10.733	0.0611	0.089	1.534	Bromide
6	16.295	3.0797	8.523	41.122	Sulfate


Sample data

Ident CCV
 Sample type Check standard 1
 Determination start 2025-03-28 12:40:10 UTC-4
 Method IC1-032125
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 10.64 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

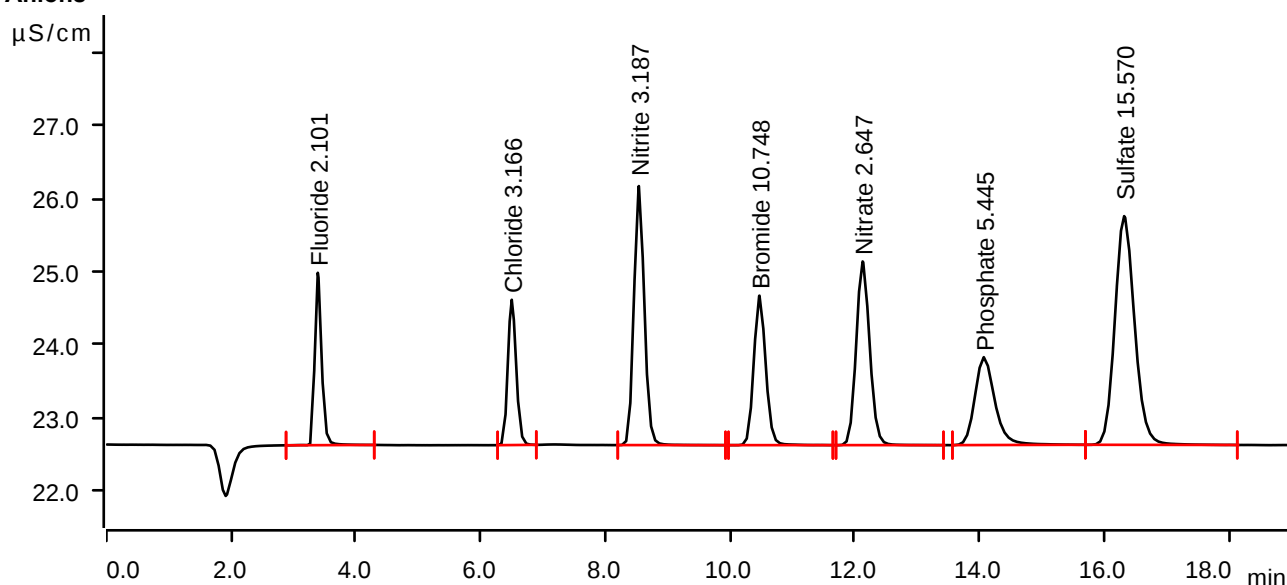

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.3000	2.355	2.101	Fluoride
2	6.500	0.3062	1.985	3.166	Chloride
3	8.538	0.6875	3.540	3.187	Nitrite
4	10.472	0.4535	2.043	10.748	Bromide
5	12.125	0.6303	2.510	2.647	Nitrate
6	14.068	0.4482	1.200	5.445	Phosphate
7	16.318	1.1463	3.126	15.570	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-03-28 13:01:40 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.64 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

