


LB135253

7471B

INSTRUMENT ID:

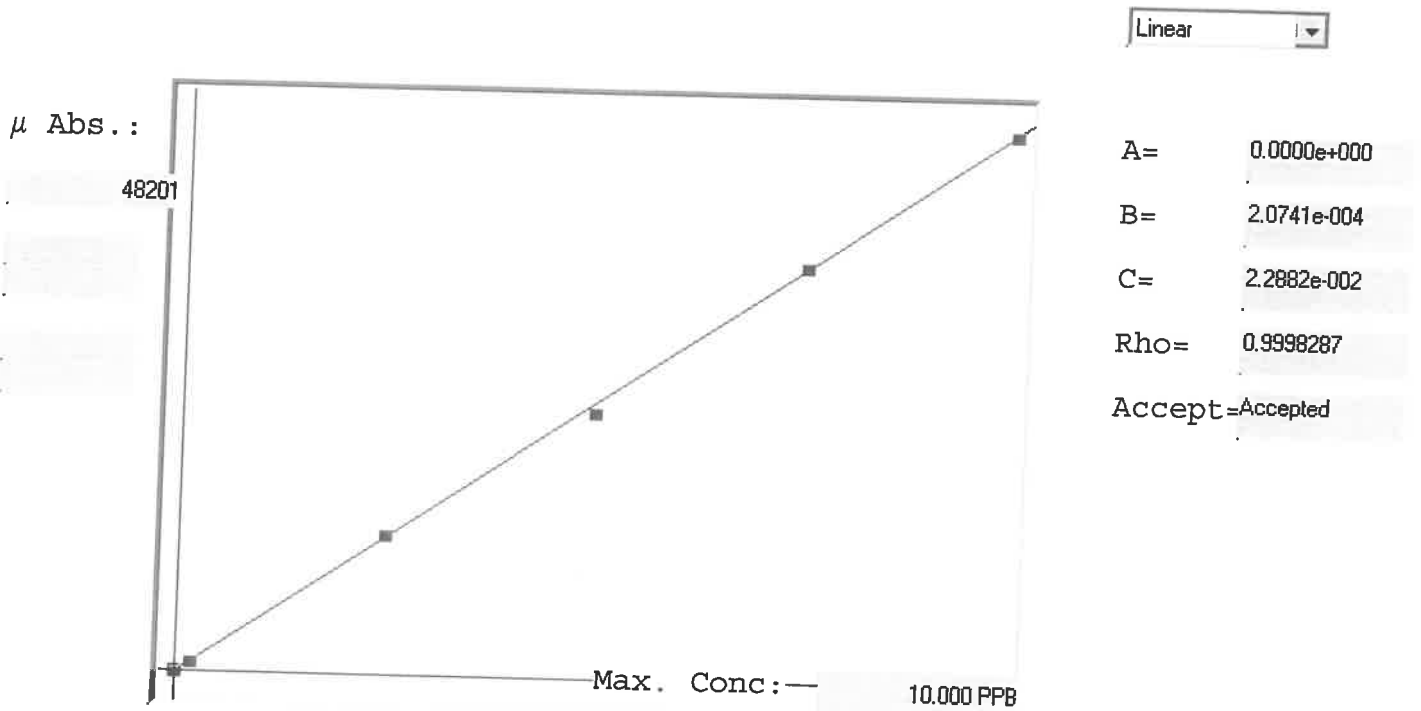

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.014	0.014	-44	0.000	-44				
0.2	0.200	0.210	0.010	901	0.0 %	901				
2.5	2.500	2.555	0.055	12207	0.0 %	12207				
5.0	5.000	4.852	-0.148	23284	0.0 %	23284				
7.5	7.500	7.549	0.049	36289	0.0 %	36289				
10.0	10.000	10.020	0.020	48201	0.0 %	48201				

0/10
152
3
0-1

LB135253 INSTRUMENT ID : CV1

Method: 7471B

Operator: Admin

Date of Analysis: 01 Apr 2025 13:32:36

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-44	-	0.0000	7471B	PPB	01 Apr 2025 13:32:51	S	Std
0.2 - 1	50.2	901	-	0.2000	7471B	PPB	01 Apr 2025 13:35:09	S	Std
2.5 - 1	52.5	12207	-	2.5000	7471B	PPB	01 Apr 2025 13:37:26	S	Std
5.0 - 1	55	23284	-	5.0000	7471B	PPB	01 Apr 2025 13:39:43	S	Std
7.5 - 1	57.7	36289	-	7.5000	7471B	PPB	01 Apr 2025 13:42:01	S	Std
10.0 - 1	59.0	48201	-	10.0000	7471B	PPB	01 Apr 2025 13:44:20	S	Std
ICV70 - 1	ICV70	18657	3.8925	-7471B	PPB	01 Apr 2025 13:47:16	U	SMPL	
ICB70 - 1	ICB70	-152	-0.0086	-7471B	PPB	01 Apr 2025 13:49:33	U	SMPL	
CCV15 - 1	CCV15	22995	4.7922	-7471B	PPB	01 Apr 2025 13:51:51	U	SMPL	
CCB15 - 1	CCB15	-145	-0.0072	-7471B	PPB	01 Apr 2025 13:54:06	U	SMPL	
CRA - 1	CRA	870	0.2033	-7471B	PPB	01 Apr 2025 13:56:26	U	SMPL	
HighStd - 1	HighStd	47244	9.8216	-7471B	PPB	01 Apr 2025 13:58:41	U	SMPL	
ChkStd - 1	ChkStd	30628	6.3754	-7471B	PPB	01 Apr 2025 14:00:56	U	SMPL	
PB167407BL - 1	PBS	-312	-0.0418	-7471B	PPB	01 Apr 2025 14:03:17	U	SMPL	
PB167407BS - 1	LCSS	18921	3.9472	-7471B	PPB	01 Apr 2025 14:08:18	U	SMPL	
Q1679-01 - 1	TP-10	1865	0.4097	-7471B	PPB	01 Apr 2025 14:10:35	U	SMPL	
Q1679-05 - 1	TP-9	1783	0.3927	-7471B	PPB	01 Apr 2025 14:12:53	U	SMPL	
Q1680-01 - 1	TP-4	3262	0.6994	-7471B	PPB	01 Apr 2025 14:31:09	U	SMPL	
Q1680-01DUP - 1	TP-4DUP	3042	0.6538	-7471B	PPB	01 Apr 2025 14:35:40	U	SMPL	
Q1680-01MS - 1	TP-4MS	21208	4.4216	-7471B	PPB	01 Apr 2025 14:37:55	U	SMPL	
CCV16 - 1	CCV16	22318	4.6518	-7471B	PPB	01 Apr 2025 14:40:11	U	SMPL	
CCB16 - 1	CCB16	-251	-0.0292	-7471B	PPB	01 Apr 2025 14:42:29	U	SMPL	
Q1680-01MSD - 1	TP-4MSD	20931	4.3641	-7471B	PPB	01 Apr 2025 14:44:47	U	SMPL	
Q1680-01LX5 - 1		832	0.1954	-7471B	PPB	01 Apr 2025 14:48:07	U	SMPL	
Q1680-01A - 1		21469	4.4757	-7471B	PPB	01 Apr 2025 14:50:22	U	SMPL	
Q1642-01DLX10 - 1		23352	4.8663	-7471B	PPB	01 Apr 2025 14:58:19	U	SMPL	
CCV17 - 1	CCV17	22519	4.6935	-7471B	PPB	01 Apr 2025 15:00:34	U	SMPL	
CCB17 - 1	CCB17	-271	-0.0333	-7471B	PPB	01 Apr 2025 15:02:54	U	SMPL	