

LG135344


7470A

INSTRUMENT ID: CV1

Linear

μ Abs.:

45223

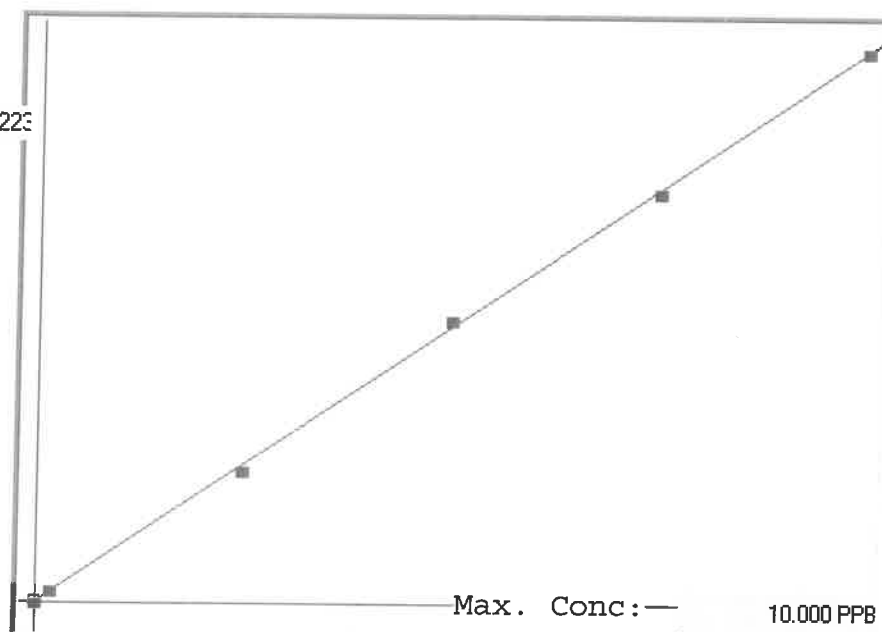

A= 0.0000e+000

B= 2.2104e-004

C= 1.0350e-003

Rho= 0.9998003

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%)
0.0	0.000	0.016	0.016	66	0.000	66	0				1
0.2	0.200	0.219	0.019	988	0.0 %	988					9
2.5	2.500	2.388	-0.112	10800	0.0 %	10800					-4
5.0	5.000	5.130	0.130	23204	0.0 %	23204					3
7.5	7.500	7.449	-0.051	33695	0.0 %	33695					-1
10.0	10.000	9.997	-0.003	45223	0.0 %	45223					0

LB135344 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 08 Apr 2025 13:30:45

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	S0	66	-	0.0000	7470A	PPB	08 Apr 2025 13:34:04	S	Std
0.2 - 1	S0.2	988	-	0.2000	7470A	PPB	08 Apr 2025 13:36:21	S	Std
2.5 - 1	S2.5	10800	-	2.5000	7470A	PPB	08 Apr 2025 13:38:38	S	Std
5.0 - 1	S5	23204	-	5.0000	7470A	PPB	08 Apr 2025 13:43:49	S	Std
7.5 - 1	S7.5	33695	-	7.5000	7470A	PPB	08 Apr 2025 13:48:59	S	Std
10.0 - 1	S10	45223	-	10.0000	7470A	PPB	08 Apr 2025 14:02:07	S	Std
ICV81 - 1	ICV81	17261	3.8165	-	7470A	PPB	08 Apr 2025 14:04:56	U	SMPL
ICB81 - 1	ICB81	-284	-0.0617	-	7470A	PPB	08 Apr 2025 14:07:12	U	SMPL
CCV46 - 1	CCV46	23042	5.0943	-	7470A	PPB	08 Apr 2025 14:09:29	U	SMPL
CCB46 - 1	CCB46	-329	-0.0717	-	7470A	PPB	08 Apr 2025 14:11:44	U	SMPL
CRA - 1	CRA	883	0.1962	-	7470A	PPB	08 Apr 2025 14:14:02	U	SMPL
HighStd - 1	HighStd	45241	10.0013	-	7470A	PPB	08 Apr 2025 14:16:17	U	SMPL
ChkStd - 1	ChkStd	28833	6.3744	-	7470A	PPB	08 Apr 2025 14:18:33	U	SMPL
PB167514BL - 1	PBW	-349	-0.0761	-	7470A	PPB	08 Apr 2025 14:20:51	U	SMPL
PB167514BS - 1	LCSW	15648	3.4599	-	7470A	PPB	08 Apr 2025 14:23:10	U	SMPL
Q1712-04 - 1	Z-05A	-210	-0.0454	-	7470A	PPB	08 Apr 2025 14:25:26	U	SMPL
Q1712-08 - 1	TT-7	-37	-0.0071	-	7470A	PPB	08 Apr 2025 14:27:45	U	SMPL
Q1732-04 - 1	TT-8	167	0.0379	-	7470A	PPB	08 Apr 2025 14:30:02	U	SMPL
Q1737-02 - 1	RT3069	26	0.0068	-	7470A	PPB	08 Apr 2025 14:32:19	U	SMPL
Q1740-04 - 1	TP-20	-23	-0.0040	-	7470A	PPB	08 Apr 2025 14:34:34	U	SMPL
CCV47 - 1	CCV47	22474	4.9688	-	7470A	PPB	08 Apr 2025 14:36:50	U	SMPL
CCB47 - 1	CCB47	-238	-0.0516	-	7470A	PPB	08 Apr 2025 14:39:05	U	SMPL
Q1740-04DUP - 1	TP-20DUP	40	0.0099	-	7470A	PPB	08 Apr 2025 14:41:23	U	SMPL
Q1740-04MS - 1	TP-20MS	14547	3.2166	-	7470A	PPB	08 Apr 2025 14:43:38	U	SMPL
Q1740-04MSD - 1	TP-20MSD	14763	3.2643	-	7470A	PPB	08 Apr 2025 14:45:53	U	SMPL
PB167467TB - 1	PB167467TB	-238	-0.0516	-	7470A	PPB	08 Apr 2025 14:48:11	U	SMPL
Q1740-04LX5 - 1		335	0.0751	-	7470A	PPB	08 Apr 2025 14:50:29	U	SMPL
Q1740-04A - 1		17257	3.8156	-	7470A	PPB	08 Apr 2025 14:52:45	U	SMPL
CCV48 - 1	CCV48	22497	4.9739	-	7470A	PPB	08 Apr 2025 14:55:02	U	SMPL
CCB48 - 1	CCB48	191	0.0433	-	7470A	PPB	08 Apr 2025 14:57:20	U	SMPL