

Ident	Instrument IC-1				Analyst: NF	Method: 300.0 / 9056A		Initial wt/ Analyst			
	Con F-	Con CL-	Con NO2	Con BR-		Con NO3	Con HPO4		Con SO4	Method name	date time
STD1	0	0	0	0	0	0	0	0	IC1-032125	3/21/2025 10:45	10 NF/IZ
STD2	0.421	0.619	0.631	2.075	0.523	1.052	3.247	IC1-032125	3/21/2025 11:07	10 NF/IZ	
STD3	0.795	1.199	1.203	3.994	1.001	1.993	5.998	IC1-032125	3/21/2025 11:28	10 NF/IZ	
STD4	0.977	1.475	1.468	4.904	1.226	2.407	7.216	IC1-032125	3/21/2025 11:50	10 NF/IZ	
STD5	1.993	3.009	2.995	10.03	2.493	4.968	14.842	IC1-032125	3/21/2025 12:11	10 NF/IZ	
STD6	4.034	5.988	5.986	19.975	5.011	10.256	30.502	IC1-032125	3/21/2025 12:32	10 NF/IZ	
STD7	4.979	7.51	7.517	25.022	6.247	12.323	36.695	IC1-032125	3/21/2025 12:54	10 NF/IZ	
ICV	2.031	3.038	3.08	10.364	2.568	5.199	15.269	IC1-032125	3/21/2025 13:37	10 NF/IZ	
ICB	0	0.122	0.08	0	0	0	0	IC1-032125	3/21/2025 13:58	10 NF/IZ	
CCV	2.123	3.246	3.205	10.778	2.74	5.408	15.725	IC1-032125	4/11/2025 8:49	10 NF/IZ	
CCB	0	0	0	0	0	0	0	IC1-032125	4/11/2025 9:14	10 NF/IZ	
Q1782-01	0.141	115.394	0	0.162	2.132	0	40.698	IC1-032125	4/11/2025 9:35	10 NF/IZ	
Q1782-03	0.224	331.594	0	0.314	2.72	0	16.551	IC1-032125	4/11/2025 9:57	10 NF/IZ	
Q1782-05	0.168	612.527	0	0.153	5.963	0	17.162	IC1-032125	4/11/2025 10:18	10 NF/IZ	
Q1782-07	0.167	615.72	0	0	6.341	0	17.163	IC1-032125	4/11/2025 10:40	10 NF/IZ	
Q1782-07MS	2.157	587.361	3.036	10.284	8.804	5.161	31.628	IC1-032125	4/11/2025 11:01	10 NF/IZ	
Q1782-07MSD	2.077	589.34	2.947	9.994	8.742	5.065	31.239	IC1-032125	4/11/2025 11:23	10 NF/IZ	
LB135389BLW	0	0	0	0	0	0	0	IC1-032125	4/11/2025 11:45	10 NF/IZ	
LB135389BSW	2.073	3.167	3.146	10.505	2.673	5.305	15.342	IC1-032125	4/11/2025 12:06	10 NF/IZ	
Q1782-01DLX2	0.079	51.843	0	0	1.073	0	27.749	IC1-032125	4/11/2025 12:28	10 NF/IZ	
CCV	2.072	3.18	3.145	10.576	2.674	5.315	15.357	IC1-032125	4/11/2025 13:11	10 NF/IZ	
CCB	0	0	0	0	0	0	0	IC1-032125	4/11/2025 13:32	10 NF/IZ	
Q1782-01DL2X50	0	1.668	0	0	0.086	0	1.377	IC1-032125	4/11/2025 14:37	10 NF/IZ	
Q1782-03DLX100	0	2.196	0	0	0.068	0	0.75	IC1-032125	4/11/2025 14:58	10 NF/IZ	
Q1782-05DLX100	0	3.912	0	0	0.098	0	0.965	IC1-032125	4/11/2025 15:20	10 NF/IZ	
Q1782-07DLX2	0.095	292.276	0	0	2.897	0	8.743	IC1-032125	4/11/2025 15:41	10 NF/IZ	
Q1782-07DL2X100	0	3.883	0	0	0.095	0	0.943	IC1-032125	4/11/2025 16:03	10 NF/IZ	
CCV	2.082	3.182	3.164	10.576	2.681	5.302	15.408	IC1-032125	4/11/2025 16:24	10 NF/IZ	
CCB	0	0	0	0	0	0	0	IC1-032125	4/11/2025 16:46	10 NF/IZ	

Clear table


Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A

ident	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0	0	0	0	0	0	0 IC1-012025	1/20/2025 11:14	10	NF/IZ
STD2	0.396	0.602	0.613	2.019	0.511	0.994	3.09 IC1-012025	1/20/2025 11:36	10	NF/IZ
STD3	0.835	1.258	1.254	4.184	1.047	2.089	6.324 IC1-012025	1/20/2025 11:57	10	NF/IZ
STD4	0.967	1.463	1.466	4.879	1.221	2.469	7.299 IC1-012025	1/20/2025 12:18	10	NF/IZ
STD5	1.996	2.973	2.959	9.912	2.468	4.936	14.741 IC1-012025	1/20/2025 12:40	10	NF/IZ
STD6	4.016	5.977	5.973	19.887	4.964	9.97	29.788 IC1-012025	1/20/2025 13:01	10	NF/IZ
STD7	4.99	7.527	7.535	25.119	6.289	12.542	37.258 IC1-012025	1/20/2025 13:23	10	NF/IZ

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	2.0000	0.5000	1.0000	1.0000	3.0000
STD3	0.8000	1.2000	4.0000	1.0000	2.0000	2.0000	6.0000
STD4	1.0000	1.5000	5.0000	1.2500	2.5000	2.5000	7.5000
STD5	2.0000	3.0000	10.0000	2.5000	5.0000	5.0000	15.0000
STD6	4.0000	6.0000	20.0000	5.0000	10.0000	10.0000	30.0000
STD7	5.0000	7.5000	25.0000	6.2500	12.5000	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1	-1.0000	0.3333	2.1667	0.9500	2.2000	-0.6000	3.0000
STD2	4.3750	4.8333	4.5000	4.6000	4.7000	4.4500	5.4000
STD3	-3.3000	-2.4667	-2.2667	-2.4200	-2.3200	-1.2400	-2.6800
STD4	-0.2000	-0.9000	-1.3667	-0.8800	-1.2800	-1.2800	-1.7267
STD5	0.4000	-0.3833	-0.4500	-0.5650	-0.7200	-0.3000	-0.7067
STD6	-0.2000	0.3600	0.4667	0.4760	0.6240	0.3360	0.6973

Fluoride (Anions)

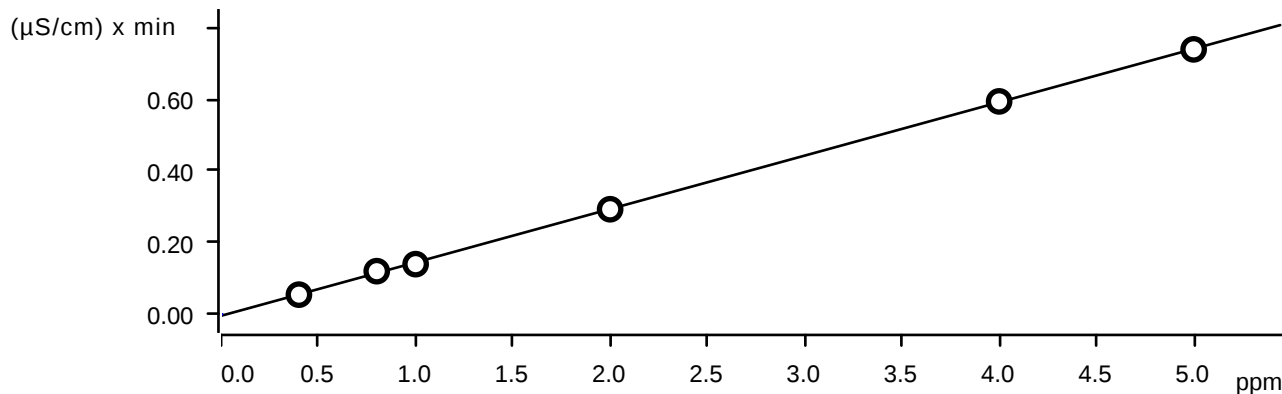


Function: $A = -4.02271E-3 + 0.0148839 \times Q$

Relative standard deviation 1.203859 %

Correlation coefficient 0.999923

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.400	10.0	1.0	1.0	0.055	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.120	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.140	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.293	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.594	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.739	STD7	2025-01-20 13:23:08 UTC-5	used

Chloride (Anions)

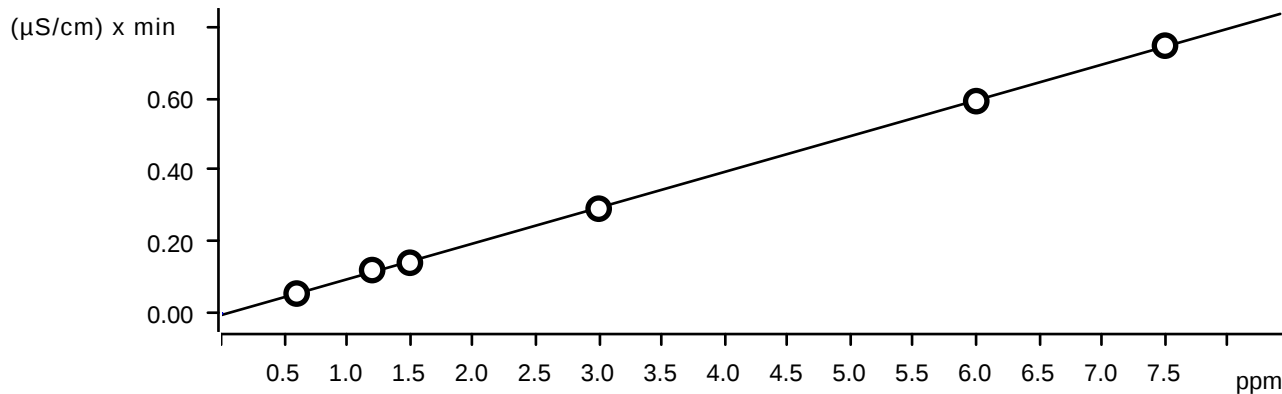

Function: $A = -4.62538E-3 + 9.98029E-3 \times Q$


Relative standard deviation 1.261416 %

Correlation coefficient 0.999916

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.055	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.121	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.141	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.292	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.592	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.747	STD7	2025-01-20 13:23:08 UTC-5	used

Nitrite (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

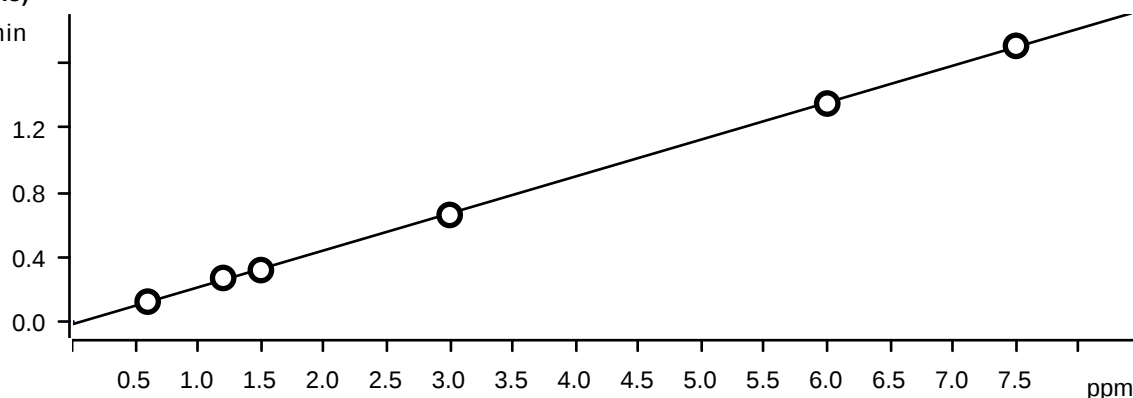

Function: $A = -0.0179856 + 0.0228967 \times Q$


Relative standard deviation 1.369596 %

Correlation coefficient 0.999903

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.122	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.269	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.318	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.660	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.350	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.707	STD7	2025-01-20 13:23:08 UTC-5	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

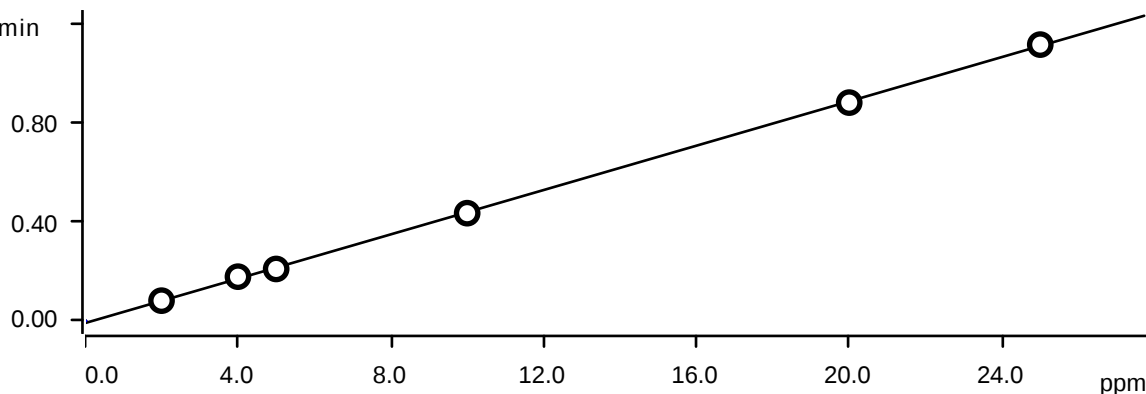

Function: $A = -8.89651E-3 + 4.46429E-3 \times Q$


Relative standard deviation 1.338167 %

Correlation coefficient 0.999906

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	2.000	10.0	1.0	1.0	0.081	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.178	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.209	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.434	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.879	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.112	STD7	2025-01-20 13:23:08 UTC-5	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

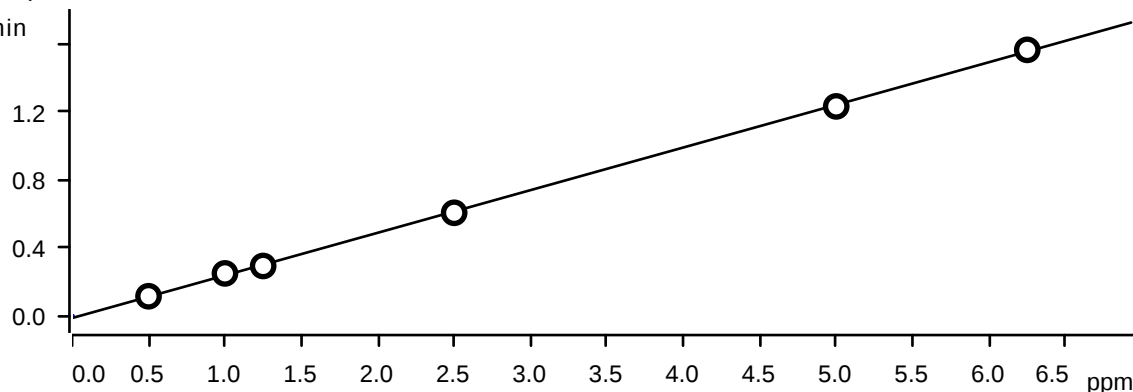

Function: $A = -0.0155875 + 0.0250988 \times Q$


Relative standard deviation 1.561944 %

Correlation coefficient 0.999873

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	0.500	10.0	1.0	1.0	0.113	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	1.000	10.0	1.0	1.0	0.247	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.291	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.604	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.230	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.563	STD7	2025-01-20 13:23:08 UTC-5	used

Phosphate (Anions)

($\mu\text{S/cm}$) $\times$ min

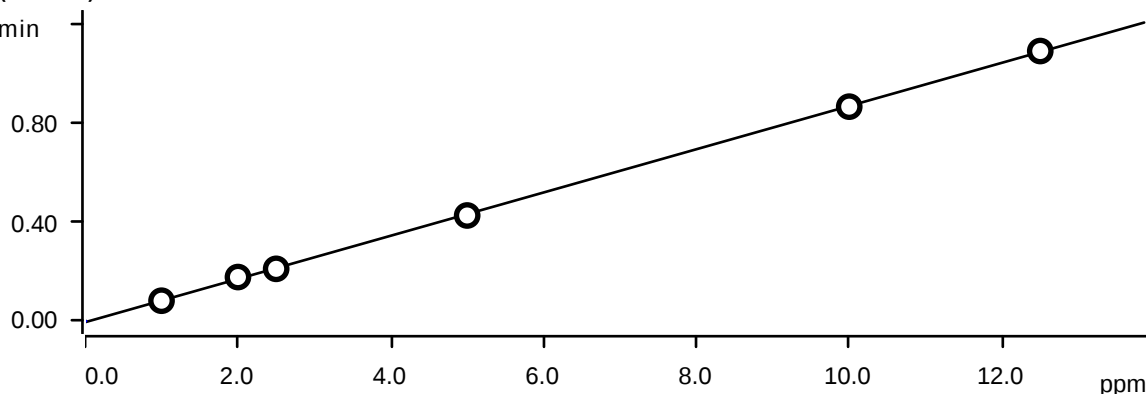


Function: $A = -4.38887E-3 + 8.70711E-3 \times Q$

Relative standard deviation 1.148005 %

Correlation coefficient 0.999929

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	1.000	10.0	1.0	1.0	0.082	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.177	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.211	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.425	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.864	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.088	STD7	2025-01-20 13:23:08 UTC-5	used

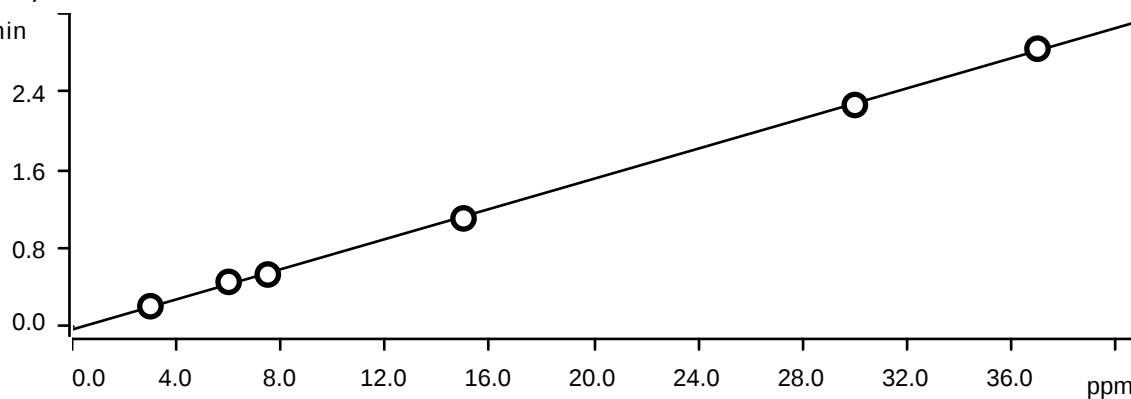Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0310554 + 7.70543E-3 \times Q$

Relative standard deviation 1.797524 %

Correlation coefficient 0.999831


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-01-20 11:14:39 UTC-5	used
Standard 2	1	3.000	10.0	1.0	1.0	0.207	STD2	2025-01-20 11:36:02 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.456	STD3	2025-01-20 11:57:26 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.531	STD4	2025-01-20 12:18:50 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.105	STD5	2025-01-20 12:40:15 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.264	STD6	2025-01-20 13:01:41 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.840	STD7	2025-01-20 13:23:08 UTC-5	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-01-20 11:14:39 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

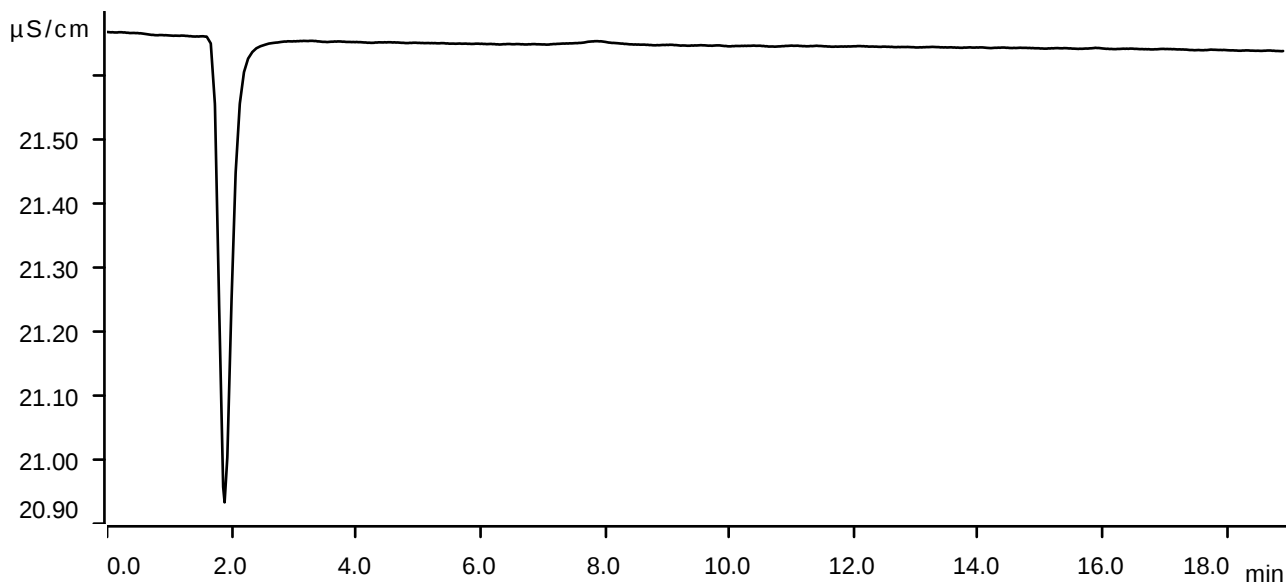Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-01-20 11:36:02 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

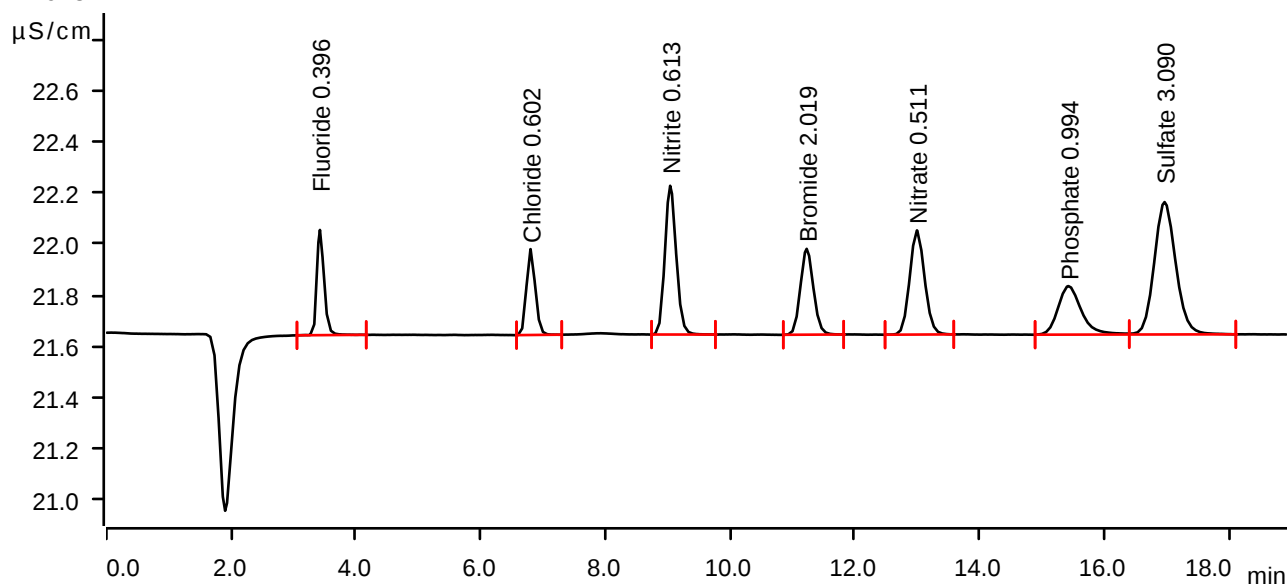

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.425	0.0549	0.411	0.396	Fluoride
2	6.802	0.0555	0.335	0.602	Chloride
3	9.040	0.1223	0.581	0.613	Nitrite
4	11.228	0.0813	0.335	2.019	Bromide
5	12.995	0.1126	0.407	0.511	Nitrate
6	15.423	0.0822	0.190	0.994	Phosphate
7	16.967	0.2070	0.517	3.090	Sulfate


Sample data

Ident STD3
 Sample type Standard 3
 Determination start 2025-01-20 11:57:26 UTC-5
 Method IC1-012025
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.99 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

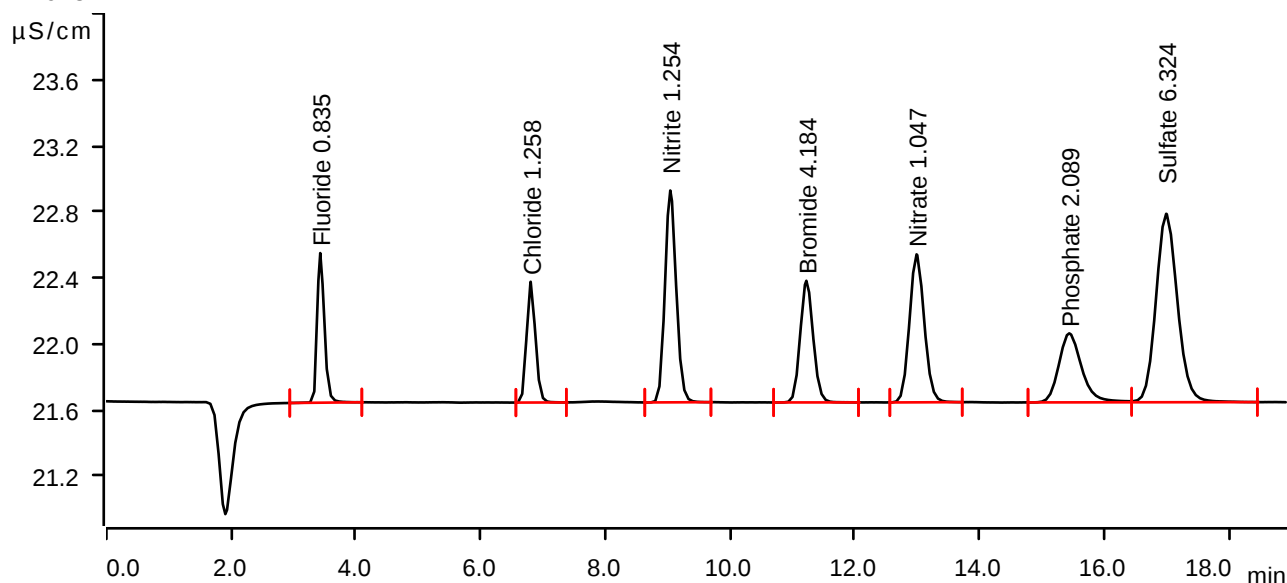

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.1203	0.906	0.835	Fluoride
2	6.803	0.1209	0.731	1.258	Chloride
3	9.042	0.2691	1.282	1.254	Nitrite
4	11.223	0.1779	0.736	4.184	Bromide
5	12.990	0.2472	0.896	1.047	Nitrate
6	15.438	0.1775	0.418	2.089	Phosphate
7	16.992	0.4562	1.141	6.324	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-01-20 12:18:50 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

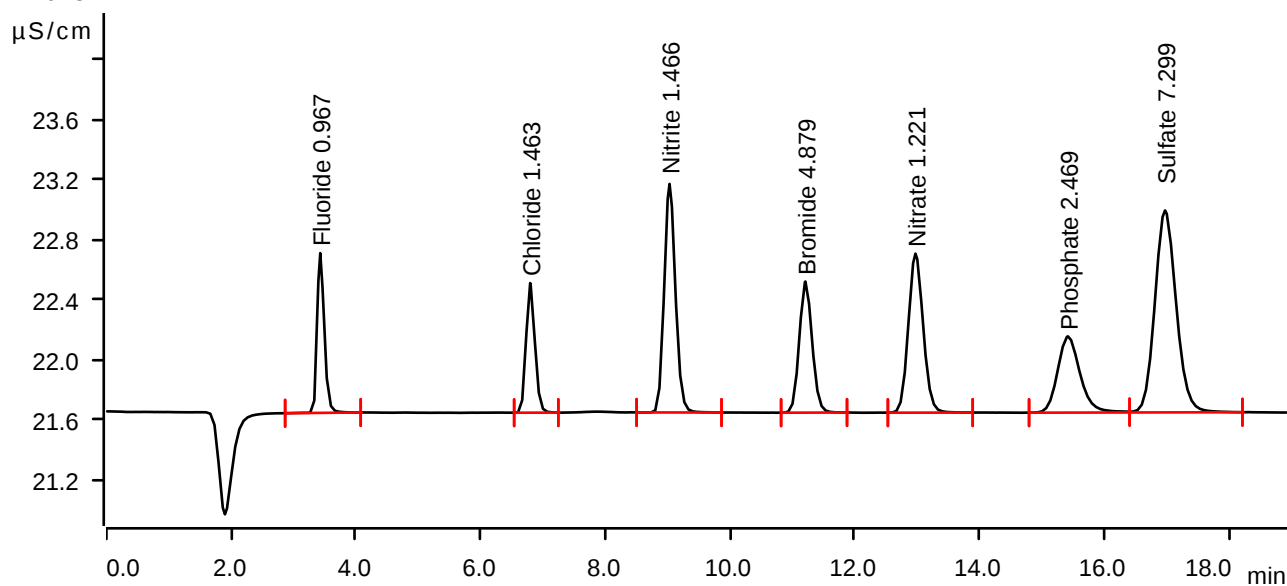

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.1399	1.061	0.967	Fluoride
2	6.795	0.1414	0.860	1.463	Chloride
3	9.030	0.3178	1.517	1.466	Nitrite
4	11.208	0.2089	0.870	4.879	Bromide
5	12.972	0.2908	1.056	1.221	Nitrate
6	15.417	0.2105	0.506	2.469	Phosphate
7	16.973	0.5314	1.341	7.299	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-01-20 12:40:15 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

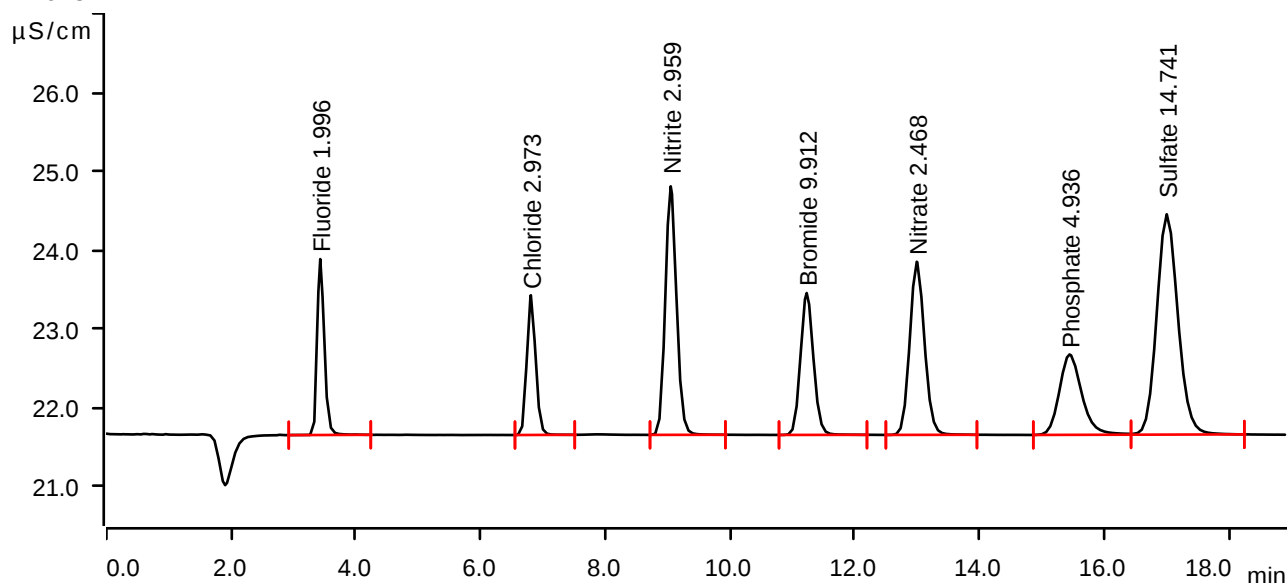

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.2930	2.233	1.996	Fluoride
2	6.807	0.2921	1.773	2.973	Chloride
3	9.048	0.6595	3.154	2.959	Nitrite
4	11.228	0.4336	1.801	9.912	Bromide
5	12.993	0.6039	2.197	2.468	Nitrate
6	15.443	0.4254	1.020	4.936	Phosphate
7	17.002	1.1048	2.795	14.741	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-01-20 13:01:41 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

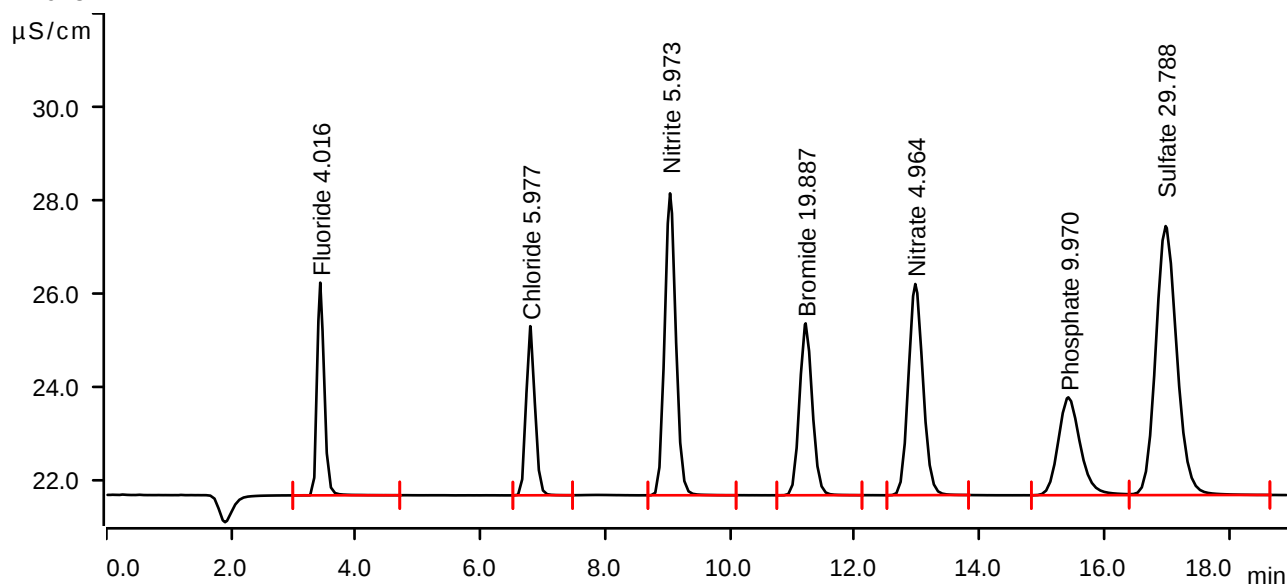

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.5937	4.568	4.016	Fluoride
2	6.797	0.5919	3.633	5.977	Chloride
3	9.038	1.3497	6.484	5.973	Nitrite
4	11.212	0.8789	3.691	19.887	Bromide
5	12.970	1.2302	4.535	4.964	Nitrate
6	15.423	0.8637	2.101	9.970	Phosphate
7	16.983	2.2643	5.777	29.788	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-01-20 13:23:08 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

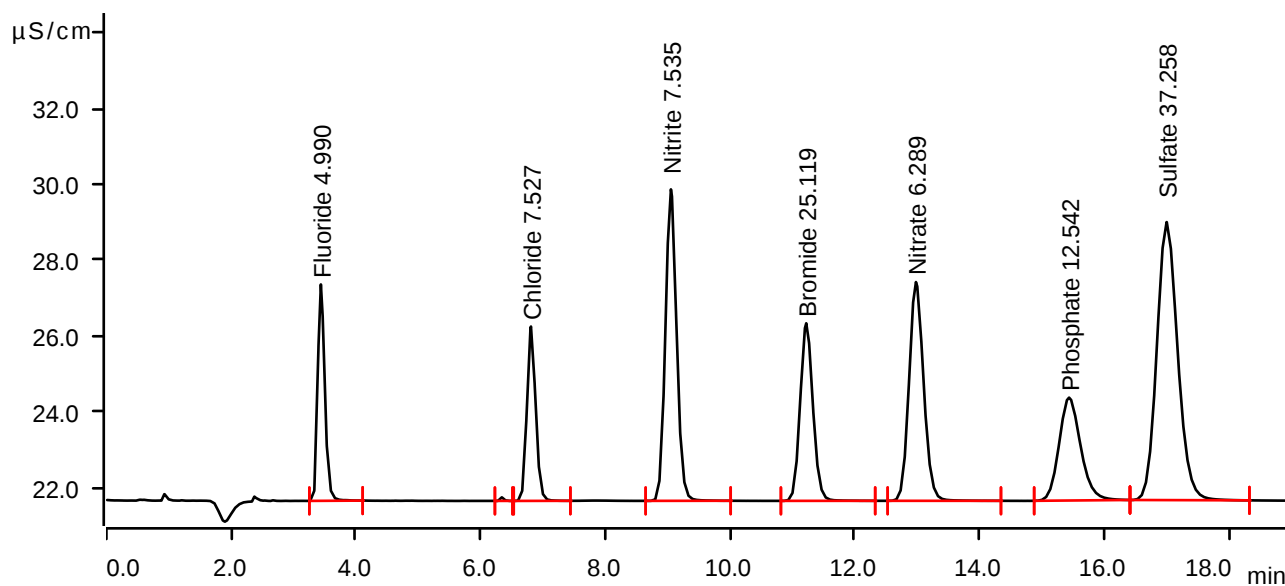

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.440	0.7387	5.703	4.990	Fluoride
2	6.342	0.0051	0.093	invalid	
3	6.808	0.7466	4.595	7.527	Chloride
4	9.052	1.7073	8.209	7.535	Nitrite
5	11.222	1.1125	4.681	25.119	Bromide
6	12.980	1.5629	5.766	6.289	Nitrate
7	15.435	1.0877	2.713	12.542	Phosphate
8	16.998	2.8398	7.327	37.258	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-01-20 13:44:36 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

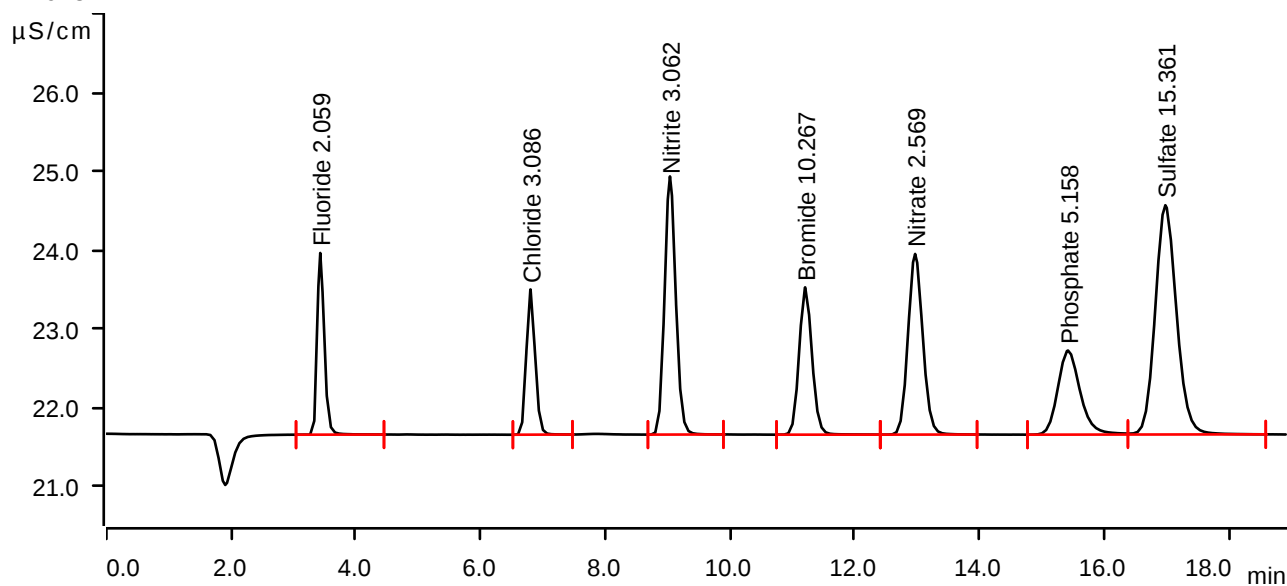

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.430	0.3025	2.306	2.059	Fluoride
2	6.798	0.3033	1.843	3.086	Chloride
3	9.037	0.6832	3.276	3.062	Nitrite
4	11.205	0.4495	1.869	10.267	Bromide
5	12.967	0.6293	2.293	2.569	Nitrate
6	15.418	0.4447	1.067	5.158	Phosphate
7	16.978	1.1525	2.909	15.361	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-01-20 14:06:05 UTC-5
Method IC1-012025
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

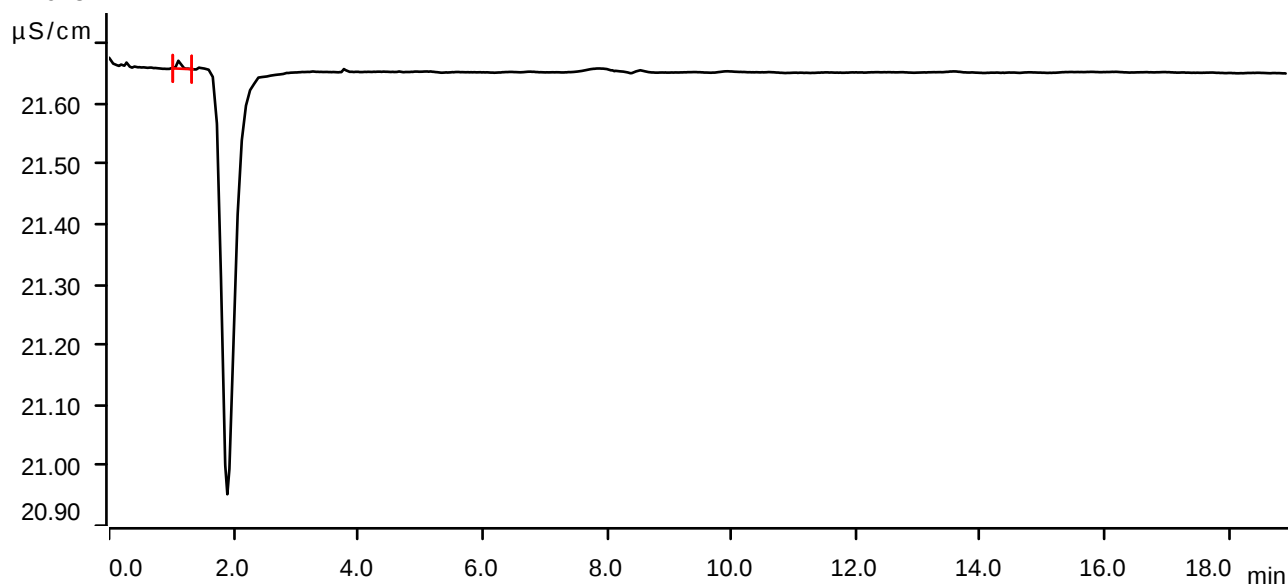

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	1.115	0.0010	0.013	invalid	


Sample data

Ident CCV
 Sample type Check standard 1
 Determination start 2025-04-11 08:49:37 UTC-4
 Method IC1-032125
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.43 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

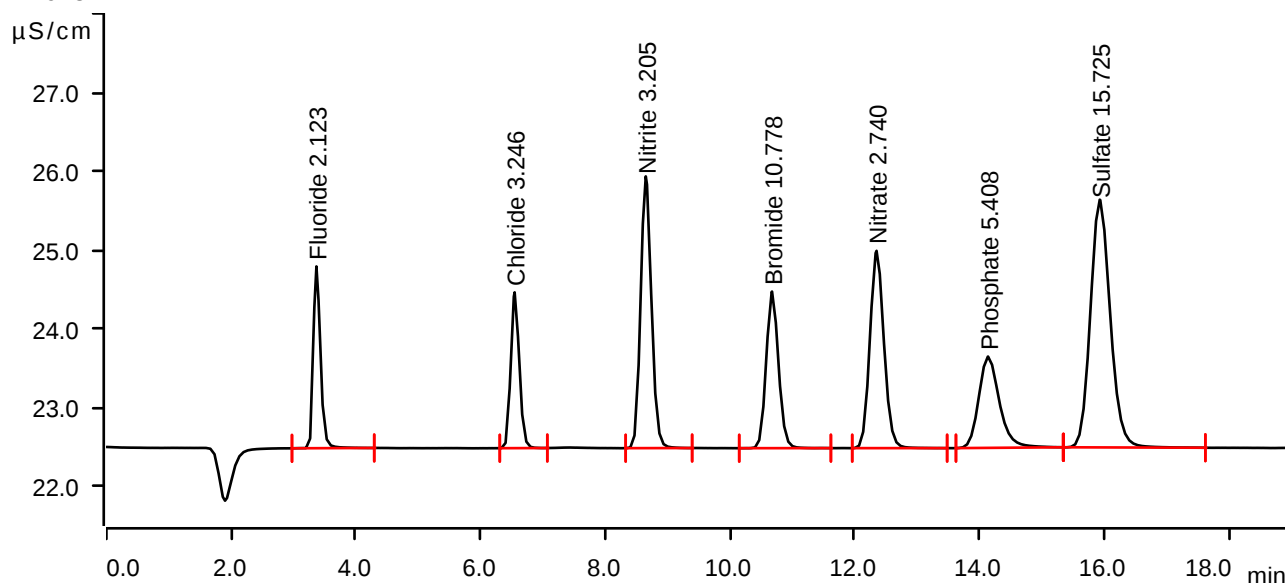


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.368	0.3032	2.306	2.123	Fluoride
2	6.547	0.3139	1.977	3.246	Chloride
3	8.648	0.6914	3.448	3.205	Nitrite
4	10.673	0.4547	1.987	10.778	Bromide
5	12.348	0.6529	2.504	2.740	Nitrate
6	14.137	0.4451	1.159	5.408	Phosphate
7	15.927	1.1580	3.144	15.725	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-04-11 09:14:13 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

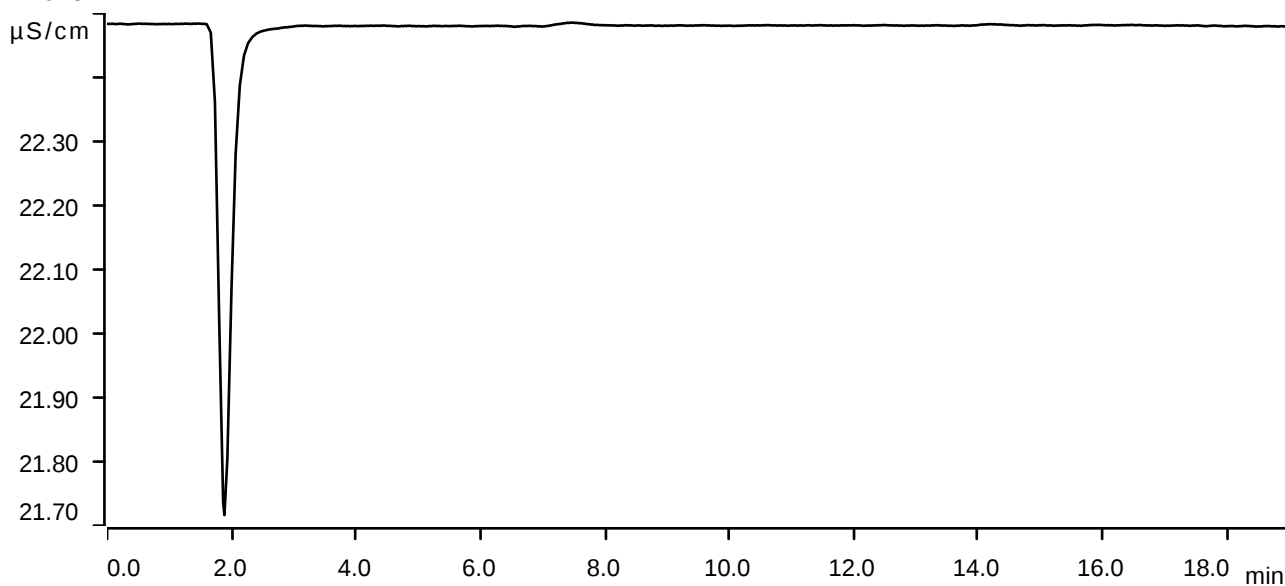Anions


Sample data

Ident Q1782-01
Sample type Sample
Determination start 2025-04-11 09:35:43 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.54 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

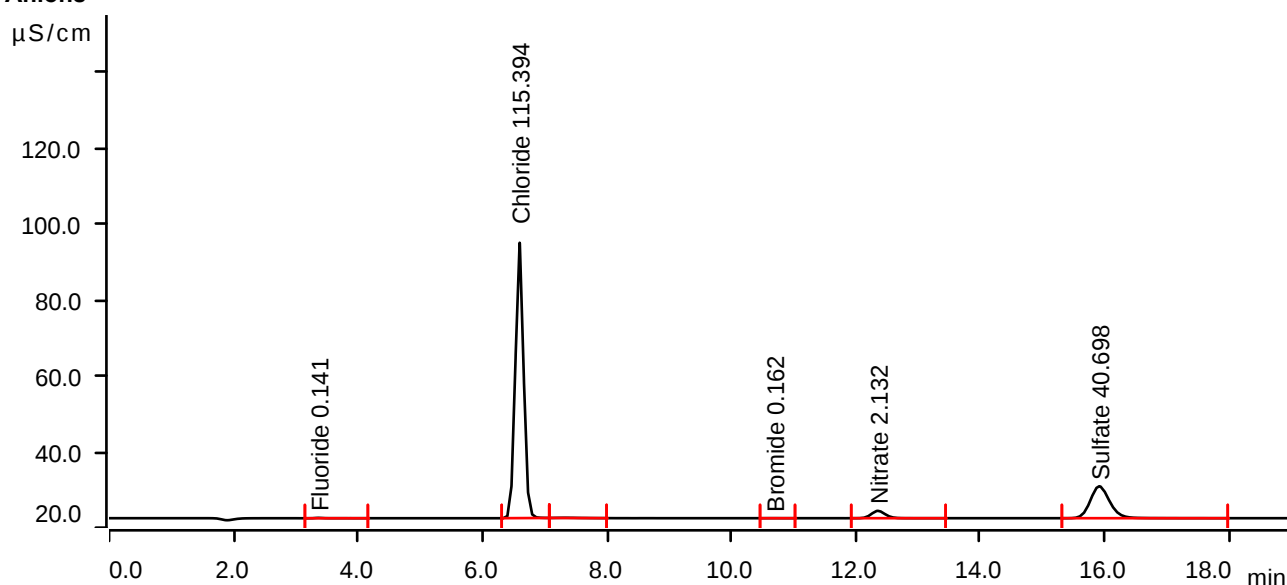

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.365	0.0164	0.100	0.141	Fluoride
2	6.598	11.2383	72.563	115.394	Chloride
3	7.313	0.0234	0.059	invalid	
4	10.688	0.0027	0.011	0.162	Bromide
5	12.355	0.5060	1.946	2.132	Nitrate
6	15.912	3.0477	8.427	40.698	Sulfate


Sample data

Ident Q1782-03
Sample type Sample
Determination start 2025-04-11 09:57:16 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

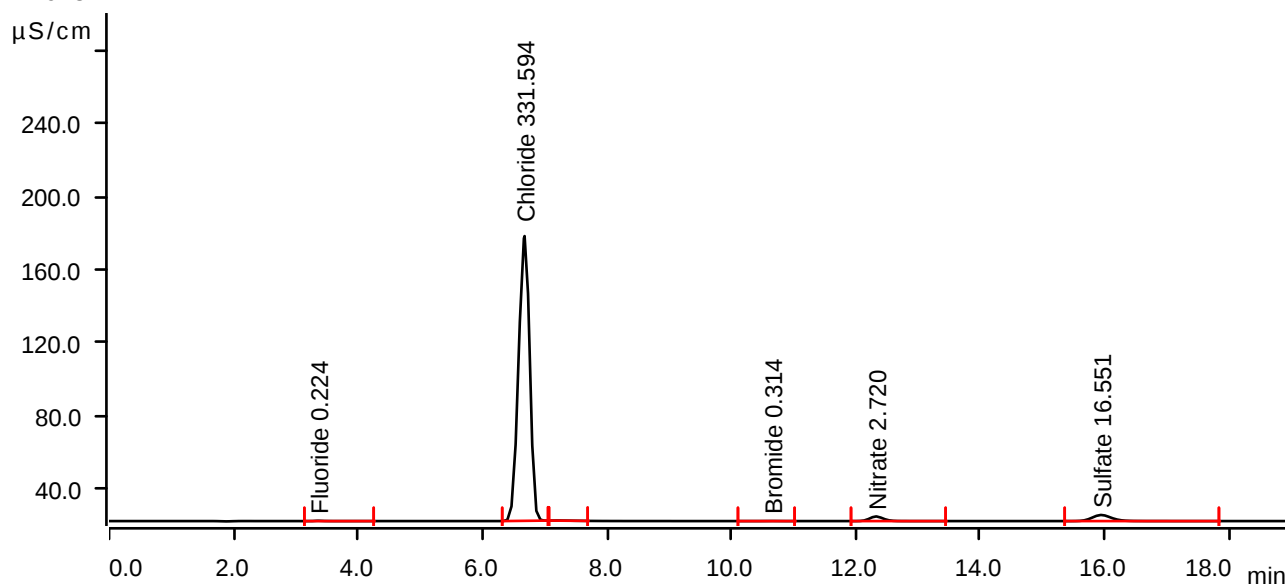

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.0284	0.184	0.224	Fluoride
2	6.678	32.2984	155.666	331.594	Chloride
3	7.190	0.0242	0.073	invalid	
4	10.655	0.0091	0.039	0.314	Bromide
5	12.325	0.6481	2.519	2.720	Nitrate
6	15.942	1.2205	3.334	16.551	Sulfate


Sample data

Ident Q1782-05
Sample type Sample
Determination start 2025-04-11 10:18:50 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

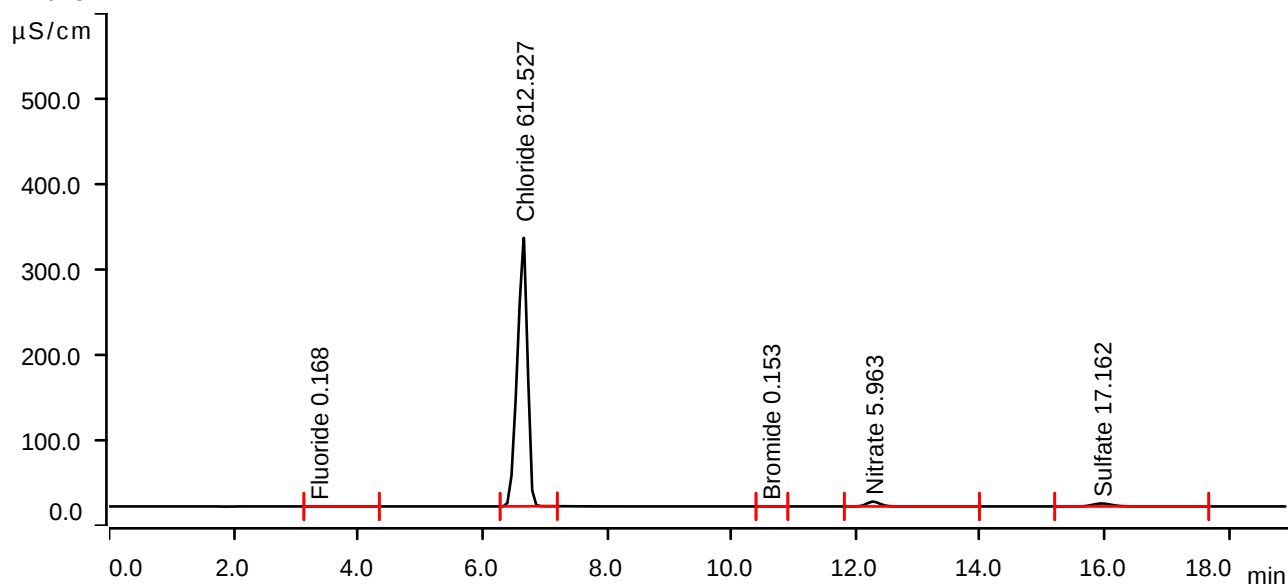

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.0203	0.131	0.168	Fluoride
2	6.663	59.6642	314.503	612.527	Chloride
3	10.623	0.0023	0.010	0.153	Bromide
4	12.277	1.4317	5.646	5.963	Nitrate
5	15.950	1.2668	3.469	17.162	Sulfate


Sample data

Ident Q1782-07
Sample type Sample
Determination start 2025-04-11 10:40:24 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

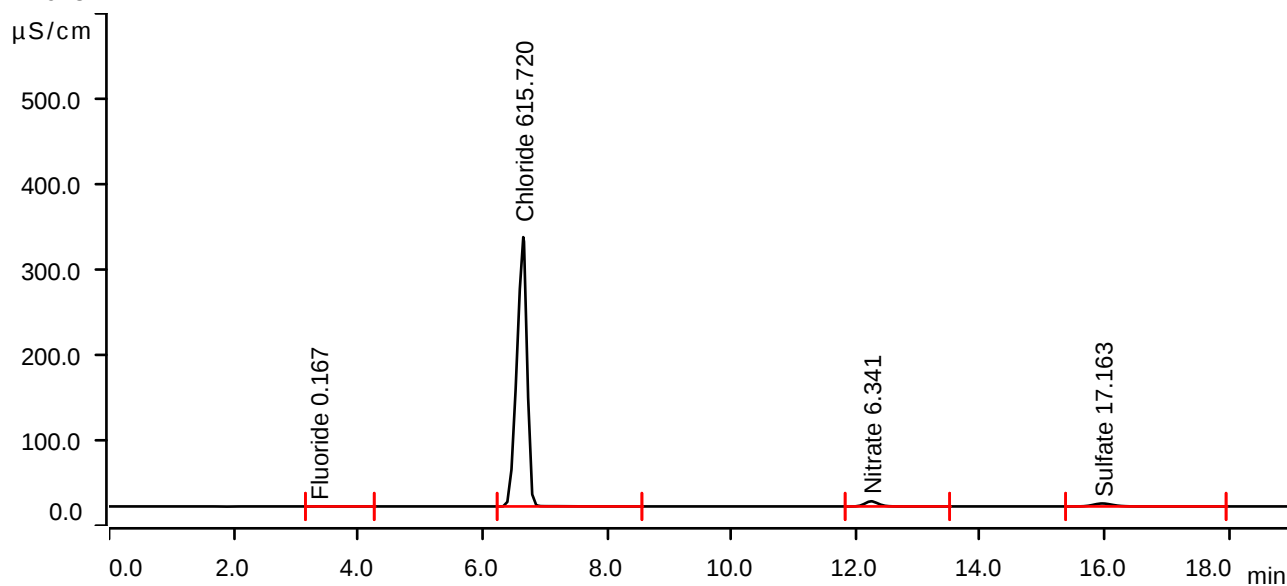

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.363	0.0202	0.132	0.167	Fluoride
2	6.657	59.9752	315.451	615.720	Chloride
3	12.247	1.5230	6.037	6.341	Nitrate
4	15.962	1.2669	3.472	17.163	Sulfate


Sample data

Ident Q1782-07MS
Sample type Sample
Determination start 2025-04-11 11:01:58 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

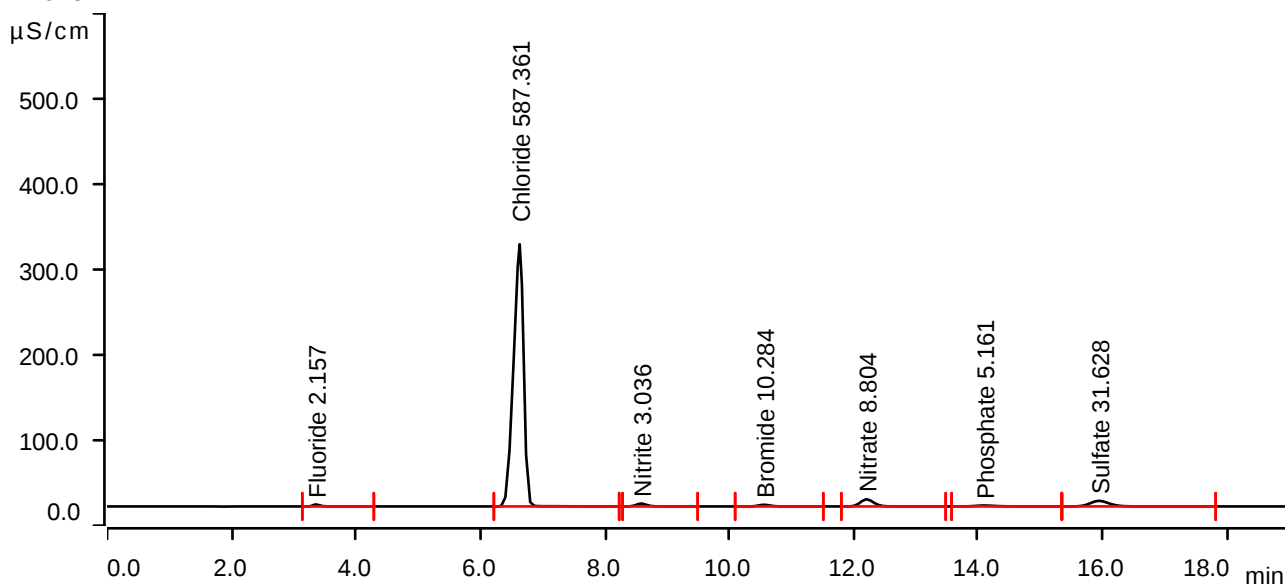

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.3081	2.330	2.157	Fluoride
2	6.632	57.2127	307.136	587.361	Chloride
3	8.583	0.6543	3.372	3.036	Nitrite
4	10.558	0.4337	1.942	10.284	Bromide
5	12.205	2.1181	8.475	8.804	Nitrate
6	14.097	0.4244	1.091	5.161	Phosphate
7	15.940	2.3614	6.557	31.628	Sulfate


Sample data

Ident Q1782-07MSD
Sample type Sample
Determination start 2025-04-11 11:23:33 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

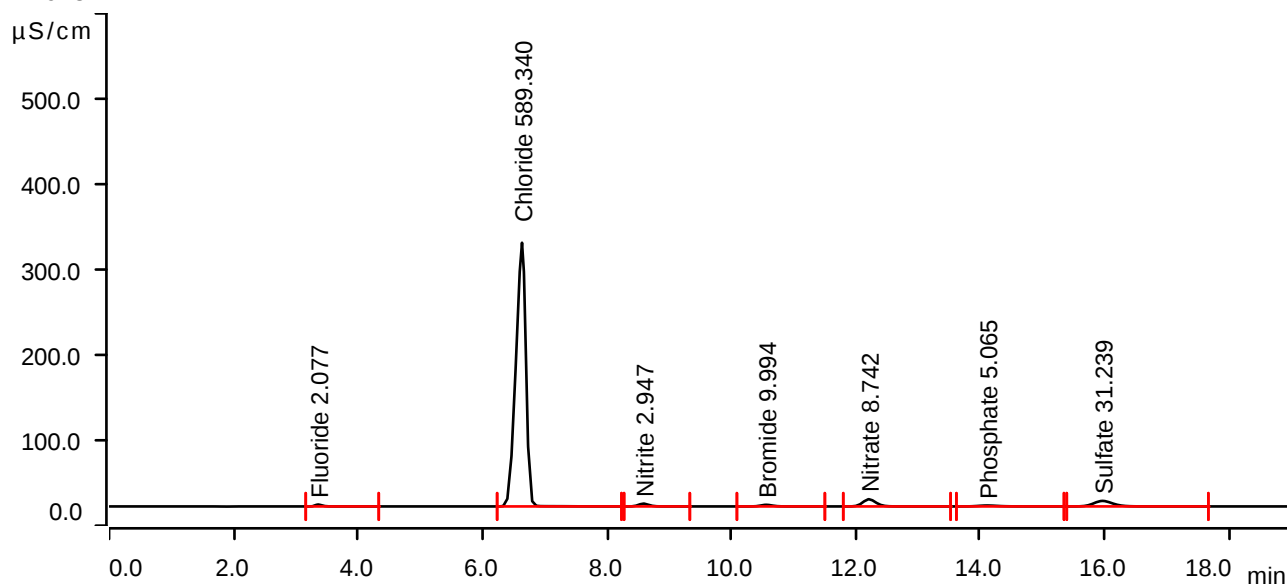


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.2965	2.244	2.077	Fluoride
2	6.637	57.4055	308.879	589.340	Chloride
3	8.588	0.6347	3.277	2.947	Nitrite
4	10.562	0.4214	1.889	9.994	Bromide
5	12.212	2.1030	8.423	8.742	Nitrate
6	14.110	0.4164	1.077	5.065	Phosphate
7	15.965	2.3319	6.480	31.239	Sulfate

Sample data

Ident LB135389BLW
Sample type Sample
Determination start 2025-04-11 11:45:06 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

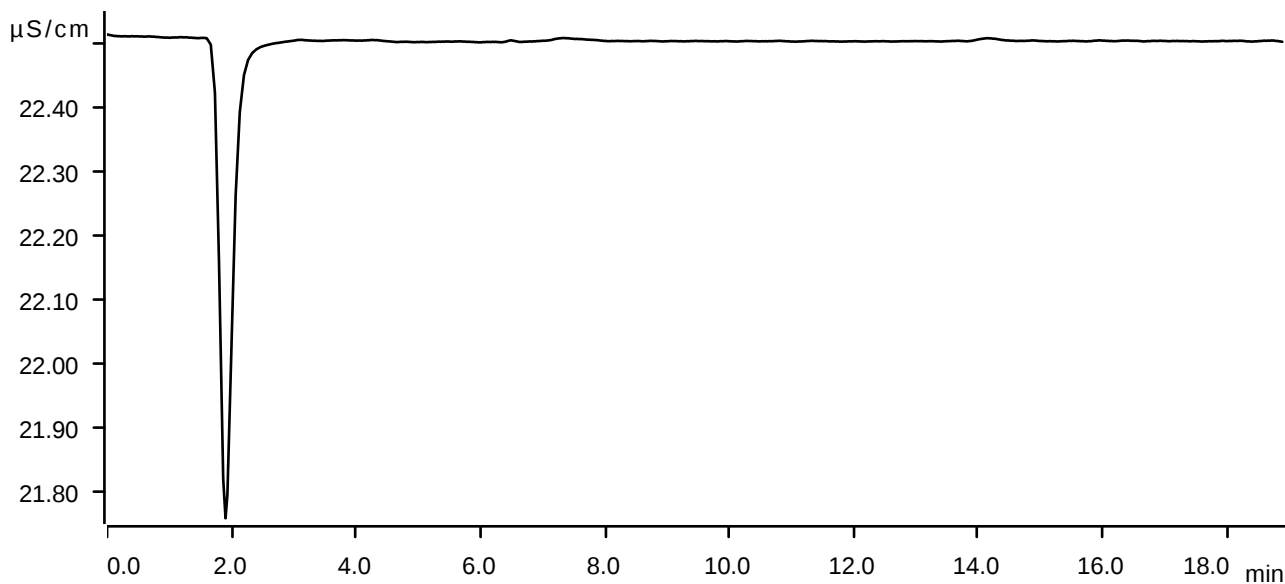Anions


Sample data

Ident LB135389BSW
Sample type Check standard 1
Determination start 2025-04-11 12:06:37 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

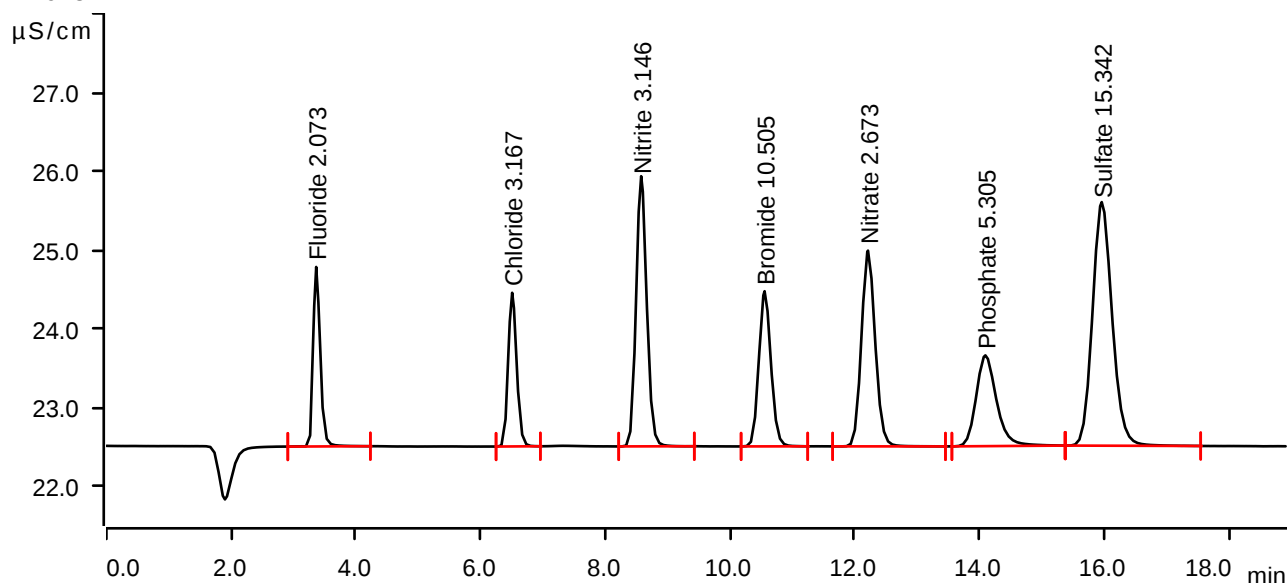

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.365	0.2959	2.277	2.073	Fluoride
2	6.507	0.3062	1.950	3.167	Chloride
3	8.575	0.6784	3.428	3.146	Nitrite
4	10.553	0.4431	1.969	10.505	Bromide
5	12.212	0.6367	2.484	2.673	Nitrate
6	14.093	0.4365	1.152	5.305	Phosphate
7	15.958	1.1290	3.091	15.342	Sulfate


Sample data

Ident Q1782-01DLX2
Sample type Sample
Determination start 2025-04-11 12:28:09 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

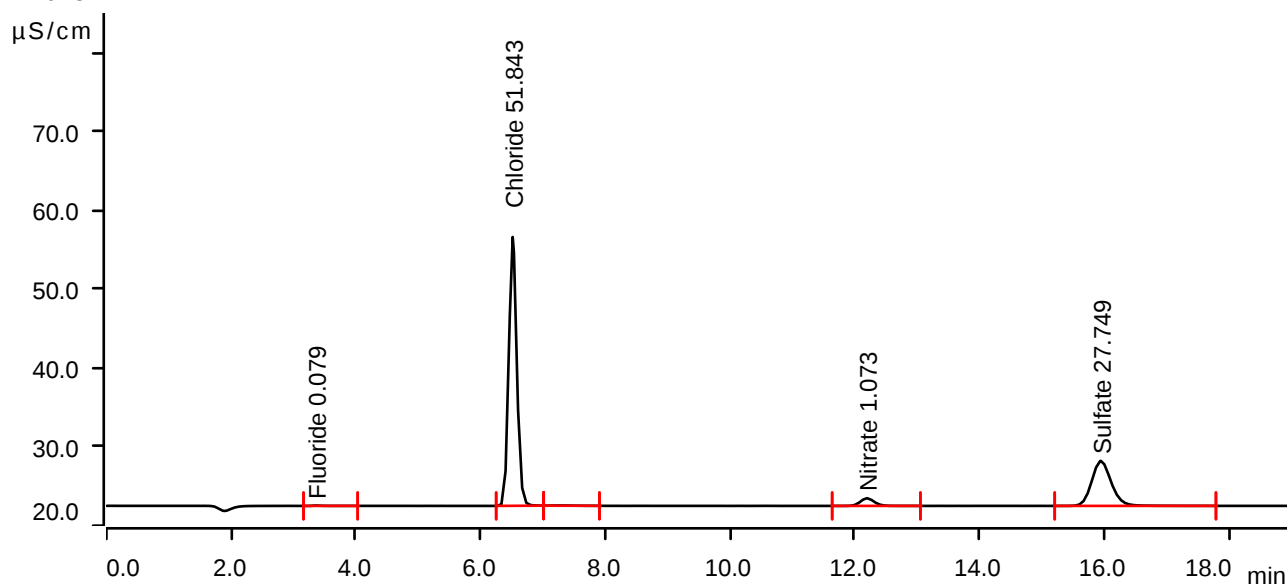

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.360	0.0075	0.048	0.079	Fluoride
2	6.515	5.0478	34.112	51.843	Chloride
3	7.270	0.0099	0.027	invalid	
4	12.195	0.2501	0.971	1.073	Nitrate
5	15.943	2.0679	5.713	27.749	Sulfate


Sample data

Ident CCV
 Sample type Check standard 1
 Determination start 2025-04-11 13:11:13 UTC-4
 Method IC1-032125
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.26 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

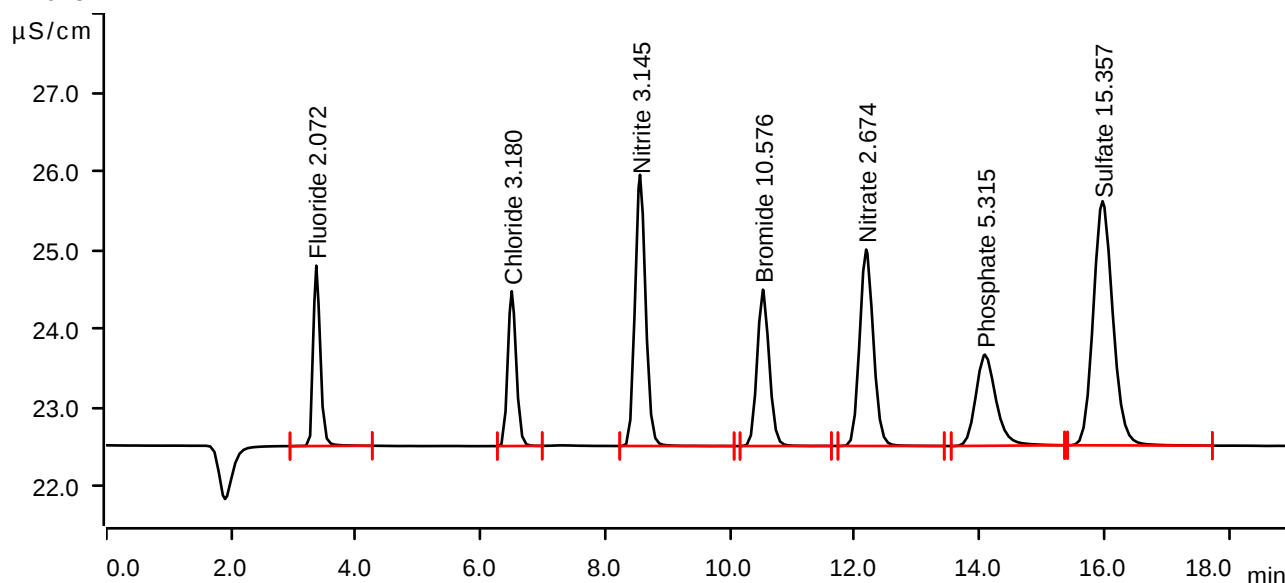


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.367	0.2958	2.288	2.072	Fluoride
2	6.500	0.3075	1.964	3.180	Chloride
3	8.557	0.6782	3.441	3.145	Nitrite
4	10.527	0.4461	1.985	10.576	Bromide
5	12.182	0.6369	2.493	2.674	Nitrate
6	14.085	0.4373	1.157	5.315	Phosphate
7	15.972	1.1302	3.099	15.357	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-04-11 13:32:43 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

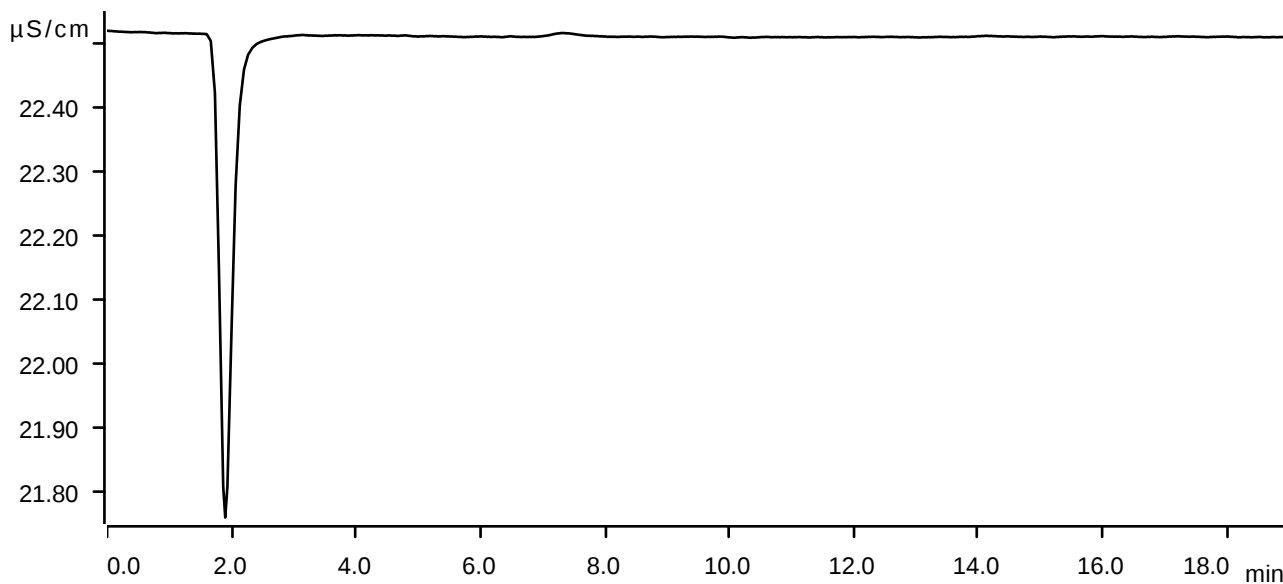Anions


Sample data

Ident Q1782-01DL2X50
Sample type Sample
Determination start 2025-04-11 14:37:14 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

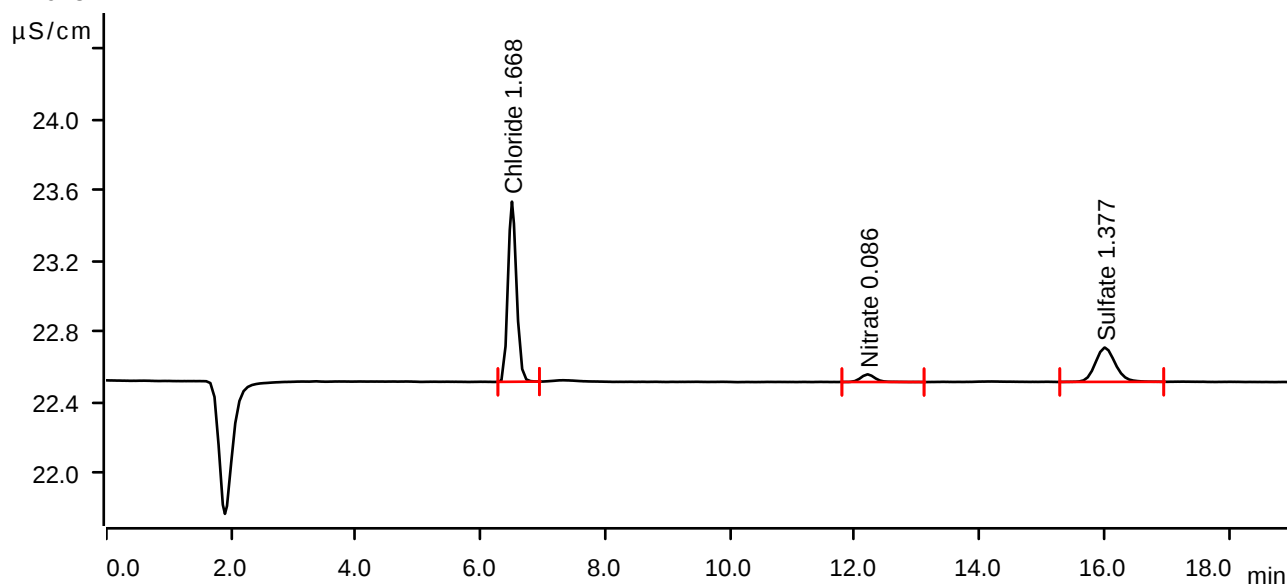

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.503	0.1602	1.020	1.668	Chloride
2	12.210	0.0116	0.043	0.086	Nitrate
3	16.010	0.0723	0.194	1.377	Sulfate


Sample data

Ident Q1782-03DLX100
Sample type Sample
Determination start 2025-04-11 14:58:42 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

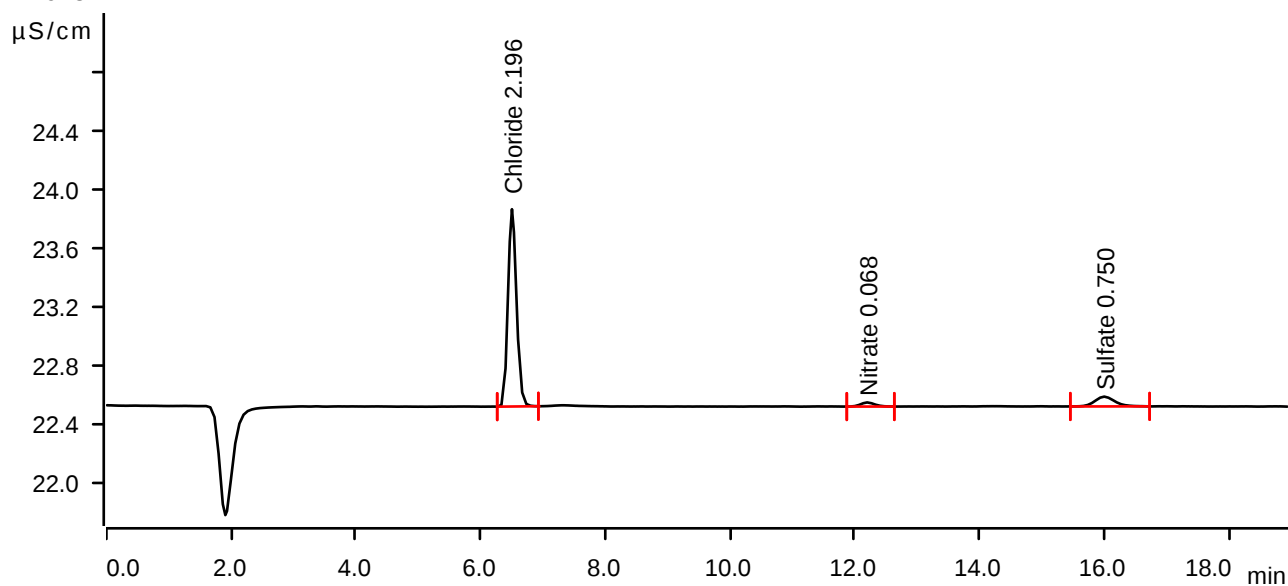

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.503	0.2116	1.348	2.196	Chloride
2	12.198	0.0073	0.028	0.068	Nitrate
3	15.997	0.0249	0.067	0.750	Sulfate


Sample data

Ident Q1782-05DLX100
Sample type Sample
Determination start 2025-04-11 15:20:09 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.15 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

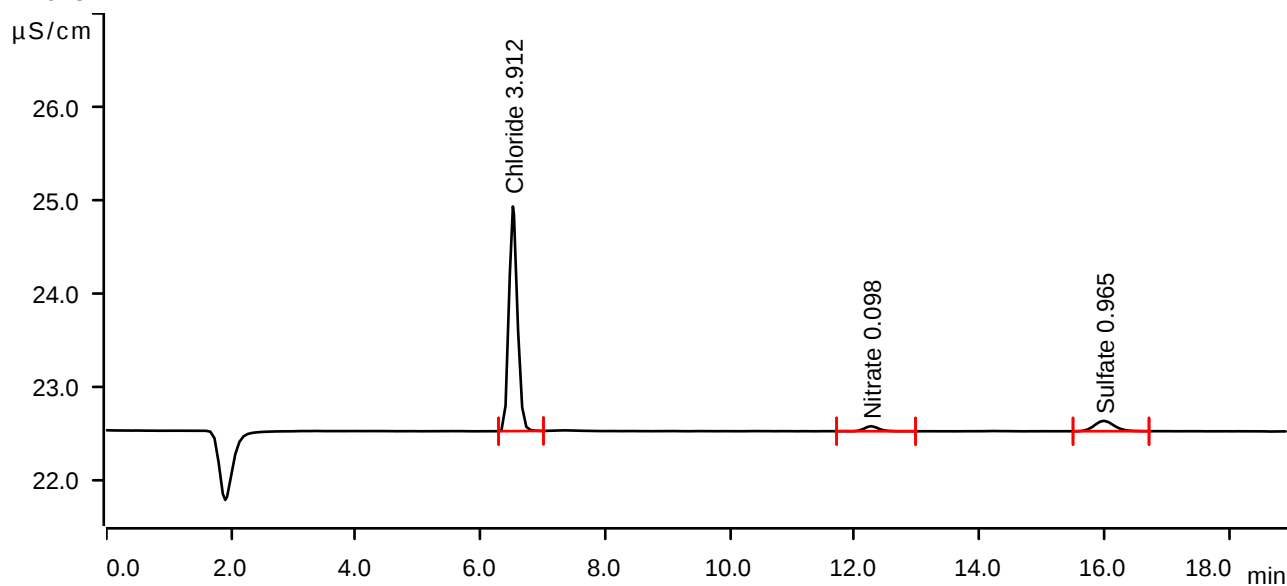

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.518	0.3788	2.412	3.912	Chloride
2	12.257	0.0145	0.054	0.098	Nitrate
3	15.990	0.0412	0.111	0.965	Sulfate


Sample data

Ident Q1782-07DLX2
Sample type Sample
Determination start 2025-04-11 15:41:36 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

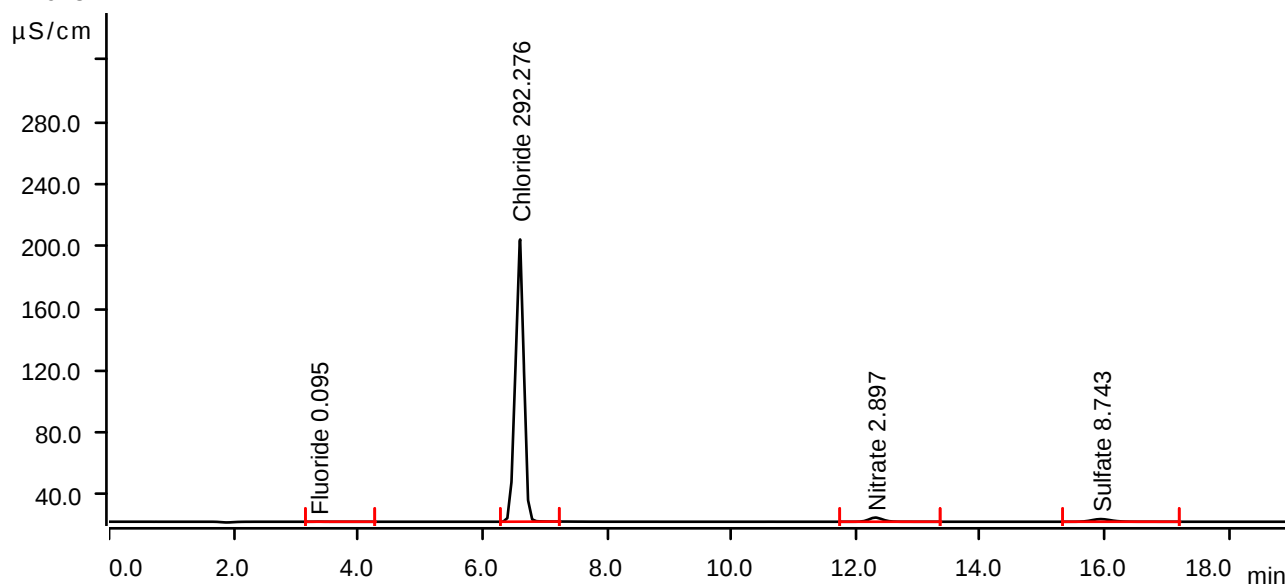

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.0098	0.065	0.095	Fluoride
2	6.607	28.4684	181.795	292.276	Chloride
3	12.315	0.6908	2.679	2.897	Nitrate
4	15.937	0.6297	1.716	8.743	Sulfate


Sample data

Ident Q1782-07DL2X100
Sample type Sample
Determination start 2025-04-11 16:03:05 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

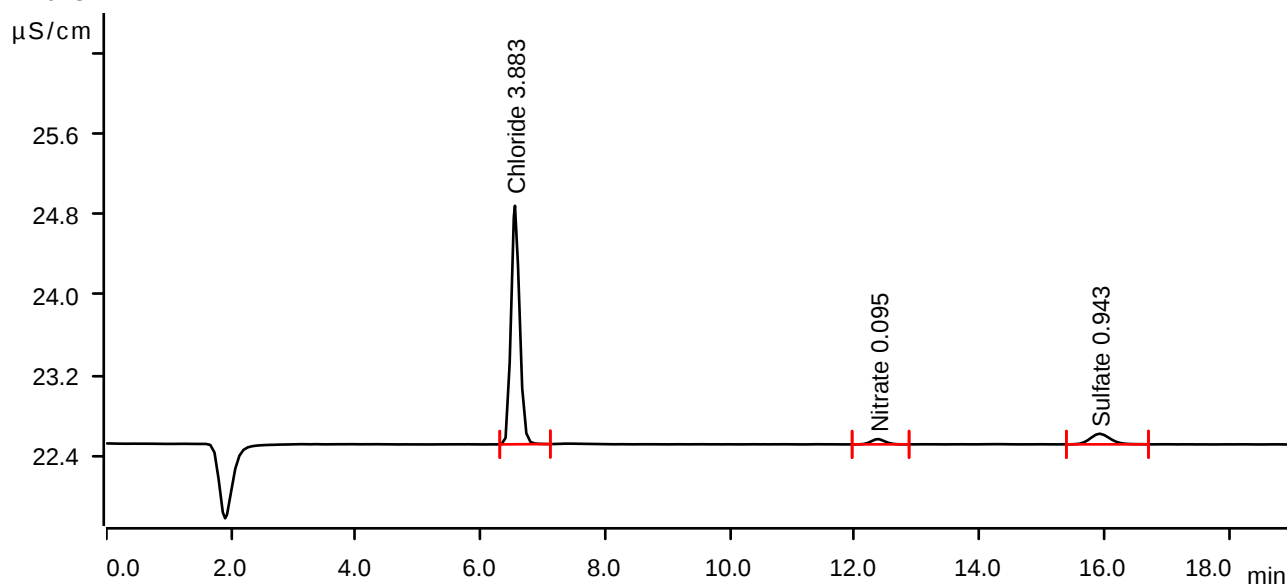

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.552	0.3760	2.375	3.883	Chloride
2	12.375	0.0137	0.052	0.095	Nitrate
3	15.925	0.0395	0.105	0.943	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-04-11 16:24:35 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

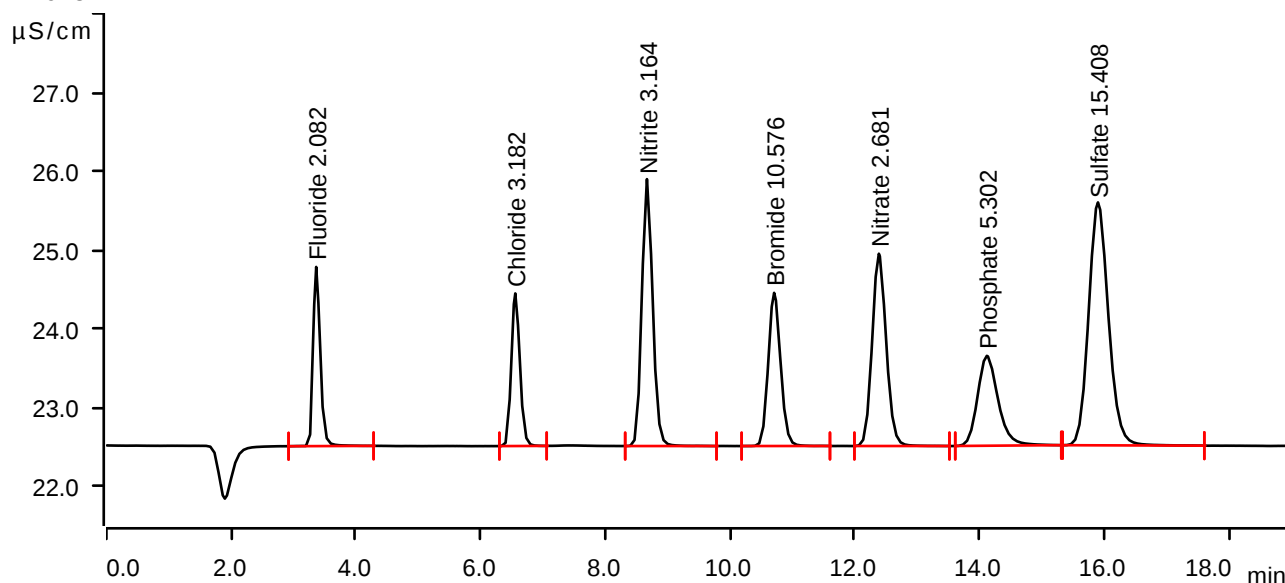

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.365	0.2973	2.273	2.082	Fluoride
2	6.557	0.3077	1.937	3.182	Chloride
3	8.668	0.6825	3.386	3.164	Nitrite
4	10.707	0.4462	1.944	10.576	Bromide
5	12.385	0.6386	2.441	2.681	Nitrate
6	14.117	0.4362	1.141	5.302	Phosphate
7	15.898	1.1340	3.083	15.408	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-04-11 16:46:05 UTC-4
Method IC1-032125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions