

Instrument IC-1			Analyst: NF		Method: 300.0 / 9056A					
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	Initial wt/ Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-042225	4/22/2025 10:37	10 NF/IZ
STD2	0.431	0.651	0.655	2.172	0.551	1.090	3.366	IC1-042225	4/22/2025 10:59	10 NF/IZ
STD3	0.810	1.217	1.222	4.049	1.011	2.010	6.091	IC1-042225	4/22/2025 11:20	10 NF/IZ
STD4	0.984	1.509	1.498	5.011	1.250	2.445	7.369	IC1-042225	4/22/2025 11:42	10 NF/IZ
STD5	1.938	2.914	2.916	9.735	2.424	4.860	14.361	IC1-042225	4/22/2025 12:03	10 NF/IZ
STD6	4.065	5.918	5.915	19.752	4.949	10.183	30.380	IC1-042225	4/22/2025 12:25	10 NF/IZ
STD7	4.972	7.591	7.594	25.280	6.316	12.412	36.933	IC1-042225	4/22/2025 12:46	10 NF/IZ
ICV	2.034	3.100	3.074	10.246	2.611	5.165	15.120	IC1-042225	4/22/2025 13:07	10 NF/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-042225	4/22/2025 13:58	10 NF/IZ
CCV	1.968	2.990	2.993	10.043	2.477	4.700	14.672	IC1-042225	5/16/2025 13:46	10 NF/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-042225	5/16/2025 14:08	10 NF/IZ
LB135822BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-042225	5/16/2025 14:29	10 NF/IZ
LB135822BSW	1.964	2.993	3.008	10.056	2.483	4.789	14.548	IC1-042225	5/16/2025 14:51	10 NF/IZ
Q2065-01	0.409	751.909	0.000	1.571	0.000	0.000	132.163	IC1-042225	5/16/2025 15:12	10 NF/IZ
Q2067-01	0.219	296.572	0.000	0.274	0.000	0.000	7.052	IC1-042225	5/16/2025 15:34	10 NF/IZ
Q2067-01MS	2.190	285.329	3.085	10.451	2.581	4.950	21.576	IC1-042225	5/16/2025 15:55	10 NF/IZ
Q2067-01MSD	2.223	285.131	3.098	10.500	2.596	5.072	21.684	IC1-042225	5/16/2025 16:17	10 NF/IZ
Q2068-03	0.609	98.816	0.200	0.396	0.291	0.316	14.260	IC1-042225	5/16/2025 16:39	10 NF/IZ
CCV	1.973	2.995	3.008	10.030	2.488	5.041	14.585	IC1-042225	5/16/2025 17:21	10 NF/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-042225	5/16/2025 17:43	10 NF/IZ


Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A									
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	Initial wt/ Final
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-042225	10 NF/IZ
STD2	0.4310	0.6510	0.6550	2.1720	0.5510	1.0900	3.3660	IC1-042225	10 NF/IZ
STD3	0.8100	1.2170	1.2220	4.0490	1.0110	2.0100	6.0910	IC1-042225	10 NF/IZ
STD4	0.9840	1.5090	1.4980	5.0110	1.2500	2.4450	7.3690	IC1-042225	10 NF/IZ
STD5	1.9380	2.9140	2.9160	9.7350	2.4240	4.8600	14.3610	IC1-042225	10 NF/IZ
STD6	4.0650	5.9180	5.9150	19.7520	4.9490	10.1830	30.3800	IC1-042225	10 NF/IZ
STD7	4.9720	7.5910	7.5940	25.2800	6.3160	12.4120	36.9330	IC1-042225	10 NF/IZ

ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000

ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4
STD1							
STD2	7.7500	8.5000	9.1667	8.6000	10.2000	9.0000	12.2000
STD3	1.2500	1.4167	1.8333	1.2250	1.1000	0.5000	1.5167
STD4	-1.6000	0.6000	-0.1333	0.2200	0.0000	-2.2000	-1.7467
STD5	-3.1000	-2.8667	-2.8000	-2.6500	-3.0400	-2.8000	-4.2600
STD6	1.6250	-1.3667	-1.4167	-1.2400	-1.0200	1.8300	1.2667
STD7	-0.5600	1.2133	1.2533	1.1200	1.0560	-0.7040	-0.1811

Fluoride (Anions)

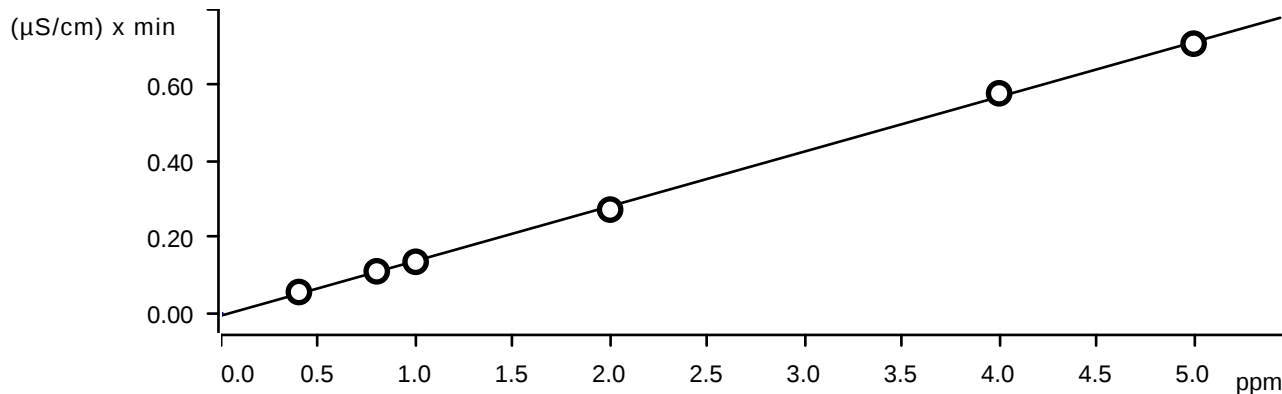


Function: $A = - 6.13443\text{E-}3 + 0.0144025 \times Q$

Relative standard deviation 2.337762 %

Correlation coefficient 0.999714

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-04-22 10:37:58 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.056	STD2	2025-04-22 10:59:20 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.110	STD3	2025-04-22 11:20:44 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.136	STD4	2025-04-22 11:42:09 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.273	STD5	2025-04-22 12:03:34 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.579	STD6	2025-04-22 12:25:01 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.710	STD7	2025-04-22 12:46:28 UTC-4	used

Chloride (Anions)

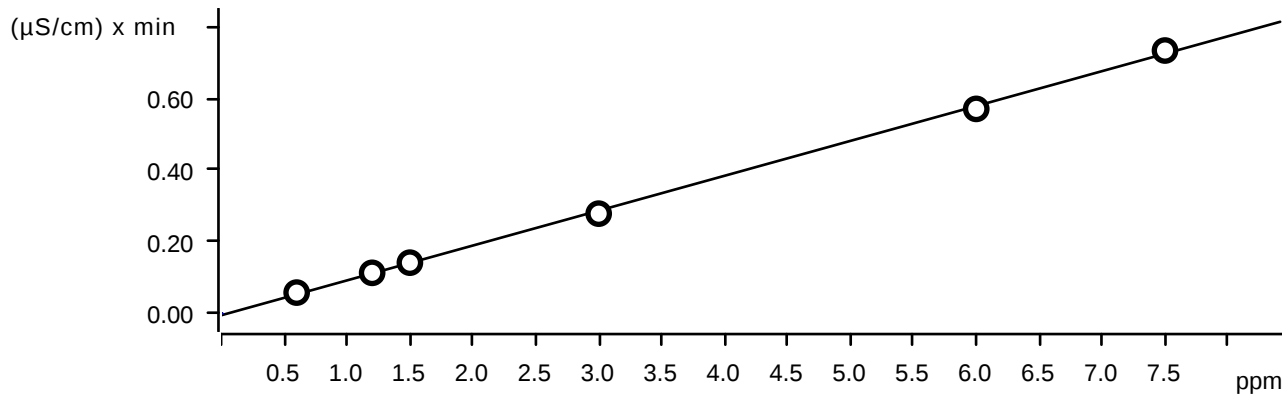

Function: $A = - 5.12446\text{E-}3 + 9.72422\text{E-}3 \times Q$


Relative standard deviation 2.452549 %

Correlation coefficient 0.999683

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-04-22 10:37:58 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.058	STD2	2025-04-22 10:59:20 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.113	STD3	2025-04-22 11:20:44 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.142	STD4	2025-04-22 11:42:09 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.278	STD5	2025-04-22 12:03:34 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.570	STD6	2025-04-22 12:25:01 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.733	STD7	2025-04-22 12:46:28 UTC-4	used

Nitrite (Anions)

($\mu\text{S/cm}$) $\times$ min

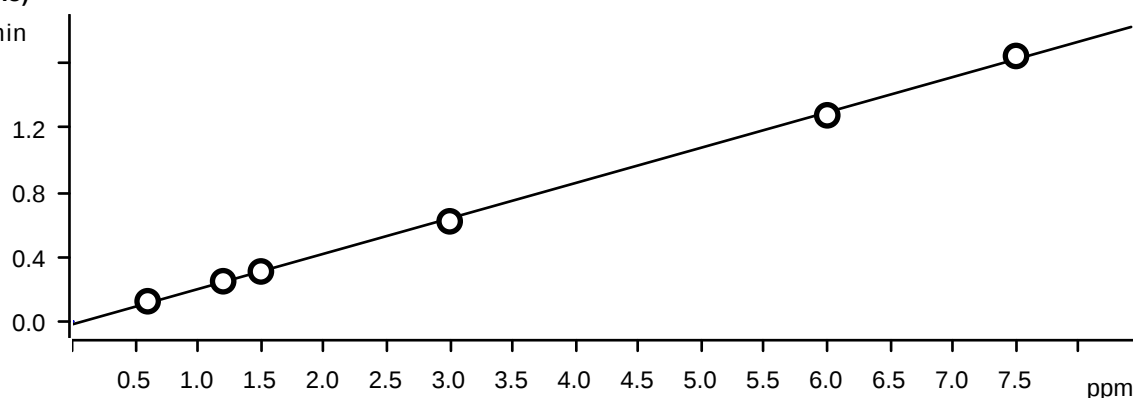

Function: $A = -0.0187238 + 0.0219021 \times Q$


Relative standard deviation 2.531721 %

Correlation coefficient 0.999669

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-04-22 10:37:58 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.125	STD2	2025-04-22 10:59:20 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.249	STD3	2025-04-22 11:20:44 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.309	STD4	2025-04-22 11:42:09 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.620	STD5	2025-04-22 12:03:34 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.277	STD6	2025-04-22 12:25:01 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.644	STD7	2025-04-22 12:46:28 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

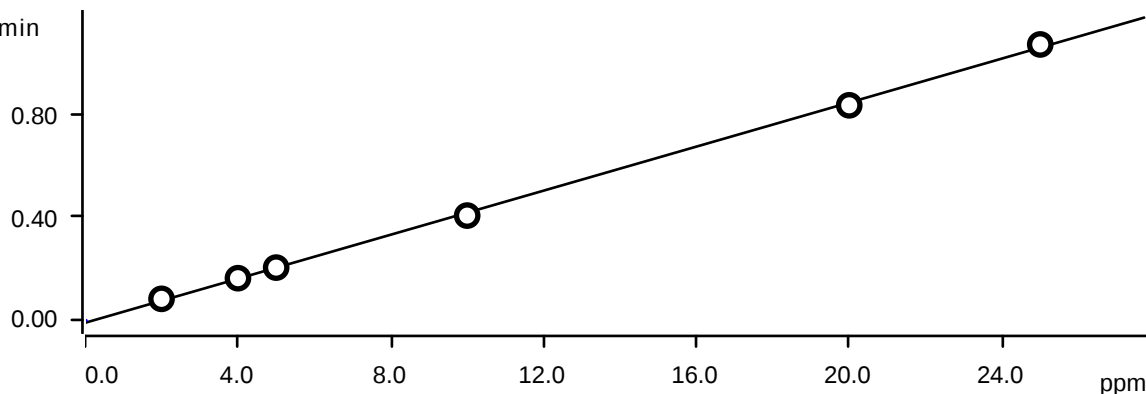

Function: $A = -9.36439E-3 + 4.26318E-3 \times Q$


Relative standard deviation 2.280508 %

Correlation coefficient 0.999728

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-04-22 10:37:58 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.083	STD2	2025-04-22 10:59:20 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.163	STD3	2025-04-22 11:20:44 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.204	STD4	2025-04-22 11:42:09 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.406	STD5	2025-04-22 12:03:34 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.833	STD6	2025-04-22 12:25:01 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.068	STD7	2025-04-22 12:46:28 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

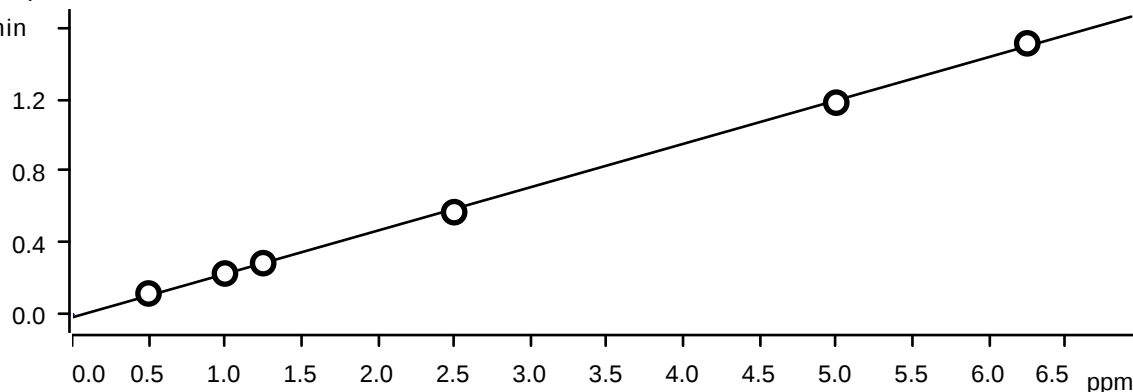


Function: $A = -0.0163950 + 0.0241967 \times Q$

Relative standard deviation 2.309177 %

Correlation coefficient 0.999724


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-04-22 10:37:58 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.117	STD2	2025-04-22 10:59:20 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.228	STD3	2025-04-22 11:20:44 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.286	STD4	2025-04-22 11:42:09 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.570	STD5	2025-04-22 12:03:34 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.181	STD6	2025-04-22 12:25:01 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.512	STD7	2025-04-22 12:46:28 UTC-4	used

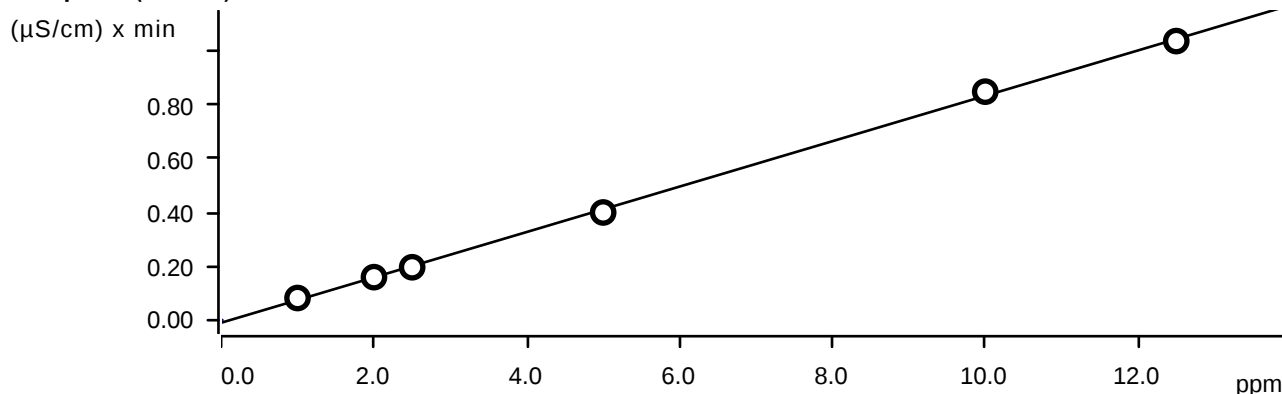Phosphate (Anions)Function: $A = -9.96993E-3 + 8.43655E-3 \times Q$

Relative standard deviation 2.492252 %

Correlation coefficient 0.999676

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-04-22 10:37:58 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.082	STD2	2025-04-22 10:59:20 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.160	STD3	2025-04-22 11:20:44 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.196	STD4	2025-04-22 11:42:09 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.400	STD5	2025-04-22 12:03:34 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.849	STD6	2025-04-22 12:25:01 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.037	STD7	2025-04-22 12:46:28 UTC-4	used

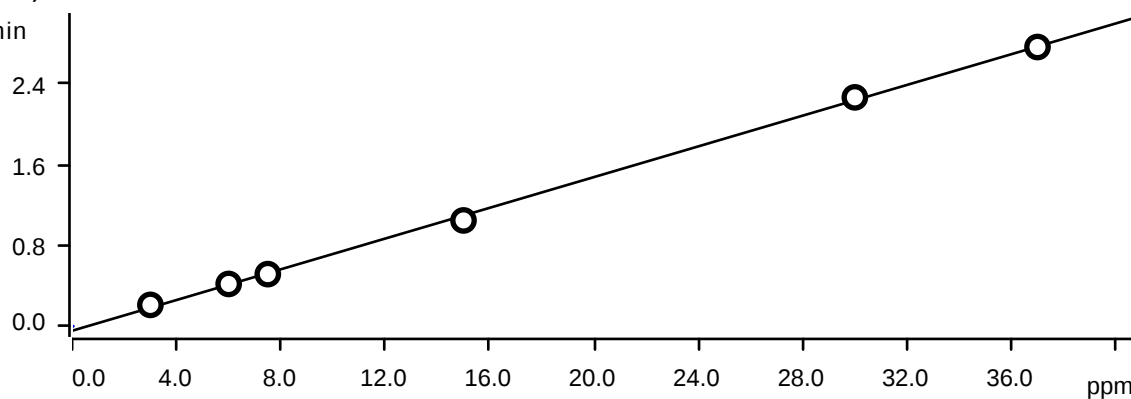Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0453007 + 7.61540E-3 \times Q$

Relative standard deviation 2.675209 %

Correlation coefficient 0.999634

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-04-22 10:37:58 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.211	STD2	2025-04-22 10:59:20 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.419	STD3	2025-04-22 11:20:44 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.516	STD4	2025-04-22 11:42:09 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.048	STD5	2025-04-22 12:03:34 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.268	STD6	2025-04-22 12:25:01 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.767	STD7	2025-04-22 12:46:28 UTC-4	used


Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-04-22 10:37:58 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

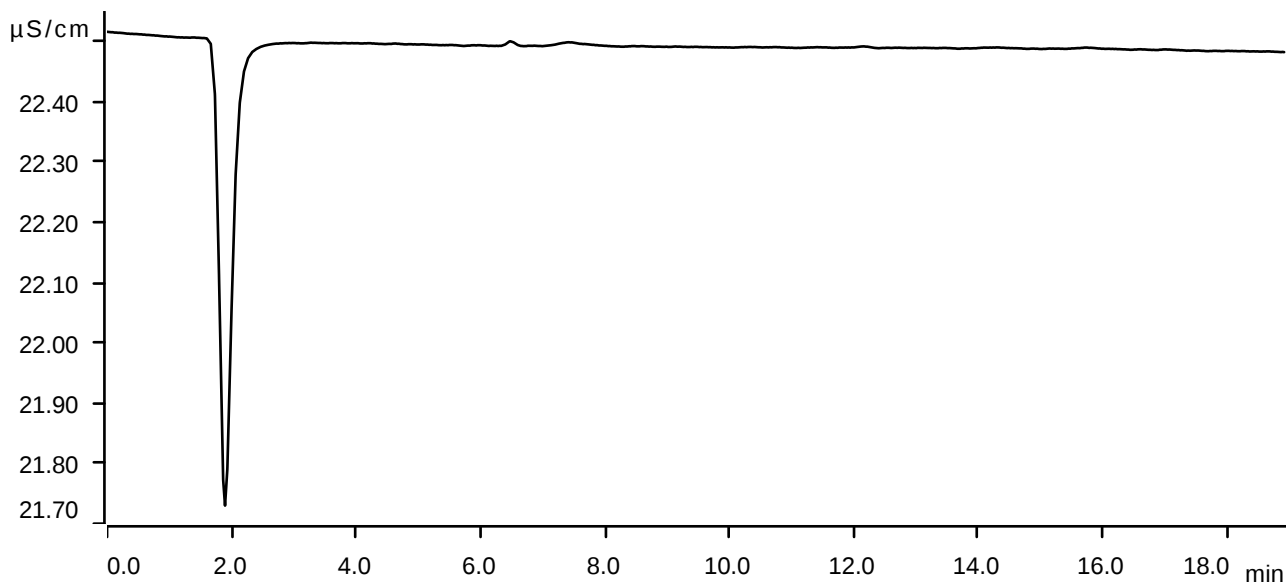


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-04-22 10:59:20 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

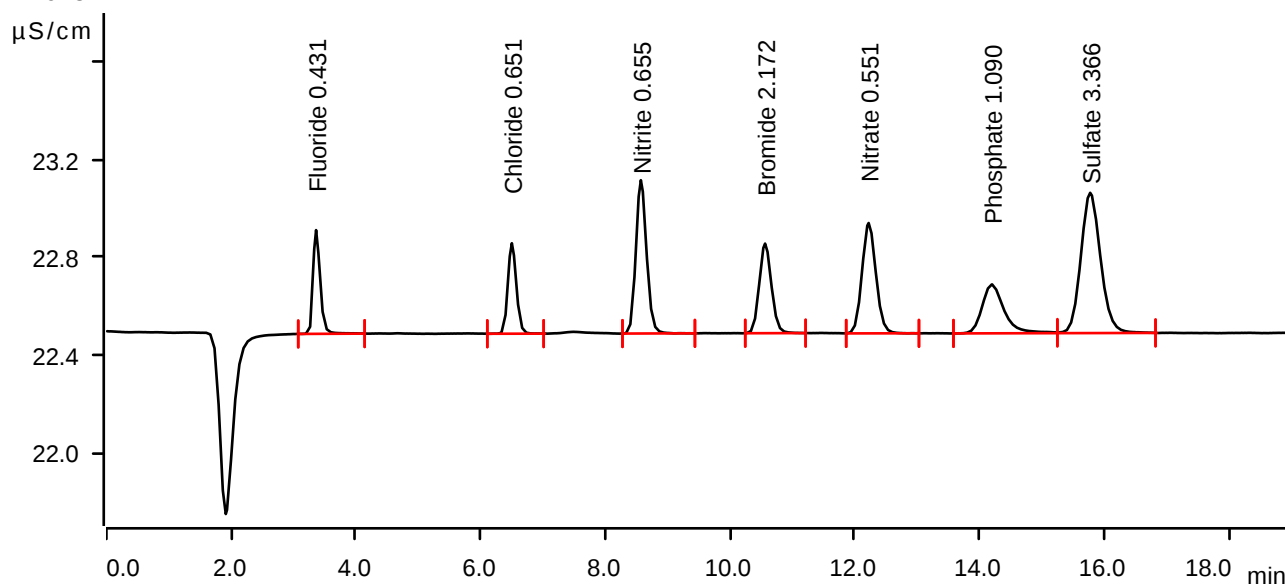

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.363	0.0560	0.425	0.431	Fluoride
2	6.502	0.0581	0.371	0.651	Chloride
3	8.570	0.1247	0.628	0.655	Nitrite
4	10.562	0.0832	0.367	2.172	Bromide
5	12.222	0.1168	0.452	0.551	Nitrate
6	14.197	0.0820	0.201	1.090	Phosphate
7	15.773	0.2111	0.575	3.366	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-04-22 11:20:44 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

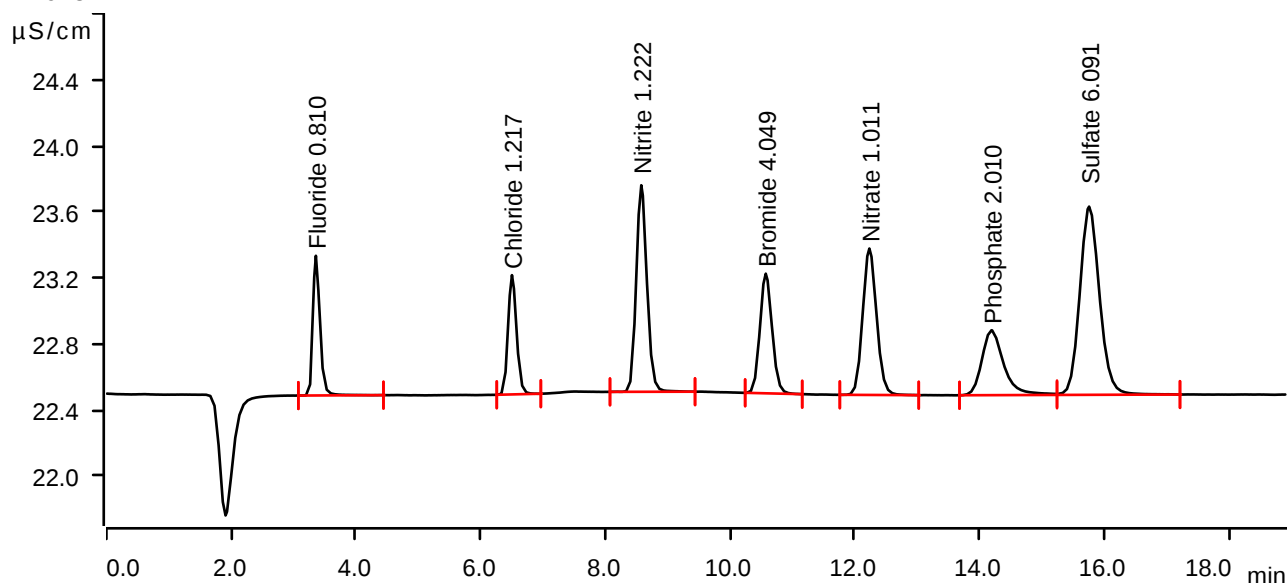

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.360	0.1105	0.845	0.810	Fluoride
2	6.503	0.1132	0.722	1.217	Chloride
3	8.577	0.2488	1.250	1.222	Nitrite
4	10.572	0.1632	0.724	4.049	Bromide
5	12.233	0.2282	0.886	1.011	Nitrate
6	14.192	0.1596	0.393	2.010	Phosphate
7	15.757	0.4185	1.139	6.091	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-04-22 11:42:09 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

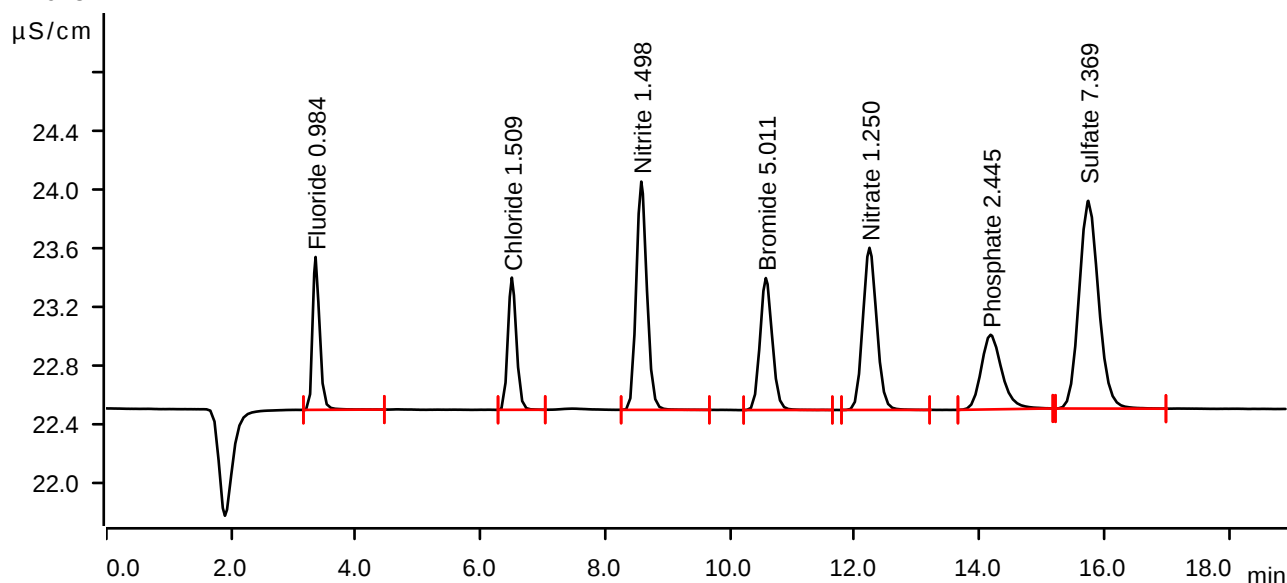

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.1356	1.044	0.984	Fluoride
2	6.502	0.1416	0.903	1.509	Chloride
3	8.577	0.3094	1.559	1.498	Nitrite
4	10.573	0.2043	0.902	5.011	Bromide
5	12.235	0.2860	1.108	1.250	Nitrate
6	14.177	0.1963	0.510	2.445	Phosphate
7	15.743	0.5159	1.419	7.369	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-04-22 12:03:34 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

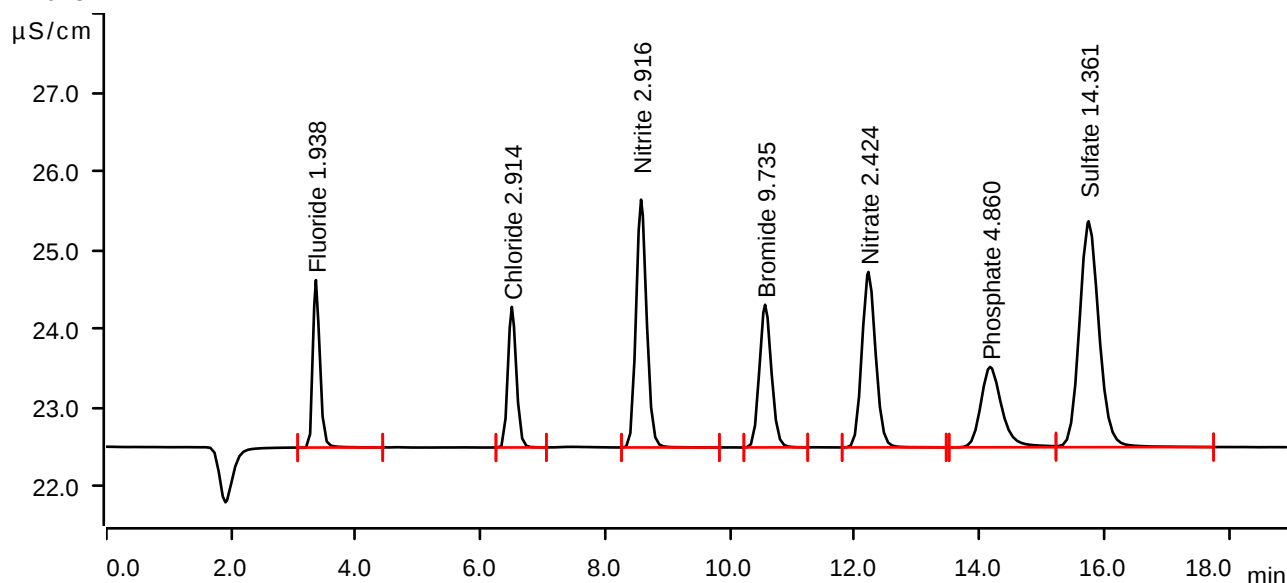

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.360	0.2730	2.125	1.938	Fluoride
2	6.502	0.2783	1.784	2.914	Chloride
3	8.573	0.6200	3.144	2.916	Nitrite
4	10.562	0.4057	1.810	9.735	Bromide
5	12.218	0.5702	2.226	2.424	Nitrate
6	14.170	0.4000	1.020	4.860	Phosphate
7	15.748	1.0484	2.866	14.361	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-04-22 12:25:01 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.49 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

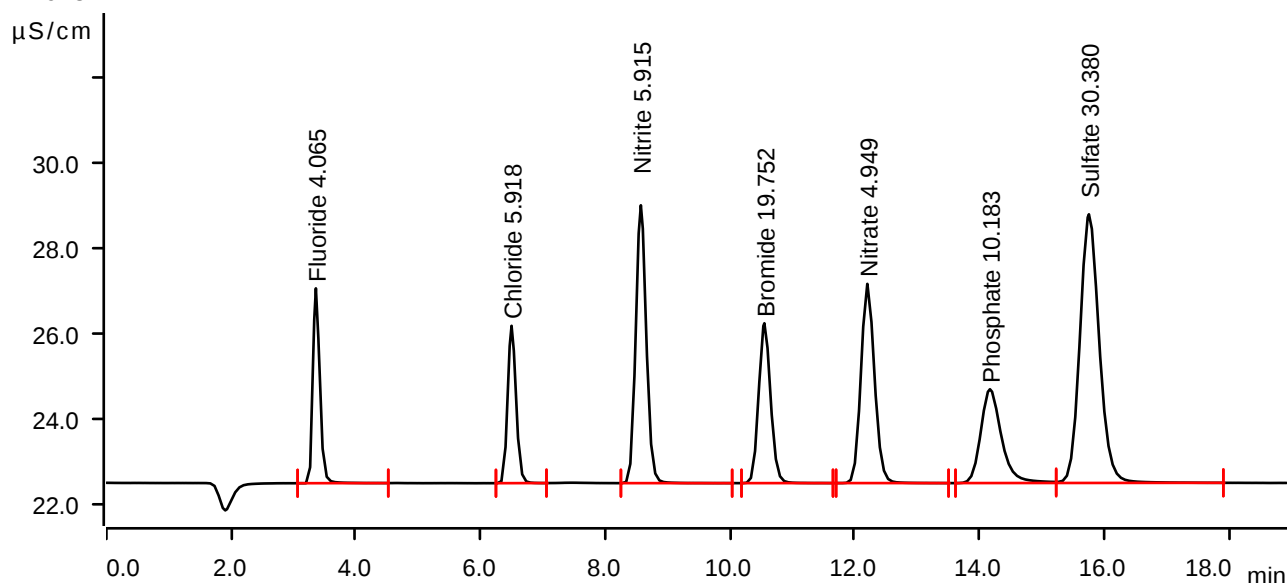

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.360	0.5793	4.564	4.065	Fluoride
2	6.497	0.5704	3.686	5.918	Chloride
3	8.570	1.2768	6.510	5.915	Nitrite
4	10.550	0.8327	3.746	19.752	Bromide
5	12.202	1.1810	4.667	4.949	Nitrate
6	14.167	0.8491	2.199	10.183	Phosphate
7	15.753	2.2683	6.294	30.380	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-04-22 12:46:28 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.43 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

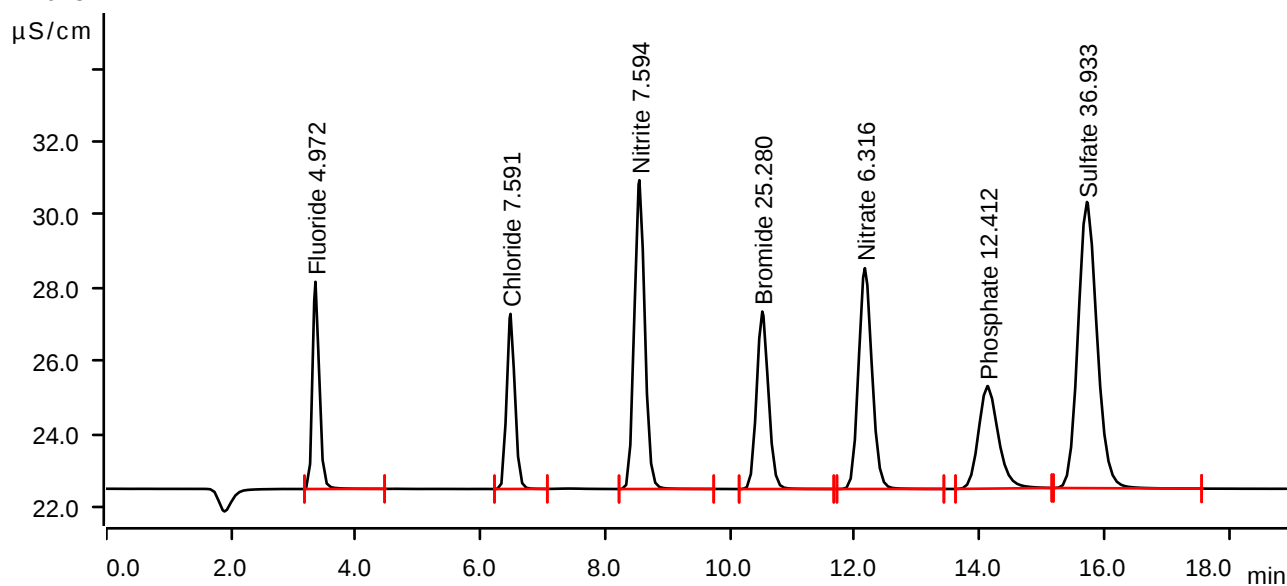

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.7100	5.662	4.972	Fluoride
2	6.480	0.7331	4.785	7.591	Chloride
3	8.547	1.6445	8.440	7.594	Nitrite
4	10.517	1.0684	4.850	25.280	Bromide
5	12.162	1.5118	6.035	6.316	Nitrate
6	14.127	1.0372	2.803	12.412	Phosphate
7	15.722	2.7673	7.822	36.933	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-04-22 13:07:56 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

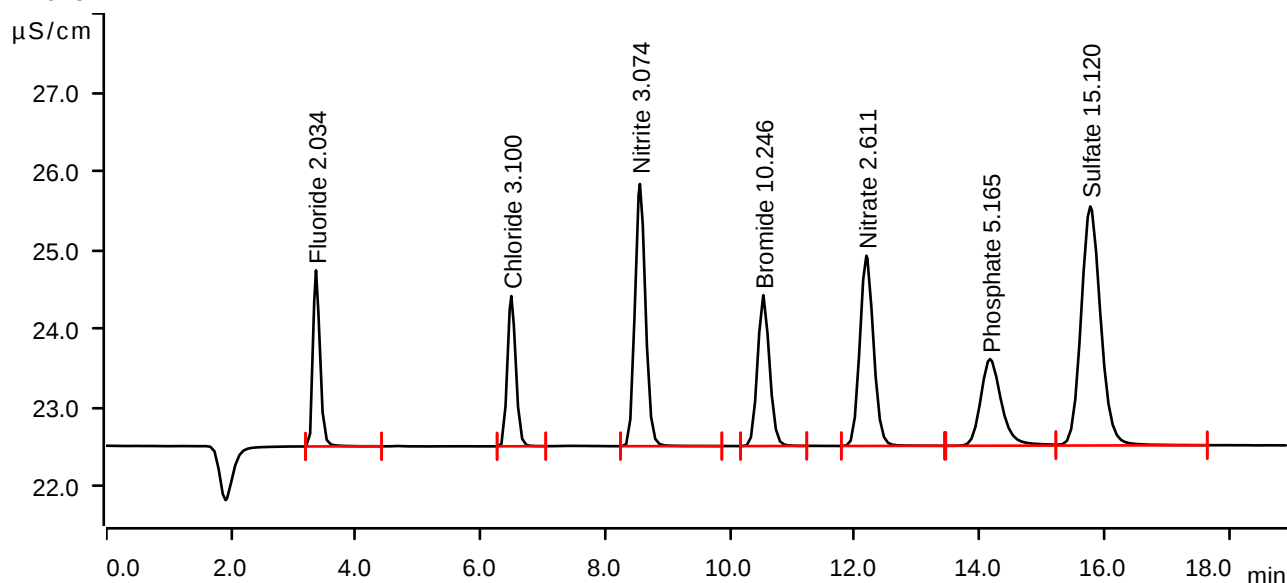

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.2867	2.234	2.034	Fluoride
2	6.493	0.2963	1.906	3.100	Chloride
3	8.555	0.6546	3.328	3.074	Nitrite
4	10.532	0.4274	1.914	10.246	Bromide
5	12.185	0.6154	2.414	2.611	Nitrate
6	14.168	0.4257	1.100	5.165	Phosphate
7	15.775	1.1062	3.034	15.120	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-04-22 13:58:31 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

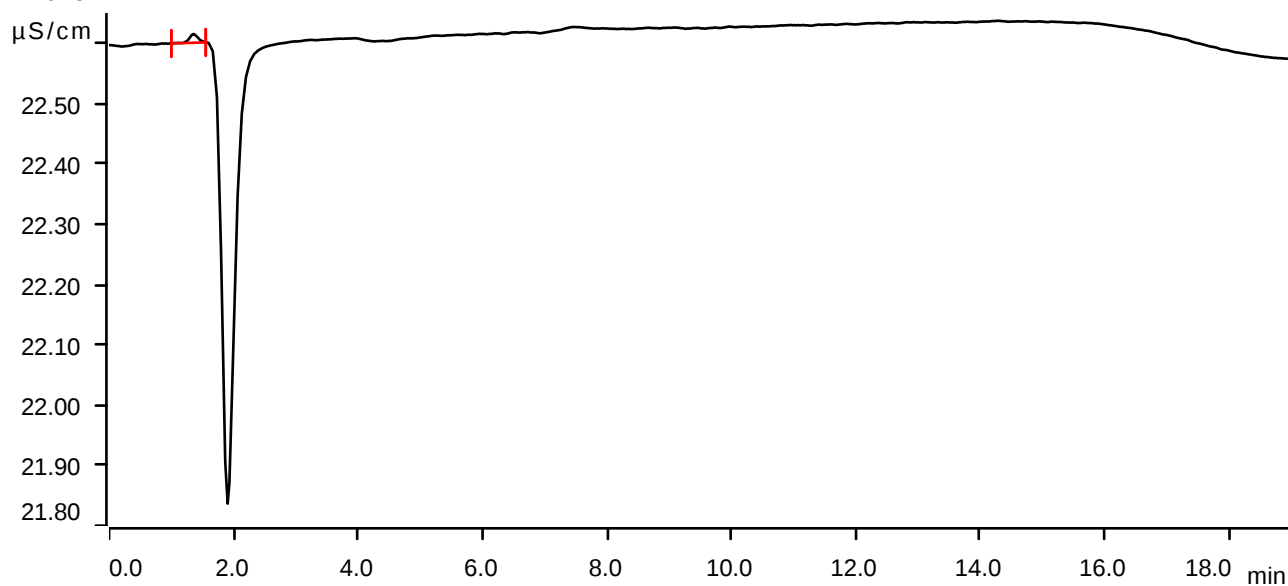

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	1.362	0.0024	0.015	invalid	


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-05-16 13:46:40 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

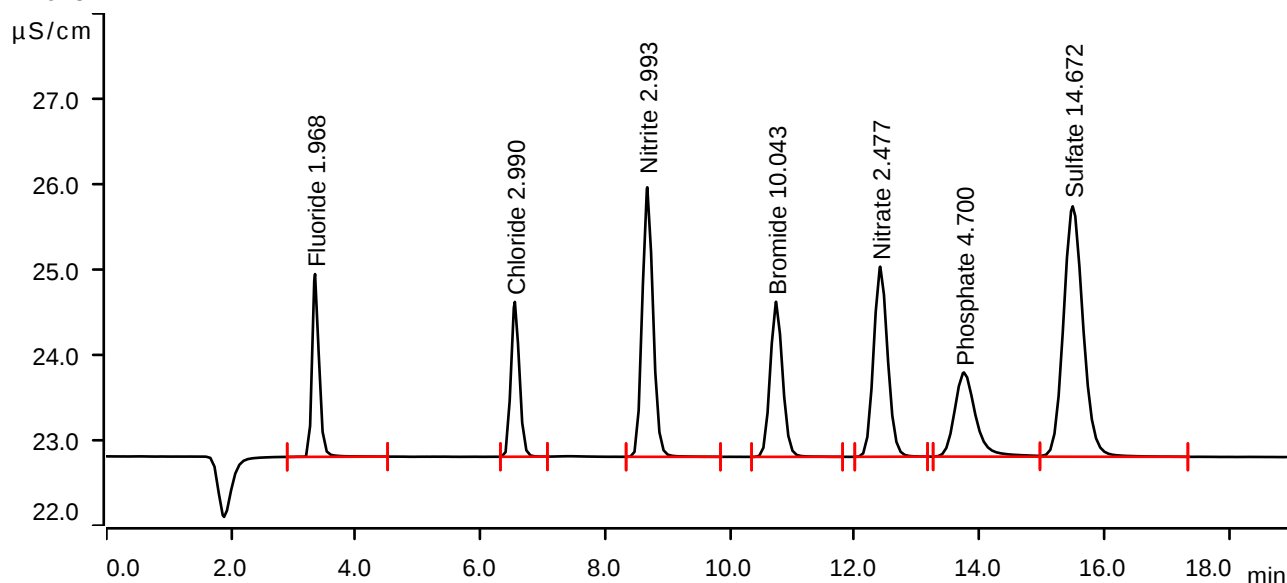


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.347	0.2773	2.140	1.968	Fluoride
2	6.550	0.2856	1.813	2.990	Chloride
3	8.673	0.6368	3.157	2.993	Nitrite
4	10.738	0.4188	1.816	10.043	Bromide
5	12.408	0.5831	2.226	2.477	Nitrate
6	13.750	0.3865	0.986	4.700	Phosphate
7	15.493	1.0721	2.933	14.672	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-05-16 14:08:11 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

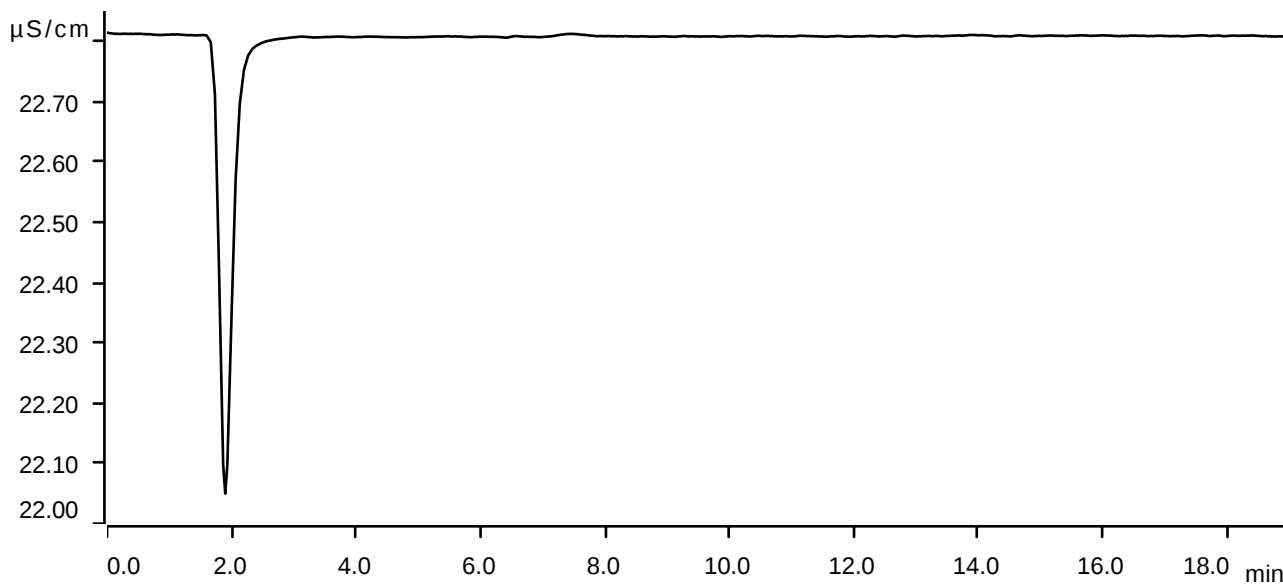Anions


Sample data

Ident LB135822BLW
Sample type Sample
Determination start 2025-05-16 14:29:42 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

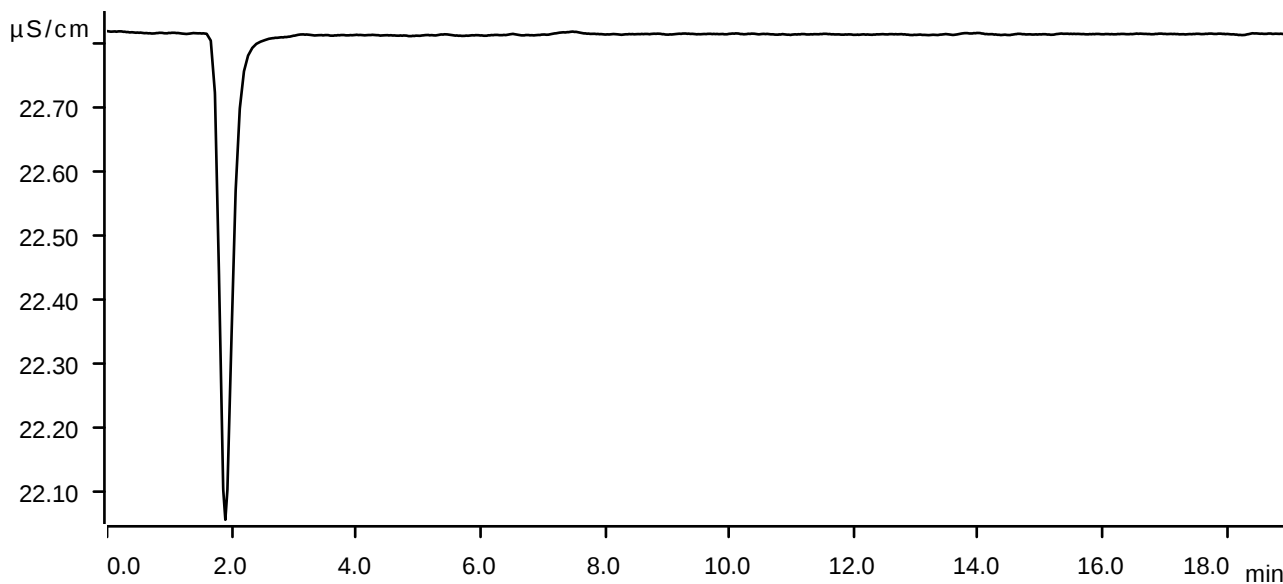


Sample data

Ident LB135822BSW
 Sample type Check standard 1
 Determination start 2025-05-16 14:51:14 UTC-4
 Method IC1-042225
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.99 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

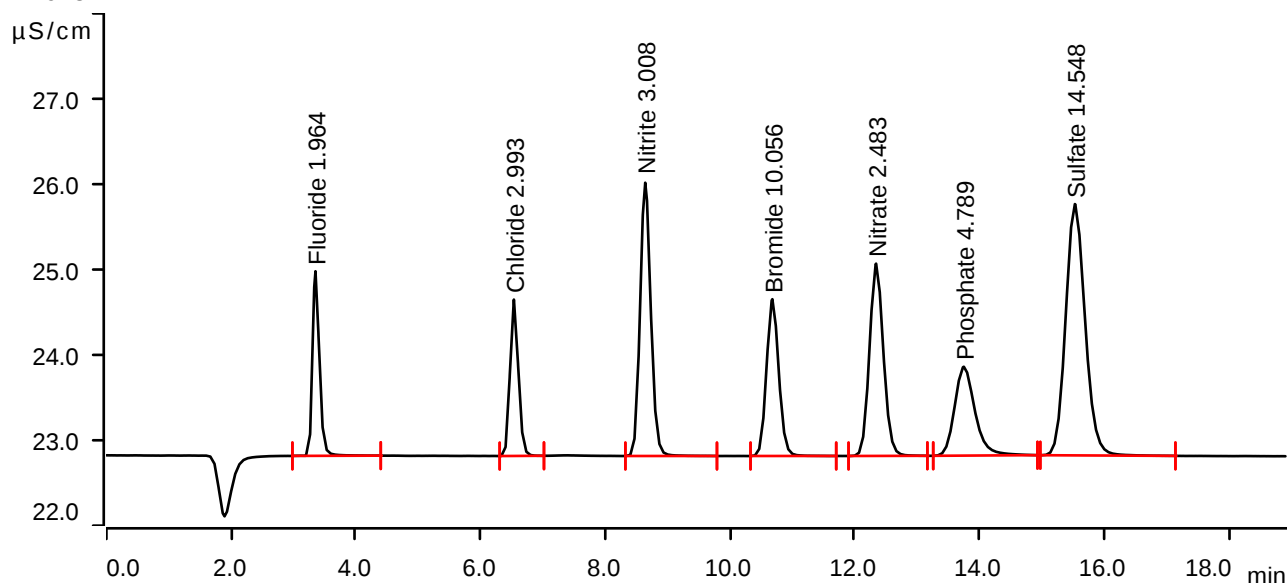

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.2767	2.162	1.964	Fluoride
2	6.535	0.2859	1.831	2.993	Chloride
3	8.640	0.6400	3.201	3.008	Nitrite
4	10.678	0.4194	1.837	10.056	Bromide
5	12.342	0.5845	2.252	2.483	Nitrate
6	13.748	0.3940	1.041	4.789	Phosphate
7	15.528	1.0626	2.944	14.548	Sulfate


Sample data

Ident Q2065-01
Sample type Sample
Determination start 2025-05-16 15:12:46 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

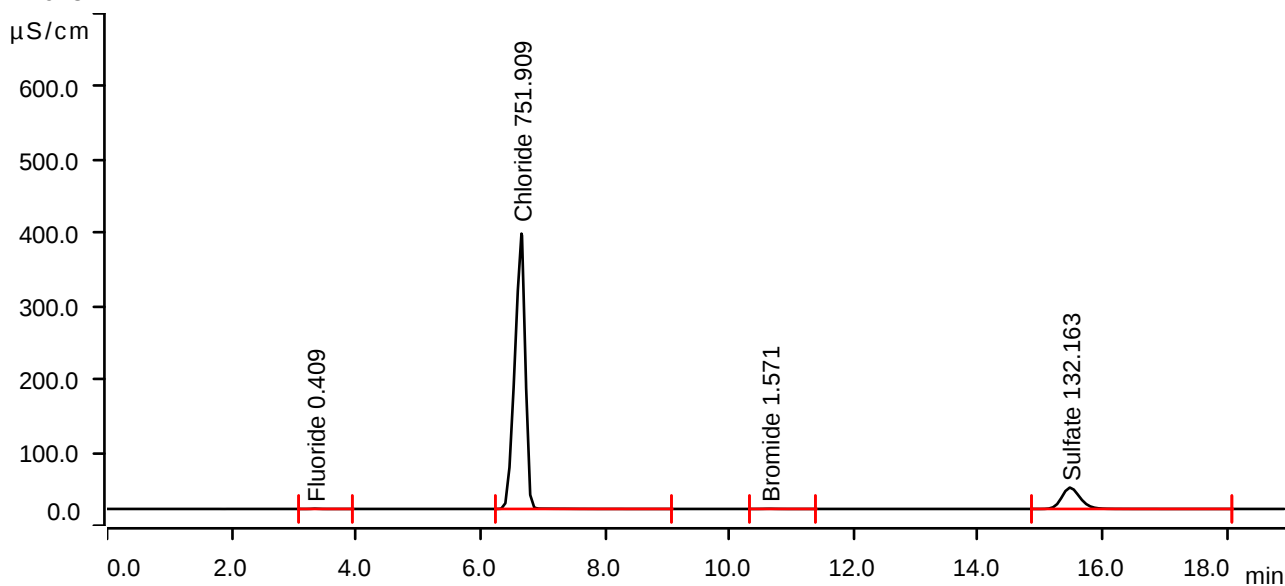

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.340	0.0528	0.388	0.409	Fluoride
2	6.660	73.1121	376.283	751.909	Chloride
3	10.647	0.0576	0.254	1.571	Bromide
4	15.475	10.0194	29.094	132.163	Sulfate


Sample data

Ident Q2067-01
Sample type Sample
Determination start 2025-05-16 15:34:19 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

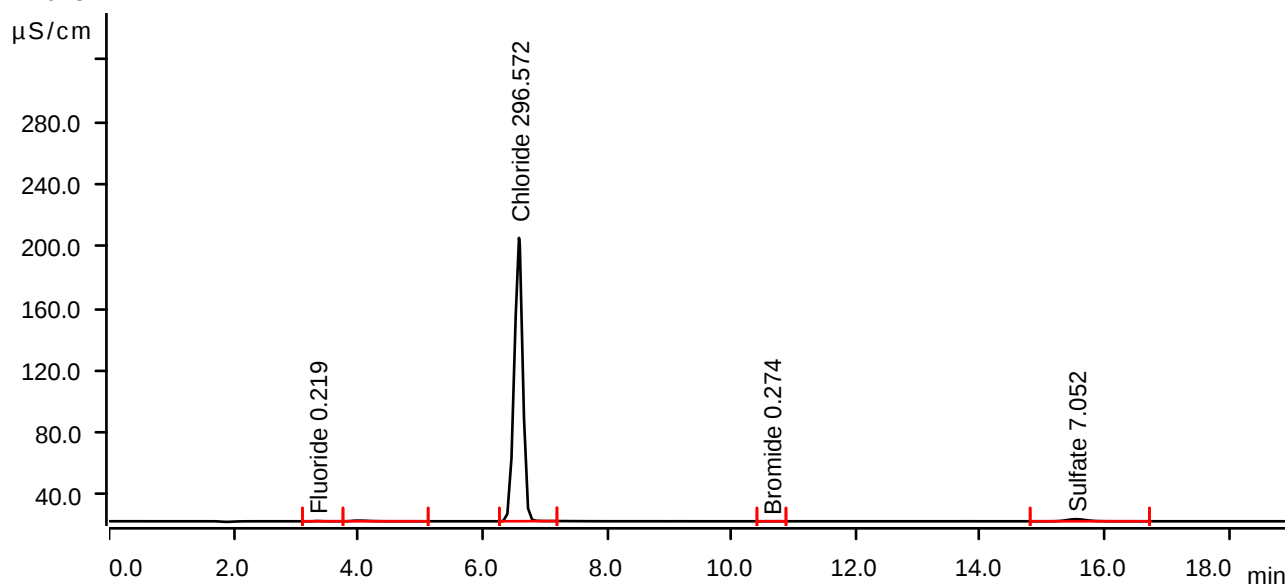

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.345	0.0253	0.180	0.219	Fluoride
2	3.993	0.1325	0.413	invalid	
3	6.588	28.8342	182.517	296.572	Chloride
4	10.642	0.0023	0.011	0.274	Bromide
5	15.540	0.4918	1.359	7.052	Sulfate


Sample data

Ident Q2067-01MS
 Sample type Sample
 Determination start 2025-05-16 15:55:53 UTC-4
 Method IC1-042225
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.88 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

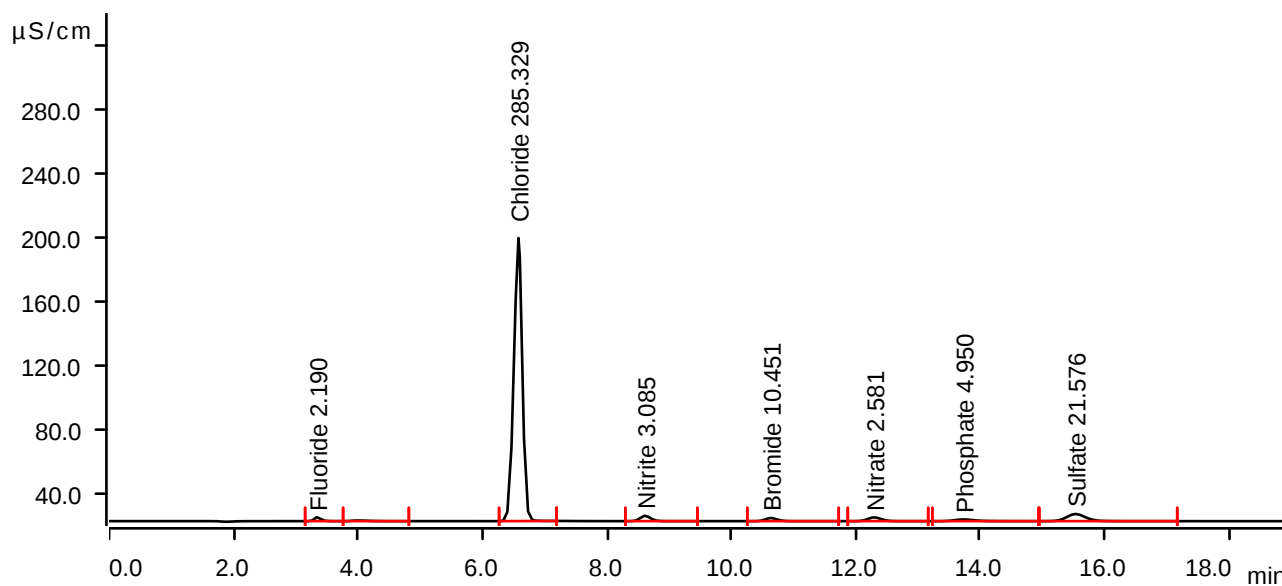

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.343	0.3093	2.406	2.190	Fluoride
2	3.987	0.1262	0.393	invalid	
3	6.580	27.7409	176.816	285.329	Chloride
4	8.615	0.6569	3.337	3.085	Nitrite
5	10.637	0.4362	1.931	10.451	Bromide
6	12.295	0.6081	2.359	2.581	Nitrate
7	13.732	0.4077	1.075	4.950	Phosphate
8	15.530	1.5978	4.467	21.576	Sulfate


Sample data

Ident Q2067-01MSD
Sample type Sample
Determination start 2025-05-16 16:17:28 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

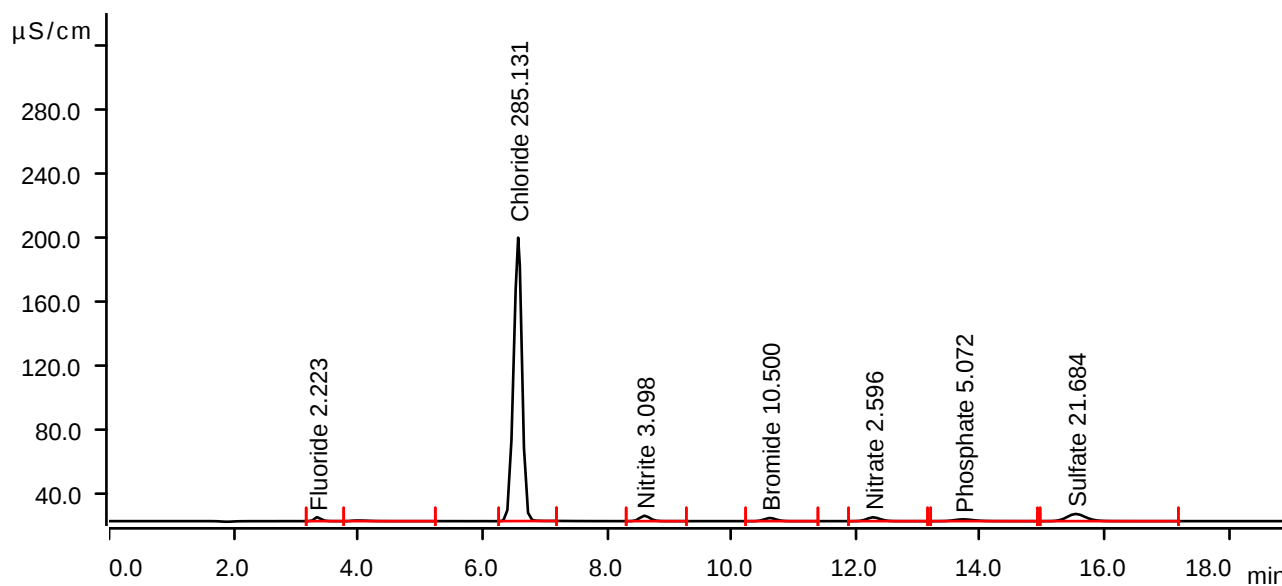

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.347	0.3141	2.439	2.223	Fluoride
2	3.993	0.1282	0.393	invalid	
3	6.575	27.7216	177.048	285.131	Chloride
4	8.607	0.6598	3.365	3.098	Nitrite
5	10.620	0.4383	1.945	10.500	Bromide
6	12.278	0.6119	2.380	2.596	Nitrate
7	13.727	0.4179	1.113	5.072	Phosphate
8	15.535	1.6060	4.492	21.684	Sulfate


Sample data

Ident Q2068-03
Sample type Sample
Determination start 2025-05-16 16:39:03 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

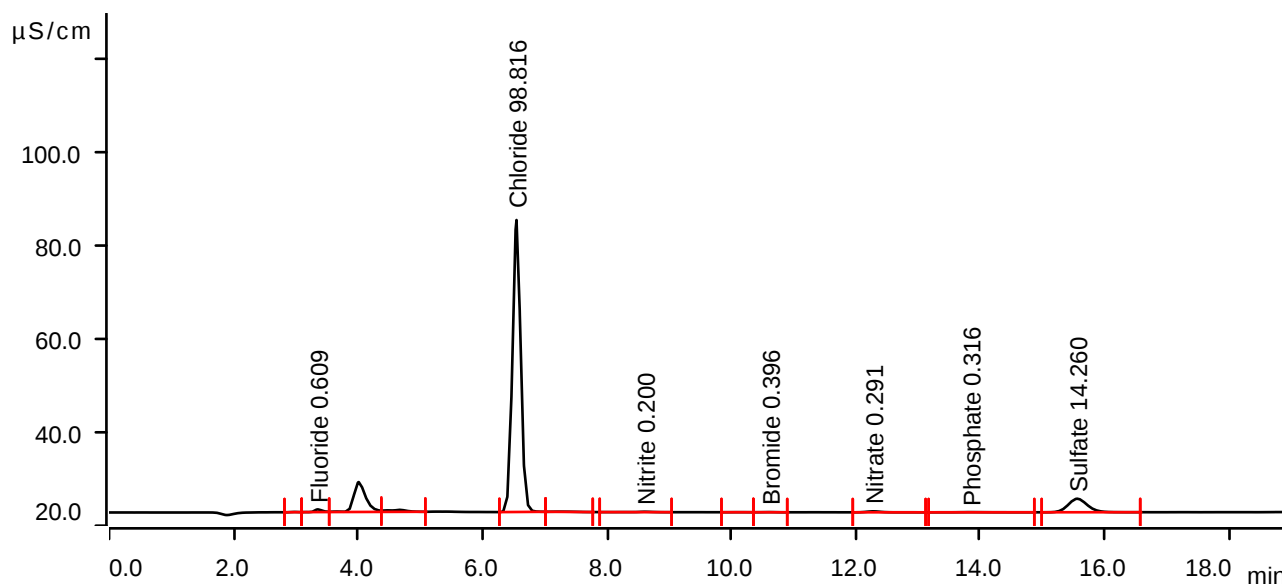

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	2.977	0.0060	0.056	invalid	
2	3.357	0.0816	0.583	0.609	Fluoride
3	4.013	1.4366	6.415	invalid	
4	4.672	0.1538	0.433	invalid	
5	6.548	9.6040	62.698	98.816	Chloride
6	7.237	0.0207	0.048	invalid	
7	8.610	0.0250	0.092	0.200	Nitrite
8	10.118	0.0033	0.015	invalid	
9	10.617	0.0075	0.034	0.396	Bromide
10	12.282	0.0540	0.205	0.291	Nitrate
11	13.845	0.0167	0.035	0.316	Phosphate
12	15.558	1.0407	2.907	14.260	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-05-16 17:21:47 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

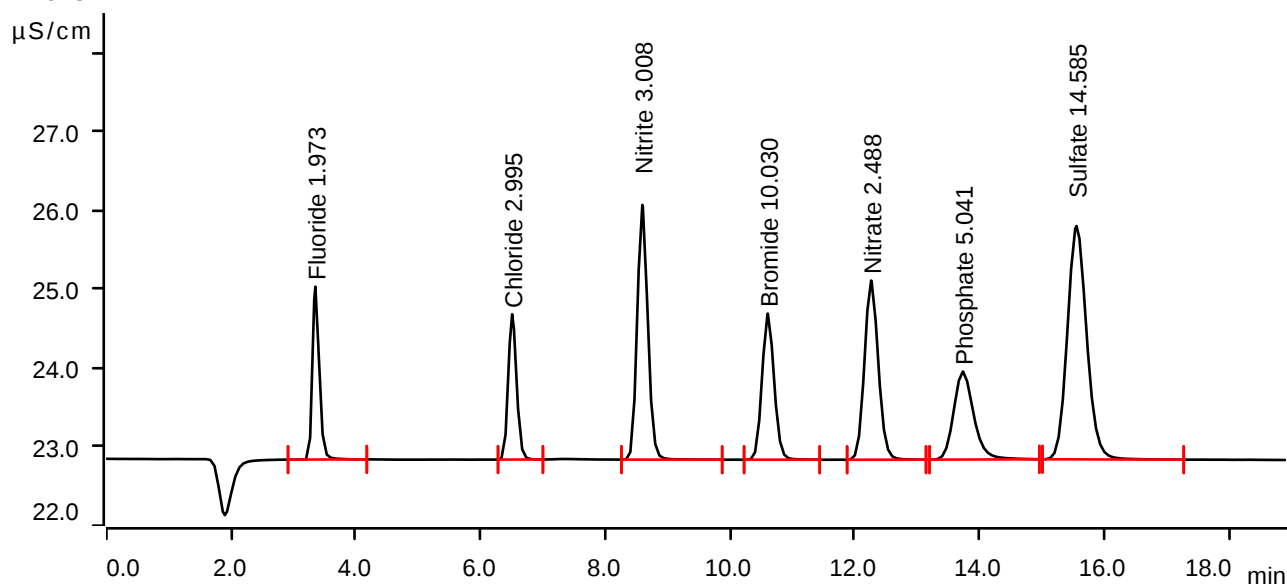

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.2781	2.192	1.973	Fluoride
2	6.507	0.2861	1.843	2.995	Chloride
3	8.593	0.6401	3.233	3.008	Nitrite
4	10.605	0.4182	1.854	10.030	Bromide
5	12.262	0.5855	2.274	2.488	Nitrate
6	13.732	0.4153	1.117	5.041	Phosphate
7	15.555	1.0654	2.961	14.585	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-05-16 17:43:17 UTC-4
Method IC1-042225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions