


Instrument IC-1		Analyst: NF		Method: 300.0 / 9056A		Initial v Analyst				
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/22/2025 11:09	10 NF/IZ
STD2	0.430	0.640	0.649	2.129	0.543	1.098	3.287	IC1-052225	5/22/2025 11:30	10 NF/IZ
STD3	0.795	1.207	1.205	4.018	1.004	1.867	6.069	IC1-052225	5/22/2025 11:52	10 NF/IZ
STD4	0.977	1.480	1.479	4.929	1.229	2.477	7.415	IC1-052225	5/22/2025 12:13	10 NF/IZ
STD5	1.991	2.968	2.960	9.916	2.467	5.110	14.621	IC1-052225	5/22/2025 12:35	10 NF/IZ
STD6	4.001	5.967	5.959	19.868	4.966	9.870	29.848	IC1-052225	5/22/2025 12:56	10 NF/IZ
STD7	5.006	7.539	7.548	25.140	6.290	12.578	37.260	IC1-052225	5/22/2025 13:17	10 NF/IZ
ICV	2.054	3.101	3.056	10.229	2.610	5.286	15.128	IC1-052225	5/22/2025 13:39	10 NF/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	5/22/2025 14:22	10 NF/IZ
CCV	2.021	3.050	3.038	10.213	2.541	4.814	15.089	IC1-052225	6/5/2025 9:50	10 NF/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	6/5/2025 10:11	10 NF/IZ
LB136017BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	6/5/2025 10:33	10 NF/IZ
LB136017BSW	2.024	3.062	3.054	10.257	2.550	4.989	15.157	IC1-052225	6/5/2025 10:54	10 NF/IZ
Q2231-01	0.038	123.754	0.131	0.228	2.836	0.000	12.502	IC1-052225	6/5/2025 11:39	10 NF/IZ
Q2231-03	0.000	195.753	0.000	0.504	3.786	0.000	31.974	IC1-052225	6/5/2025 12:00	10 NF/IZ
Q2231-04	0.124	301.974	0.000	0.403	5.572	0.000	57.925	IC1-052225	6/5/2025 12:22	10 NF/IZ
Q2231-04MS	1.680	293.513	2.336	8.126	7.482	4.056	68.858	IC1-052225	6/5/2025 12:43	10 NF/IZ
Q2331-04MSD	1.312	295.422	1.815	6.351	7.048	3.188	66.381	IC1-052225	6/5/2025 13:05	10 NF/IZ
Q2231-05	0.084	170.890	0.000	0.268	7.695	0.000	8.959	IC1-052225	6/5/2025 13:26	10 NF/IZ
Q2231-04DLX5	0.036	48.728	0.000	0.000	1.108	0.000	10.987	IC1-052225	6/5/2025 13:48	10 NF/IZ
CCV	2.034	3.063	3.055	10.226	2.552	5.287	15.145	IC1-052225	6/5/2025 14:09	10 NF/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-052225	6/5/2025 14:31	10 NF/IZ

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A											
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-052225	5/22/2025 11:09	10	NF/IZ
STD2	0.4300	0.6400	0.6490	2.1290	0.5430	1.0980	3.2870	IC1-052225	5/22/2025 11:30	10	NF/IZ
STD3	0.7950	1.2070	1.2050	4.0180	1.0040	1.8670	6.0690	IC1-052225	5/22/2025 11:52	10	NF/IZ
STD4	0.9770	1.4800	1.4790	4.9290	1.2290	2.4770	7.4150	IC1-052225	5/22/2025 12:13	10	NF/IZ
STD5	1.9910	2.9680	2.9600	9.9160	2.4670	5.1100	14.6210	IC1-052225	5/22/2025 12:35	10	NF/IZ
STD6	4.0010	5.9670	5.9590	19.8680	4.9660	9.8700	29.8480	IC1-052225	5/22/2025 12:56	10	NF/IZ
STD7	5.0060	7.5390	7.5480	25.1400	6.2900	12.5780	37.2600	IC1-052225	5/22/2025 13:17	10	NF/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1	7.5000	6.6667	8.1667	6.4500	8.6000	9.8000	9.5667				
STD2	-0.6250	0.5833	0.4167	0.4500	0.4000	-6.6500	1.1500				
STD3	-2.3000	-1.3333	-1.4000	-1.4200	-1.6800	-0.9200	-1.1333				
STD4	-0.4500	-1.0667	-1.3333	-0.8400	-1.3200	2.2000	-2.5267				
STD5	0.0250	-0.5500	-0.6833	-0.6600	-0.6800	-1.3000	-0.5067				
STD6	0.1200	0.5200	0.6400	0.5600	0.6400	0.6240	0.7027				
STD7											

Initial
wt/
Final


Analyst

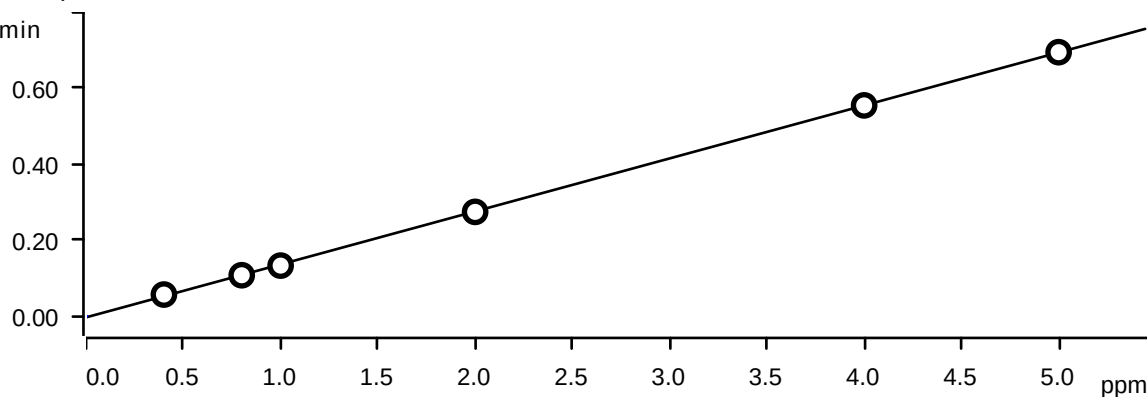Fluoride (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -2.82659E-3 + 0.0139492 \times Q$

Relative standard deviation 0.920519 %

Correlation coefficient 0.999955

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.108	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.133	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.275	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.555	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.695	STD7	2025-05-22 13:17:57 UTC-4	used

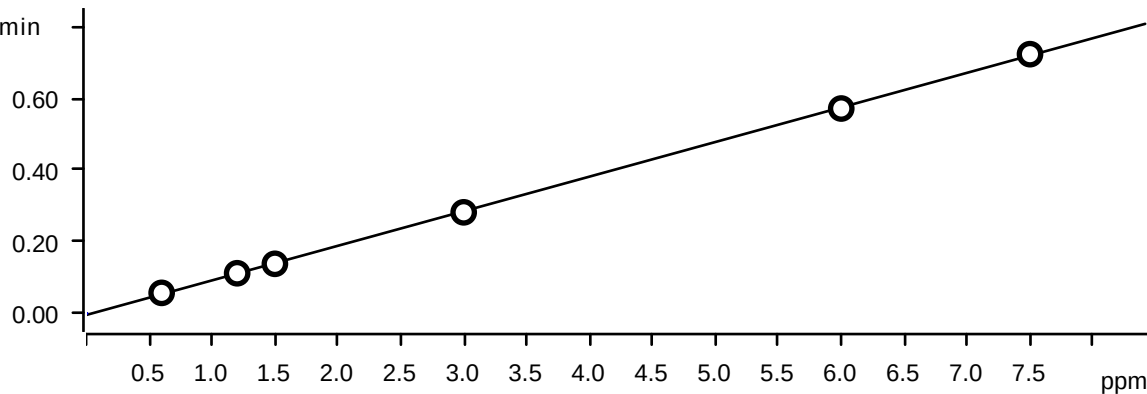Chloride (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -4.33057E-3 + 9.64673E-3 \times Q$


Relative standard deviation 1.154335 %

Correlation coefficient 0.999929

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.057	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.112	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.138	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.282	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.571	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.723	STD7	2025-05-22 13:17:57 UTC-4	used

Nitrite (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

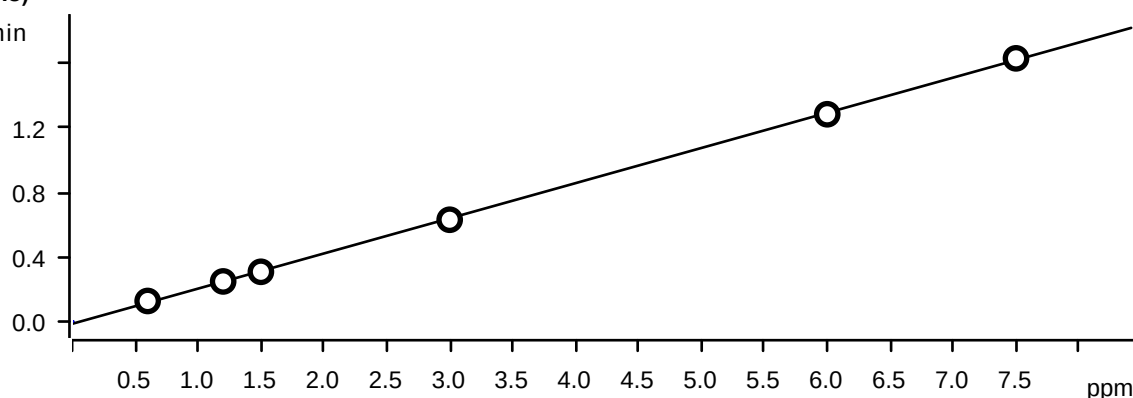

Function: $A = -0.0150155 + 0.0217890 \times Q$


Relative standard deviation 1.428639 %

Correlation coefficient 0.999893

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.126	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.248	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.307	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.630	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.283	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.630	STD7	2025-05-22 13:17:57 UTC-4	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

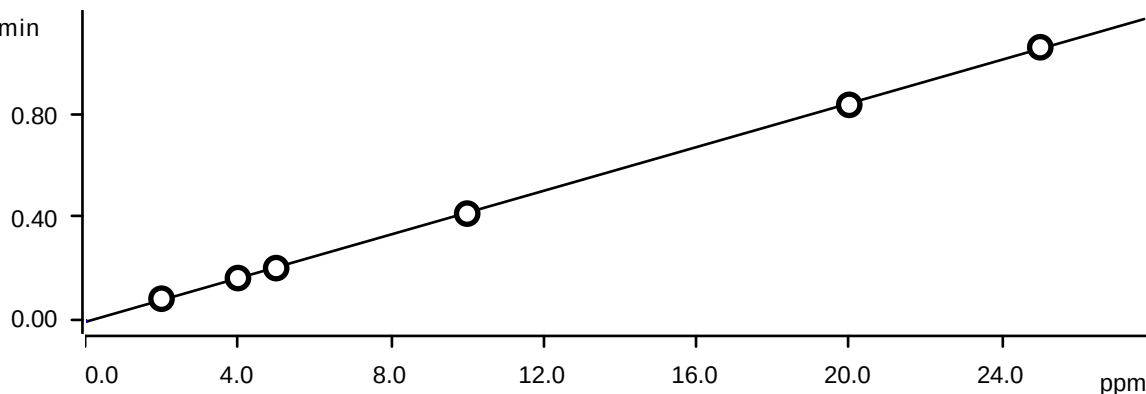

Function: $A = -6.27114E-3 + 4.23162E-3 \times Q$


Relative standard deviation: 1.185575 %

Correlation coefficient: 0.999925

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.084	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.164	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.202	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.413	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.834	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.058	STD7	2025-05-22 13:17:57 UTC-4	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

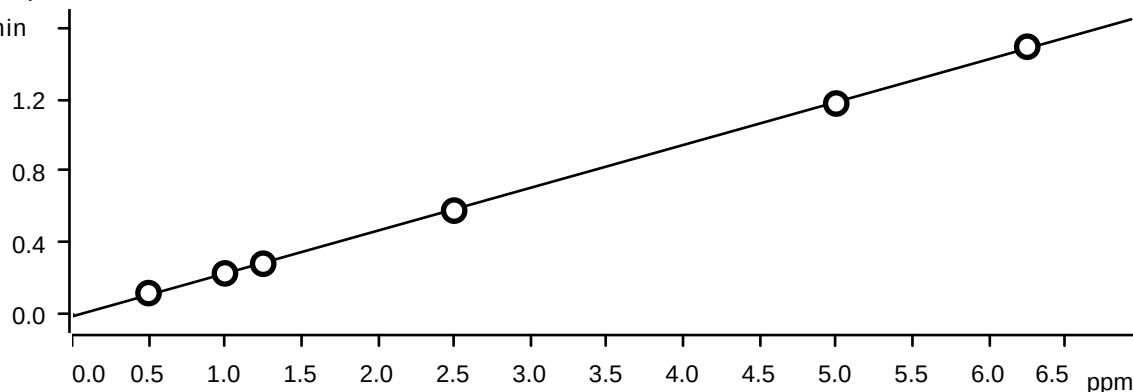


Function: $A = -0.0109593 + 0.0239055 \times Q$

Relative standard deviation: 1.451672 %

Correlation coefficient 0.999889


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.119	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.229	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.283	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.579	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.176	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.493	STD7	2025-05-22 13:17:57 UTC-4	used

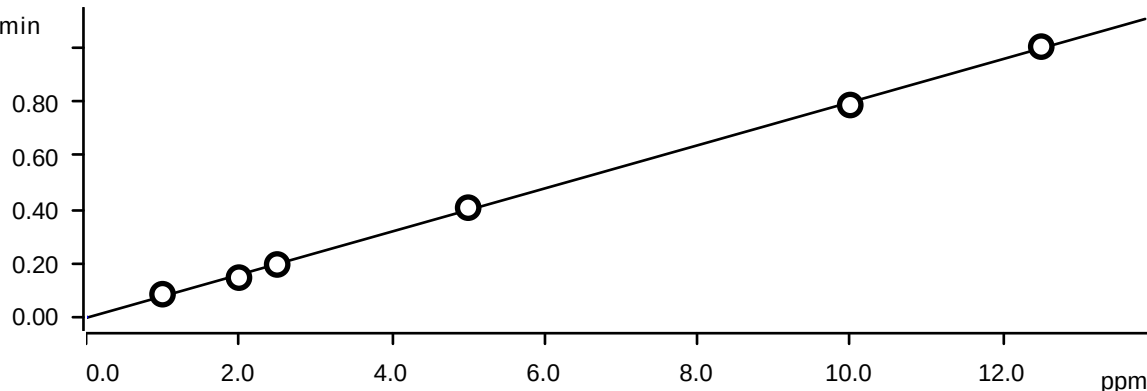Phosphate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -3.02035E-3 + 8.01761E-3 \times Q$

Relative standard deviation 2.297726 %

Correlation coefficient 0.999716

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.085	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.147	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.196	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.407	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.788	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.005	STD7	2025-05-22 13:17:57 UTC-4	used

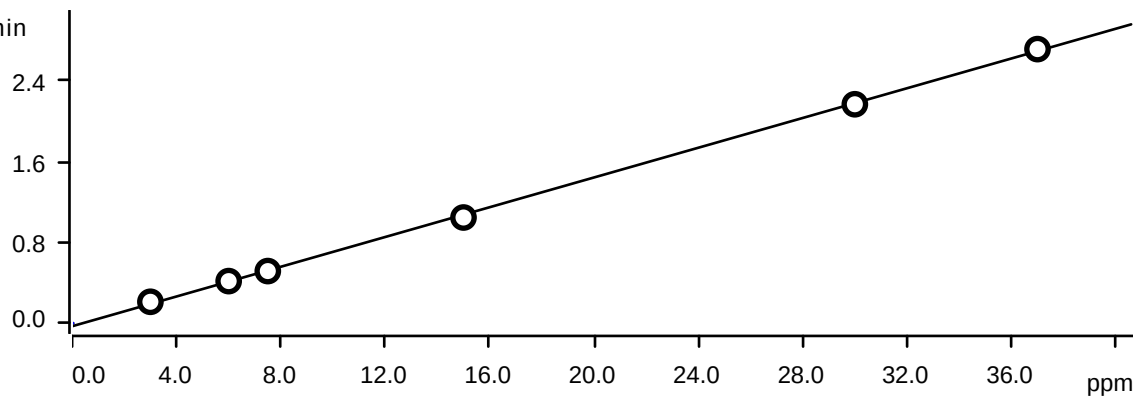Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0303663 + 7.37295E-3 \times Q$

Relative standard deviation 1.792871 %

Correlation coefficient 0.999832


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-05-22 11:09:38 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.212	STD2	2025-05-22 11:30:53 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.417	STD3	2025-05-22 11:52:16 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.516	STD4	2025-05-22 12:13:41 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.048	STD5	2025-05-22 12:35:06 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.170	STD6	2025-05-22 12:56:31 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.717	STD7	2025-05-22 13:17:57 UTC-4	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-05-22 11:09:38 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

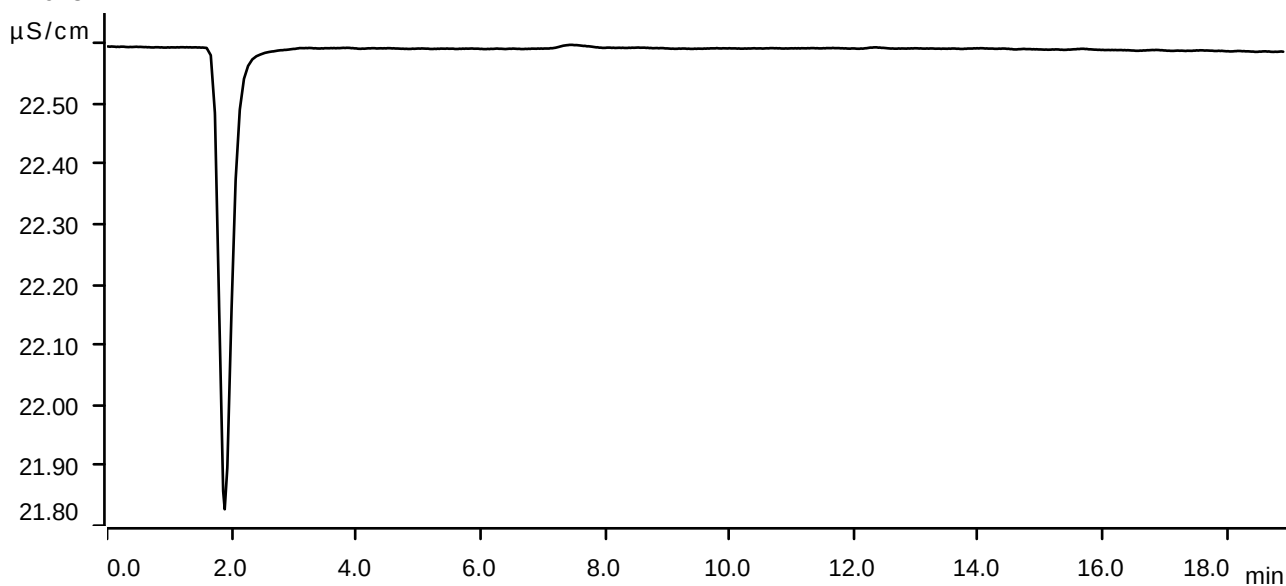Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-05-22 11:30:53 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

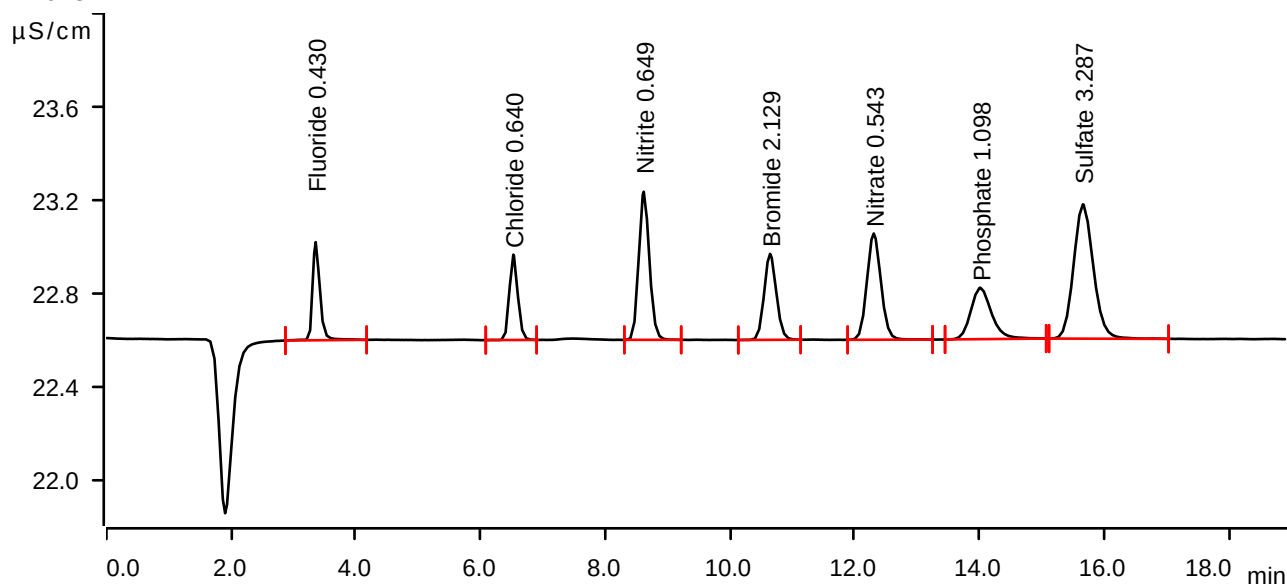

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.0572	0.421	0.430	Fluoride
2	6.525	0.0574	0.366	0.640	Chloride
3	8.617	0.1264	0.636	0.649	Nitrite
4	10.642	0.0838	0.369	2.129	Bromide
5	12.303	0.1190	0.456	0.543	Nitrate
6	14.013	0.0850	0.221	1.098	Phosphate
7	15.657	0.2120	0.577	3.287	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-05-22 11:52:16 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

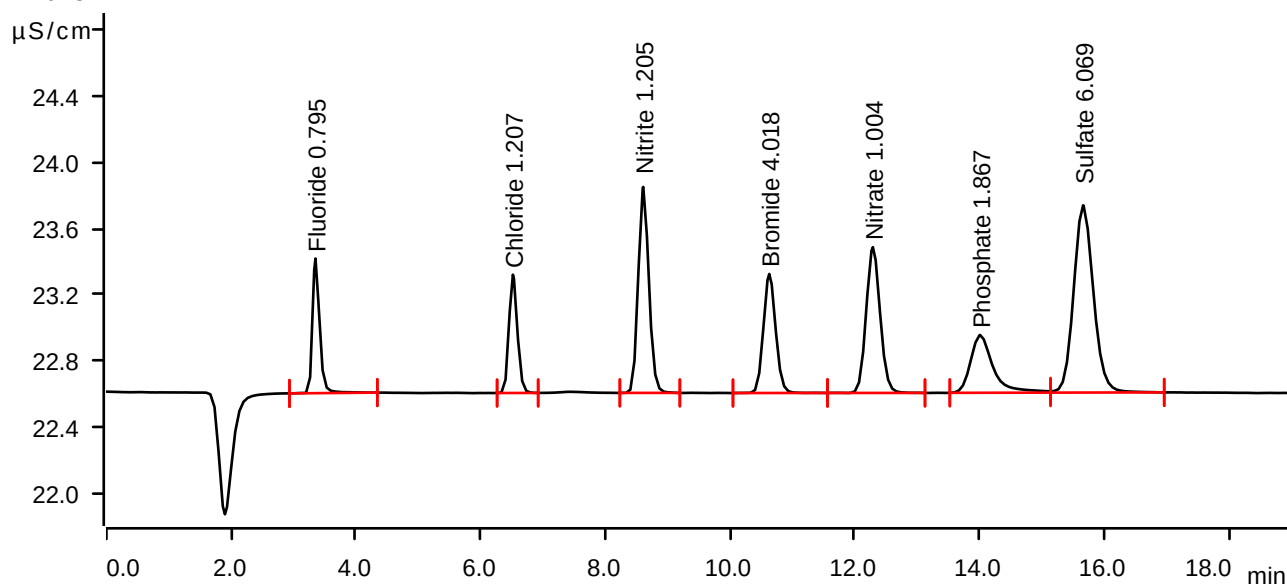

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.1081	0.814	0.795	Fluoride
2	6.518	0.1121	0.716	1.207	Chloride
3	8.608	0.2475	1.247	1.205	Nitrite
4	10.628	0.1637	0.720	4.018	Bromide
5	12.290	0.2290	0.882	1.004	Nitrate
6	14.008	0.1467	0.350	1.867	Phosphate
7	15.660	0.4171	1.133	6.069	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-05-22 12:13:41 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.71 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

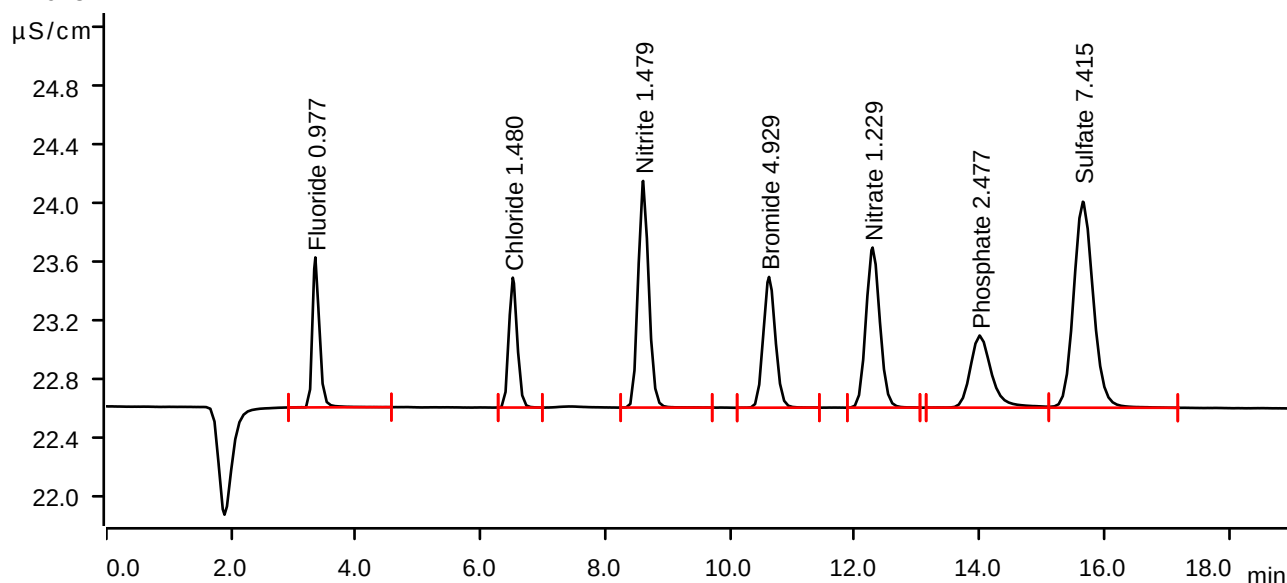

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.1334	1.024	0.977	Fluoride
2	6.517	0.1384	0.888	1.480	Chloride
3	8.607	0.3073	1.549	1.479	Nitrite
4	10.625	0.2023	0.894	4.929	Bromide
5	12.285	0.2828	1.094	1.229	Nitrate
6	14.003	0.1955	0.493	2.477	Phosphate
7	15.657	0.5164	1.408	7.415	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-05-22 12:35:06 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

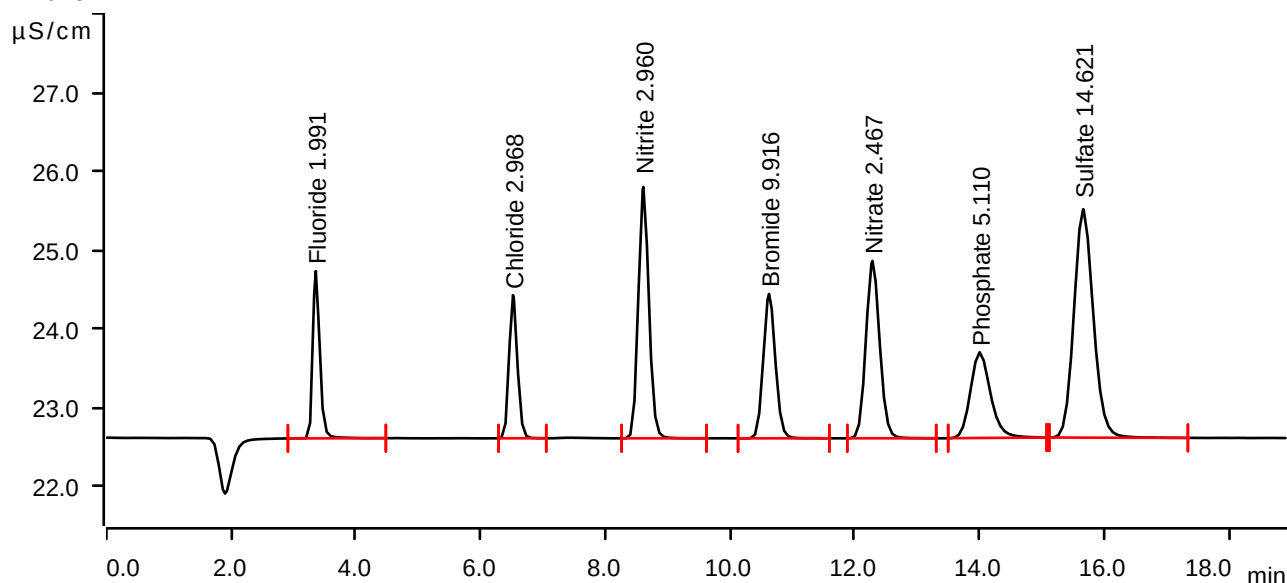

Peak number	Retention time	Area	Height	Concentration	Component name
	min	(µS/cm) x min	µS/cm	ppm	
1	3.358	0.2749	2.123	1.991	Fluoride
2	6.520	0.2820	1.816	2.968	Chloride
3	8.610	0.6298	3.190	2.960	Nitrite
4	10.625	0.4133	1.833	9.916	Bromide
5	12.283	0.5789	2.251	2.467	Nitrate
6	14.002	0.4067	1.087	5.110	Phosphate
7	15.660	1.0476	2.898	14.621	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-05-22 12:56:31 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

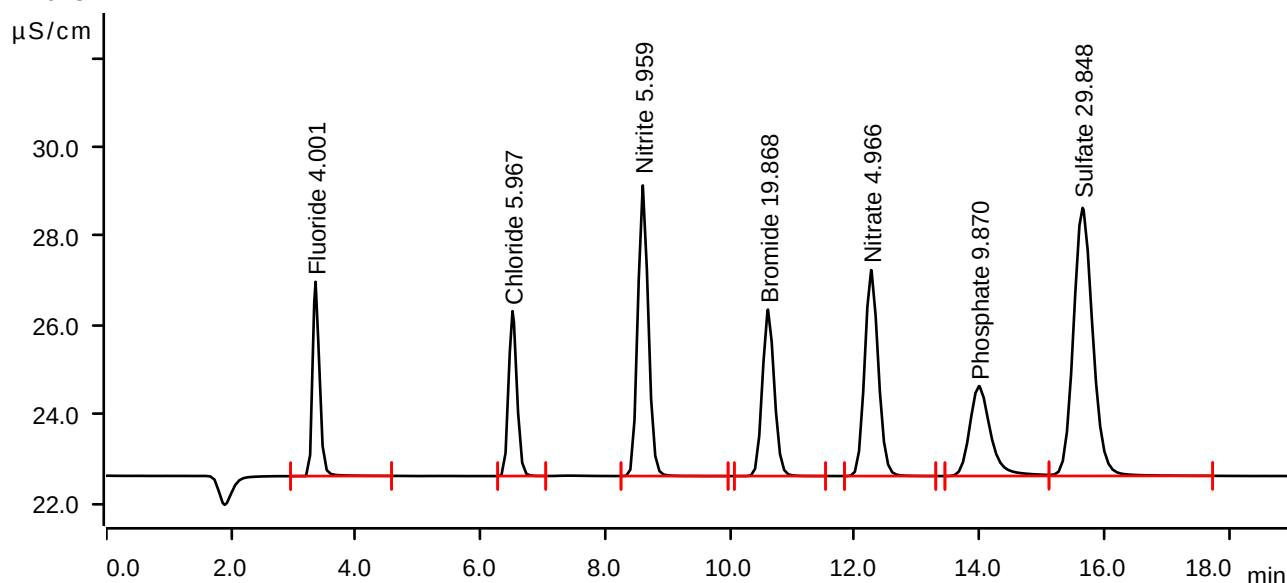

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.5553	4.361	4.001	Fluoride
2	6.512	0.5713	3.701	5.967	Chloride
3	8.602	1.2834	6.525	5.959	Nitrite
4	10.608	0.8345	3.739	19.868	Bromide
5	12.262	1.1762	4.624	4.966	Nitrate
6	13.990	0.7883	2.019	9.870	Phosphate
7	15.652	2.1703	6.019	29.848	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-05-22 13:17:57 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

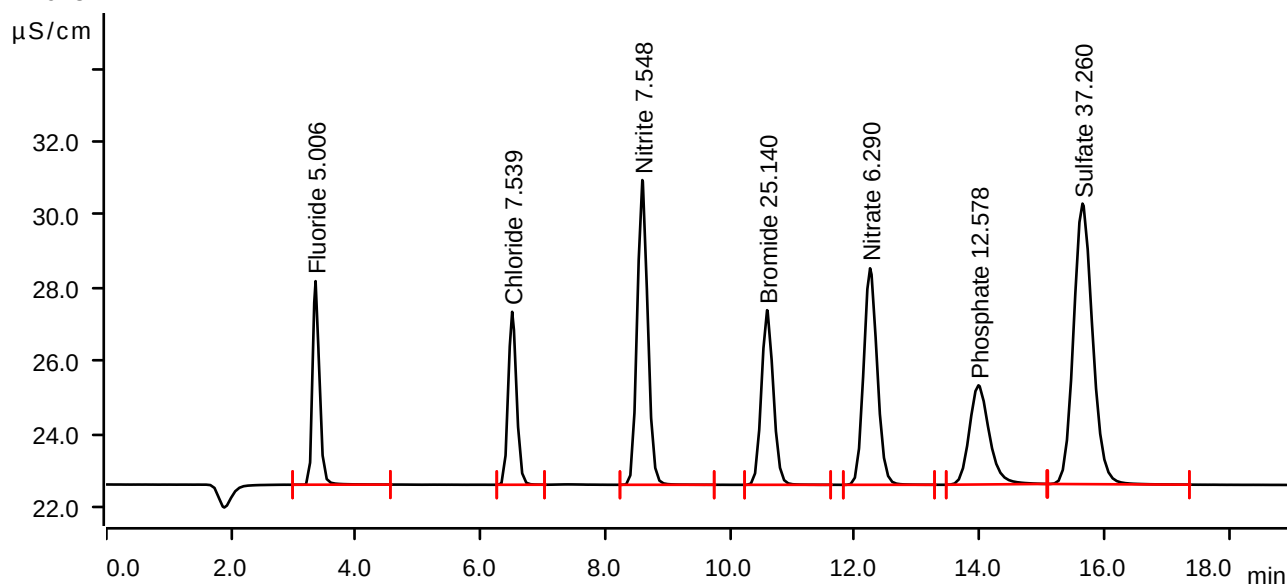

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.355	0.6954	5.562	5.006	Fluoride
2	6.507	0.7229	4.726	7.539	Chloride
3	8.593	1.6297	8.328	7.548	Nitrite
4	10.593	1.0576	4.774	25.140	Bromide
5	12.245	1.4927	5.918	6.290	Nitrate
6	13.982	1.0054	2.711	12.578	Phosphate
7	15.650	2.7168	7.668	37.260	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-05-22 13:39:25 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

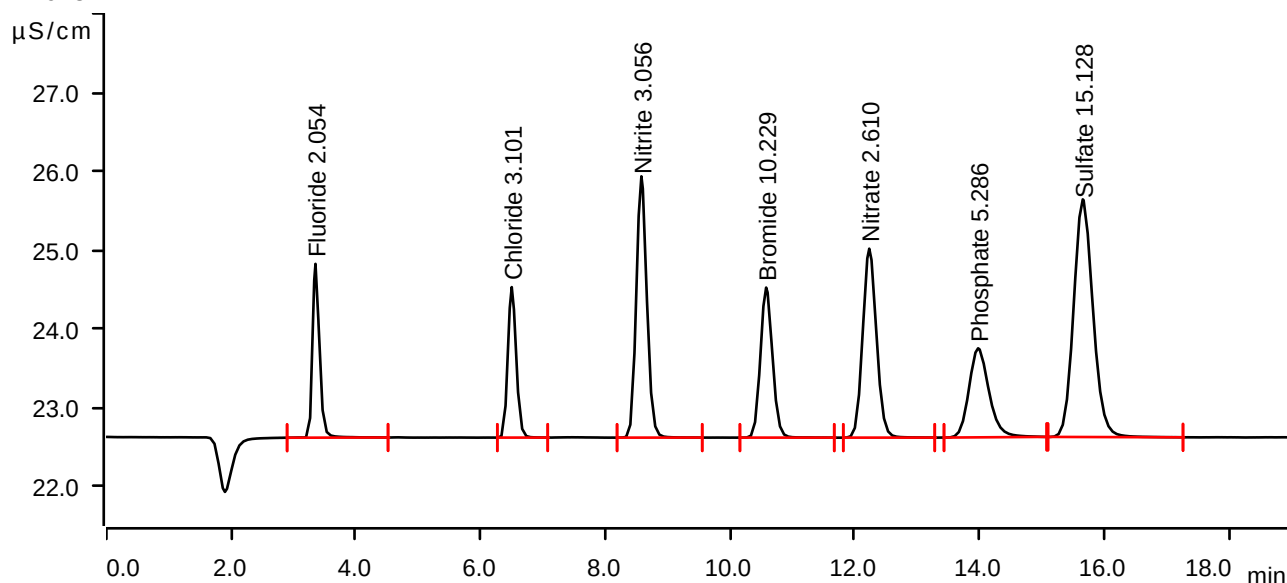

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.2837	2.205	2.054	Fluoride
2	6.500	0.2948	1.910	3.101	Chloride
3	8.578	0.6509	3.316	3.056	Nitrite
4	10.578	0.4266	1.904	10.229	Bromide
5	12.232	0.6129	2.398	2.610	Nitrate
6	13.977	0.4208	1.130	5.286	Phosphate
7	15.655	1.0850	3.016	15.128	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-05-22 14:22:21 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.66 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

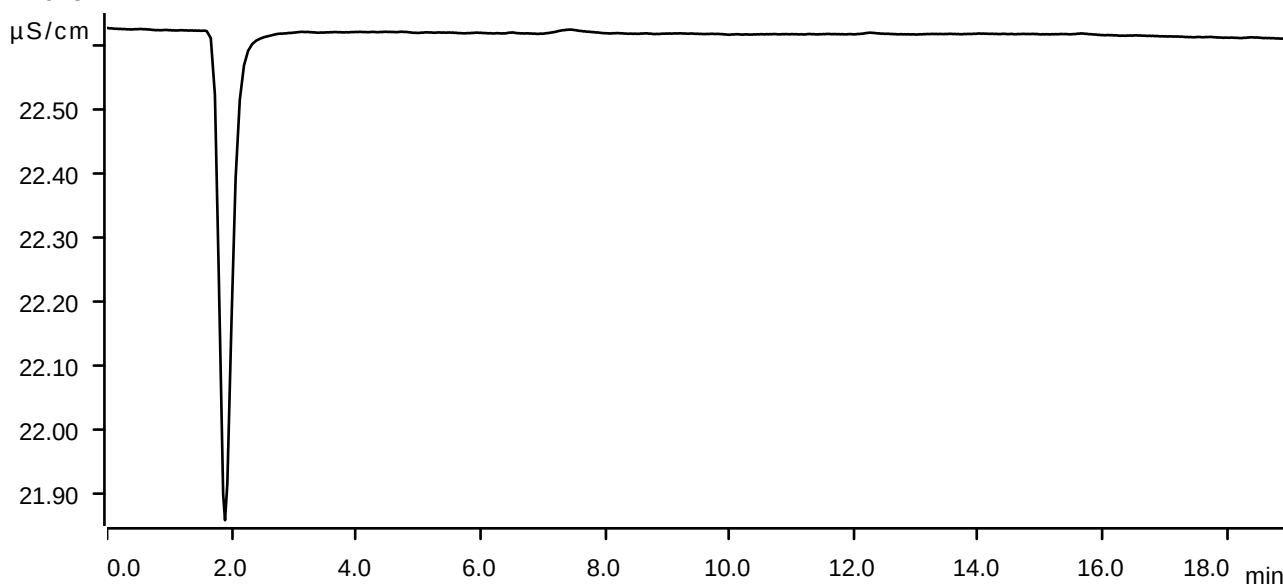


Sample data

Ident CCV
 Sample type Check standard 1
 Determination start 2025-06-05 09:50:16 UTC-4
 Method IC1-052225
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.32 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

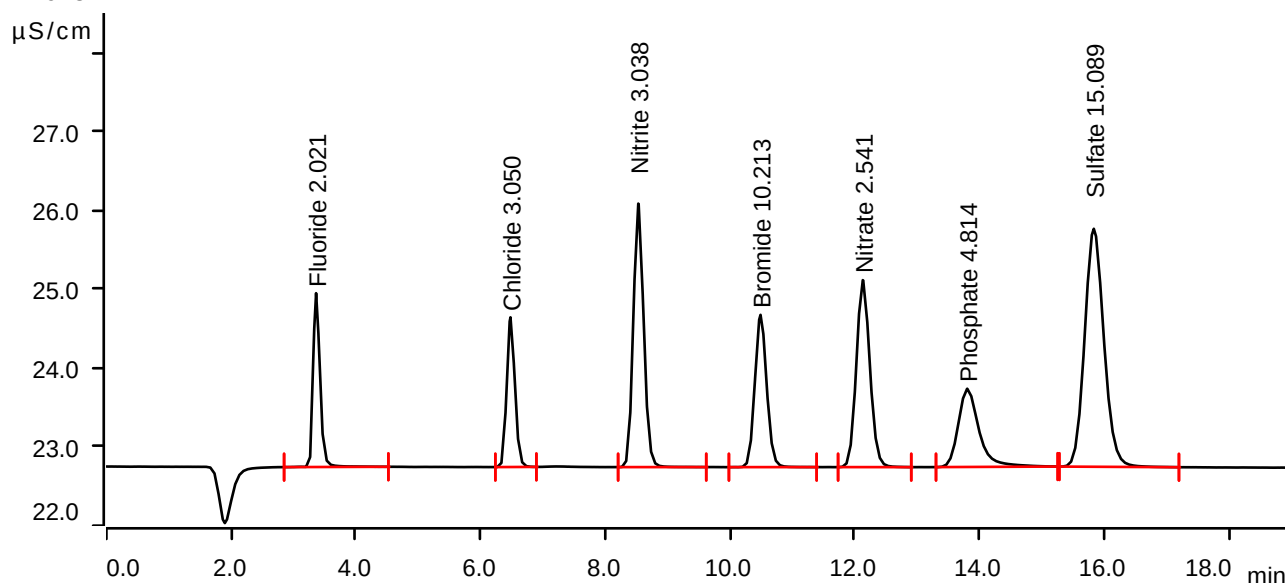

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.363	0.2791	2.206	2.021	Fluoride
2	6.480	0.2899	1.900	3.050	Chloride
3	8.528	0.6470	3.344	3.038	Nitrite
4	10.488	0.4259	1.933	10.213	Bromide
5	12.128	0.5964	2.373	2.541	Nitrate
6	13.803	0.3829	0.993	4.814	Phosphate
7	15.832	1.0821	3.020	15.089	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2025-06-05 10:11:45 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

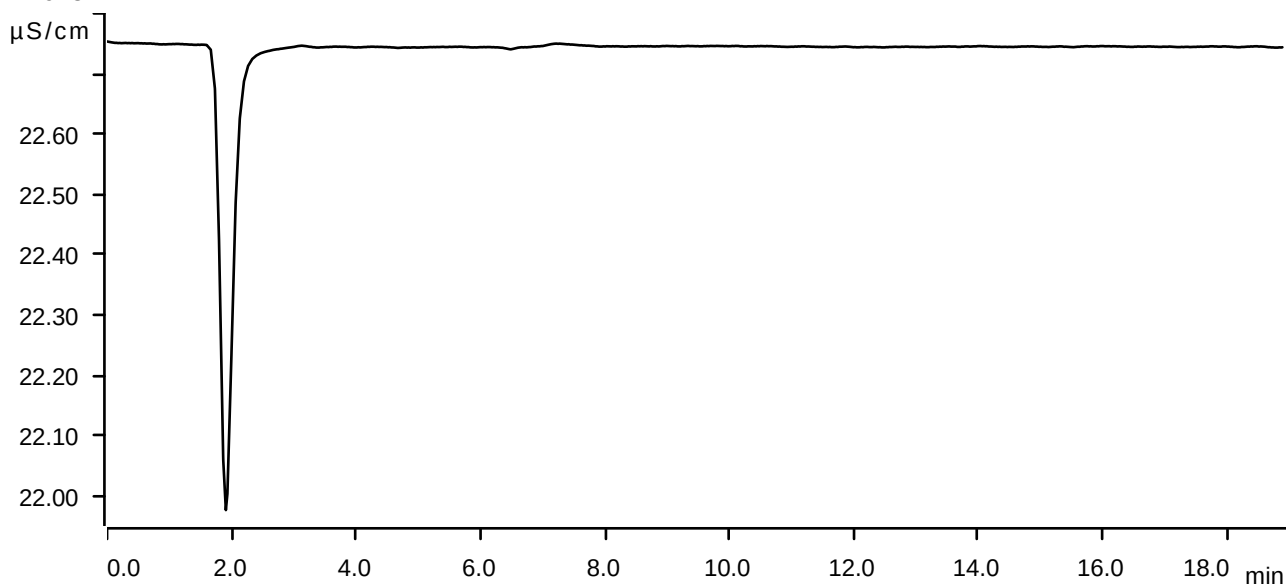


Sample data

Ident LB136017BLW
Sample type Sample
Determination start 2025-06-05 10:33:15 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

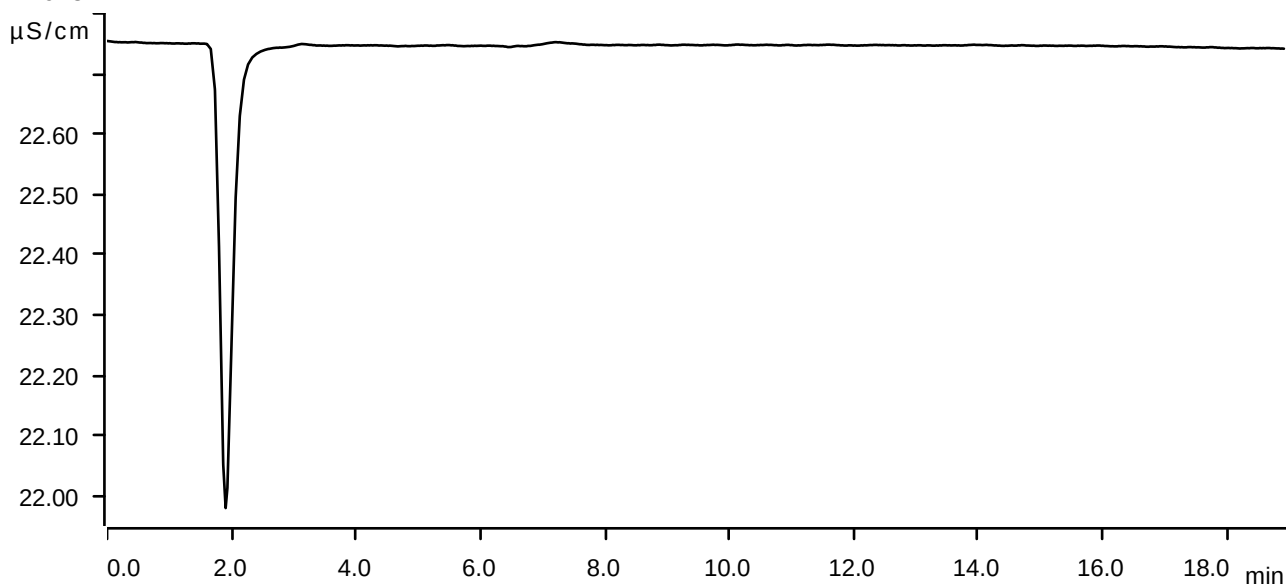Anions


Sample data

Ident LB136017BSW
Sample type Check standard 1
Determination start 2025-06-05 10:54:46 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.32 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

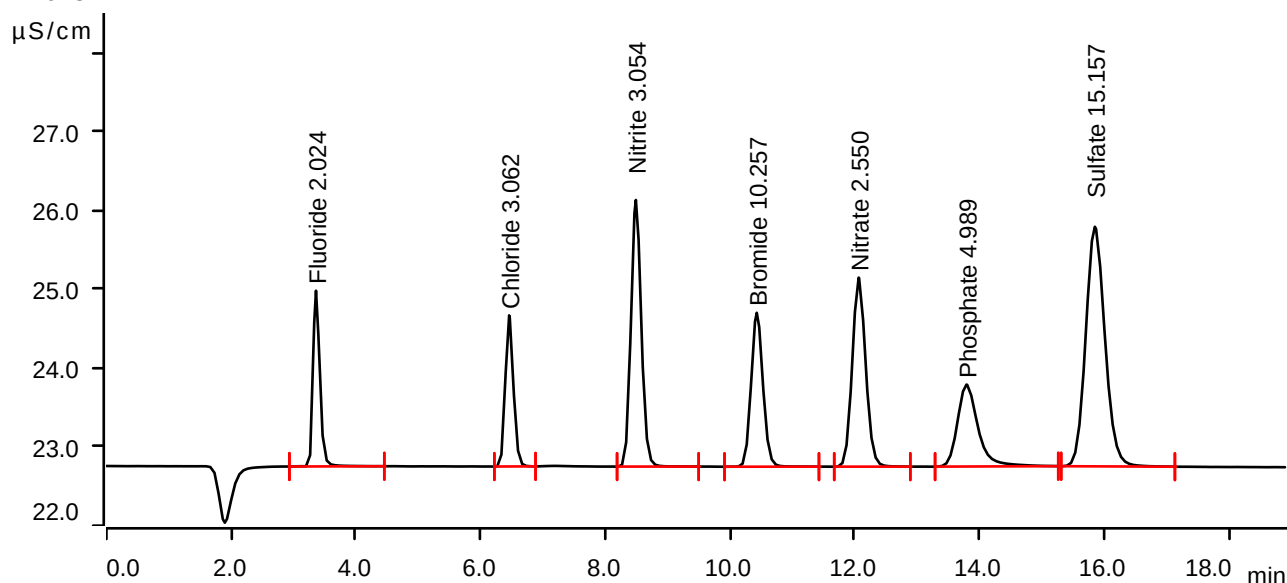

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.362	0.2796	2.229	2.024	Fluoride
2	6.458	0.2911	1.917	3.062	Chloride
3	8.490	0.6504	3.383	3.054	Nitrite
4	10.428	0.4278	1.953	10.257	Bromide
5	12.062	0.5987	2.399	2.550	Nitrate
6	13.790	0.3970	1.040	4.989	Phosphate
7	15.848	1.0872	3.041	15.157	Sulfate


Sample data

Ident Q2231-01
Sample type Sample
Determination start 2025-06-05 11:39:06 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.20 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

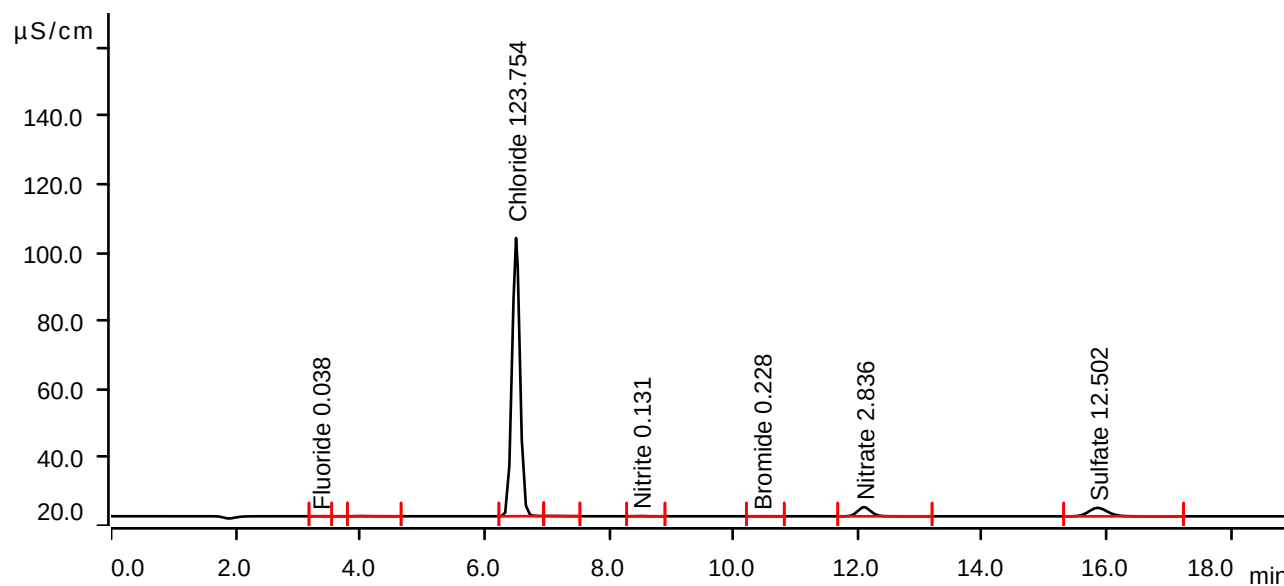

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.365	0.0025	0.017	0.038	Fluoride
2	3.635	0.0008	0.004	invalid	
3	3.992	0.0159	0.063	invalid	
4	6.508	11.9339	81.458	123.754	Chloride
5	7.102	0.0068	0.022	invalid	
6	8.515	0.0135	0.071	0.131	Nitrite
7	10.455	0.0034	0.014	0.228	Bromide
8	12.100	0.6671	2.682	2.836	Nitrate
9	15.855	0.8914	2.487	12.502	Sulfate


Sample data

Ident Q2231-03
Sample type Sample
Determination start 2025-06-05 12:00:43 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.20 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

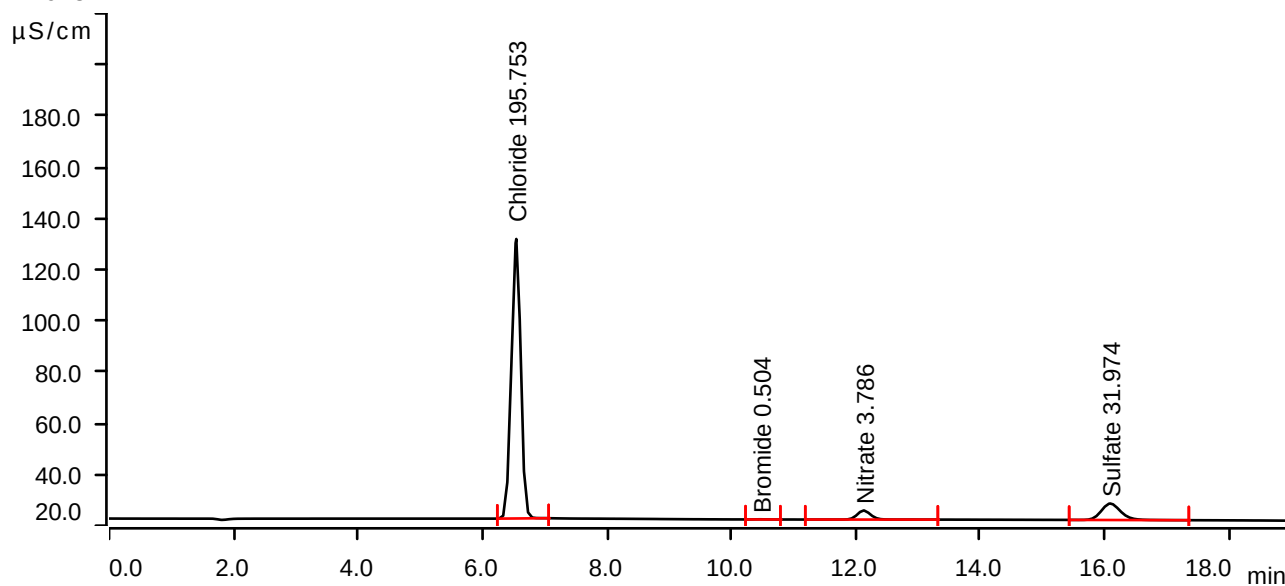

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.545	18.8795	109.136	195.753	Chloride
2	10.468	0.0150	0.071	0.504	Bromide
3	12.127	0.8940	3.548	3.786	Nitrate
4	16.088	2.3270	6.432	31.974	Sulfate


Sample data

Ident Q2231-04
Sample type Sample
Determination start 2025-06-05 12:22:16 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.09 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

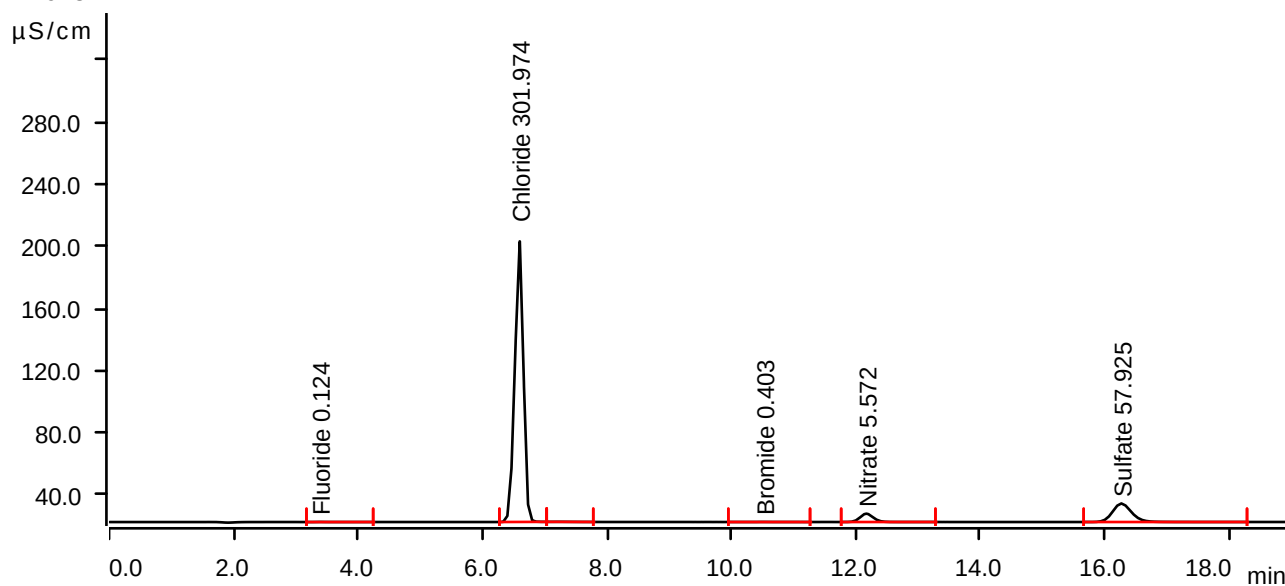

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.0144	0.073	0.124	Fluoride
2	6.600	29.1263	180.769	301.974	Chloride
3	7.243	0.0186	0.054	invalid	
4	10.527	0.0108	0.046	0.403	Bromide
5	12.170	1.3211	5.367	5.572	Nitrate
6	16.267	4.2404	11.935	57.925	Sulfate


Sample data

Ident Q2231-04MS
 Sample type Sample
 Determination start 2025-06-05 12:43:50 UTC-4
 Method IC1-052225
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.15 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

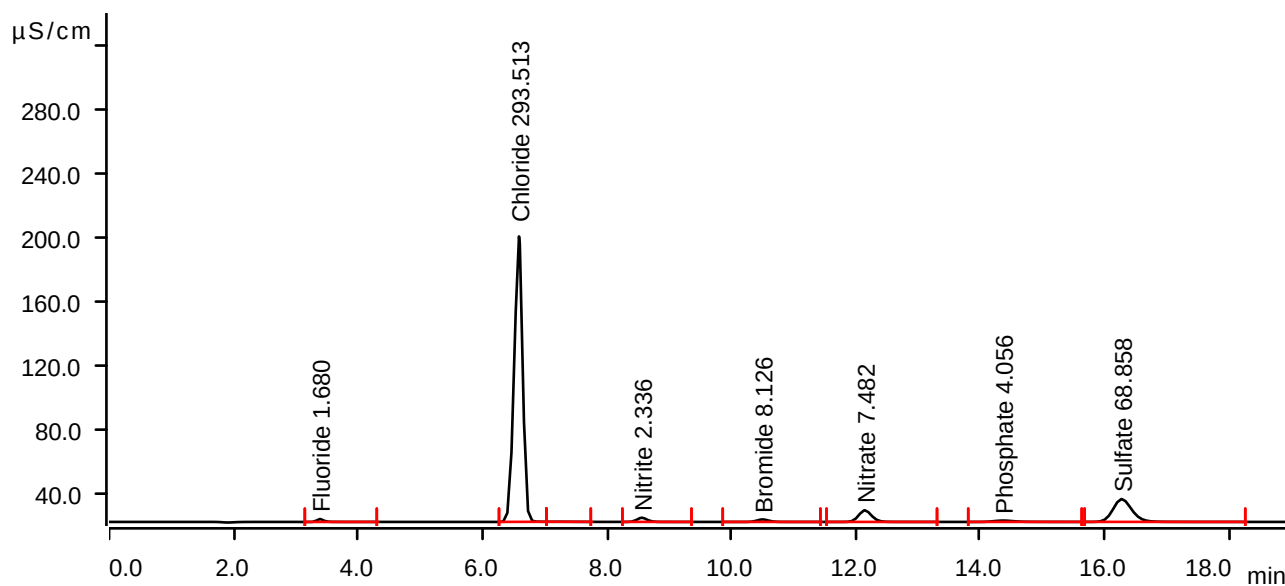

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.387	0.2315	1.800	1.680	Fluoride
2	6.588	28.3101	178.307	293.513	Chloride
3	7.227	0.0169	0.050	invalid	
4	8.562	0.4940	2.600	2.336	Nitrite
5	10.502	0.3376	1.544	8.126	Bromide
6	12.145	1.7775	7.270	7.482	Nitrate
7	14.363	0.3222	0.832	4.056	Phosphate
8	16.273	5.0465	14.273	68.858	Sulfate


Sample data

Ident Q2331-04MSD
Sample type Sample
Determination start 2025-06-05 13:05:25 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.04 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

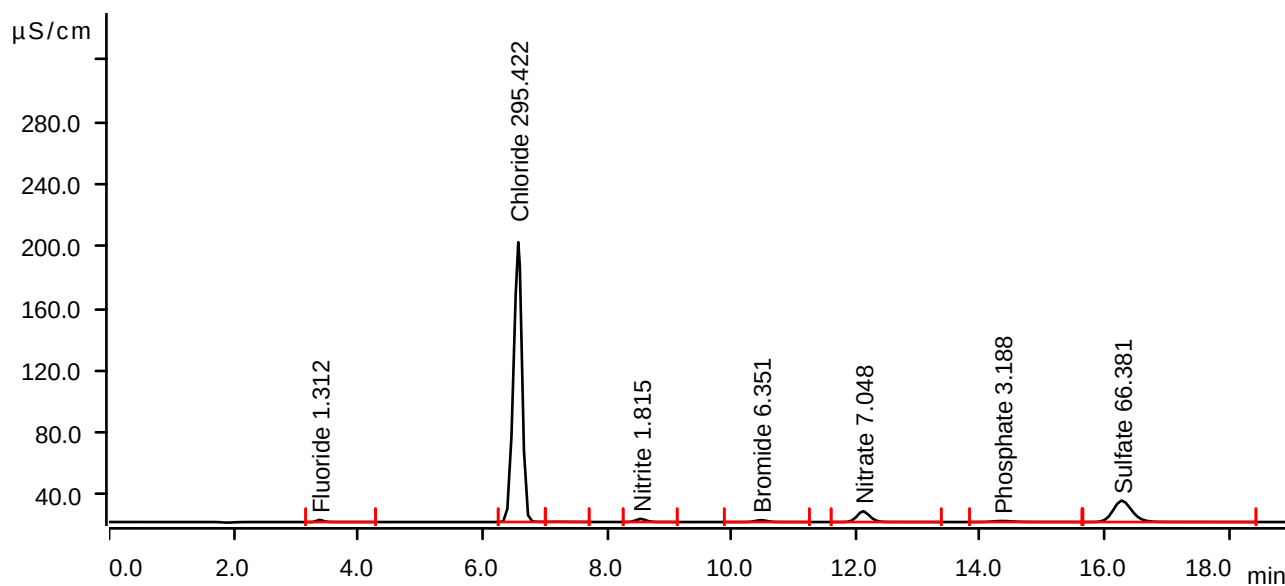

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.383	0.1802	1.395	1.312	Fluoride
2	6.577	28.4942	180.236	295.422	Chloride
3	7.215	0.0165	0.049	invalid	
4	8.543	0.3804	2.011	1.815	Nitrite
5	10.477	0.2625	1.207	6.351	Bromide
6	12.117	1.6740	6.866	7.048	Nitrate
7	14.352	0.2525	0.654	3.188	Phosphate
8	16.275	4.8639	13.774	66.381	Sulfate


Sample data

Ident Q2231-05
Sample type Sample
Determination start 2025-06-05 13:26:50 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.04 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

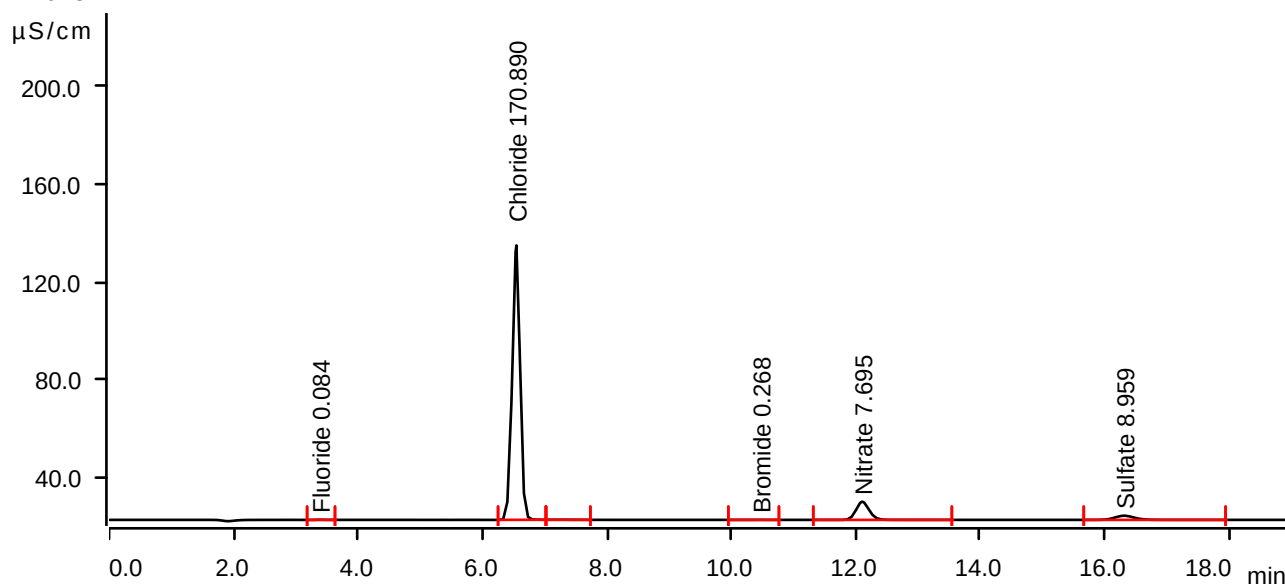

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.387	0.0089	0.069	0.084	Fluoride
2	6.547	16.4810	112.486	170.890	Chloride
3	7.240	0.0103	0.031	invalid	
4	10.470	0.0051	0.023	0.268	Bromide
5	12.103	1.8285	7.492	7.695	Nitrate
6	16.312	0.6302	1.719	8.959	Sulfate


Sample data

Ident Q2231-04DLX5
Sample type Sample
Determination start 2025-06-05 13:48:23 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.04 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

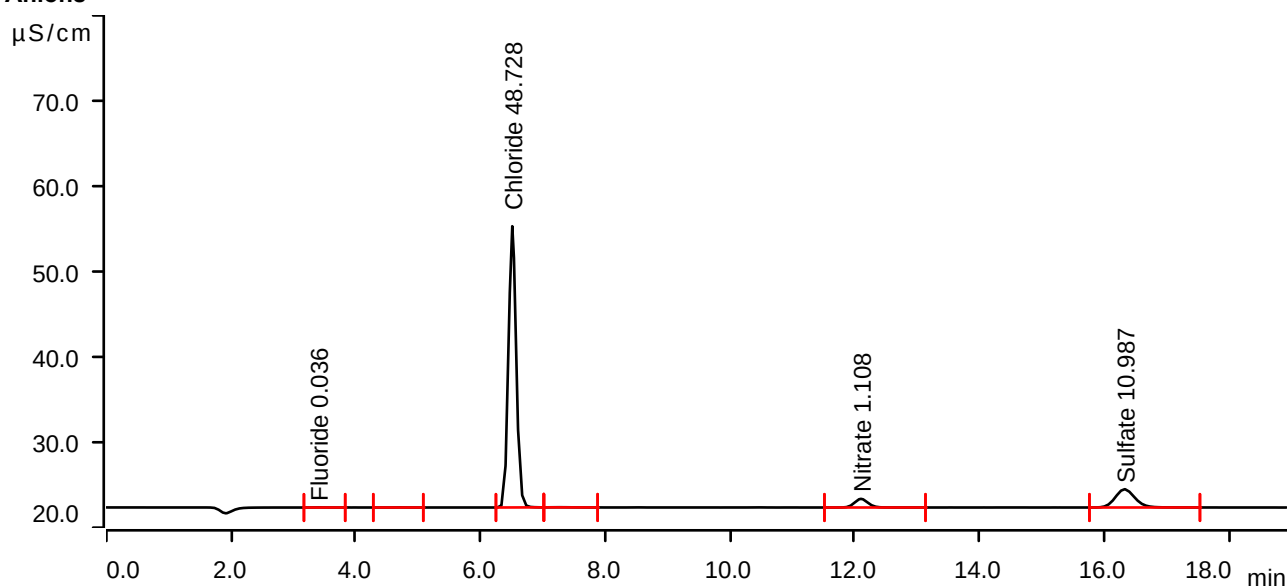

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.0022	0.014	0.036	Fluoride
2	4.708	0.0019	0.011	invalid	
3	6.508	4.6963	32.939	48.728	Chloride
4	7.253	0.0059	0.017	invalid	
5	12.098	0.2539	1.012	1.108	Nitrate
6	16.325	0.7797	2.137	10.987	Sulfate


Sample data

Ident CCV
 Sample type Check standard 1
 Determination start 2025-06-05 14:09:56 UTC-4
 Method IC1-052225
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 10.92 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

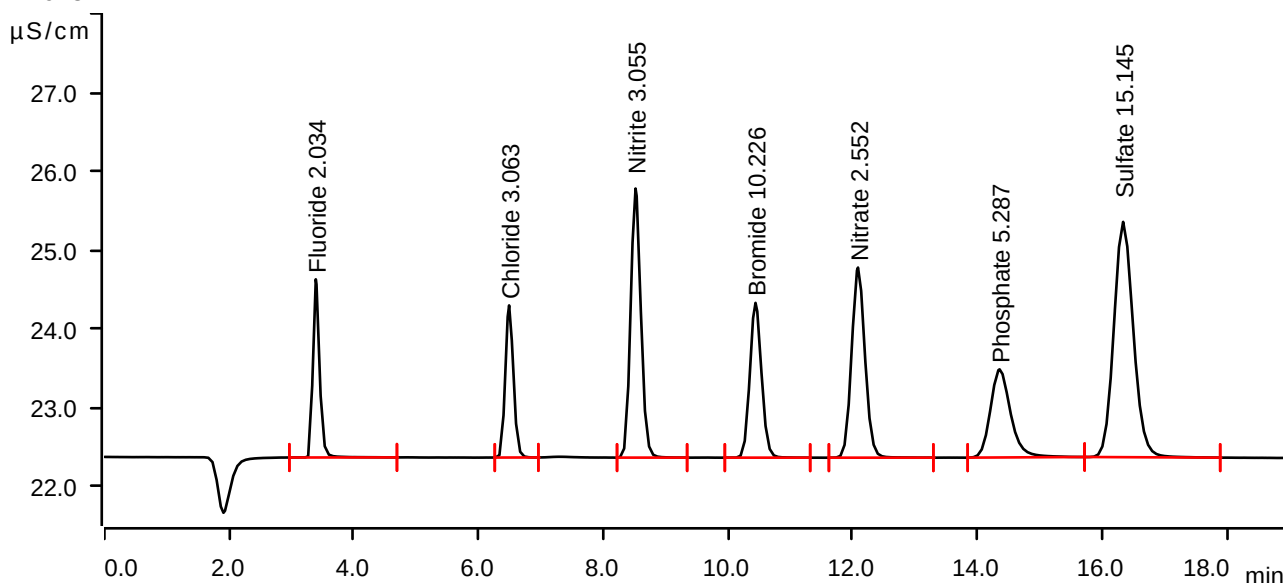

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.390	0.2809	2.260	2.034	Fluoride
2	6.490	0.2911	1.930	3.063	Chloride
3	8.517	0.6506	3.415	3.055	Nitrite
4	10.440	0.4265	1.964	10.226	Bromide
5	12.083	0.5990	2.413	2.552	Nitrate
6	14.353	0.4209	1.119	5.287	Phosphate
7	16.333	1.0863	2.986	15.145	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-06-05 14:31:25 UTC-4
Method IC1-052225
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 10.92 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions