

66136087

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

6/10/2025 13:48

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.004	0.0	0.059	
ICB1	-0.005	0.0	0.006	
CCV1	1.001	0.0	0.059	
CCB1	-0.003	0.0	0.006	
PB168386BL	-0.002	0.0	0.006	
PB168386BS	1.001	0.0	0.059	
Q2126-03	0.023	0.0	0.008	
PB168388BL	0.001	0.0	0.007	
PB168388BS	1.012	0.0	0.060	
Q2126-09	0.024	0.0	0.008	
CCV2	0.999	0.0	0.059	
CCB2	-0.002	0.0	0.006	

N	12
Mean	0.421
SD	0.5142
CV%	122.10

Aquakem v. 7.2AQ1

Results from time period:

Tue Jun 10 11:56:36 2025

Tue Jun 10 13:43:05 2025

Sample Id	Sam/Ctr/cA	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0072	mg/l	6/10/2025 12:36:09	
0.05PPM	A	Phenolics-	P	0.0573	mg/l	6/10/2025 12:36:10	
0.1PPM	A	Phenolics-	P	0.1053	mg/l	6/10/2025 12:36:11	
0.25PPM	A	Phenolics-	P	0.2503	mg/l	6/10/2025 12:36:12	
0.50PPM	A	Phenolics-	P	0.5049	mg/l	6/10/2025 12:36:13	
1.0PPM	A	Phenolics-	P	0.9822	mg/l	6/10/2025 12:36:14	
2.0PPM	A	Phenolics-	P	2.0072	mg/l	6/10/2025 12:36:15	
ICV1	S	Phenolics-	P	1.004	mg/l	6/10/2025 13:32:53	
ICB1	S	Phenolics-	P	-0.0049	mg/l	6/10/2025 13:32:55	
CCV1	S	Phenolics-	P	1.0009	mg/l	6/10/2025 13:32:56	
CCB1	S	Phenolics-	P	-0.0025	mg/l	6/10/2025 13:32:59	
PB168386BL	S	Phenolics-	P	-0.0021	mg/l	6/10/2025 13:33:01	
PB168386BS	S	Phenolics-	P	1.001	mg/l	6/10/2025 13:33:03	
Q2126-03	S	Phenolics-	P	0.0226	mg/l	6/10/2025 13:42:55	
PB168388BL	S	Phenolics-	P	0.0012	mg/l	6/10/2025 13:42:57	
PB168388BS	S	Phenolics-	P	1.0124	mg/l	6/10/2025 13:42:59	
Q2126-09	S	Phenolics-	P	0.0235	mg/l	6/10/2025 13:43:01	
CCV2	S	Phenolics-	P	0.9992	mg/l	6/10/2025 13:43:02	
CCB2	S	Phenolics-	P	-0.0019	mg/l	6/10/2025 13:43:04	

CHEMTECH CONSULTING GROUP INC
284 Sheffield Street, Mountainside, NJ 07092

6/10/2025 12:39

Reviewed by : RM

Instrument ID : Konelab


Test Phenolics-

Accepted 6/10/2025 12:39

Factor 18.97
Bias 0.007

Coeff. of det. 0.999834

Errors

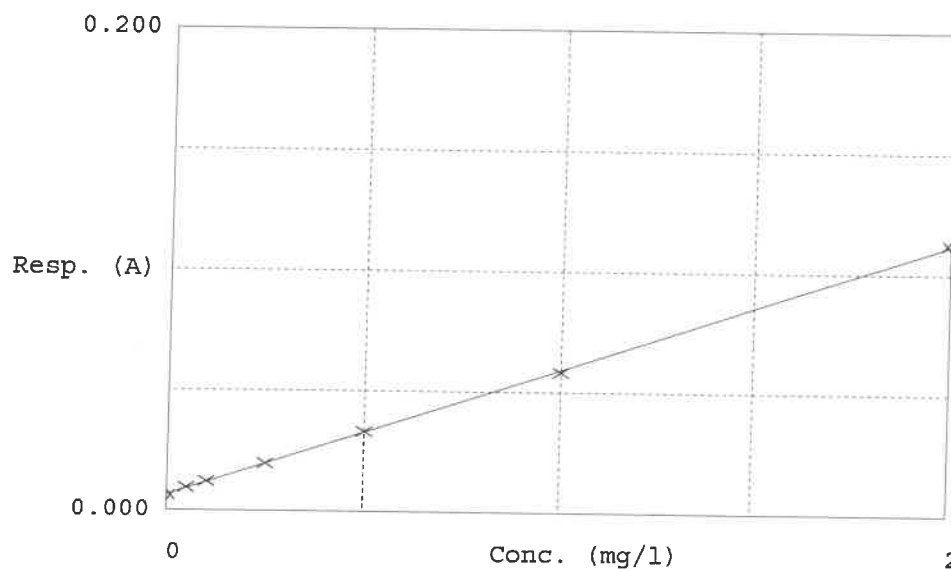

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.006	-0.0072	0.0000	-
2	Phenol-2	0.010	0.0573	0.0500	14.6
3	Phenol-2	0.012	0.1053	0.1000	5.3
4	Phenol-2	0.020	0.2503	0.2500	0.1
5	Phenol-2	0.033	0.5049	0.5000	1.0
6	Phenol-2	0.058	0.9822	1.0000	-1.8
7	Phenol-2	0.112	2.0072	2.0000	0.4

06/10/2025
RM