

LB186107


7470A

INSTRUMENT ID: CV1

Linear

 μ Abs.:

41243

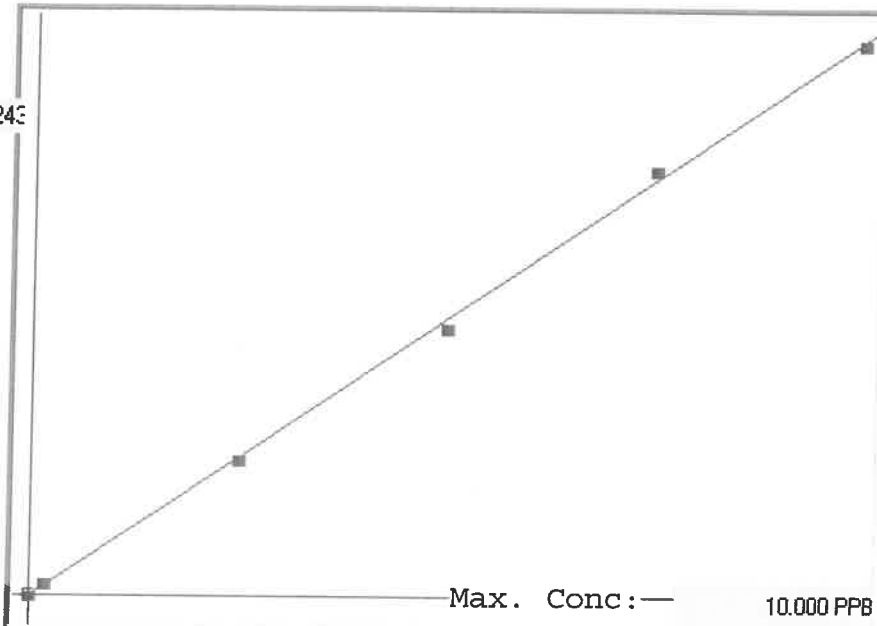

A= 0.0000e+000

B= 2.4060e-004

C= 2.1216e-002

Rho= 0.9995560

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%RSD
0.0	0.000	0.034	0.034	52	0.000	52	0				
0.2	0.200	0.239	0.039	906	0.0 %	906					
2.5	2.500	2.464	-0.036	10155	0.0 %	10155					
5.0	5.000	4.829	-0.171	19981	0.0 %	19981					
7.5	7.500	7.690	0.190	31874	0.0 %	31874					
10.0	10.000	9.944	-0.056	41243	0.0 %	41243					

0/100
 1
 20
 1
 3
 3
 1

LB136107 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 11 Jun 2025 12:31:05

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	30	52	-	0.0000	7470A	PPB	11 Jun 2025 12:38:14	S	Std
0.2 - 1	50-2	906	-	0.2000	7470A	PPB	11 Jun 2025 12:40:32	S	Std
2.5 - 1	52-7	10155	-	2.5000	7470A	PPB	11 Jun 2025 12:42:49	S	Std
5.0 - 1	55	19981	-	5.0000	7470A	PPB	11 Jun 2025 12:45:06	S	Std
7.5 - 1	57-5	31874	-	7.5000	7470A	PPB	11 Jun 2025 12:47:23	S	Std
10.0 - 1	58	41243	-	10.0000	7470A	PPB	11 Jun 2025 12:49:41	S	Std
ICV34 - 1	ICV34	15766	3.8144	-	7470A	PPB	11 Jun 2025 12:52:32	U	SMPL
ICB34 - 1	ICB34	-192	-0.0250	-	7470A	PPB	11 Jun 2025 12:54:47	U	SMPL
CCV27 - 1	CCV27	20065	4.8488	-	7470A	PPB	11 Jun 2025 12:57:04	U	SMPL
CCB27 - 1	CCB27	-188	-0.0240	-	7470A	PPB	11 Jun 2025 12:59:19	U	SMPL
CRA - 1	CRA	809	0.2159	-	7470A	PPB	11 Jun 2025 13:01:36	U	SMPL
HighStd - 1	HighStd	39685	9.5693	-	7470A	PPB	11 Jun 2025 13:03:51	U	SMPL
ChkStd - 1	ChkStd	27860	6.7242	-	7470A	PPB	11 Jun 2025 13:06:06	U	SMPL
PB168420BL - 1	PBW	-325	-0.0570	-	7470A	PPB	11 Jun 2025 13:08:26	U	SMPL
PB168420BS - 1	LCSW	16830	4.0704	-	7470A	PPB	11 Jun 2025 13:10:44	U	SMPL
Q2279-01 - 1	301-469-5TH-AVE	1974	0.4962	-	7470A	PPB	11 Jun 2025 13:13:01	U	SMPL
Q2279-01DUP - 1	301-469-5TH-AVEDUP	2093	0.5248	-	7470A	PPB	11 Jun 2025 13:15:19	U	SMPL
Q2279-01MS - 1	301-469-5TH-AVEMS	18364	4.4395	-	7470A	PPB	11 Jun 2025 13:17:37	U	SMPL
Q2279-01MSD - 1	301-469-5TH-AVEMSD	16342	3.9530	-	7470A	PPB	11 Jun 2025 13:19:55	U	SMPL
Q2282-04 - 1	251233	23796	5.7464	-	7470A	PPB	11 Jun 2025 13:22:14	U	SMPL
CCV28 - 1	CCV28	21530	5.2012	-	7470A	PPB	11 Jun 2025 13:33:02	U	SMPL
CCB28 - 1	CCB28	-286	-0.0476	-	7470A	PPB	11 Jun 2025 13:35:17	U	SMPL
Q2284-02 - 1	TRE-GAS-25-0068	911	0.2404	-	7470A	PPB	11 Jun 2025 13:37:35	U	SMPL
Q2286-03 - 1	LAW-25-0084	569	0.1581	-	7470A	PPB	11 Jun 2025 13:39:50	U	SMPL
Q2279-01LX5 - 1		492	0.1396	-	7470A	PPB	11 Jun 2025 13:45:44	U	SMPL
Q2279-01A - 1		17824	4.3096	-	7470A	PPB	11 Jun 2025 13:47:59	U	SMPL
CCV29 - 1	CCV29	19178	4.6354	-	7470A	PPB	11 Jun 2025 13:50:14	U	SMPL
CCB29 - 1	CCB29	-289	-0.0483	-	7470A	PPB	11 Jun 2025 13:52:34	U	SMPL