

| Ident       | Instrument IC-1 |         |         |         | Analyst: NF |          | Method: 300.0 / 9056A |                            | Initial Analyst |
|-------------|-----------------|---------|---------|---------|-------------|----------|-----------------------|----------------------------|-----------------|
|             | Con F-          | Con CL- | Con NO2 | Con BR- | Con NO3     | Con HPO4 | Con SO4               | Method nar date time       |                 |
| STD1        | 0.000           | 0.000   | 0.000   | 0.000   | 0.000       | 0.000    | 0.000                 | IC1-052225 5/22/2025 11:09 | 10 NF/IZ        |
| STD2        | 0.430           | 0.640   | 0.649   | 2.129   | 0.543       | 1.098    | 3.287                 | IC1-052225 5/22/2025 11:30 | 10 NF/IZ        |
| STD3        | 0.795           | 1.207   | 1.205   | 4.018   | 1.004       | 1.867    | 6.069                 | IC1-052225 5/22/2025 11:52 | 10 NF/IZ        |
| STD4        | 0.977           | 1.480   | 1.479   | 4.929   | 1.229       | 2.477    | 7.415                 | IC1-052225 5/22/2025 12:13 | 10 NF/IZ        |
| STD5        | 1.991           | 2.968   | 2.960   | 9.916   | 2.467       | 5.110    | 14.621                | IC1-052225 5/22/2025 12:35 | 10 NF/IZ        |
| STD6        | 4.001           | 5.967   | 5.959   | 19.868  | 4.966       | 9.870    | 29.848                | IC1-052225 5/22/2025 12:56 | 10 NF/IZ        |
| STD7        | 5.006           | 7.539   | 7.548   | 25.140  | 6.290       | 12.578   | 37.260                | IC1-052225 5/22/2025 13:17 | 10 NF/IZ        |
| ICV         | 2.054           | 3.101   | 3.056   | 10.229  | 2.610       | 5.286    | 15.128                | IC1-052225 5/22/2025 13:39 | 10 NF/IZ        |
| ICB         | 0.000           | 0.000   | 0.000   | 0.000   | 0.000       | 0.000    | 0.000                 | IC1-052225 5/22/2025 14:22 | 10 NF/IZ        |
| CCV         | 2.056           | 3.048   | 3.044   | 10.190  | 2.531       | 5.283    | 15.071                | IC1-052225 6/20/2025 13:39 | 10 NF/IZ        |
| CCB         | 0.000           | 0.000   | 0.000   | 0.000   | 0.000       | 0.000    | 0.000                 | IC1-052225 6/20/2025 14:01 | 10 NF/IZ        |
| LB136234BLW | 0.000           | 0.000   | 0.000   | 0.000   | 0.000       | 0.000    | 0.000                 | IC1-052225 6/20/2025 14:22 | 10 NF/IZ        |
| LB136234BSW | 2.059           | 3.049   | 3.050   | 10.208  | 2.534       | 5.287    | 15.100                | IC1-052225 6/20/2025 14:44 | 10 NF/IZ        |
| Q2385-01    | 0.090           | 163.638 | 0.000   | 0.216   | 0.653       | 0.000    | 18.371                | IC1-052225 6/20/2025 15:37 | 10 NF/IZ        |
| Q2385-01MS  | 2.124           | 159.399 | 3.025   | 10.220  | 3.137       | 5.118    | 32.980                | IC1-052225 6/20/2025 16:21 | 10 NF/IZ        |
| Q2385-01MSD | 2.133           | 159.243 | 3.025   | 10.205  | 3.135       | 5.309    | 33.039                | IC1-052225 6/20/2025 16:42 | 10 NF/IZ        |
| CCV         | 2.067           | 3.047   | 3.045   | 10.194  | 2.530       | 5.343    | 15.067                | IC1-052225 6/20/2025 17:04 | 10 NF/IZ        |
| CCB         | 0.000           | 0.000   | 0.000   | 0.000   | 0.000       | 0.000    | 0.000                 | IC1-052225 6/20/2025 17:25 | 10 NF/IZ        |

Clear table


| Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A |                      |                       |                       |                       |                       |                        |                       |            |                 |                         |         |
|--------------------------------------------------------|----------------------|-----------------------|-----------------------|-----------------------|-----------------------|------------------------|-----------------------|------------|-----------------|-------------------------|---------|
| ident                                                  | concentra<br>tion F- | concentratio<br>n CL- | concentrati<br>on NO2 | concentrati<br>on BR- | concentrati<br>on NO3 | concentrati<br>on HPO4 | concentrati<br>on SO4 | file name  | date time       | Initial<br>wt/<br>Final | Analyst |
| STD1                                                   | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                | IC1-052225 | 5/22/2025 11:09 | 10                      | NF/IZ   |
| STD2                                                   | 0.4300               | 0.6400                | 0.6490                | 2.1290                | 0.5430                | 1.0980                 | 3.2870                | IC1-052225 | 5/22/2025 11:30 | 10                      | NF/IZ   |
| STD3                                                   | 0.7950               | 1.2070                | 1.2050                | 4.0180                | 1.0040                | 1.8670                 | 6.0690                | IC1-052225 | 5/22/2025 11:52 | 10                      | NF/IZ   |
| STD4                                                   | 0.9770               | 1.4800                | 1.4790                | 4.9290                | 1.2290                | 2.4770                 | 7.4150                | IC1-052225 | 5/22/2025 12:13 | 10                      | NF/IZ   |
| STD5                                                   | 1.9910               | 2.9680                | 2.9600                | 9.9160                | 2.4670                | 5.1100                 | 14.6210               | IC1-052225 | 5/22/2025 12:35 | 10                      | NF/IZ   |
| STD6                                                   | 4.0010               | 5.9670                | 5.9590                | 19.8680               | 4.9660                | 9.8700                 | 29.8480               | IC1-052225 | 5/22/2025 12:56 | 10                      | NF/IZ   |
| STD7                                                   | 5.0060               | 7.5390                | 7.5480                | 25.1400               | 6.2900                | 12.5780                | 37.2600               | IC1-052225 | 5/22/2025 13:17 | 10                      | NF/IZ   |
|                                                        |                      |                       |                       |                       |                       |                        |                       |            |                 |                         |         |
| ident                                                  | True<br>Value F-     | True Value<br>CL-     | True Value<br>NO2     | True Value<br>BR-     | True Value<br>NO3     | True Value<br>HPO4     | True Value<br>SO4     |            |                 |                         |         |
| STD1                                                   | 0.0000               | 0.0000                | 0.0000                | 0.0000                | 0.0000                | 0.0000                 | 0.0000                |            |                 |                         |         |
| STD2                                                   | 0.4000               | 0.6000                | 0.6000                | 2.0000                | 0.5000                | 1.0000                 | 3.0000                |            |                 |                         |         |
| STD3                                                   | 0.8000               | 1.2000                | 1.2000                | 4.0000                | 1.0000                | 2.0000                 | 6.0000                |            |                 |                         |         |
| STD4                                                   | 1.0000               | 1.5000                | 1.5000                | 5.0000                | 1.2500                | 2.5000                 | 7.5000                |            |                 |                         |         |
| STD5                                                   | 2.0000               | 3.0000                | 3.0000                | 10.0000               | 2.5000                | 5.0000                 | 15.0000               |            |                 |                         |         |
| STD6                                                   | 4.0000               | 6.0000                | 6.0000                | 20.0000               | 5.0000                | 10.0000                | 30.0000               |            |                 |                         |         |
| STD7                                                   | 5.0000               | 7.5000                | 7.5000                | 25.0000               | 6.2500                | 12.5000                | 37.0000               |            |                 |                         |         |
|                                                        |                      |                       |                       |                       |                       |                        |                       |            |                 |                         |         |
| ident                                                  | Relative<br>Error F- | Relative<br>Error CL- | Relative<br>Error NO2 | Relative<br>Error BR- | Relative<br>Error NO3 | Relative<br>Error HPO4 | Relative<br>Error SO4 |            |                 |                         |         |
| STD1                                                   |                      |                       |                       |                       |                       |                        |                       |            |                 |                         |         |
| STD2                                                   | 7.5000               | 6.6667                | 8.1667                | 6.4500                | 8.6000                | 9.8000                 | 9.5667                |            |                 |                         |         |
| STD3                                                   | -0.6250              | 0.5833                | 0.4167                | 0.4500                | 0.4000                | -6.6500                | 1.1500                |            |                 |                         |         |
| STD4                                                   | -2.3000              | -1.3333               | -1.4000               | -1.4200               | -1.6800               | -0.9200                | -1.1333               |            |                 |                         |         |
| STD5                                                   | -0.4500              | -1.0667               | -1.3333               | -0.8400               | -1.3200               | 2.2000                 | -2.5267               |            |                 |                         |         |
| STD6                                                   | 0.0250               | -0.5500               | -0.6833               | -0.6600               | -0.6800               | -1.3000                | -0.5067               |            |                 |                         |         |
| STD7                                                   | 0.1200               | 0.5200                | 0.6400                | 0.5600                | 0.6400                | 0.6240                 | 0.7027                |            |                 |                         |         |

Initial  
wt/  
Final

Analyst

# Fluoride (Anions)

( $\mu\text{S}/\text{cm}$ ) x min

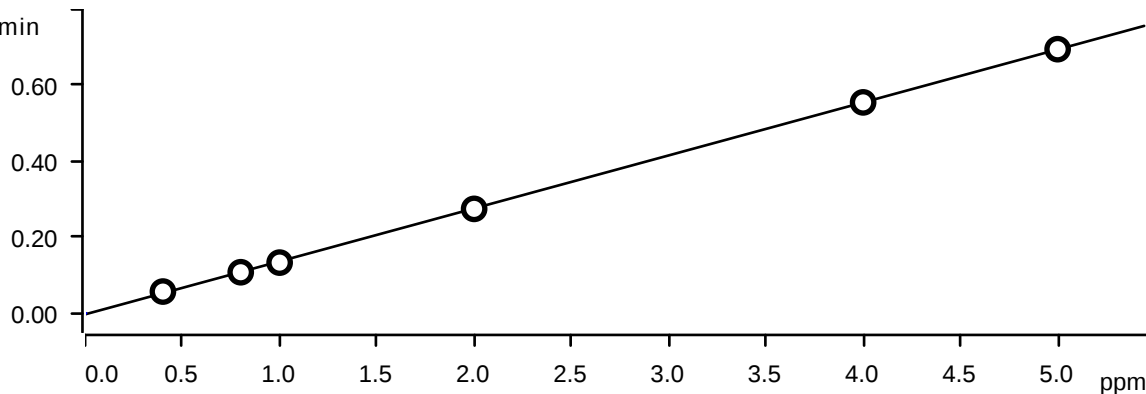

Function: . . . . .  $A = -2.82659E-3 + 0.0139492 \times Q$


Relative standard deviation . . . . . 0.920519 %

Correlation coefficient . . . . . 0.999955

| Sample type | Index | Conc. | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|-------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000 | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2025-05-22 11:09:38 UTC-4 | used |
| Standard 2  | 1     | 0.400 | 10.0   | 1.0      | 1.0           | 0.057 | STD2  | 2025-05-22 11:30:53 UTC-4 | used |
| Standard 3  | 1     | 0.800 | 10.0   | 1.0      | 1.0           | 0.108 | STD3  | 2025-05-22 11:52:16 UTC-4 | used |
| Standard 4  | 1     | 1.000 | 10.0   | 1.0      | 1.0           | 0.133 | STD4  | 2025-05-22 12:13:41 UTC-4 | used |
| Standard 5  | 1     | 2.000 | 10.0   | 1.0      | 1.0           | 0.275 | STD5  | 2025-05-22 12:35:06 UTC-4 | used |
| Standard 6  | 1     | 4.000 | 10.0   | 1.0      | 1.0           | 0.555 | STD6  | 2025-05-22 12:56:31 UTC-4 | used |
| Standard 7  | 1     | 5.000 | 10.0   | 1.0      | 1.0           | 0.695 | STD7  | 2025-05-22 13:17:57 UTC-4 | used |

# Chloride (Anions)

( $\mu\text{S}/\text{cm}$ ) x min

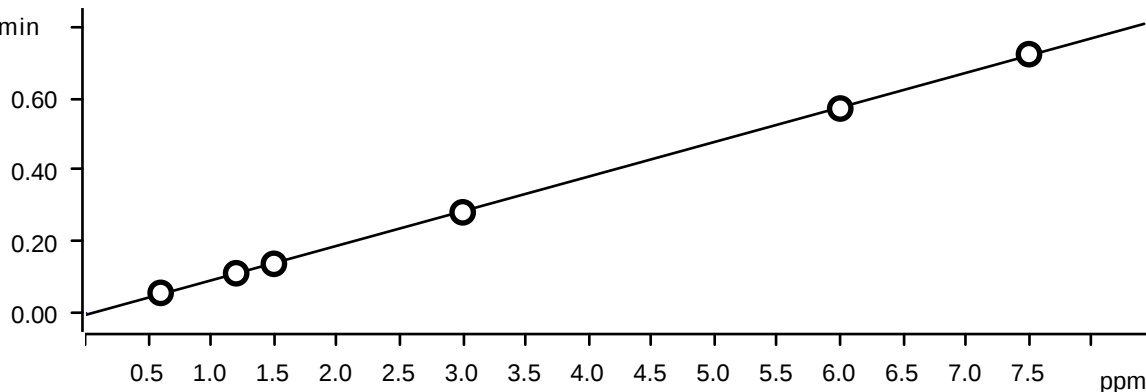

Function: . . . . .  $A = -4.33057E-3 + 9.64673E-3 \times Q$


Relative standard deviation . . . . . 1.154335 %

Correlation coefficient . . . . . 0.999929

| Sample type | Index | Conc. | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|-------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000 | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2025-05-22 11:09:38 UTC-4 | used |
| Standard 2  | 1     | 0.600 | 10.0   | 1.0      | 1.0           | 0.057 | STD2  | 2025-05-22 11:30:53 UTC-4 | used |
| Standard 3  | 1     | 1.200 | 10.0   | 1.0      | 1.0           | 0.112 | STD3  | 2025-05-22 11:52:16 UTC-4 | used |
| Standard 4  | 1     | 1.500 | 10.0   | 1.0      | 1.0           | 0.138 | STD4  | 2025-05-22 12:13:41 UTC-4 | used |
| Standard 5  | 1     | 3.000 | 10.0   | 1.0      | 1.0           | 0.282 | STD5  | 2025-05-22 12:35:06 UTC-4 | used |
| Standard 6  | 1     | 6.000 | 10.0   | 1.0      | 1.0           | 0.571 | STD6  | 2025-05-22 12:56:31 UTC-4 | used |
| Standard 7  | 1     | 7.500 | 10.0   | 1.0      | 1.0           | 0.723 | STD7  | 2025-05-22 13:17:57 UTC-4 | used |

#### Nitrite (Anions)

( $\mu\text{S}/\text{cm}$ )  $\times$  min

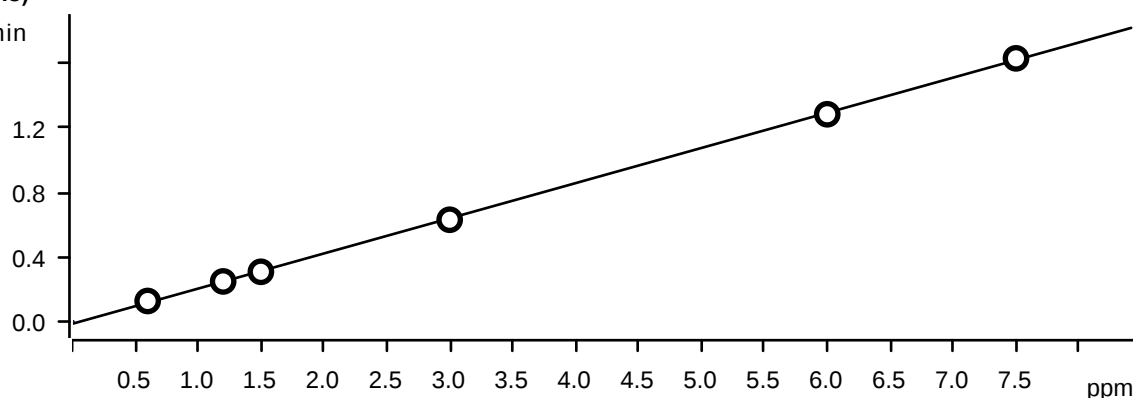

Function: . . . . .  $A = -0.0150155 + 0.0217890 \times Q$


Relative standard deviation . . . . . 1.428639 %

Correlation coefficient . . . . . 0.999893

| Sample type | Index | Conc. | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|-------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000 | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2025-05-22 11:09:38 UTC-4 | used |
| Standard 2  | 1     | 0.600 | 10.0   | 1.0      | 1.0           | 0.126 | STD2  | 2025-05-22 11:30:53 UTC-4 | used |
| Standard 3  | 1     | 1.200 | 10.0   | 1.0      | 1.0           | 0.248 | STD3  | 2025-05-22 11:52:16 UTC-4 | used |
| Standard 4  | 1     | 1.500 | 10.0   | 1.0      | 1.0           | 0.307 | STD4  | 2025-05-22 12:13:41 UTC-4 | used |
| Standard 5  | 1     | 3.000 | 10.0   | 1.0      | 1.0           | 0.630 | STD5  | 2025-05-22 12:35:06 UTC-4 | used |
| Standard 6  | 1     | 6.000 | 10.0   | 1.0      | 1.0           | 1.283 | STD6  | 2025-05-22 12:56:31 UTC-4 | used |
| Standard 7  | 1     | 7.500 | 10.0   | 1.0      | 1.0           | 1.630 | STD7  | 2025-05-22 13:17:57 UTC-4 | used |

# Bromide (Anions)

( $\mu\text{S}/\text{cm}$ )  $\times$  min

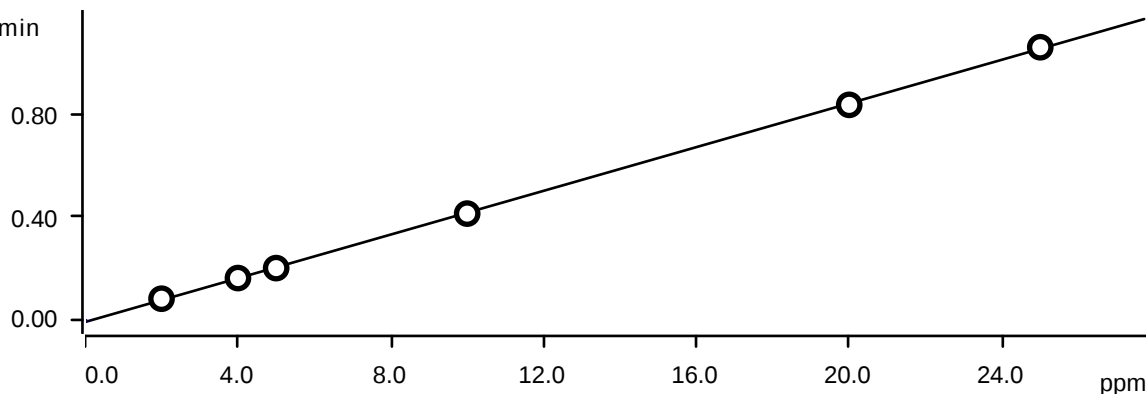

Function: . . . . .  $A = -6.27114E-3 + 4.23162E-3 \times Q$


Relative standard deviation . . . . . 1.185575 %

Correlation coefficient . . . . . 0.999925

| Sample type | Index | Conc.  | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|--------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000  | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2025-05-22 11:09:38 UTC-4 | used |
| Standard 2  | 1     | 2.000  | 10.0   | 1.0      | 1.0           | 0.084 | STD2  | 2025-05-22 11:30:53 UTC-4 | used |
| Standard 3  | 1     | 4.000  | 10.0   | 1.0      | 1.0           | 0.164 | STD3  | 2025-05-22 11:52:16 UTC-4 | used |
| Standard 4  | 1     | 5.000  | 10.0   | 1.0      | 1.0           | 0.202 | STD4  | 2025-05-22 12:13:41 UTC-4 | used |
| Standard 5  | 1     | 10.000 | 10.0   | 1.0      | 1.0           | 0.413 | STD5  | 2025-05-22 12:35:06 UTC-4 | used |
| Standard 6  | 1     | 20.000 | 10.0   | 1.0      | 1.0           | 0.834 | STD6  | 2025-05-22 12:56:31 UTC-4 | used |
| Standard 7  | 1     | 25.000 | 10.0   | 1.0      | 1.0           | 1.058 | STD7  | 2025-05-22 13:17:57 UTC-4 | used |

# Nitrate (Anions)

( $\mu\text{S}/\text{cm}$ )  $\times$  min

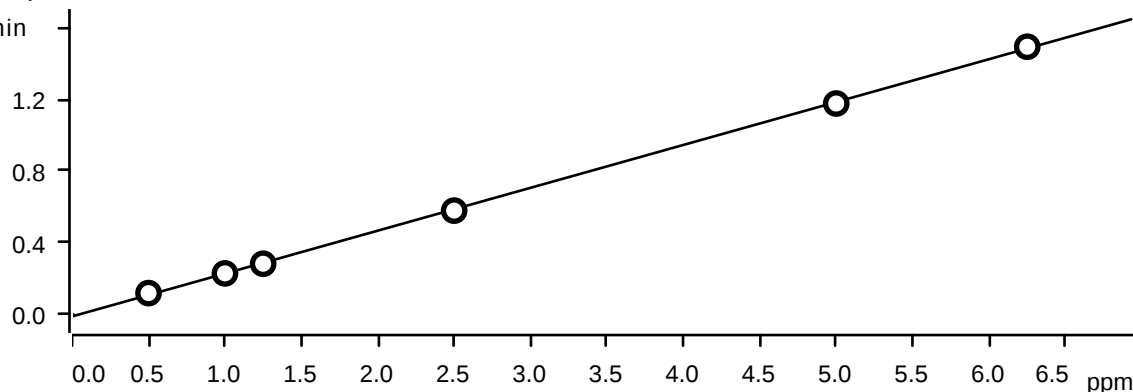

Function: . . . . .  $A = -0.0109593 + 0.0239055 \times Q$


Relative standard deviation . . . . . 1.451672 %

Correlation coefficient . . . . . 0.999889

| Sample type | Index | Conc. | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|-------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000 | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2025-05-22 11:09:38 UTC-4 | used |
| Standard 2  | 1     | 0.500 | 10.0   | 1.0      | 1.0           | 0.119 | STD2  | 2025-05-22 11:30:53 UTC-4 | used |
| Standard 3  | 1     | 1.000 | 10.0   | 1.0      | 1.0           | 0.229 | STD3  | 2025-05-22 11:52:16 UTC-4 | used |
| Standard 4  | 1     | 1.250 | 10.0   | 1.0      | 1.0           | 0.283 | STD4  | 2025-05-22 12:13:41 UTC-4 | used |
| Standard 5  | 1     | 2.500 | 10.0   | 1.0      | 1.0           | 0.579 | STD5  | 2025-05-22 12:35:06 UTC-4 | used |
| Standard 6  | 1     | 5.000 | 10.0   | 1.0      | 1.0           | 1.176 | STD6  | 2025-05-22 12:56:31 UTC-4 | used |
| Standard 7  | 1     | 6.250 | 10.0   | 1.0      | 1.0           | 1.493 | STD7  | 2025-05-22 13:17:57 UTC-4 | used |

**Phosphate (Anions)**

(μS/cm) x min

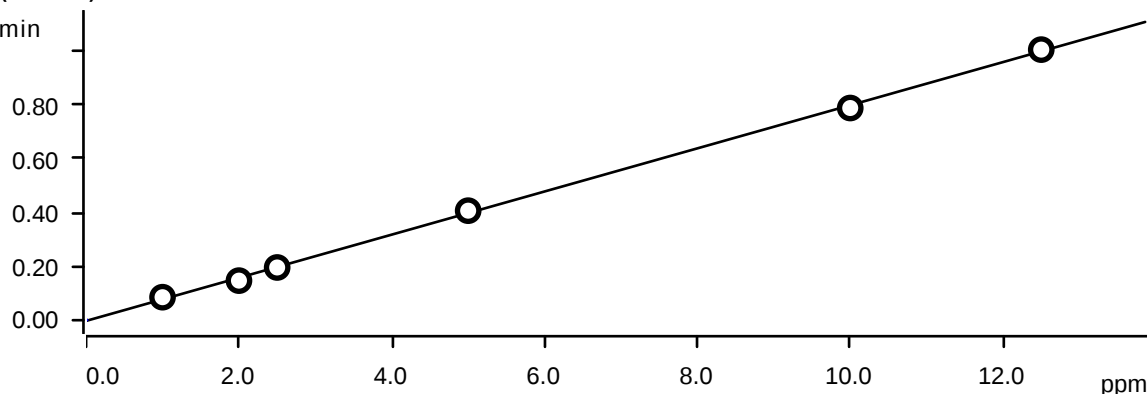Function: . . . . .  $A = -3.02035E-3 + 8.01761E-3 \times Q$ 


Relative standard deviation . . . . . 2.297726 %

Correlation coefficient . . . . . 0.999716

| Sample type | Index | Conc.  | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|--------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000  | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2025-05-22 11:09:38 UTC-4 | used |
| Standard 2  | 1     | 1.000  | 10.0   | 1.0      | 1.0           | 0.085 | STD2  | 2025-05-22 11:30:53 UTC-4 | used |
| Standard 3  | 1     | 2.000  | 10.0   | 1.0      | 1.0           | 0.147 | STD3  | 2025-05-22 11:52:16 UTC-4 | used |
| Standard 4  | 1     | 2.500  | 10.0   | 1.0      | 1.0           | 0.196 | STD4  | 2025-05-22 12:13:41 UTC-4 | used |
| Standard 5  | 1     | 5.000  | 10.0   | 1.0      | 1.0           | 0.407 | STD5  | 2025-05-22 12:35:06 UTC-4 | used |
| Standard 6  | 1     | 10.000 | 10.0   | 1.0      | 1.0           | 0.788 | STD6  | 2025-05-22 12:56:31 UTC-4 | used |
| Standard 7  | 1     | 12.500 | 10.0   | 1.0      | 1.0           | 1.005 | STD7  | 2025-05-22 13:17:57 UTC-4 | used |

**Sulfate (Anions)**

( $\mu\text{S}/\text{cm}$ )  $\times$  min

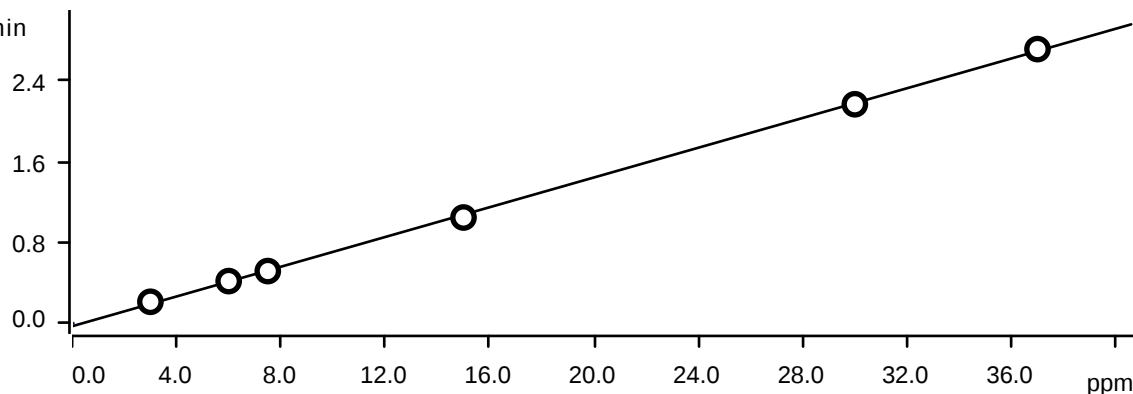

Function: . . . . .  $A = -0.0303663 + 7.37295E-3 \times Q$

Relative standard deviation . . . . . 1.792871 %

Correlation coefficient . . . . . 0.999832


| Sample type | Index | Conc.  | Volume | Dilution | Sample amount | Area  | Ident | Date                      | Used |
|-------------|-------|--------|--------|----------|---------------|-------|-------|---------------------------|------|
| Standard 1  | 1     | 0.000  | 10.0   | 1.0      | 1.0           | n. d. | STD1  | 2025-05-22 11:09:38 UTC-4 | used |
| Standard 2  | 1     | 3.000  | 10.0   | 1.0      | 1.0           | 0.212 | STD2  | 2025-05-22 11:30:53 UTC-4 | used |
| Standard 3  | 1     | 6.000  | 10.0   | 1.0      | 1.0           | 0.417 | STD3  | 2025-05-22 11:52:16 UTC-4 | used |
| Standard 4  | 1     | 7.500  | 10.0   | 1.0      | 1.0           | 0.516 | STD4  | 2025-05-22 12:13:41 UTC-4 | used |
| Standard 5  | 1     | 15.000 | 10.0   | 1.0      | 1.0           | 1.048 | STD5  | 2025-05-22 12:35:06 UTC-4 | used |
| Standard 6  | 1     | 30.000 | 10.0   | 1.0      | 1.0           | 2.170 | STD6  | 2025-05-22 12:56:31 UTC-4 | used |
| Standard 7  | 1     | 37.000 | 10.0   | 1.0      | 1.0           | 2.717 | STD7  | 2025-05-22 13:17:57 UTC-4 | used |

**Sample data**

Ident . . . . . STD1  
Sample type . . . . . Standard 1  
Determination start . . . . . 2025-05-22 11:09:38 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

**Anions**

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.82 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

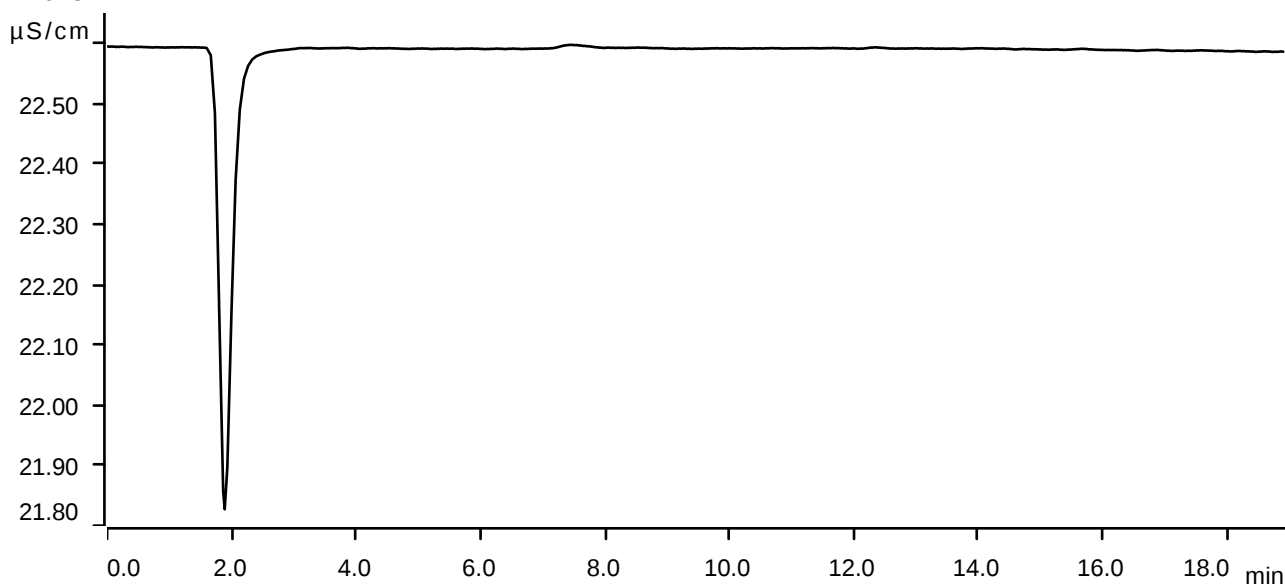**Anions**


## Sample data

Ident . . . . . STD2  
Sample type . . . . . Standard 2  
Determination start . . . . . 2025-05-22 11:30:53 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.77 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

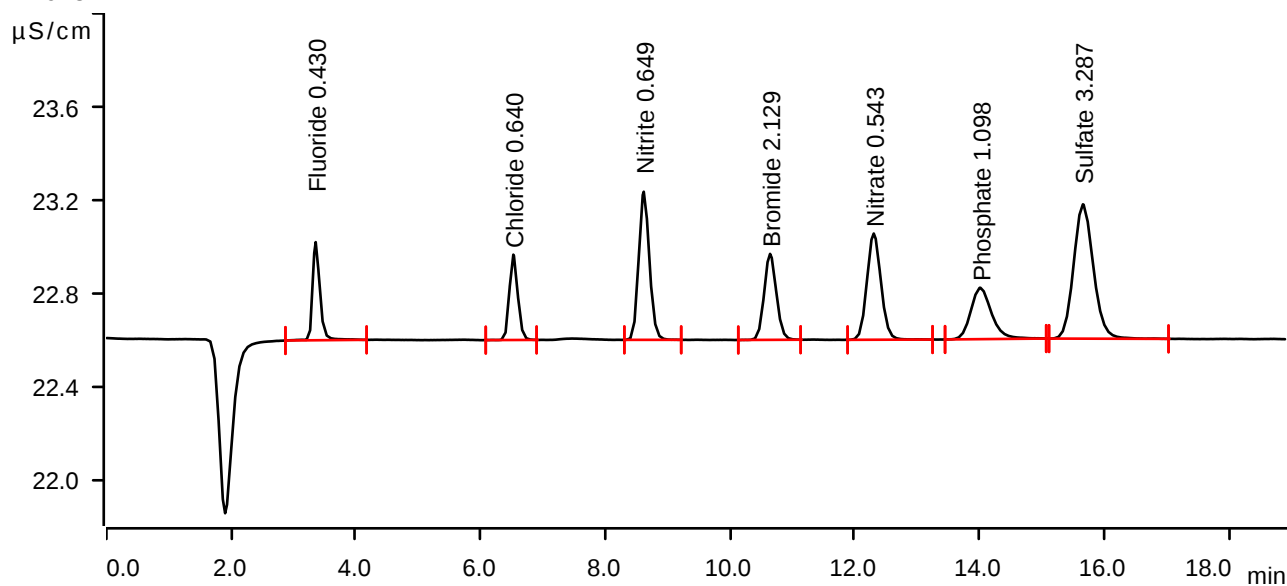

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.357                 | 0.0572                | 0.421           | 0.430                | Fluoride       |
| 2           | 6.525                 | 0.0574                | 0.366           | 0.640                | Chloride       |
| 3           | 8.617                 | 0.1264                | 0.636           | 0.649                | Nitrite        |
| 4           | 10.642                | 0.0838                | 0.369           | 2.129                | Bromide        |
| 5           | 12.303                | 0.1190                | 0.456           | 0.543                | Nitrate        |
| 6           | 14.013                | 0.0850                | 0.221           | 1.098                | Phosphate      |
| 7           | 15.657                | 0.2120                | 0.577           | 3.287                | Sulfate        |


## Sample data

Ident . . . . . STD3  
Sample type . . . . . Standard 3  
Determination start . . . . . 2025-05-22 11:52:16 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.71 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

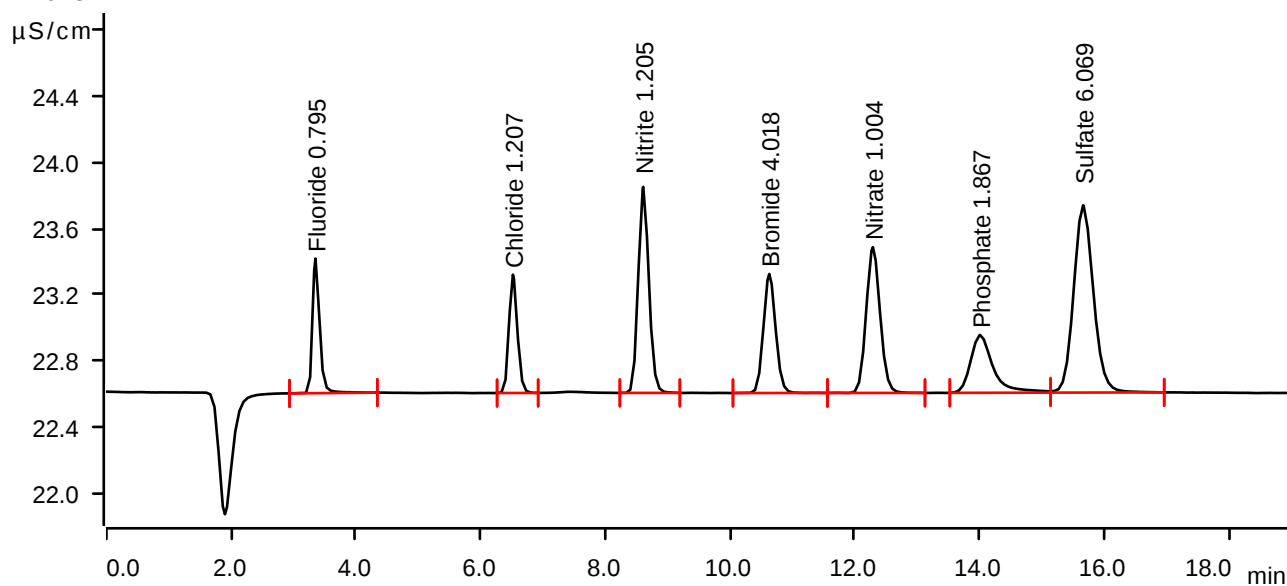

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.353                 | 0.1081                | 0.814           | 0.795                | Fluoride       |
| 2           | 6.518                 | 0.1121                | 0.716           | 1.207                | Chloride       |
| 3           | 8.608                 | 0.2475                | 1.247           | 1.205                | Nitrite        |
| 4           | 10.628                | 0.1637                | 0.720           | 4.018                | Bromide        |
| 5           | 12.290                | 0.2290                | 0.882           | 1.004                | Nitrate        |
| 6           | 14.008                | 0.1467                | 0.350           | 1.867                | Phosphate      |
| 7           | 15.660                | 0.4171                | 1.133           | 6.069                | Sulfate        |


## Sample data

Ident . . . . . STD4  
Sample type . . . . . Standard 4  
Determination start . . . . . 2025-05-22 12:13:41 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.71 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

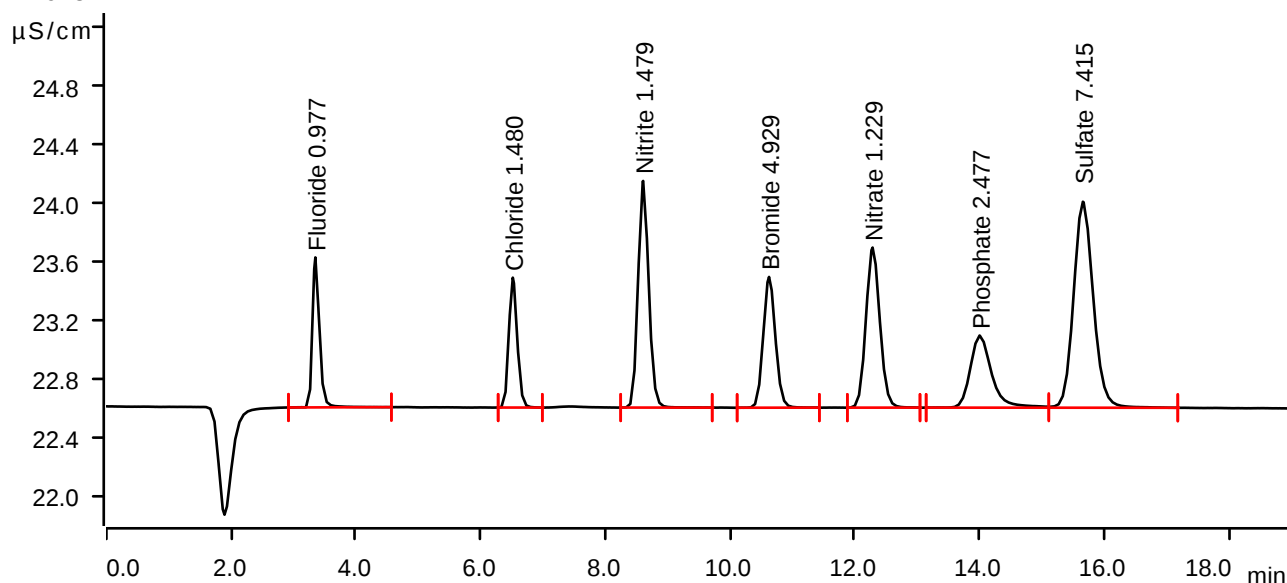

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.352                 | 0.1334                | 1.024           | 0.977                | Fluoride       |
| 2           | 6.517                 | 0.1384                | 0.888           | 1.480                | Chloride       |
| 3           | 8.607                 | 0.3073                | 1.549           | 1.479                | Nitrite        |
| 4           | 10.625                | 0.2023                | 0.894           | 4.929                | Bromide        |
| 5           | 12.285                | 0.2828                | 1.094           | 1.229                | Nitrate        |
| 6           | 14.003                | 0.1955                | 0.493           | 2.477                | Phosphate      |
| 7           | 15.657                | 0.5164                | 1.408           | 7.415                | Sulfate        |


## Sample data

Ident . . . . . STD5  
Sample type . . . . . Standard 5  
Determination start . . . . . 2025-05-22 12:35:06 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.66 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

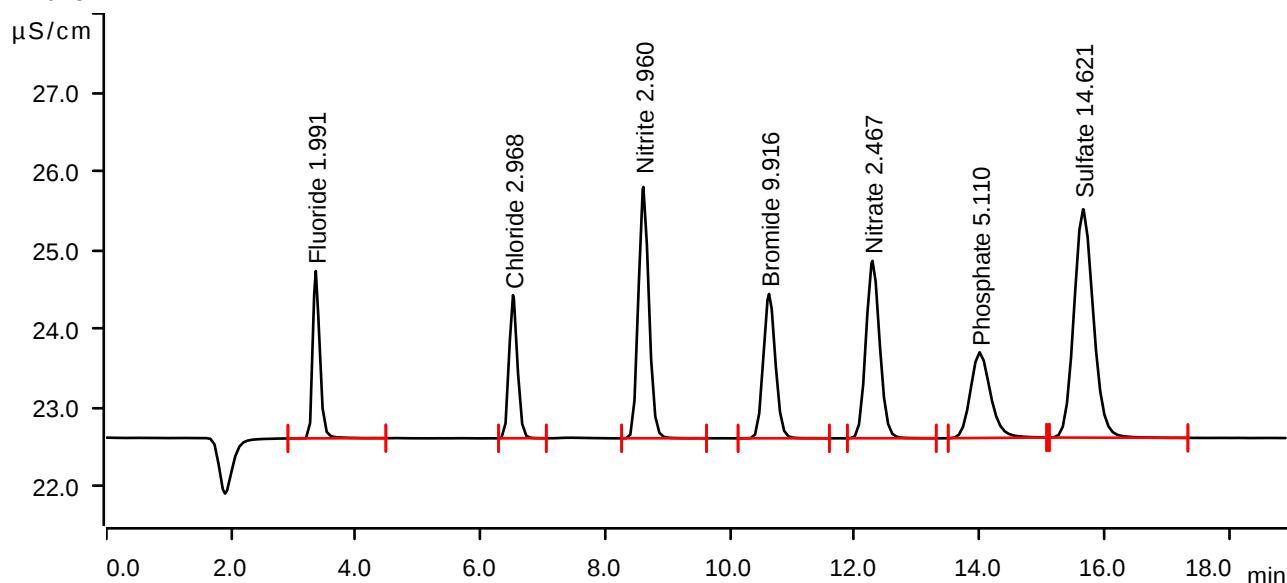

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.358                 | 0.2749                | 2.123           | 1.991                | Fluoride       |
| 2           | 6.520                 | 0.2820                | 1.816           | 2.968                | Chloride       |
| 3           | 8.610                 | 0.6298                | 3.190           | 2.960                | Nitrite        |
| 4           | 10.625                | 0.4133                | 1.833           | 9.916                | Bromide        |
| 5           | 12.283                | 0.5789                | 2.251           | 2.467                | Nitrate        |
| 6           | 14.002                | 0.4067                | 1.087           | 5.110                | Phosphate      |
| 7           | 15.660                | 1.0476                | 2.898           | 14.621               | Sulfate        |


## Sample data

Ident . . . . . STD6  
Sample type . . . . . Standard 6  
Determination start . . . . . 2025-05-22 12:56:31 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.66 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

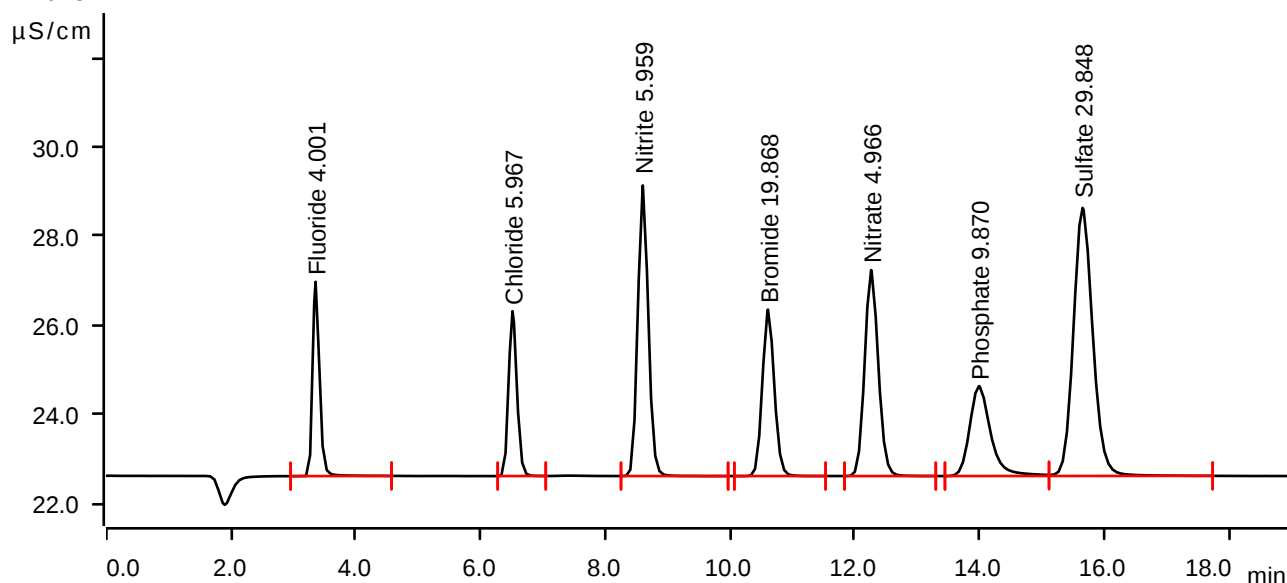

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.355                 | 0.5553                | 4.361           | 4.001                | Fluoride       |
| 2           | 6.512                 | 0.5713                | 3.701           | 5.967                | Chloride       |
| 3           | 8.602                 | 1.2834                | 6.525           | 5.959                | Nitrite        |
| 4           | 10.608                | 0.8345                | 3.739           | 19.868               | Bromide        |
| 5           | 12.262                | 1.1762                | 4.624           | 4.966                | Nitrate        |
| 6           | 13.990                | 0.7883                | 2.019           | 9.870                | Phosphate      |
| 7           | 15.652                | 2.1703                | 6.019           | 29.848               | Sulfate        |


## Sample data

Ident . . . . . STD7  
Sample type . . . . . Standard 7  
Determination start . . . . . 2025-05-22 13:17:57 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.66 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

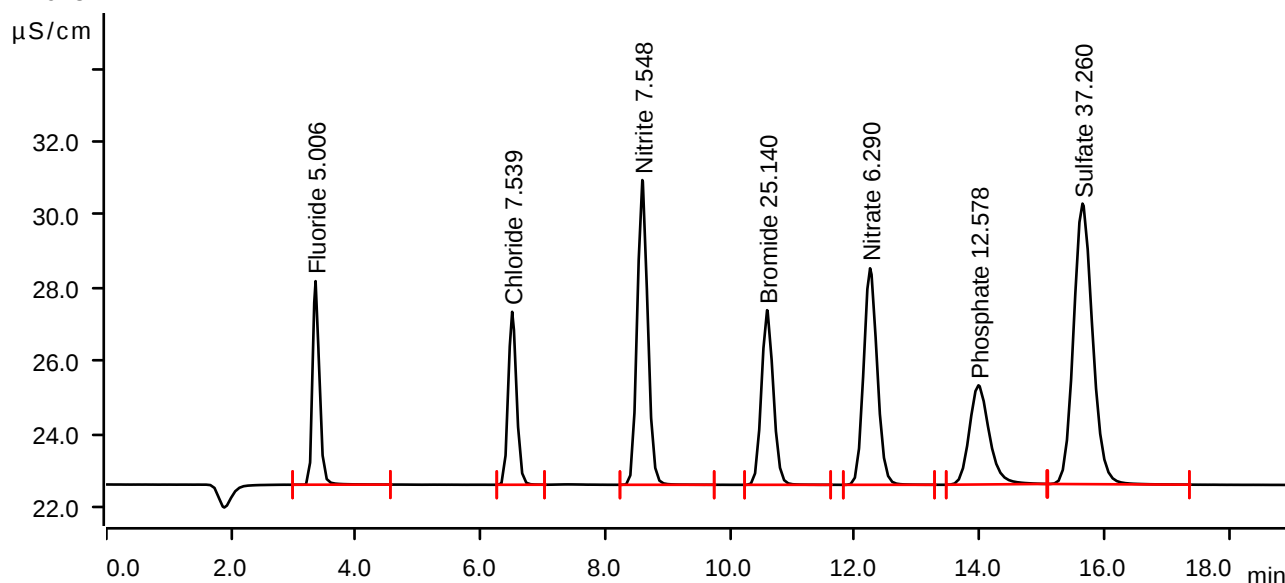

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.355                 | 0.6954                | 5.562           | 5.006                | Fluoride       |
| 2           | 6.507                 | 0.7229                | 4.726           | 7.539                | Chloride       |
| 3           | 8.593                 | 1.6297                | 8.328           | 7.548                | Nitrite        |
| 4           | 10.593                | 1.0576                | 4.774           | 25.140               | Bromide        |
| 5           | 12.245                | 1.4927                | 5.918           | 6.290                | Nitrate        |
| 6           | 13.982                | 1.0054                | 2.711           | 12.578               | Phosphate      |
| 7           | 15.650                | 2.7168                | 7.668           | 37.260               | Sulfate        |


## Sample data

Ident . . . . . ICV  
 Sample type . . . . . Check standard 1  
 Determination start . . . . . 2025-05-22 13:39:25 UTC-4  
 Method . . . . . IC1-052225  
 Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
 Channel . . . . . Conductivity  
 Recording time . . . . . 19.0 min  
 Integration . . . . . Automatically  
 Column type . . . . . Metrosep A Supp 19 - 150/4.0  
 Eluent composition . . . . . not defined  
 Flow . . . . . 0.700 mL/min  
 Maximum flow monitored . . . . . yes  
 Pressure . . . . . 11.60 MPa  
 Maximum pressure monitored . . . . . yes  
 Temperature . . . . . ---- °C

## Anions

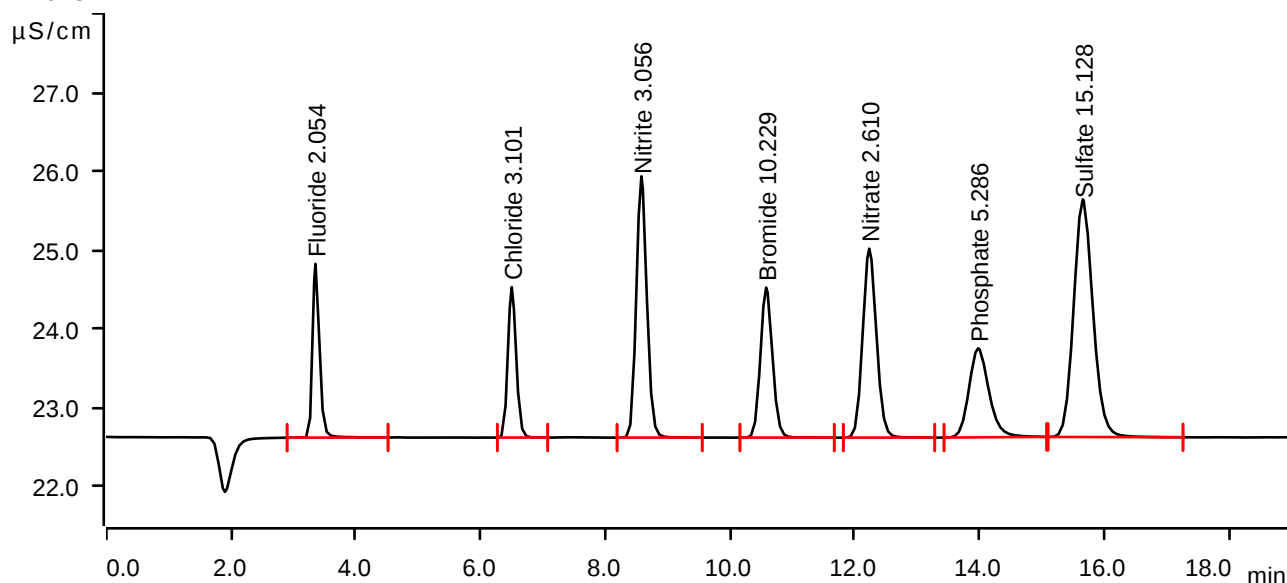

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.353                 | 0.2837                | 2.205           | 2.054                | Fluoride       |
| 2           | 6.500                 | 0.2948                | 1.910           | 3.101                | Chloride       |
| 3           | 8.578                 | 0.6509                | 3.316           | 3.056                | Nitrite        |
| 4           | 10.578                | 0.4266                | 1.904           | 10.229               | Bromide        |
| 5           | 12.232                | 0.6129                | 2.398           | 2.610                | Nitrate        |
| 6           | 13.977                | 0.4208                | 1.130           | 5.286                | Phosphate      |
| 7           | 15.655                | 1.0850                | 3.016           | 15.128               | Sulfate        |


## Sample data

Ident . . . . . ICB  
Sample type . . . . . Sample  
Determination start . . . . . 2025-05-22 14:22:21 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 11.66 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

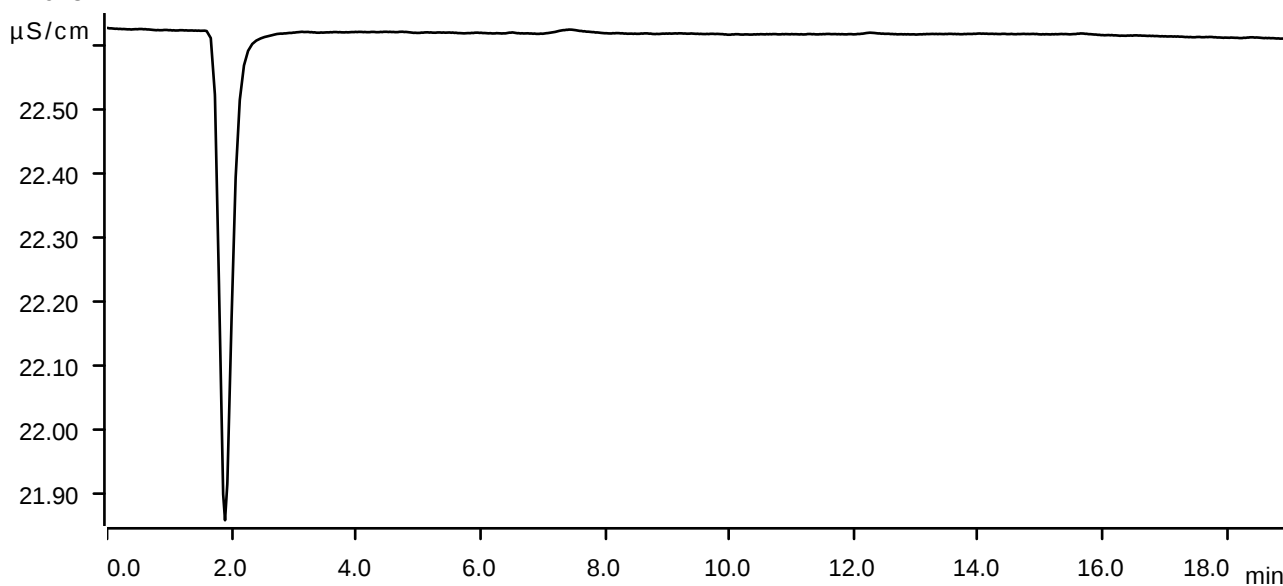


## Sample data

Ident . . . . . CCV  
Sample type . . . . . Check standard 1  
Determination start . . . . . 2025-06-20 13:39:56 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 12.50 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

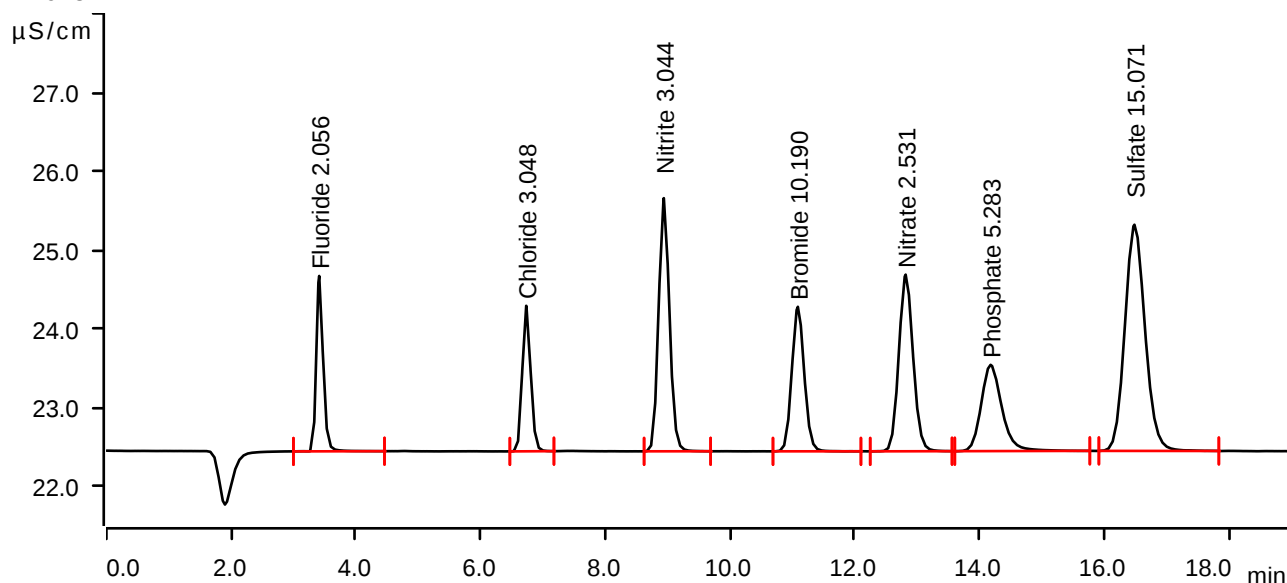


| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.413                 | 0.2839                | 2.225           | 2.056                | Fluoride       |
| 2           | 6.732                 | 0.2897                | 1.846           | 3.048                | Chloride       |
| 3           | 8.938                 | 0.6482                | 3.213           | 3.044                | Nitrite        |
| 4           | 11.087                | 0.4249                | 1.834           | 10.190               | Bromide        |
| 5           | 12.815                | 0.5941                | 2.242           | 2.531                | Nitrate        |
| 6           | 14.177                | 0.4205                | 1.095           | 5.283                | Phosphate      |
| 7           | 16.483                | 1.0808                | 2.870           | 15.071               | Sulfate        |

**Sample data**

Ident . . . . . CCB  
Sample type . . . . . Sample  
Determination start . . . . . 2025-06-20 14:01:26 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

**Anions**

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 12.44 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

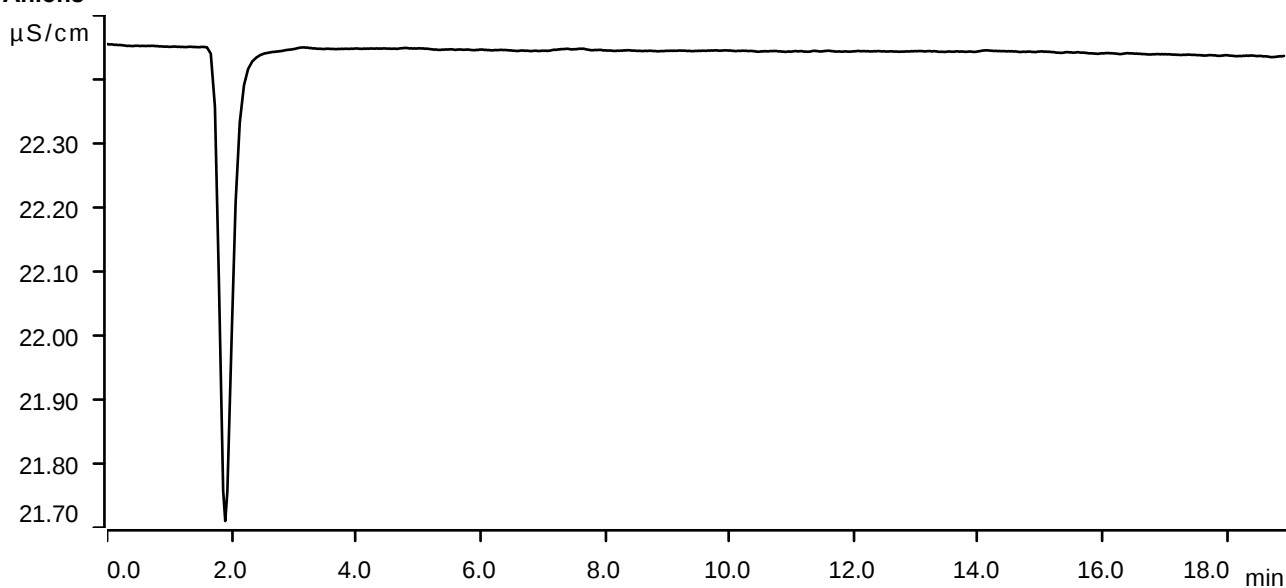
**Anions**

**Sample data**

Ident . . . . . LB136234BLW  
Sample type . . . . . Sample  
Determination start . . . . . 2025-06-20 14:22:56 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

**Anions**

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 12.44 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

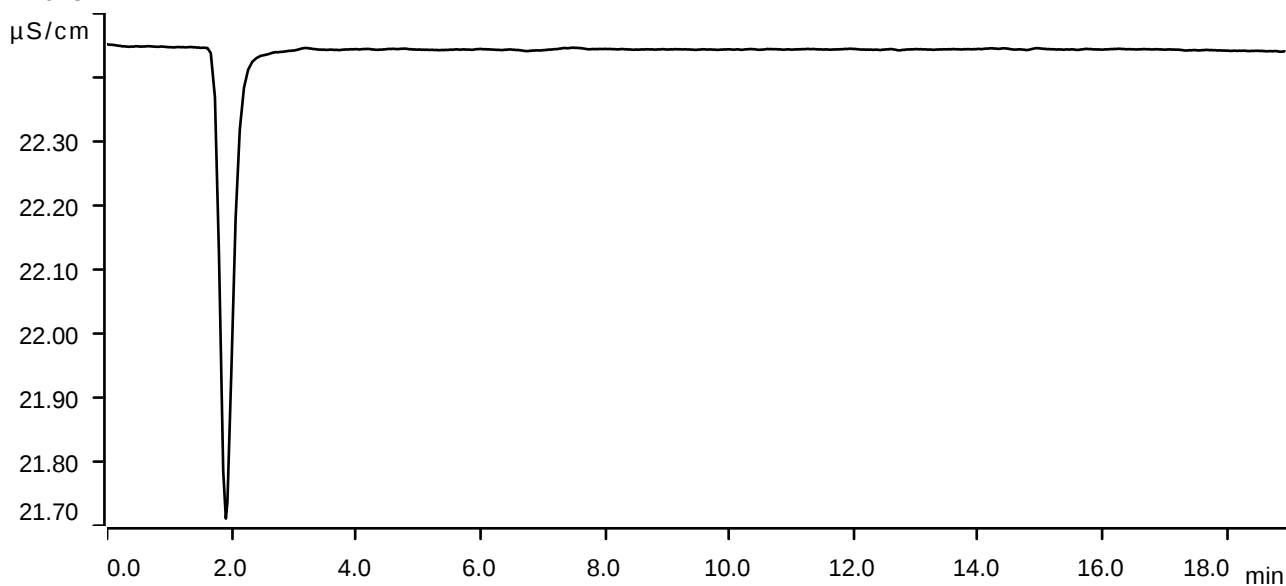**Anions**


## Sample data

Ident . . . . . LB136234BSW  
Sample type . . . . . Check standard 1  
Determination start . . . . . 2025-06-20 14:44:27 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 12.44 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

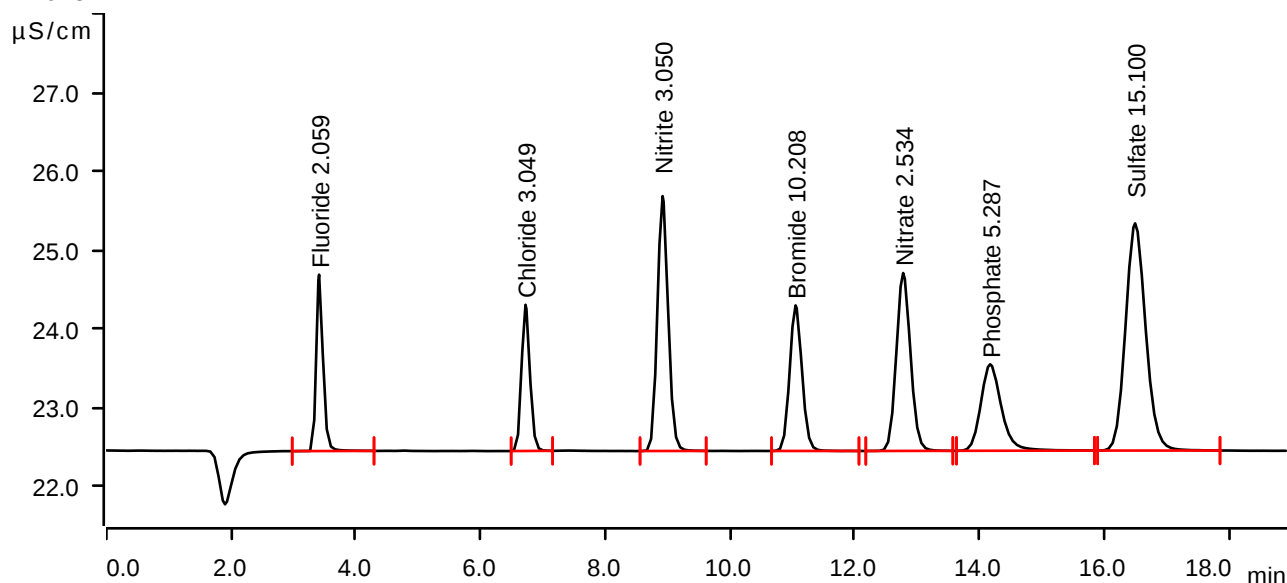

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.412                 | 0.2844                | 2.238           | 2.059                | Fluoride       |
| 2           | 6.720                 | 0.2898                | 1.855           | 3.049                | Chloride       |
| 3           | 8.918                 | 0.6495                | 3.235           | 3.050                | Nitrite        |
| 4           | 11.050                | 0.4257                | 1.847           | 10.208               | Bromide        |
| 5           | 12.775                | 0.5947                | 2.257           | 2.534                | Nitrate        |
| 6           | 14.170                | 0.4208                | 1.097           | 5.287                | Phosphate      |
| 7           | 16.493                | 1.0829                | 2.883           | 15.100               | Sulfate        |


## Sample data

Ident . . . . . Q2385-01  
Sample type . . . . . Sample  
Determination start . . . . . 2025-06-20 15:37:46 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 12.50 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

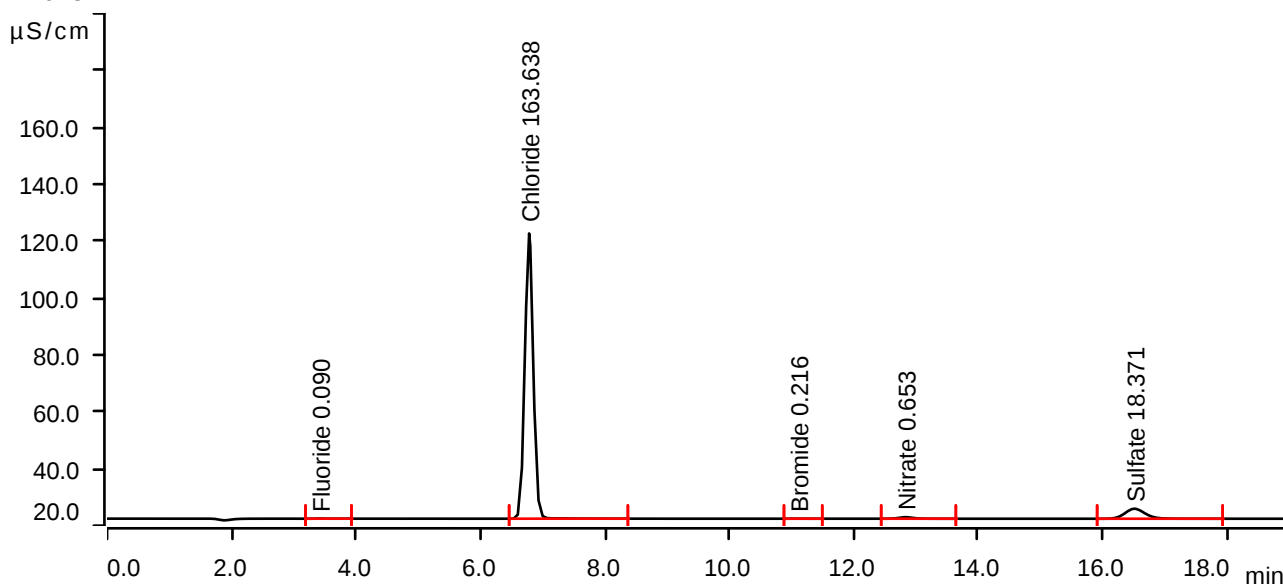

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.420                 | 0.0098                | 0.064           | 0.090                | Fluoride       |
| 2           | 6.783                 | 15.7813               | 100.226         | 163.638              | Chloride       |
| 3           | 11.107                | 0.0029                | 0.012           | 0.216                | Bromide        |
| 4           | 12.833                | 0.1451                | 0.544           | 0.653                | Nitrate        |
| 5           | 16.510                | 1.3241                | 3.527           | 18.371               | Sulfate        |


## Sample data

Ident . . . . . Q2385-01MS  
Sample type . . . . . Sample  
Determination start . . . . . 2025-06-20 16:21:01 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 12.44 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

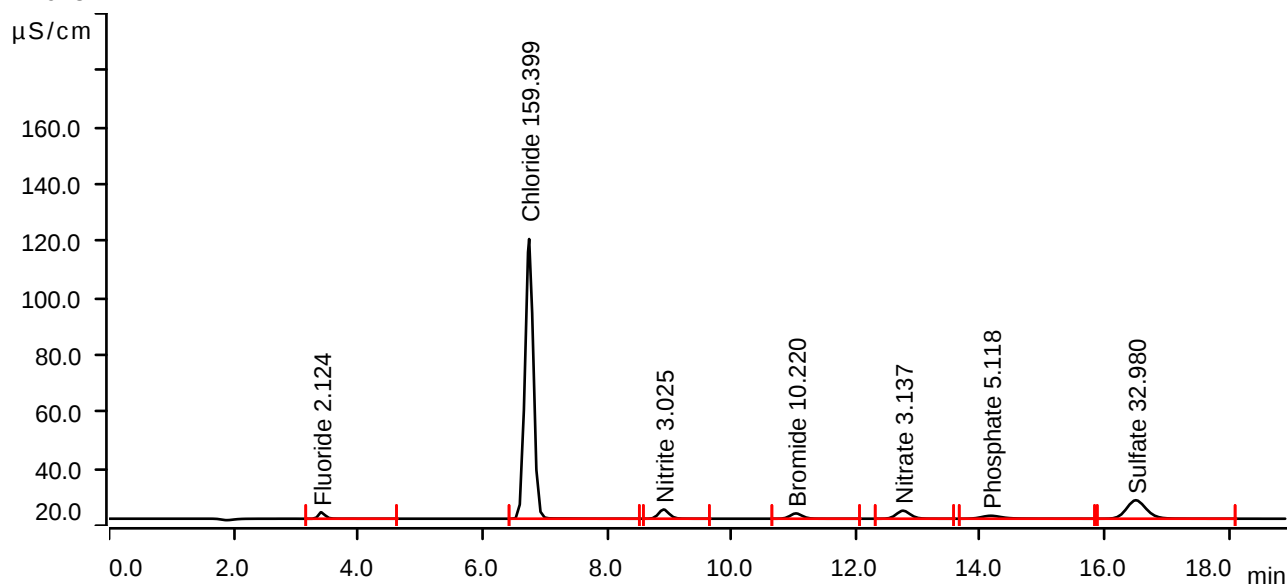

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.412                 | 0.2934                | 2.292           | 2.124                | Fluoride       |
| 2           | 6.752                 | 15.3724               | 98.278          | 159.399              | Chloride       |
| 3           | 8.912                 | 0.6441                | 3.243           | 3.025                | Nitrite        |
| 4           | 11.038                | 0.4262                | 1.866           | 10.220               | Bromide        |
| 5           | 12.758                | 0.7390                | 2.830           | 3.137                | Nitrate        |
| 6           | 14.168                | 0.4073                | 1.037           | 5.118                | Phosphate      |
| 7           | 16.500                | 2.4012                | 6.497           | 32.980               | Sulfate        |


## Sample data

Ident . . . . . Q2385-01MSD  
Sample type . . . . . Sample  
Determination start . . . . . 2025-06-20 16:42:34 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 12.33 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

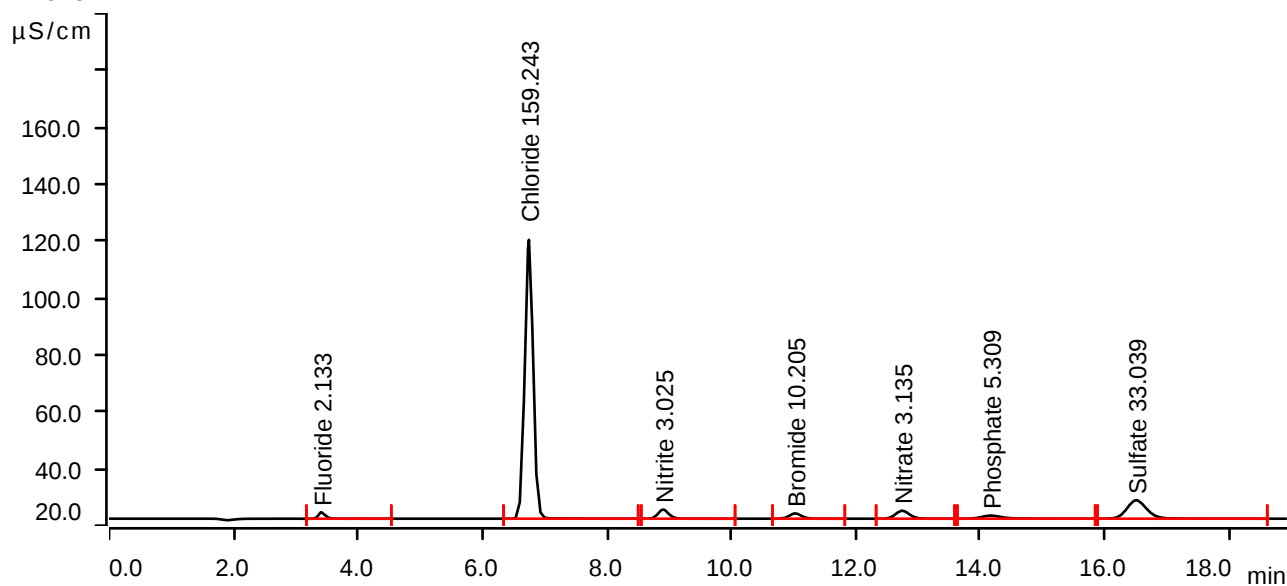

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.413                 | 0.2947                | 2.299           | 2.133                | Fluoride       |
| 2           | 6.748                 | 15.3574               | 98.003          | 159.243              | Chloride       |
| 3           | 8.905                 | 0.6440                | 3.240           | 3.025                | Nitrite        |
| 4           | 11.025                | 0.4256                | 1.864           | 10.205               | Bromide        |
| 5           | 12.745                | 0.7385                | 2.829           | 3.135                | Nitrate        |
| 6           | 14.168                | 0.4226                | 1.088           | 5.309                | Phosphate      |
| 7           | 16.507                | 2.4056                | 6.493           | 33.039               | Sulfate        |


## Sample data

Ident . . . . . CCV  
Sample type . . . . . Check standard 1  
Determination start . . . . . 2025-06-20 17:04:08 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

## Anions

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 12.33 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

## Anions

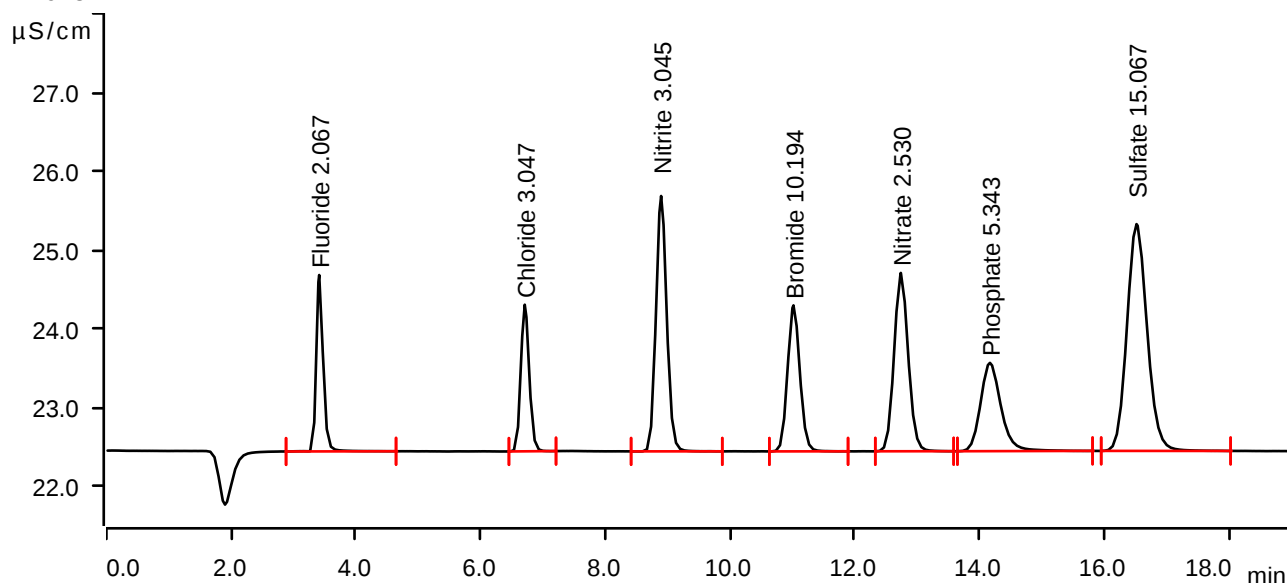

| Peak number | Retention time<br>min | Area<br>(µS/cm) x min | Height<br>µS/cm | Concentration<br>ppm | Component name |
|-------------|-----------------------|-----------------------|-----------------|----------------------|----------------|
| 1           | 3.413                 | 0.2855                | 2.238           | 2.067                | Fluoride       |
| 2           | 6.708                 | 0.2896                | 1.860           | 3.047                | Chloride       |
| 3           | 8.895                 | 0.6485                | 3.241           | 3.045                | Nitrite        |
| 4           | 11.017                | 0.4251                | 1.853           | 10.194               | Bromide        |
| 5           | 12.738                | 0.5939                | 2.263           | 2.530                | Nitrate        |
| 6           | 14.167                | 0.4254                | 1.120           | 5.343                | Phosphate      |
| 7           | 16.517                | 1.0805                | 2.878           | 15.067               | Sulfate        |

**Sample data**

Ident . . . . . CCB  
Sample type . . . . . Sample  
Determination start . . . . . 2025-06-20 17:25:27 UTC-4  
Method . . . . . IC1-052225  
Operator . . . . .

**Anions**

Data source . . . . . Conductivity detector 1 (Eco IC 1)  
Channel . . . . . Conductivity  
Recording time . . . . . 19.0 min  
Integration . . . . . Automatically  
Column type . . . . . Metrosep A Supp 19 - 150/4.0  
Eluent composition . . . . . not defined  
Flow . . . . . 0.700 mL/min  
Maximum flow monitored . . . . . yes  
Pressure . . . . . 12.33 MPa  
Maximum pressure monitored . . . . . yes  
Temperature . . . . . ---- °C

**Anions**