

LB136446 INSTRUMENT ID:CV1

Method: 7471B


Operator: Admin

Date of Analysis: 29 Jul 2025 12:29:13

Type	Sample ID	Extended ID	Conc.	μ Abs.	Units	Type	Std Conc	Method	Date
S	0.0 - 1	50	-	59	PPB	Std	0.0000	7471B	29 Jul 2025 13:03:38
S	0.2 - 1	50.2	-	1161	PPB	Std	0.2000	7471B	29 Jul 2025 13:05:55
S	2.5 - 1	52.5	-	12715	PPB	Std	2.5000	7471B	29 Jul 2025 13:08:12
S	5.0 - 1	55.0	-	27800	PPB	Std	5.0000	7471B	29 Jul 2025 13:10:30
S	7.5 - 1	57.5	-	40400	PPB	Std	7.5000	7471B	29 Jul 2025 13:12:49
S	10.0 - 1	510.0	-	51423	PPB	Std	10.0000	7471B	29 Jul 2025 13:15:08
U	ICV44 - 1	ICV44	4.2067	22295	PPB	SMPL	-7471B		29 Jul 2025 13:18:15
U	ICB44 - 1	ICB44	-0.0900	-223	PPB	SMPL	-7471B		29 Jul 2025 13:20:31
U	CCV62 - 1	CCV62	5.3262	28162	PPB	SMPL	-7471B		29 Jul 2025 13:24:59
U	CCB62 - 1	CCB62	-0.0873	-209	PPB	SMPL	-7471B		29 Jul 2025 13:27:14
U	CRA - 1	CRA	0.1850	1218	PPB	SMPL	-7471B		29 Jul 2025 13:29:34
U	HighStd - 1	HighStd	9.8502	51871	PPB	SMPL	-7471B		29 Jul 2025 13:32:22
U	ChkStd - 1	ChkStd	7.2176	38074	PPB	SMPL	-7471B		29 Jul 2025 13:34:37
U	PB169034BL - 1	PB169034BL	-0.0681	-108	PPB	SMPL	-7471B		29 Jul 2025 13:37:01
U	PB169034BS - 1	PB169034BS	3.9701	21055	PPB	SMPL	-7471B		29 Jul 2025 13:42:08
U	Q2700-01 - 1	EO-03-072525	1.1896	6483	PPB	SMPL	-7471B		29 Jul 2025 13:44:26
U	Q2703-01 - 1	TP-4	4.3979	23297	PPB	SMPL	-7471B		29 Jul 2025 13:46:48
U	Q2706-01 - 1	RT-5417	0.1170	862	PPB	SMPL	-7471B		29 Jul 2025 13:49:07
U	Q2706-03 - 1	ETGI-361	0.2540	1580	PPB	SMPL	-7471B		29 Jul 2025 13:51:26
U	Q2706-03DUP - 1	ETGI-361DUP	0.1945	1268	PPB	SMPL	-7471B		29 Jul 2025 13:56:21
U	CCV63 - 1	CCV63	5.0175	26544	PPB	SMPL	-7471B		29 Jul 2025 13:58:35
U	CCB63 - 1	CCB63	-0.0457	9	PPB	SMPL	-7471B		29 Jul 2025 14:04:02
U	Q2706-03MS - 1	ETGI-361MS	3.6696	19480	PPB	SMPL	-7471B		29 Jul 2025 14:06:17
U	Q2706-03MSD - 1	ETGI-361MSD	3.5816	19019	PPB	SMPL	-7471B		29 Jul 2025 14:08:33
U	Q2709-01 - 1	7211935-295	0.1250	904	PPB	SMPL	-7471B		29 Jul 2025 14:10:51
U	Q2710-01 - 1	JC-03-07282025	0.3231	1942	PPB	SMPL	-7471B		29 Jul 2025 14:13:10
U	Q2706-03LX5 - 1		-0.0539	-34	PPB	SMPL	-7471B		29 Jul 2025 14:15:29
U	Q2706-03A - 1		-0.0474	0	PPB	SMPL	-7471B		29 Jul 2025 14:17:46
U	CCV64 - 1	CCV64	4.1016	21744	PPB	SMPL	-7471B		29 Jul 2025 14:19:32
U	CCB64 - 1	CCB64	5.1551	27265	PPB	SMPL	-7471B		29 Jul 2025 14:21:48
U			-0.0387	46	PPB	SMPL	-7471B		29 Jul 2025 14:26:45

LB136646
INSTRUMENT ID : CV1

7471B

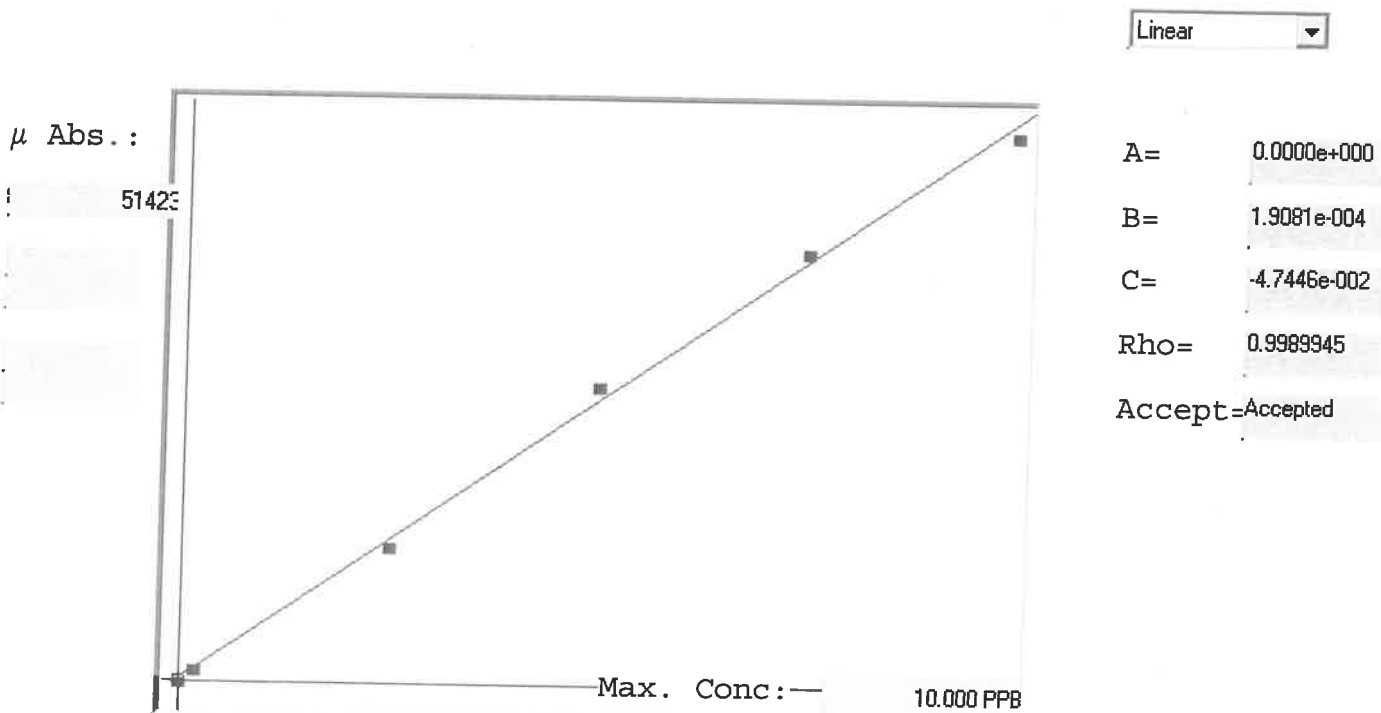

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.0	0.000	-0.036	-0.036	59	0.000	59					0
0.2	0.200	0.174	-0.026	1161	0.0 %	1161					-13
2.5	2.500	2.379	-0.121	12715	0.0 %	12715					-5
5.0	5.000	5.257	0.257	27800	0.0 %	27800					5
7.5	7.500	7.661	0.161	40400	0.0 %	40400					2
10.0	10.000	9.765	-0.235	51423	0.0 %	51423					-2