

LB136686 INSTRUMENT ID:CV1

Method: 7470A

Operator: Admin


Date of Analysis: 04 Aug 2025 11:35:49

Type	Sample ID	Extended ID	Conc.	μ Abs.	Units	Type	Std ConcMethod	Date
S	0.0 - 1	50	-	-	PPB	Std	0.00007470A	04 Aug 2025 11:43:02
S	0.2 - 1	50.2	-	-	PPB	Std	0.20007470A	04 Aug 2025 11:45:19
S	0.2 - 1	52.5	-	803	PPB	Std	0.20007470A	04 Aug 2025 11:49:24
S	2.5 - 1	5.56	-	11331	PPB	Std	2.50007470A	04 Aug 2025 11:51:40
S	5.0 - 1	5.75	-	22475	PPB	Std	5.00007470A	04 Aug 2025 11:53:57
S	7.5 - 1	5.10	-	34167	PPB	Std	7.50007470A	04 Aug 2025 11:56:14
S	10.0 - 1		-	46090	PPB	Std	10.00007470A	04 Aug 2025 11:58:33
U	ICV50 - 1	ICV50	4.2138	19207	PPB	SMPL	-7470A	04 Aug 2025 12:08:18
U	ICB50 - 1	ICB50	-0.0464	-381	PPB	SMPL	-7470A	04 Aug 2025 12:10:33
U	CCV78 - 1	CCV78	4.9941	22795	PPB	SMPL	-7470A	04 Aug 2025 12:12:50
U	CCB78 - 1	CCB78	0.0364	0	PPB	SMPL	-7470A	04 Aug 2025 12:15:05
U	CCV78 - 1	CCV78	5.0546	23073	PPB	SMPL	-7470A	04 Aug 2025 12:16:43
U	CCB78 - 1	CCB78	-0.0469	-383	PPB	SMPL	-7470A	04 Aug 2025 12:18:57
U	CRA - 1	CRA	0.1952	730	PPB	SMPL	-7470A	04 Aug 2025 12:21:15
U	HighStd - 1	HighStd	10.0021	45821	PPB	SMPL	-7470A	04 Aug 2025 12:27:01
U	ChkStd - 1	ChkStd	7.4757	34205	PPB	SMPL	-7470A	04 Aug 2025 12:29:16
U	PB169103BL - 1	PBW	0.0121	-112	PPB	SMPL	-7470A	04 Aug 2025 12:34:26
U	PB169103BS - 1	LCSW	3.4112	15517	PPB	SMPL	-7470A	04 Aug 2025 12:36:41
U	Q2728-02 - 1	7211931-VNJ240	-0.0242	-279	PPB	SMPL	-7470A	04 Aug 2025 12:38:58
U	Q2728-02DUP - 1	7211931-VNJ240DUP	0.0364	0	PPB	SMPL	-7470A	04 Aug 2025 12:41:16
U	Q2728-02DUP - 1	7211931-VNJ240DUP	0.0343	-10	PPB	SMPL	-7470A	04 Aug 2025 12:42:48
U	Q2728-02MS - 1	7211931-VNJ240MS	3.2549	14798	PPB	SMPL	-7470A	04 Aug 2025 12:45:06
U	Q2728-02MSD - 1	7211931-VNJ240MSD	3.6092	16427	PPB	SMPL	-7470A	04 Aug 2025 12:47:24
U	PB169060TB - 1	PB169060TB	-0.0434	-367	PPB	SMPL	-7470A	04 Aug 2025 12:49:41
U	CCV79 - 1	CCV79	5.0148	22890	PPB	SMPL	-7470A	04 Aug 2025 12:51:58
U	CCB79 - 1	CCB79	-0.0593	-440	PPB	SMPL	-7470A	04 Aug 2025 12:54:13
U	Q2728-02LX5 - 1		0.0573	96	PPB	SMPL	-7470A	04 Aug 2025 12:56:30
U	Q2728-02A - 1		3.9193	17853	PPB	SMPL	-7470A	04 Aug 2025 12:58:46
U	CCV80 - 1	CCV80	4.9391	22542	PPB	SMPL	-7470A	04 Aug 2025 13:01:02
U	CCB80 - 1	CCB80	-0.0619	-452	PPB	SMPL	-7470A	04 Aug 2025 13:03:20

LB136686

INSTRUMENT ID: CV₁

7470A

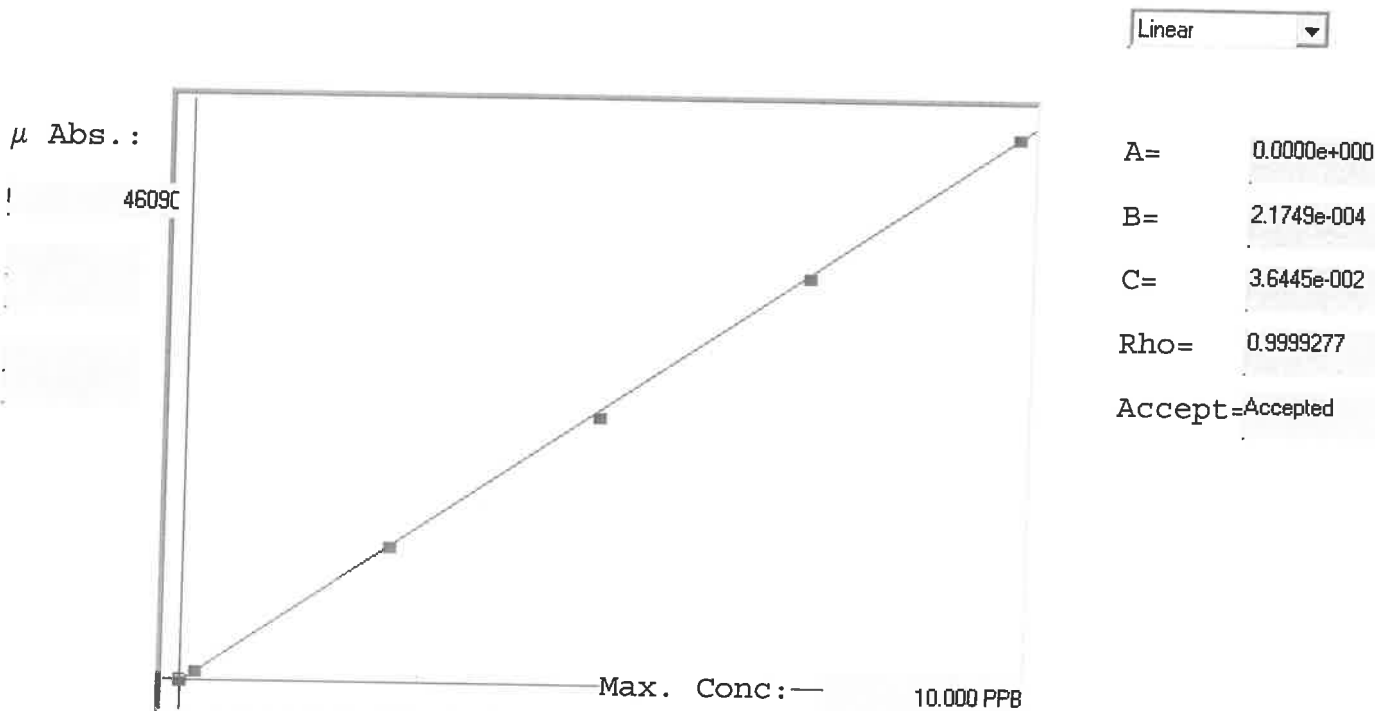

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.036	0.036	-4	0.000	-4	0				
0.2	0.200	0.211	0.011	803	0.0 %	803					
2.5	2.500	2.501	0.001	11331	0.0 %	11331	0				
5.0	5.000	4.925	-0.075	22475	0.0 %	22475					
7.5	7.500	7.467	-0.033	34167	0.0 %	34167					
10.0	10.000	10.061	0.061	46090	0.0 %	46090					