

LB136689 INSTRUMENT ID:CV1

Method: 7471B


Operator: Admin

Date of Analysis: 04 Aug 2025 13:32:14

Type	Sample ID	Extended ID	Conc.	μ Abs.	Units	Type	Std ConcMethod	Date
S	0.0 - 1	50	-	488	PPB	Std	0.00007471B	04 Aug 2025 13:39:19
S	0.2 - 1	50.2	-	1439	PPB	Std	0.20007471B	04 Aug 2025 13:45:14
S	2.5 - 1	52.5	-	14091	PPB	Std	2.50007471B	04 Aug 2025 13:47:31
S	5.0 - 1	5.50	-	28064	PPB	Std	5.00007471B	04 Aug 2025 13:52:39
S	7.5 - 1	5.75	-	42131	PPB	Std	7.50007471B	04 Aug 2025 13:54:57
S	10.0 - 1	5.10	-	56676	PPB	Std	10.00007471B	04 Aug 2025 13:57:19
U	ICV51 - 1	ICV51	3.9561	22446	PPB	SMPL	-7471B	04 Aug 2025 14:00:11
U	ICB51 - 1	ICB51	-0.0479	-24	PPB	SMPL	-7471B	04 Aug 2025 14:02:28
U	CCV80 - 1	CCV80	5.0272	28457	PPB	SMPL	-7471B	04 Aug 2025 14:04:46
U	CCB80 - 1	CCB80	-0.0543	-60	PPB	SMPL	-7471B	04 Aug 2025 14:07:02
U	CRA - 1	CRA	0.2187	1472	PPB	SMPL	-7471B	04 Aug 2025 14:12:00
U	HighStd - 1	HighStd	10.0053	56394	PPB	SMPL	-7471B	04 Aug 2025 14:14:15
U	ChkStd - 1	ChkStd	7.4317	41951	PPB	SMPL	-7471B	04 Aug 2025 14:16:31
U	PB169099BL - 1	PB169099BL	-0.0930	-277	PPB	SMPL	-7471B	04 Aug 2025 14:19:02
U	PB169099BS - 1	PB169099BS	3.4447	19576	PPB	SMPL	-7471B	04 Aug 2025 14:27:19
U	Q2734-01 - 1	VNJ-253	2.8005	15961	PPB	SMPL	-7471B	04 Aug 2025 14:29:35
U	Q2740-01 - 1	OR-02-07312025	0.4197	2600	PPB	SMPL	-7471B	04 Aug 2025 14:31:57
U	Q2740-01DUP - 1	OR-02-07312025DUP	0.4193	2598	PPB	SMPL	-7471B	04 Aug 2025 14:34:19
U	Q2740-01MS - 1	OR-02-07312025MS	5.0915	28818	PPB	SMPL	-7471B	04 Aug 2025 15:05:15
U	Q2740-01MSD - 1	OR-02-07312025MSD	5.8276	32949	PPB	SMPL	-7471B	04 Aug 2025 15:17:55
U	CCV81 - 1	CCV81	4.6412	26291	PPB	SMPL	-7471B	04 Aug 2025 15:23:28
U	CCB81 - 1	CCB81	0.0079	289	PPB	SMPL	-7471B	04 Aug 2025 15:28:27
U	Q2741-01 - 1	TR-05-07312025	3.0322	17261	PPB	SMPL	-7471B	04 Aug 2025 15:30:42
U	Q2753-01 - 1	289	4.9091	27794	PPB	SMPL	-7471B	04 Aug 2025 15:32:57
U	Q2758-01 - 1	WASTE	78.1841	439010	PPB	SMPL	-7471B	04 Aug 2025 15:35:17
U	Q2740-01LX5 - 1		-0.0436	0	PPB	SMPL	-7471B	04 Aug 2025 15:37:43
U	Q2740-01LX5 - 1		-0.0382	30	PPB	SMPL	-7471B	04 Aug 2025 15:42:40
U	Q2740-01A - 1		3.8082	21616	PPB	SMPL	-7471B	04 Aug 2025 15:44:55
U	Q2758-01DLX20 - 1		3.5199	19998	PPB	SMPL	-7471B	04 Aug 2025 15:47:11
U	CCV82 - 1	CCV82	4.7708	27018	PPB	SMPL	-7471B	04 Aug 2025 15:49:31
U	CCB82 - 1	CCB82	-0.0664	-128	PPB	SMPL	-7471B	04 Aug 2025 15:51:52

LB136689
INSTRUMENT ID: CV₁

7471B

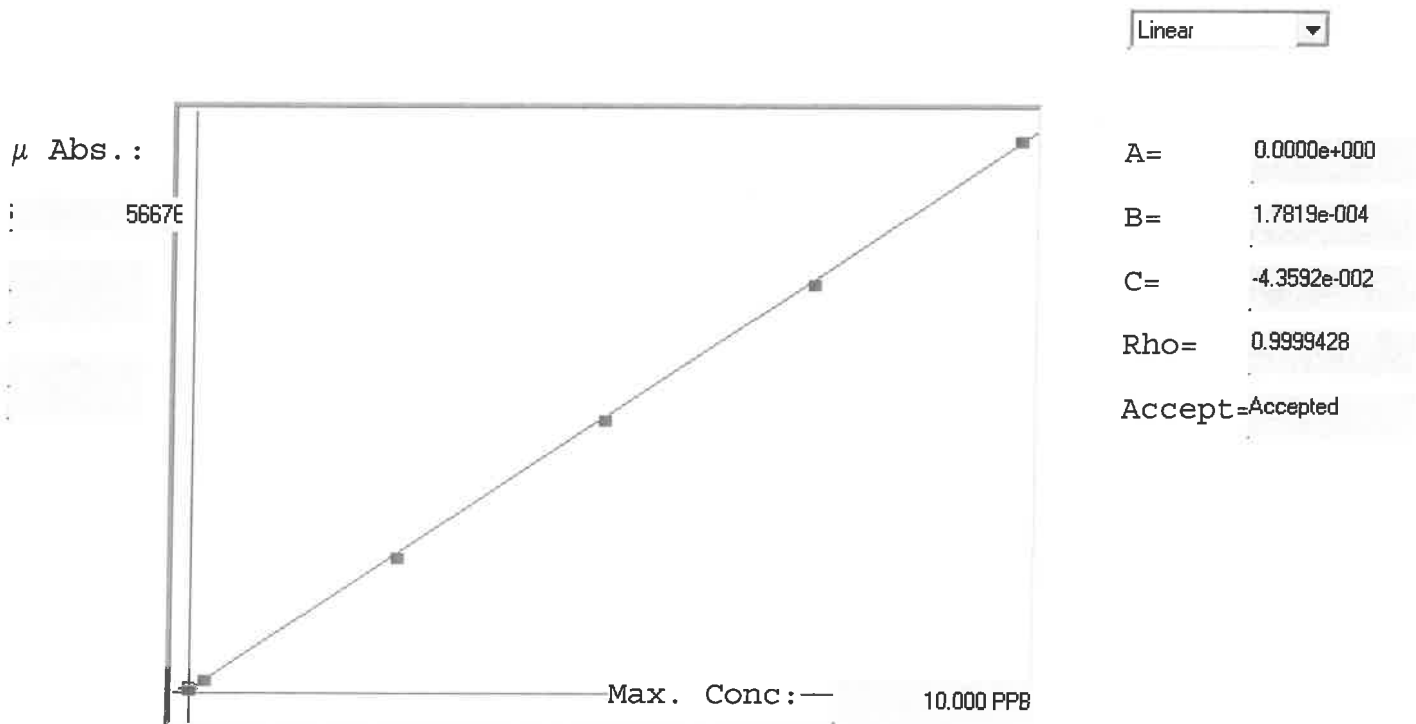

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.043	0.043	488	0.000	488					6
0.2	0.200	0.213	0.013	1439	0.0 %	1439					-1
2.5	2.500	2.467	-0.033	14091	0.0 %	14091					-1
5.0	5.000	4.957	-0.043	28064	0.0 %	28064					0
7.5	7.500	7.464	-0.036	42131	0.0 %	42131					1
10.0	10.000	10.056	0.056	56676	0.0 %	56676					1