


LB 136708 INSTRUMENT ID : CV1

7471B

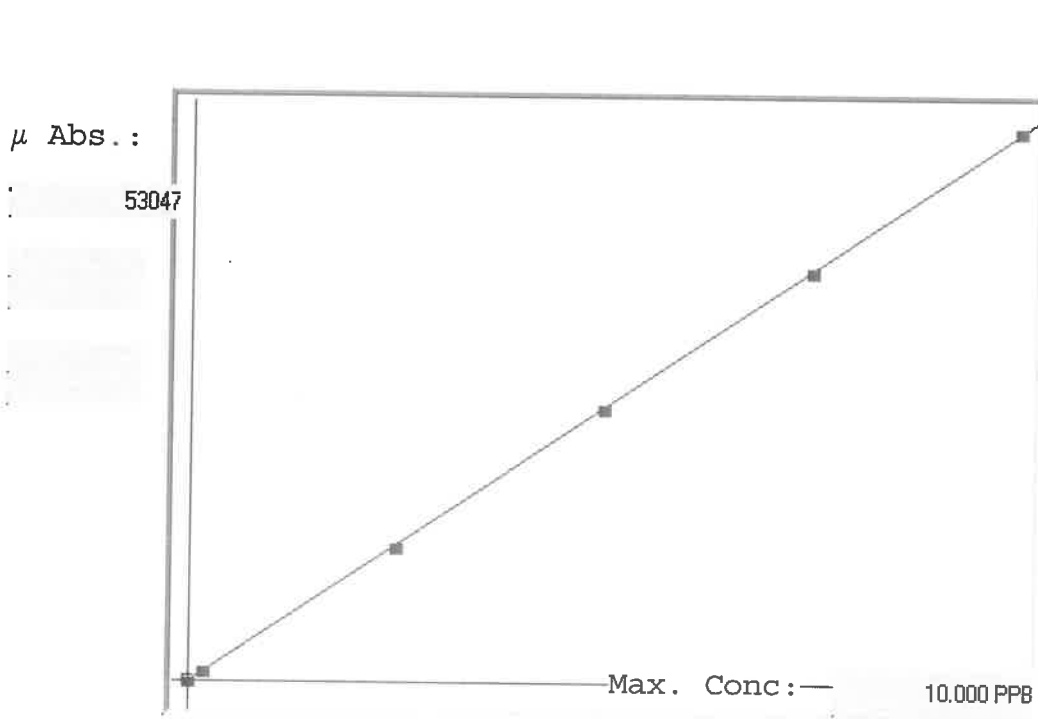

Linear

A= 0.0000e+000

B= 1.8864e-004

C= 2.2103e-002

Rho= 0.9999623

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.0	0.000	0.047	0.047	131	0.000	131					
0.2	0.200	0.204	0.004	964	0.0 %	964					
2.5	2.500	2.448	-0.052	12859	0.0 %	12859					
5.0	5.000	4.984	-0.016	26302	0.0 %	26302					
7.5	7.500	7.489	-0.011	39580	0.0 %	39580					
10.0	10.000	10.029	0.029	53047	0.0 %	53047					

LB136708 INSTRUMENT ID:CV1

Method: 7471B

Operator: Admin

Date of Analysis: 05 Aug 2025 13:15:43

Type	Sample ID	Extended ID	Conc.	µ Abs.	Units	Type	Std CondMethod	Date
S	0.0 - 1	50	-	131	PPB	Std	0.00007471B	05 Aug 2025 13:24:03
S	0.2 - 1	50.2	-	964	PPB	Std	0.20007471B	05 Aug 2025 13:26:20
S	2.5 - 1		-	12859	PPB	Std	2.50007471B	05 Aug 2025 13:28:37
S	5.0 - 1	52.5	-	26302	PPB	Std	5.00007471B	05 Aug 2025 13:30:54
S	7.5 - 1	55.0	-	39580	PPB	Std	7.50007471B	05 Aug 2025 13:33:14
S	10.0 - 1	57.5	-	53047	PPB	Std	10.00007471B	05 Aug 2025 13:35:33
U	ICV53 - 1	ICV53 510	3.7843	21482	PPB	SMPL	-7471B	05 Aug 2025 13:38:44
U	ICB53 - 1	ICB53	-0.0951	-289	PPB	SMPL	-7471B	05 Aug 2025 13:40:59
U	CCV86 - 1	CCV86	4.6435	26304	PPB	SMPL	-7471B	05 Aug 2025 13:43:17
U	CCB86 - 1	CCB86	-0.0217	123	PPB	SMPL	-7471B	05 Aug 2025 13:48:08
U	CRA - 1	CRA	0.1770	1238	PPB	SMPL	-7471B	05 Aug 2025 14:01:46
U	HighStd - 1	HighStd	9.4230	53126	PPB	SMPL	-7471B	05 Aug 2025 14:04:52
U	ChkStd - 1	ChkStd	6.9558	39280	PPB	SMPL	-7471B	05 Aug 2025 14:07:06
U	PB169125BL - 1	PB169125BL	-0.0222	120	PPB	SMPL	-7471B	05 Aug 2025 14:12:11
U	PB169125BS - 1	PB169125BS	3.0928	17601	PPB	SMPL	-7471B	05 Aug 2025 14:14:26
U	Q2759-01 - 1	SOLID-DRUMS	6.9860	39450	PPB	SMPL	-7471B	05 Aug 2025 14:16:42
U	Q2760-01 - 1	NB-07-08042025	0.0002	246	PPB	SMPL	-7471B	05 Aug 2025 14:19:01
U	Q2760-01DUP - 1	NB-07-08042025DUP	0.1405	1033	PPB	SMPL	-7471B	05 Aug 2025 14:21:34
U	Q2760-01MS - 1	NB-07-08042025MS	3.2057	18235	PPB	SMPL	-7471B	05 Aug 2025 14:23:51
U	Q2760-01MSD - 1	NB-07-08042025MSD	2.6198	14947	PPB	SMPL	-7471B	05 Aug 2025 14:26:06
U	CCV87 - 1	CCV87	4.8297	25485	PPB	SMPL	-7471B	05 Aug 2025 14:30:01
U	CCB87 - 1	CCB87	-0.0717	-497	PPB	SMPL	-7471B	05 Aug 2025 14:32:16
U	Q2763-01 - 1	TP-2	5.1769	27326	PPB	SMPL	-7471B	05 Aug 2025 14:34:37
U	Q2760-01LX5 - 1		-0.1120	-711	PPB	SMPL	-7471B	05 Aug 2025 14:36:52
U	Q2760-01A - 1		3.9504	20824	PPB	SMPL	-7471B	05 Aug 2025 14:39:15
U	CCV88 - 1	CCV88	4.8023	25340	PPB	SMPL	-7471B	05 Aug 2025 14:41:31
U	CCB88 - 1	CCB88	-0.0717	-497	PPB	SMPL	-7471B	05 Aug 2025 14:43:49