

LB136741 INSTRUMENT ID:CV1

Method: 7470A

Operator: Admin

Date of Analysis: 07 Aug 2025 14:11:51


Type	Sample ID	Extended ID	Conc.	μ Abs.	Units	Type	Std CondMethod	Date
S	0.0 - 1	50.0	-	-80	PPB	Std	0.00007470A	07 Aug 2025 14:12:11
S	0.2 - 1	50.2	-	811	PPB	Std	0.20007470A	07 Aug 2025 14:17:22
S	2.5 - 1	52.5	-	9201	PPB	Std	2.50007470A	07 Aug 2025 14:19:39
S	5.0 - 1	55.0	-	17089	PPB	Std	5.00007470A	07 Aug 2025 14:21:56
S	7.5 - 1	57.5	-	25698	PPB	Std	7.50007470A	07 Aug 2025 14:24:13
S	10.0 - 1	510.0	-	33885	PPB	Std	10.00007470A	07 Aug 2025 14:26:30
U	ICV03 - 1	ICV03	3.9997	13756	PPB	SMPL	-7470A	07 Aug 2025 14:29:29
U	CCV05 - 1	CCV05	4.9264	16893	PPB	SMPL	-7470A	07 Aug 2025 14:36:32
U	CCB05 - 1	CCB05	-0.0510	43	PPB	SMPL	-7470A	07 Aug 2025 14:41:21
U	CRA - 1	CRA	0.1676	783	PPB	SMPL	-7470A	07 Aug 2025 14:43:36
U	HighStd - 1	HighStd	10.0231	34147	PPB	SMPL	-7470A	07 Aug 2025 14:45:51
U	ChkStd - 1	ChkStd	7.3793	25197	PPB	SMPL	-7470A	07 Aug 2025 14:48:07
U	PB169163BL - 1	PBW	0.0001	216	PPB	SMPL	-7470A	07 Aug 2025 14:50:25
U	PB169163BS - 1	LCSW	3.7114	12780	PPB	SMPL	-7470A	07 Aug 2025 14:52:43
U	Q2758-02 - 1	WASTE	-0.1145	-172	PPB	SMPL	-7470A	07 Aug 2025 14:54:59
U	Q2759-02 - 1	SOLID-DRUMS	-0.0811	-59	PPB	SMPL	-7470A	07 Aug 2025 14:57:17
U	Q2763-04 - 1	TP-2	-0.0661	-8	PPB	SMPL	-7470A	07 Aug 2025 14:59:34
U	Q2773-01 - 1	COMP-1	-0.0617	7	PPB	SMPL	-7470A	07 Aug 2025 15:01:51
U	Q2773-02 - 1	COMP-2	-0.0519	40	PPB	SMPL	-7470A	07 Aug 2025 15:04:06
U	CCV06 - 1	CCV06	4.9349	16922	PPB	SMPL	-7470A	07 Aug 2025 15:06:22
U	CCB06 - 1	CCB06	-0.0407	78	PPB	SMPL	-7470A	07 Aug 2025 15:11:18
U	Q2773-03 - 1	COMP-3	-0.0711	-25	PPB	SMPL	-7470A	07 Aug 2025 15:13:34
U	Q2780-04 - 1	TP-3	-0.0439	67	PPB	SMPL	-7470A	07 Aug 2025 15:15:49
U	Q2780-08 - 1	TP-1	-0.0271	124	PPB	SMPL	-7470A	07 Aug 2025 15:18:04
U	Q2780-08DUP - 1	TP-1DUP	-0.0221	141	PPB	SMPL	-7470A	07 Aug 2025 15:20:20
U	Q2780-08MS - 1	TP-1MS	3.9563	13609	PPB	SMPL	-7470A	07 Aug 2025 15:22:37
U	Q2780-08MSD - 1	TP-1MSD	4.4289	15209	PPB	SMPL	-7470A	07 Aug 2025 15:24:54
U	Q2780-08LX5 - 1		-0.1432	-269	PPB	SMPL	-7470A	07 Aug 2025 15:27:12
U	Q2780-08A - 1		4.0942	14076	PPB	SMPL	-7470A	07 Aug 2025 15:29:31
U	PB169122TB - 1	PB169122TB	0.0131	260	PPB	SMPL	-7470A	07 Aug 2025 15:31:48
U	CCV07 - 1	CCV07	5.0209	17213	PPB	SMPL	-7470A	07 Aug 2025 15:34:05
U	CCB07 - 1	CCB07	-0.0720	-28	PPB	SMPL	-7470A	07 Aug 2025 15:36:20

LB136741
INSTRUMENT ID: CV₁

7470A

μ Abs.:

33885

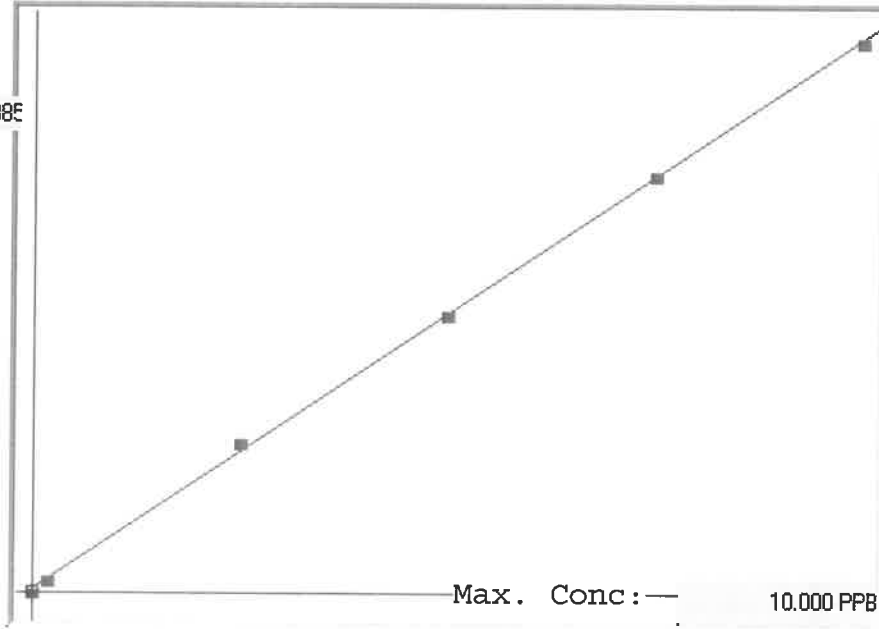

Linear

A= 0.0000e+000

B= 2.9539e-004

C= -6.3720e-002

Rho= 0.9997801

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.0	0.000	-0.087	-0.087	-80	0.000	-80	0				-12
0.2	0.200	0.176	-0.024	811	0.0 %	811					6
2.5	2.500	2.654	0.154	9201	0.0 %	9201	0				0
5.0	5.000	4.984	-0.016	17089	0.0 %	17089					0
7.5	7.500	7.527	0.027	25698	0.0 %	25698					0
10.0	10.000	9.946	-0.054	33885	0.0 %	33885					-1