

LB136748 INSTRUMENT ID: CV1

Method: 7471B

Operator: Admin

Date of Analysis: 08 Aug 2025 10:56:30

Type	Sample ID	Extended ID	Conc.	µ Abs.	Units	Type	Std Conc	Method	Date
S	0.0 - 1	50	-	63	PPB	Std	0.0000	7471B	08 Aug 2025 11:06:15
S	0.2 - 1	50.2	-	822	PPB	Std	0.2000	7471B	08 Aug 2025 11:08:32
S	2.5 - 1	52.5	-	12839	PPB	Std	2.5000	7471B	08 Aug 2025 11:10:49
S	5.0 - 1	55.0	-	24887	PPB	Std	5.0000	7471B	08 Aug 2025 11:13:06
S	7.5 - 1	57.5	-	38754	PPB	Std	7.5000	7471B	08 Aug 2025 11:15:25
S	10.0 - 1	510.0	-	53125	PPB	Std	10.0000	7471B	08 Aug 2025 11:17:45
U	ICV04 - 1	ICV04	4.0691	21058	PPB	SMPL	-7471B		08 Aug 2025 11:20:34
U	ICB04 - 1	ICB04	0.0319	-238	PPB	SMPL	-7471B		08 Aug 2025 11:22:51
U	CCV08 - 1	CCV08	5.0047	25993	PPB	SMPL	-7471B		08 Aug 2025 11:25:09
U	CCB08 - 1	CCB08	0.0256	-271	PPB	SMPL	-7471B		08 Aug 2025 11:27:25
U	CRA - 1	CRA	0.2761	1050	PPB	SMPL	-7471B		08 Aug 2025 11:29:45
U	HighStd - 1	HighStd	9.8467	51534	PPB	SMPL	-7471B		08 Aug 2025 11:32:00
U	ChkStd - 1	ChkStd	7.5342	39336	PPB	SMPL	-7471B		08 Aug 2025 11:34:15
U	PB169169BL - 1	PB169169BL	-0.0079	-448	PPB	SMPL	-7471B		08 Aug 2025 11:36:41
U	PB169169BS - 1	PB169169BS	3.3156	17083	PPB	SMPL	-7471B		08 Aug 2025 11:39:07
U	Q2772-01 - 1	500-3B-SOIL	0.2668	1001	PPB	SMPL	-7471B		08 Aug 2025 11:41:23
U	Q2774-03 - 1	256	5.0333	26144	PPB	SMPL	-7471B		08 Aug 2025 11:43:43
U	Q2774-05 - 1	R5	9.6620	50560	PPB	SMPL	-7471B		08 Aug 2025 11:46:01
U	Q2774-07 - 1	RT3826	1.4973	7492	PPB	SMPL	-7471B		08 Aug 2025 11:48:24
U	Q2774-07DUP - 1	RT3826DUP	1.2837	6365	PPB	SMPL	-7471B		08 Aug 2025 11:50:54
U	CCV09 - 1	CCV09	4.8769	25319	PPB	SMPL	-7471B		08 Aug 2025 11:53:13
U	CCB09 - 1	CCB09	-0.0210	-517	PPB	SMPL	-7471B		08 Aug 2025 11:55:31
U	Q2774-07MS - 1	RT3826MS	4.8487	25170	PPB	SMPL	-7471B		08 Aug 2025 11:57:49
U	Q2774-07MSD - 1	RT3826MSD	4.7086	24431	PPB	SMPL	-7471B		08 Aug 2025 12:00:06
U	Q2774-09 - 1	248	1.2014	5931	PPB	SMPL	-7471B		08 Aug 2025 12:02:27
U	Q2774-11 - 1	224	2.8538	14647	PPB	SMPL	-7471B		08 Aug 2025 12:04:49
U	Q2774-13 - 1	254	1.1648	5738	PPB	SMPL	-7471B		08 Aug 2025 12:07:09
U	Q2780-01 - 1	TP-3	2.6200	13414	PPB	SMPL	-7471B		08 Aug 2025 12:09:28
U	Q2780-05 - 1	TP-1	12.6242	66185	PPB	SMPL	-7471B		08 Aug 2025 12:11:47
U	Q2783-01 - 1	RT5414	1.2825	6359	PPB	SMPL	-7471B		08 Aug 2025 12:14:06
U	Q2784-01 - 1	EO-01-080625	0.6160	2843	PPB	SMPL	-7471B		08 Aug 2025 12:16:37
U	Q2786-01 - 1	PL-01-08062025	0.4979	2220	PPB	SMPL	-7471B		08 Aug 2025 12:18:55
U	CCV10 - 1	CCV10	4.9871	25900	PPB	SMPL	-7471B		08 Aug 2025 12:21:11
U	CCB10 - 1	CCB10	0.0074	-367	PPB	SMPL	-7471B		08 Aug 2025 12:23:29
U	Q2786-04 - 1	PL-03-08062025	0.3635	1511	PPB	SMPL	-7471B		08 Aug 2025 12:25:47
U	Q2774-07LX5 - 1		0.2892	1119	PPB	SMPL	-7471B		08 Aug 2025 12:28:03
U	Q2774-07A - 1		4.2183	21845	PPB	SMPL	-7471B		08 Aug 2025 12:30:18
U	Q2780-05DXL5 - 1	Q2780-05DXL5	2.3436	11956	PPB	SMPL	-7471B		08 Aug 2025 12:32:34
U	CCV11 - 1	CCV11	4.8676	25270	PPB	SMPL	-7471B		08 Aug 2025 12:34:55
U	CCB11 - 1	CCB11	0.0135	-335	PPB	SMPL	-7471B		08 Aug 2025 12:37:15


LB136748
INSTRUMENT ID: CV1

7471B

Linear

μ Abs. :

53125

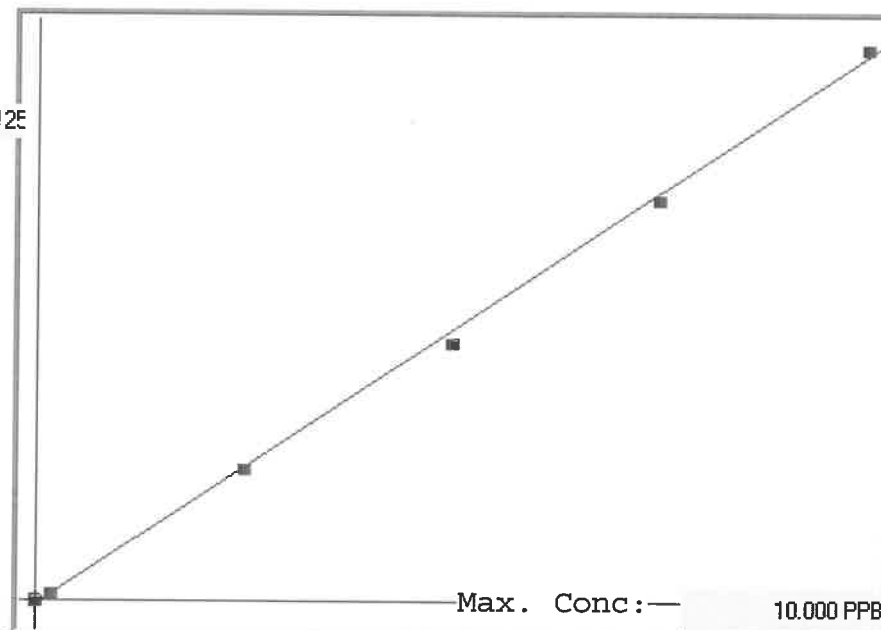

A= 0.0000e+000

B= 1.8958e-004

C= 7.7023e-002

Rho= 0.9995169

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.089	0.089	63	0.000	63					0
0.2	0.200	0.233	0.033	822	0.0 %	822					17
2.5	2.500	2.511	0.011	12839	0.0 %	12839					0
5.0	5.000	4.795	-0.205	24887	0.0 %	24887					4
7.5	7.500	7.424	-0.076	38754	0.0 %	38754					-1
10.0	10.000	10.148	0.148	53125	0.0 %	53125					1