

## LB136774 INSTRUMENT ID:CV1

Method: 7470A

Operator: Admin

Date of Analysis: 11 Aug 2025 14:44:41

| Type | Sample ID       | Extended ID | Conc.   | µ Abs. | Units | Type | Std CondMethod | Date                 |
|------|-----------------|-------------|---------|--------|-------|------|----------------|----------------------|
| S    | 0.0 - 1         | 50.0        | -       | 189    | PPB   | Std  | 0.00007470A    | 11 Aug 2025 16:17:40 |
| S    | 0.2 - 1         | 50.2        | -       | 749    | PPB   | Std  | 0.20007470A    | 11 Aug 2025 16:22:09 |
| S    | 2.5 - 1         | 52.5        | -       | 9410   | PPB   | Std  | 2.50007470A    | 11 Aug 2025 16:24:26 |
| S    | 5.0 - 1         | 55.0        | -       | 20627  | PPB   | Std  | 5.00007470A    | 11 Aug 2025 16:32:36 |
| S    | 7.5 - 1         | 57.5        | -       | 28372  | PPB   | Std  | 7.50007470A    | 11 Aug 2025 16:50:05 |
| S    | 10.0 - 1        | 510.0       | -       | 39436  | PPB   | Std  | 10.00007470A   | 11 Aug 2025 17:01:57 |
| U    | ICV07 - 1       | ICV07       | 3.7640  | 14758  | PPB   | SMPL | -7470A         | 11 Aug 2025 17:07:40 |
| U    | ICB07 - 1       | ICB07       | 0.0607  | 268    | PPB   | SMPL | -7470A         | 11 Aug 2025 17:09:55 |
| U    | CCV19 - 1       | CCV19       | 5.0621  | 19837  | PPB   | SMPL | -7470A         | 11 Aug 2025 17:22:05 |
| U    | CCB19 - 1       | CCB19       | 0.0615  | 271    | PPB   | SMPL | -7470A         | 11 Aug 2025 17:24:22 |
| U    | CRA - 1         | CRA         | 0.2023  | 822    | PPB   | SMPL | -7470A         | 11 Aug 2025 17:26:39 |
| U    | HighStd - 1     | HighStd     | 9.8117  | 38421  | PPB   | SMPL | -7470A         | 11 Aug 2025 17:37:57 |
| U    | ChkStd - 1      | ChkStd      | 6.7147  | 26303  | PPB   | SMPL | -7470A         | 11 Aug 2025 17:42:57 |
| U    | PB169166BL - 1  | PBW         | -0.1683 | -628   | PPB   | SMPL | -7470A         | 11 Aug 2025 17:45:13 |
| U    | PB169166BS - 1  | LCSW        | 4.1484  | 16262  | PPB   | SMPL | -7470A         | 11 Aug 2025 17:47:54 |
| U    | Q2779-04 - 1    | TP-4        | -0.0954 | -343   | PPB   | SMPL | -7470A         | 11 Aug 2025 17:50:10 |
| U    | Q2779-08 - 1    | TP-5        | -0.0185 | -42    | PPB   | SMPL | -7470A         | 11 Aug 2025 17:52:28 |
| U    | Q2783-03 - 1    | RT5414      | -0.0108 | -12    | PPB   | SMPL | -7470A         | 11 Aug 2025 17:54:46 |
| U    | Q2791-01 - 1    | SLUDGE      | 0.0025  | 40     | PPB   | SMPL | -7470A         | 11 Aug 2025 17:57:04 |
| U    | Q2798-04 - 1    | TP-6        | 0.0526  | 236    | PPB   | SMPL | -7470A         | 11 Aug 2025 17:59:19 |
| U    | CCV20 - 1       | CCV20       | 4.7996  | 18810  | PPB   | SMPL | -7470A         | 11 Aug 2025 18:01:35 |
| U    | CCB20 - 1       | CCB20       | 0.0030  | 42     | PPB   | SMPL | -7470A         | 11 Aug 2025 18:03:50 |
| U    | Q2800-02 - 1    | VNJ-222     | 0.0152  | 90     | PPB   | SMPL | -7470A         | 11 Aug 2025 18:06:08 |
| U    | Q2800-02DUP - 1 | VNJ-222DUP  | 0.0152  | 90     | PPB   | SMPL | -7470A         | 11 Aug 2025 18:08:24 |
| U    | Q2800-02MS - 1  | VNJ-222MS   | 3.4589  | 13564  | PPB   | SMPL | -7470A         | 11 Aug 2025 18:10:39 |
| U    | Q2800-02MSD - 1 | VNJ-222MSD  | 3.4057  | 13356  | PPB   | SMPL | -7470A         | 11 Aug 2025 18:12:55 |
| U    | Q2800-02LX5 - 1 |             | -0.0456 | -148   | PPB   | SMPL | -7470A         | 11 Aug 2025 18:15:12 |
| U    | Q2800-02A - 1   |             | 3.3998  | 13333  | PPB   | SMPL | -7470A         | 11 Aug 2025 18:17:30 |
| U    | PB169149TB - 1  | PB169149TB  | -0.0387 | -121   | PPB   | SMPL | -7470A         | 11 Aug 2025 18:19:47 |
| U    | CCV21 - 1       | CCV21       | 4.8607  | 19049  | PPB   | SMPL | -7470A         | 11 Aug 2025 18:22:05 |
| U    | CCB21 - 1       | CCB21       | -0.0446 | -144   | PPB   | SMPL | -7470A         | 11 Aug 2025 18:24:22 |

LB 136773


INSTRUMENT ID: CV2

7470A

Linear ▼

 $\mu$  Abs.:

: 3943E

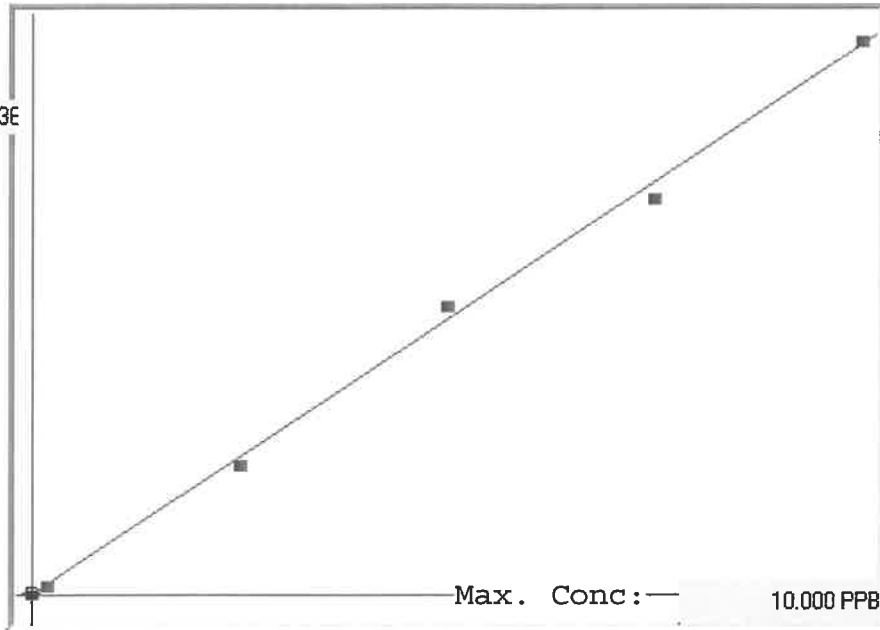

A= 0.0000e+000

B= 2.5558e-004

C= -7.7607e-003

Rho= 0.9990629

Accept=Accepted

| Std ID | Conc.  | Calc.  | Dev.   | Mean  | SD or %RSD | Rep 1 | Rep 2 | Rep 3 | Rep 4 | Rep 5 | %D |
|--------|--------|--------|--------|-------|------------|-------|-------|-------|-------|-------|----|
| 0.0    | 0.000  | 0.041  | 0.041  | 189   | 0.000      | 189   | 0     |       |       |       | -8 |
| 0.2    | 0.200  | 0.184  | -0.016 | 749   | 0.0 %      | 749   |       |       |       |       | -4 |
| 2.5    | 2.500  | 2.397  | -0.103 | 9410  | 0.0 %      | 9410  | 0     |       |       |       | 5  |
| 5.0    | 5.000  | 5.264  | 0.264  | 20627 | 0.0 %      | 20627 |       |       |       |       | -3 |
| 7.5    | 7.500  | 7.243  | -0.257 | 28372 | 0.0 %      | 28372 |       |       |       |       | 1  |
| 10.0   | 10.000 | 10.071 | 0.071  | 39436 | 0.0 %      | 39436 |       |       |       |       |    |