

LB136791 INSTRUMENT ID:CV1

Method: 245.1

Operator: Admin

Date of Analysis: 12 Aug 2025 16:16:33


Type	Sample ID	Extended ID	Conc.	μ Abs.	Units	Type	Std Cond	Method	Date
S	0.0 - 1	50	-	-116	PPB	Std	0.0000	245.1	12 Aug 2025 16:58:13
S	0.05 - 1	50.05	-	124	PPB	Std	0.0500	245.1	12 Aug 2025 17:00:30
S	0.2 - 1	50.2	-	775	PPB	Std	0.2000	245.1	12 Aug 2025 17:02:47
S	2.5 - 1	52.5	-	10491	PPB	Std	2.5000	245.1	12 Aug 2025 17:05:04
S	5.0 - 1	55.0	-	20947	PPB	Std	5.0000	245.1	12 Aug 2025 17:07:20
S	7.5 - 1	57.5	-	31480	PPB	Std	7.5000	245.1	12 Aug 2025 17:09:38
S	10.0 - 1	510.0	-	42035	PPB	Std	10.0000	245.1	12 Aug 2025 17:28:26
U	ICV11 - 1	ICV11	4.0583	17005	PPB	SMPL	-245.1		12 Aug 2025 17:35:31
U	ICB11 - 1	ICB11	0.0115	-35	PPB	SMPL	-245.1		12 Aug 2025 17:40:32
U	CCV32 - 1	CCV32	4.9722	20853	PPB	SMPL	-245.1		12 Aug 2025 17:42:47
U	CCB32 - 1	CCB32	-0.0393	-249	PPB	SMPL	-245.1		12 Aug 2025 17:45:02
U	CRA - 1	CRA	0.0381	77	PPB	SMPL	-245.1		12 Aug 2025 17:47:19
U	HighStd - 1	HighStd	9.9432	41784	PPB	SMPL	-245.1		12 Aug 2025 17:49:34
U	ChkStd - 1	ChkStd	7.1709	30111	PPB	SMPL	-245.1		12 Aug 2025 17:51:49
U	PB169219BL - 1	PBW	0.0198	0	PPB	SMPL	-245.1		12 Aug 2025 17:57:00
U	PB169219BS - 1	LCSW	3.9137	16396	PPB	SMPL	-245.1		12 Aug 2025 17:59:15
U	Q2785-01 - 1	WATER	-0.0469	-281	PPB	SMPL	-245.1		12 Aug 2025 18:01:31
U	Q2785-01DUP - 1	WATERDUP	0.0010	-79	PPB	SMPL	-245.1		12 Aug 2025 18:03:49
U	Q2785-01MS - 1	WATERMS	3.8346	16063	PPB	SMPL	-245.1		12 Aug 2025 18:11:38
U	Q2785-01MSD - 1	WATERMSD	3.8263	16028	PPB	SMPL	-245.1		12 Aug 2025 18:13:55
U	Q2789-02 - 1	Comp	0.1100	380	PPB	SMPL	-245.1		12 Aug 2025 18:16:12
U	CCV33 - 1	CCV33	4.6561	19522	PPB	SMPL	-245.1		12 Aug 2025 18:18:30
U	CCB33 - 1	CCB33	-0.0391	-248	PPB	SMPL	-245.1		12 Aug 2025 18:20:45
U	Q2799-01 - 1	CC-071325-RW	-0.0403	-253	PPB	SMPL	-245.1		12 Aug 2025 18:23:02
U	Q2785-01LX5 - 1		-0.0496	-292	PPB	SMPL	-245.1		12 Aug 2025 18:25:18
U	Q2785-01A - 1		3.7817	15840	PPB	SMPL	-245.1		12 Aug 2025 18:27:56
U	CCV34 - 1	CCV34	4.7494	19915	PPB	SMPL	-245.1		12 Aug 2025 18:30:11
U	CCB34 - 1	CCB34	-0.0094	-123	PPB	SMPL	-245.1		12 Aug 2025 18:32:29

LB136791
INSTRUMENT ID: CV1

245.1

μ Abs.:

42035

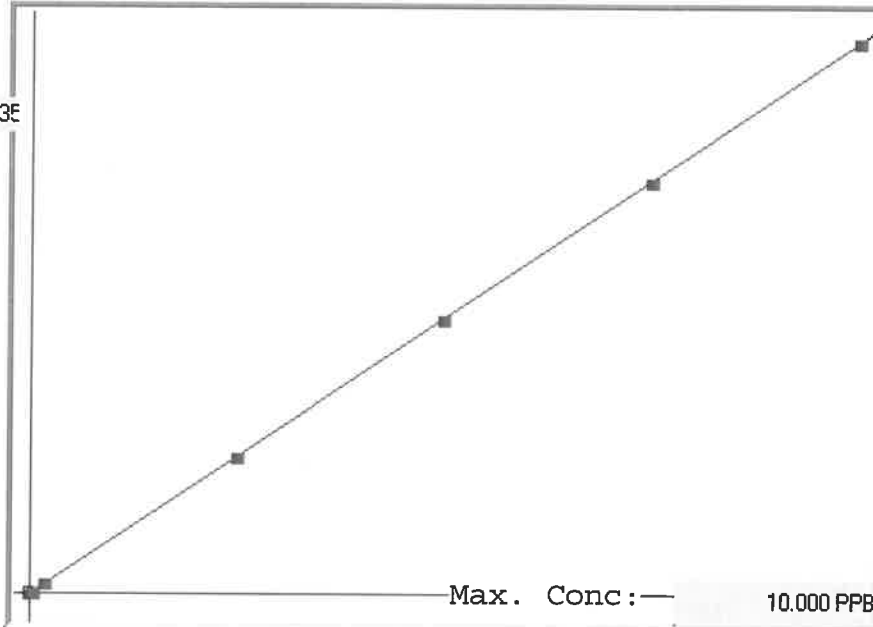

Linear

A= 0.0000e+000

B= 2.3749e-004

C= 1.9791e-002

Rho= 0.9999987

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%
0.0	0.000	-0.008	-0.008	-116	0.000	-116					
0.05	0.050	0.049	-0.001	124	0.0 %	124					
0.2	0.200	0.204	0.004	775	0.0 %	775					
2.5	2.500	2.511	0.011	10491	0.0 %	10491					
5.0	5.000	4.995	-0.005	20947	0.0 %	20947					
7.5	7.500	7.496	-0.004	31480	0.0 %	31480					
10.0	10.000	10.003	0.003	42035	0.0 %	42035					

0.00001
0.00001
0.00001
0.00001
0.00001
0.00001
0.00001