

LB136797 INSTRUMENT ID: CV1

Method: 7470A

Operator: Admin

Date of Analysis: 13 Aug 2025 10:42:51


Type	Sample ID	Extended ID	Conc.	μ Abs.	Units	Type	Std CondMethod	Date
S	0.0 - 1	50.0	-	-97	PPB	Std	0.00007470A	13 Aug 2025 10:55:11
S	0.2 - 1	50.2	-	687	PPB	Std	0.20007470A	13 Aug 2025 10:57:29
S	2.5 - 1	52.5	-	9657	PPB	Std	2.50007470A	13 Aug 2025 10:59:46
S	5.0 - 1	55.0	-	18787	PPB	Std	5.00007470A	13 Aug 2025 11:02:04
S	7.5 - 1	57.5	-	29412	PPB	Std	7.50007470A	13 Aug 2025 11:04:23
S	10.0 - 1	510.0	-	38526	PPB	Std	10.00007470A	13 Aug 2025 11:06:43
U	ICV12 - 1	ICV12	4.1031	15786	PPB	SMPL	-7470A	13 Aug 2025 11:10:50
U	ICB12 - 1	ICB12	0.0134	-77	PPB	SMPL	-7470A	13 Aug 2025 11:19:45
U	CCV35 - 1	CCV35	5.0616	19504	PPB	SMPL	-7470A	13 Aug 2025 11:22:01
U	CCB35 - 1	CCB35	-0.0443	-301	PPB	SMPL	-7470A	13 Aug 2025 11:24:17
U	CRA - 1	CRA	0.2027	657	PPB	SMPL	-7470A	13 Aug 2025 11:26:36
U	HighStd - 1	HighStd	10.1843	39374	PPB	SMPL	-7470A	13 Aug 2025 11:28:56
U	ChkStd - 1	ChkStd	7.6100	29389	PPB	SMPL	-7470A	13 Aug 2025 11:31:13
U	PB169233BL - 1	PBW	-0.1003	-518	PPB	SMPL	-7470A	13 Aug 2025 11:33:31
U	PB169233BS - 1	LCSW	4.0188	15459	PPB	SMPL	-7470A	13 Aug 2025 11:35:49
U	Q2808-04 - 1	TP-7	-0.0299	-245	PPB	SMPL	-7470A	13 Aug 2025 11:38:06
U	Q2826-02 - 1	WC1	0.0067	-103	PPB	SMPL	-7470A	13 Aug 2025 11:40:25
U	Q2827-04 - 1	TP-8	0.0511	69	PPB	SMPL	-7470A	13 Aug 2025 11:42:41
U	Q2827-08 - 1	TP-9	0.0160	-67	PPB	SMPL	-7470A	13 Aug 2025 11:44:59
U	Q2831-03 - 1	VNJ-238	-0.0013	-134	PPB	SMPL	-7470A	13 Aug 2025 11:47:14
U	CCV36 - 1	CCV36	4.9538	19086	PPB	SMPL	-7470A	13 Aug 2025 11:49:29
U	CCB36 - 1	CCB36	-0.0152	-188	PPB	SMPL	-7470A	13 Aug 2025 11:51:44
U	Q2831-03DUP - 1	VNJ-238DUP	0.0147	-72	PPB	SMPL	-7470A	13 Aug 2025 11:54:02
U	Q2831-03MS - 1	VNJ-238MS	4.1314	15896	PPB	SMPL	-7470A	13 Aug 2025 11:56:19
U	Q2831-03MSD - 1	VNJ-238MSD	4.1701	16046	PPB	SMPL	-7470A	13 Aug 2025 11:58:40
U	Q2831-03LX5 - 1		-0.0206	-209	PPB	SMPL	-7470A	13 Aug 2025 12:01:01
U	Q2831-03A - 1		4.2023	16171	PPB	SMPL	-7470A	13 Aug 2025 12:03:21
U	PB169200TB - 1	PB169200TB	-0.0317	-252	PPB	SMPL	-7470A	13 Aug 2025 12:05:42
U	CCV37 - 1	CCV37	4.9608	19113	PPB	SMPL	-7470A	13 Aug 2025 12:08:04
U	CCB37 - 1	CCB37	-0.0446	-302	PPB	SMPL	-7470A	13 Aug 2025 12:10:22

LB136797
INSTRUMENT ID: CV₂

7470A

μ Abs.:

3852E

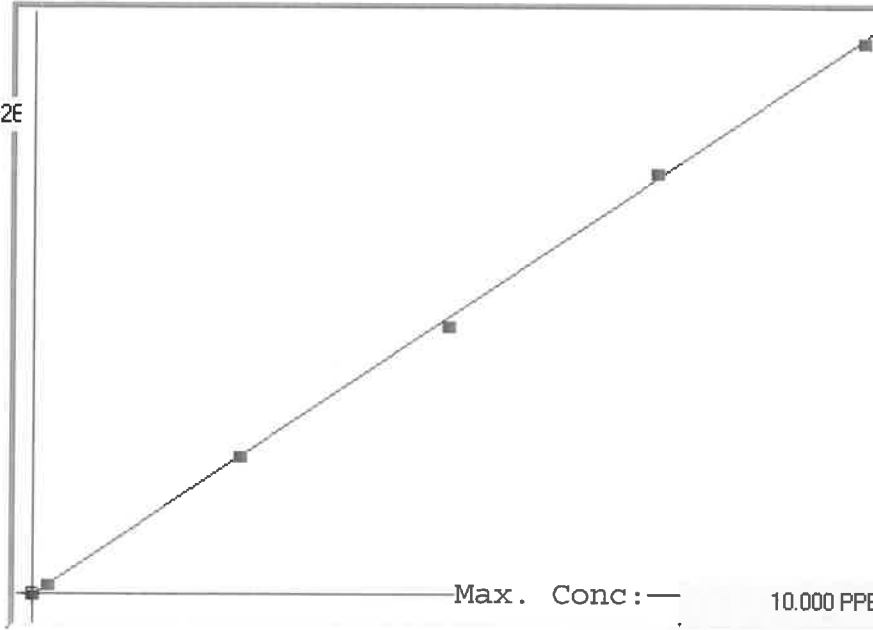

Linear

A= 0.0000e+000

B= 2.5781e-004

C= 3.3286e-002

Rho= 0.9998132

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.008	0.008	-97	0.000	-97	0				
0.2	0.200	0.210	0.010	687	0.0 %	687					
2.5	2.500	2.523	0.023	9657	0.0 %	9657	0				
5.0	5.000	4.877	-0.123	18787	0.0 %	18787					
7.5	7.500	7.616	0.116	29412	0.0 %	29412					
10.0	10.000	9.966	-0.034	38526	0.0 %	38526					

100000