

LB136799 INSTRUMENT ID:CV1

Method: 7471B

Operator: Admin

Date of Analysis: 13 Aug 2025 13:56:07

Type	Sample ID	Extended ID	Conc.	µ Abs.	Units	Type	Stdnd Conc	Method	Date
S	0.0 - 1	50.0	-	-829	PPB	Std	0.00007471B		13 Aug 2025 14:11:01
S	0.2 - 1	50.2	-	109	PPB	Std	0.20007471B		13 Aug 2025 14:13:18
S	2.5 - 1	52.5	-	11015	PPB	Std	2.50007471B		13 Aug 2025 14:15:35
S	5.0 - 1	55.0	-	22669	PPB	Std	5.00007471B		13 Aug 2025 14:17:52
S	7.5 - 1	57.5	-	35161	PPB	Std	7.50007471B		13 Aug 2025 14:20:11
S	10.0 - 1	510.0	-	47856	PPB	Std	10.00007471B		13 Aug 2025 14:22:30
U	ICV13 - 1	ICV13	3.9393	18066	PPB	SMPL	-7471B		13 Aug 2025 14:39:23
U	ICB13 - 1	ICB13	-0.0192	-1129	PPB	SMPL	-7471B		13 Aug 2025 14:41:40
U	CCV38 - 1	CCV38	4.9836	23130	PPB	SMPL	-7471B		13 Aug 2025 14:44:01
U	CCB38 - 1	CCB38	-0.0347	-1204	PPB	SMPL	-7471B		13 Aug 2025 14:46:15
U	CRA - 1	CRA	0.2332	95	PPB	SMPL	-7471B		13 Aug 2025 14:48:35
U	HighStd - 1	HighStd	10.1669	48264	PPB	SMPL	-7471B		13 Aug 2025 14:50:50
U	ChkStd - 1	ChkStd	7.7431	36511	PPB	SMPL	-7471B		13 Aug 2025 14:53:08
U	PB169231BL - 1	PB169231BL	-0.0912	-1478	PPB	SMPL	-7471B		13 Aug 2025 14:55:33
U	PB169231BS - 1	PB169231BS	3.4679	15780	PPB	SMPL	-7471B		13 Aug 2025 14:57:54
U	Q2832-01 - 1	TG-S01	21.3213	102352	PPB	SMPL	-7471B		13 Aug 2025 15:00:11
U	Q2832-03 - 1	TG-S02	5.1868	24115	PPB	SMPL	-7471B		13 Aug 2025 15:02:30
U	Q2832-05 - 1	TG-S03	7.2954	34340	PPB	SMPL	-7471B		13 Aug 2025 15:05:13
U	Q2832-07 - 1	TG-S04	6.5899	30919	PPB	SMPL	-7471B		13 Aug 2025 15:08:55
U	Q2832-09 - 1	TG-S05	9.4773	44920	PPB	SMPL	-7471B		13 Aug 2025 15:11:11
U	CCV39 - 1	CCV39	4.8834	22644	PPB	SMPL	-7471B		13 Aug 2025 15:13:34
U	CCB39 - 1	CCB39	-0.0621	-1337	PPB	SMPL	-7471B		13 Aug 2025 15:15:59
U	Q2838-01 - 1	TP-11	0.0622	-734	PPB	SMPL	-7471B		13 Aug 2025 15:18:19
U	Q2838-05 - 1	TP-10	0.2738	292	PPB	SMPL	-7471B		13 Aug 2025 15:20:35
U	Q2840-01 - 1	0804-SOIL	2.2317	9786	PPB	SMPL	-7471B		13 Aug 2025 15:22:51
U	Q2840-01DUP - 1	0804-SOILDUP	1.6417	6925	PPB	SMPL	-7471B		13 Aug 2025 15:25:07
U	Q2840-01MS - 1	0804-SOILMS	5.0152	23283	PPB	SMPL	-7471B		13 Aug 2025 15:27:27
U	Q2840-01MSD - 1	0804-SOILMSD	6.5726	30835	PPB	SMPL	-7471B		13 Aug 2025 15:32:57
U	Q2840-02 - 1	0804-D	0.0928	-586	PPB	SMPL	-7471B		13 Aug 2025 15:37:52
U	Q2840-01LX5 - 1		0.3873	842	PPB	SMPL	-7471B		13 Aug 2025 15:40:12
U	Q2840-01A - 1		4.0915	18804	PPB	SMPL	-7471B		13 Aug 2025 15:42:29
U	Q2832-01DLX5 - 1		4.2286	19469	PPB	SMPL	-7471B		13 Aug 2025 15:44:45
U	CCV40 - 1	CCV40	4.7574	22033	PPB	SMPL	-7471B		13 Aug 2025 15:47:03
U	CCB40 - 1	CCB40	-0.0270	-1167	PPB	SMPL	-7471B		13 Aug 2025 15:49:29

LB136799

7471B

INSTRUMENT ID: GV₁

Linear

 μ Abs.:

4785E


A= 0.0000e+000

B= 2.0623e-004

C= 2.1362e-001

Rho= 0.9998540

Accept=Accepted

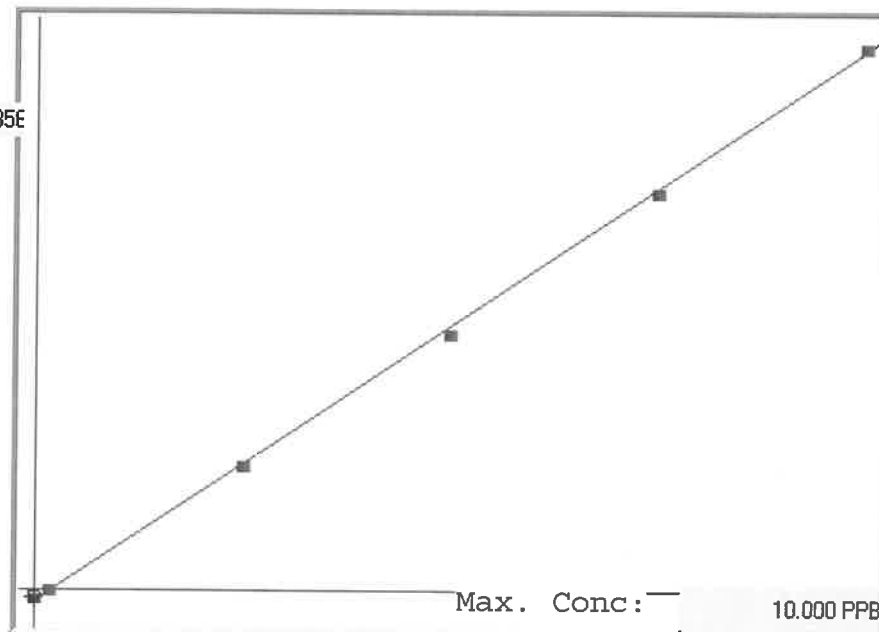

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	Handwritten
0.0	0.000	0.043	0.043	-829	0.000	-829					10000
0.2	0.200	0.236	0.036	109	0.0 %	109					10000
2.5	2.500	2.485	-0.015	11015	0.0 %	11015					10000
5.0	5.000	4.889	-0.111	22669	0.0 %	22669					10000
7.5	7.500	7.465	-0.035	35161	0.0 %	35161					10000
10.0	10.000	10.083	0.083	47856	0.0 %	47856					10000