

LB136819 INSTRUMENT ID:CV1

Method: 7470A

Operator: Admin

Date of Analysis: 14 Aug 2025 10:27:03

Type	Sample ID	Extended ID	Conc.	µ Abs.	Units	Type	Std CondMethod	Date
S	0.0 - 1	50.0	-	-73	PPB	Std	0.00007470A	14 Aug 2025 10:40:26
S	0.2 - 1	50.2	-	460	PPB	Std	0.20007470A	14 Aug 2025 10:42:46
S	2.5 - 1	52.5	-	9017	PPB	Std	2.50007470A	14 Aug 2025 10:48:03
S	5.0 - 1	55.0	-	18875	PPB	Std	5.00007470A	14 Aug 2025 10:50:22
S	7.5 - 1	57.5	-	28739	PPB	Std	7.50007470A	14 Aug 2025 10:52:38
S	10.0 - 1	510.0	-	37490	PPB	Std	10.00007470A	14 Aug 2025 10:54:56
U	ICV14 - 1	ICV14	3.9561	14824	PPB	SMPL	-7470A	14 Aug 2025 10:58:01
U	ICB14 - 1	ICB14	0.0063	-193	PPB	SMPL	-7470A	14 Aug 2025 11:00:59
U	CCV41 - 1	CCV41	5.1271	19276	PPB	SMPL	-7470A	14 Aug 2025 11:03:15
U	CCB41 - 1	CCB41	-0.0502	-408	PPB	SMPL	-7470A	14 Aug 2025 11:05:31
U	CRA - 1	CRA	0.2146	599	PPB	SMPL	-7470A	14 Aug 2025 11:07:48
U	HighStd - 1	HighStd	10.1189	38255	PPB	SMPL	-7470A	14 Aug 2025 11:10:05
U	ChkStd - 1	ChkStd	7.4969	28286	PPB	SMPL	-7470A	14 Aug 2025 11:12:23
U	PB169234BL - 1	PBW	-0.1378	-741	PPB	SMPL	-7470A	14 Aug 2025 11:17:21
U	PB169234BS - 1	LCSW	3.9351	14744	PPB	SMPL	-7470A	14 Aug 2025 11:19:39
U	Q2732-03 - 1	WC-A7-01-C	-0.0844	-538	PPB	SMPL	-7470A	14 Aug 2025 11:21:58
U	Q2832-02 - 1	TG-S01	-0.0155	-276	PPB	SMPL	-7470A	14 Aug 2025 11:24:43
U	Q2832-04 - 1	TG-S02	-0.0247	-311	PPB	SMPL	-7470A	14 Aug 2025 11:27:00
U	Q2832-06 - 1	TG-S03	-0.1073	-625	PPB	SMPL	-7470A	14 Aug 2025 11:29:52
U	Q2832-10 - 1	TG-S05	-0.0934	-572	PPB	SMPL	-7470A	14 Aug 2025 11:32:08
U	CCV42 - 1	CCV42	5.0887	19130	PPB	SMPL	-7470A	14 Aug 2025 11:34:25
U	CCB42 - 1	CCB42	-0.0323	-340	PPB	SMPL	-7470A	14 Aug 2025 11:36:40
U	Q2836-03 - 1	WC-A2-15-C	-0.1220	-681	PPB	SMPL	-7470A	14 Aug 2025 11:38:57
U	Q2836-07 - 1	WC-A2-16-C	-0.0970	-586	PPB	SMPL	-7470A	14 Aug 2025 11:41:13
U	Q2836-11 - 1	WC-A2-17-C	-0.1433	-762	PPB	SMPL	-7470A	14 Aug 2025 11:43:28
U	Q2836-15 - 1	WC-A5-02-C	-0.1252	-693	PPB	SMPL	-7470A	14 Aug 2025 11:45:46
U	Q2838-04 - 1	TP-11	-0.1446	-767	PPB	SMPL	-7470A	14 Aug 2025 11:48:07
U	Q2838-08 - 1	TP-10	-0.1465	-774	PPB	SMPL	-7470A	14 Aug 2025 11:50:24
U	Q2838-08DUP - 1	TP-10DUP	-0.1383	-743	PPB	SMPL	-7470A	14 Aug 2025 11:52:41
U	Q2838-08MS - 1	TP-10MS	3.9385	14757	PPB	SMPL	-7470A	14 Aug 2025 11:55:00
U	Q2838-08MSD - 1	TP-10MSD	3.5752	13376	PPB	SMPL	-7470A	14 Aug 2025 11:57:17
U	Q2832-08 - 1	TG-S04	-0.1499	-787	PPB	SMPL	-7470A	14 Aug 2025 11:59:34
U	CCV43 - 1	CCV43	5.0266	18894	PPB	SMPL	-7470A	14 Aug 2025 12:01:52
U	CCB43 - 1	CCB43	-0.0360	-354	PPB	SMPL	-7470A	14 Aug 2025 12:04:08
U	Q2838-08LX5 - 1		-0.1552	-807	PPB	SMPL	-7470A	14 Aug 2025 12:06:31
U	Q2838-08A - 1		3.9479	14793	PPB	SMPL	-7470A	14 Aug 2025 12:08:47
U	PB169212TB - 1	PB169212TB	-0.1057	-619	PPB	SMPL	-7470A	14 Aug 2025 12:11:07
U	CCV44 - 1	CCV44	4.9816	18723	PPB	SMPL	-7470A	14 Aug 2025 12:13:28
U	CCB44 - 1	CCB44	-0.0468	-395	PPB	SMPL	-7470A	14 Aug 2025 12:15:46


7470A

LB 136819
INSTRUMENT ID: CV1

Linear

 μ Abs.:

37490

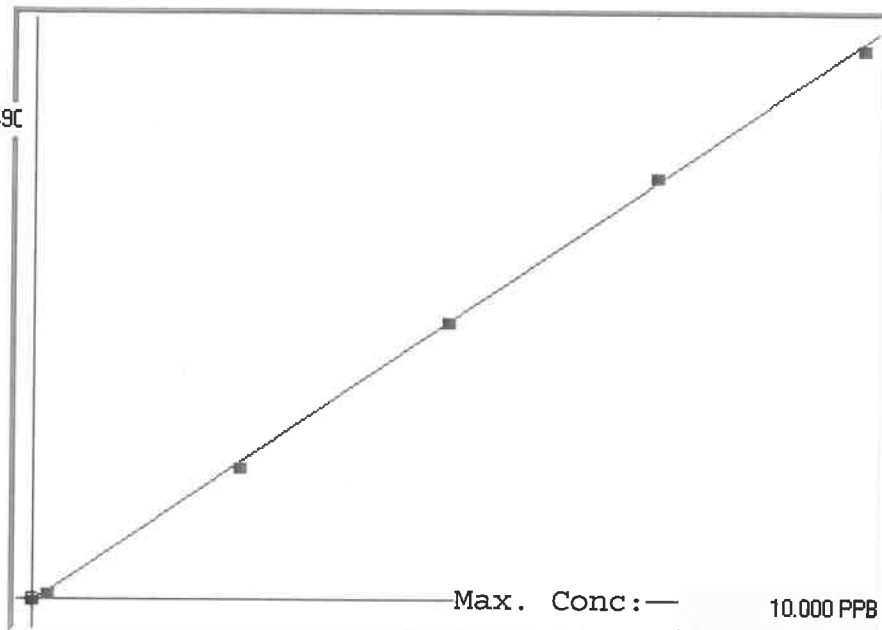

A= 0.0000e+000

B= 2.6302e-004

C= 5.7097e-002

Rho= 0.9998305

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.0	0.000	0.038	0.038	-73	0.000	-73	0				0.0000
0.2	0.200	0.178	-0.022	460	0.0 %	460					0.0000
2.5	2.500	2.429	-0.071	9017	0.0 %	9017	0				0.0000
5.0	5.000	5.022	0.022	18875	0.0 %	18875					0.0000
7.5	7.500	7.616	0.116	28739	0.0 %	28739					0.0000
10.0	10.000	9.918	-0.082	37490	0.0 %	37490					0.0000