

LB136888 INSTRUMENT ID:CV1

Method: 7470A

Operator: Admin

Date of Analysis: 20 Aug 2025 10:03:12

Type	Sample ID	Extended ID	Conc.	μ Abs.	Units	Type	Std Conc	Method	Date
S	0.0 - 1	50.0	-	379	PPB	Std	0.0000	7470A	20 Aug 2025 10:34:15
S	0.2 - 1	50.2	-	1046	PPB	Std	0.2000	7470A	20 Aug 2025 10:36:32
S	2.5 - 1	52.5	-	11067	PPB	Std	2.5000	7470A	20 Aug 2025 10:38:49
S	5.0 - 1	55.0	-	22101	PPB	Std	5.0000	7470A	20 Aug 2025 10:41:05
S	7.5 - 1	57.5	-	32949	PPB	Std	7.5000	7470A	20 Aug 2025 10:43:21
S	10.0 - 1	59.0	-	41928	PPB	Std	10.0000	7470A	20 Aug 2025 10:45:38
U	ICV26 - 1	ICV26	4.0914	17786	PPB	SMPL	-7470A	-7470A	20 Aug 2025 10:48:50
U	ICB26 - 1	ICB26	-0.0560	253	PPB	SMPL	-7470A	-7470A	20 Aug 2025 10:51:05
U	CCV81 - 1	CCV81	5.0511	21843	PPB	SMPL	-7470A	-7470A	20 Aug 2025 10:53:23
U	CCB81 - 1	CCB81	-0.0681	202	PPB	SMPL	-7470A	-7470A	20 Aug 2025 10:55:39
U	CRA - 1	CRA	0.1623	1176	PPB	SMPL	-7470A	-7470A	20 Aug 2025 10:58:06
U	HighStd - 1	HighStd	9.7878	41867	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:00:22
U	ChkStd - 1	ChkStd	7.7215	33132	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:02:43
U	PB169310BL - 1	PBW	-0.0787	157	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:07:04
U	PB169310BS - 1	LCSW	4.1186	17901	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:09:20
U	Q2865-03 - 1	LAW-25-0109	0.2822	1683	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:11:36
U	Q2865-03DUP - 1	LAW-25-0109DUP	0.2640	1606	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:13:54
U	Q2865-03MS - 1	LAW-25-0109MS	3.6621	15971	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:22:21
U	Q2865-03MSD - 1	LAW-25-0109MSD	3.5317	15420	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:27:16
U	Q2867-01 - 1	Tre-2005	-0.0995	69	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:29:32
U	CCV82 - 1	CCV82	4.5075	19545	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:31:48
U	CCB82 - 1	CCB82	-0.0276	373	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:40:07
U	Q2867-02 - 1	Tre-2006	0.5966	3012	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:42:22
U	PB169308BL - 1	PBW	-0.0279	372	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:47:27
U	PB169308BS - 1	LCSW	3.6954	16112	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:53:23
U	Q2884-04 - 1	302	-0.0929	97	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:55:39
U	Q2888-02 - 1	VNJ-210	-0.0567	250	PPB	SMPL	-7470A	-7470A	20 Aug 2025 11:57:56
U	Q2888-02DUP - 1	VNJ-210DUP	-0.0470	291	PPB	SMPL	-7470A	-7470A	20 Aug 2025 12:00:15
U	Q2888-02MS - 1	VNJ-210MS	3.7936	16527	PPB	SMPL	-7470A	-7470A	20 Aug 2025 12:02:32
U	Q2888-02MSD - 1	VNJ-210MSD	3.2531	14242	PPB	SMPL	-7470A	-7470A	20 Aug 2025 12:04:48
U	Q2865-03LX5 - 1		0.3042	1776	PPB	SMPL	-7470A	-7470A	20 Aug 2025 12:07:08
U	Q2865-03A - 1		3.4419	15040	PPB	SMPL	-7470A	-7470A	20 Aug 2025 12:09:24
U	CCV83 - 1	CCV83	4.8924	21172	PPB	SMPL	-7470A	-7470A	20 Aug 2025 12:11:42
U	CCB83 - 1	CCB83	-0.0510	274	PPB	SMPL	-7470A	-7470A	20 Aug 2025 12:13:57
U	PB169291TB - 1	PB169291TB	-0.0532	265	PPB	SMPL	-7470A	-7470A	20 Aug 2025 12:16:13
U	Q2888-02LX5 - 1		-0.1175	-7	PPB	SMPL	-7470A	-7470A	20 Aug 2025 12:18:29
U	Q2888-02A - 1		3.4875	15233	PPB	SMPL	-7470A	-7470A	20 Aug 2025 12:20:45
U	CCV84 - 1	CCV84	5.2018	22480	PPB	SMPL	-7470A	-7470A	20 Aug 2025 12:23:01
U	CCB84 - 1	CCB84	-0.0671	206	PPB	SMPL	-7470A	-7470A	20 Aug 2025 12:25:17


LB136888

Instrument ID: CV1

7470A

 μ Abs.:

41928

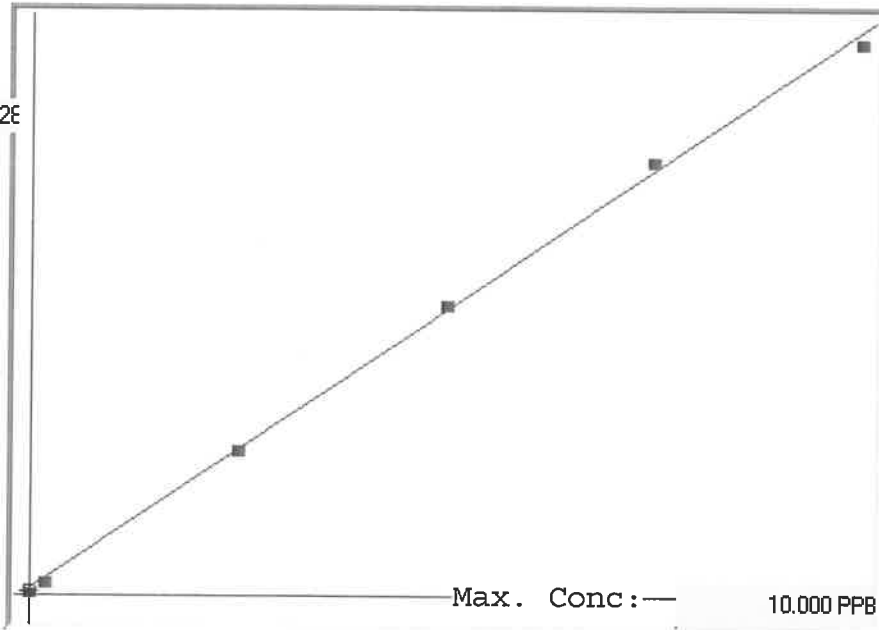

Linear

A= 0.0000e+000

B= 2.3655e-004

C= -1.1586e-001

Rho= 0.9994562

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.0	0.000	-0.026	-0.026	379	0.000	379	0				-5
0.2	0.200	0.132	-0.068	1046	0.0 %	1046					0
2.5	2.500	2.502	0.002	11067	0.0 %	11067	0				2
5.0	5.000	5.112	0.112	22101	0.0 %	22101					2
7.5	7.500	7.678	0.178	32949	0.0 %	32949					-2
10.0	10.000	9.802	-0.198	41928	0.0 %	41928					