

6b136895

Test results

Aquakem 7.2AQ1

Page: 1

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

8/20/2025 14:25

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.015	0.0	0.109	
ICB1	0.003	0.0	0.008	
CCV1	0.986	0.0	0.106	
CCB1	0.001	0.0	0.008	
PB169315BL	-0.001	0.0	0.008	
PB169315BS	1.014	0.0	0.109	
Q2893-01	0.027	0.0	0.011	
Q2893-02	0.048	0.0	0.013	
PB169317BL	0.001	0.0	0.008	
PB169317BS	1.014	0.0	0.109	
Q2893-07	0.026	0.0	0.011	
Q2893-08	0.050	0.0	0.013	
CCV2	0.986	0.0	0.106	
CCB2	0.002	0.0	0.008	

N	14
Mean	0.369
SD	0.4904
CV%	132.75

Aquakem v. 7.2AQ1

Results from time period:

Wed Aug 20 13:17:31 2025

Wed Aug 20 14:24:32 2025

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0004	mg/l	8/20/2025 13:37:35	
0.05PPM	A	Phenolics-	P	0.0524	mg/l	8/20/2025 13:37:36	
0.1PPM	A	Phenolics-	P	0.1032	mg/l	8/20/2025 13:37:37	
0.25PPM	A	Phenolics-	P	0.2535	mg/l	8/20/2025 13:37:38	
0.50PPM	A	Phenolics-	P	0.5003	mg/l	8/20/2025 13:37:39	
1.0PPM	A	Phenolics-	P	0.9835	mg/l	8/20/2025 13:37:40	
2.0PPM	A	Phenolics-	P	2.0075	mg/l	8/20/2025 13:37:41	
ICV1	S	Phenolics-	P	1.0146	mg/l	8/20/2025 14:09:33	
ICB1	S	Phenolics-	P	0.0026	mg/l	8/20/2025 14:09:35	
CCV1	S	Phenolics-	P	0.9862	mg/l	8/20/2025 14:09:37	
CCB1	S	Phenolics-	P	0.0007	mg/l	8/20/2025 14:09:39	
PB169315BL	S	Phenolics-	P	-0.0006	mg/l	8/20/2025 14:09:41	
PB169315BS	S	Phenolics-	P	1.014	mg/l	8/20/2025 14:09:44	
Q2893-01	S	Phenolics-	P	0.0268	mg/l	8/20/2025 14:19:36	
Q2893-02	S	Phenolics-	P	0.0483	mg/l	8/20/2025 14:19:37	
PB169317BL	S	Phenolics-	P	0.0014	mg/l	8/20/2025 14:19:40	
PB169317BS	S	Phenolics-	P	1.0142	mg/l	8/20/2025 14:19:41	
Q2893-07	S	Phenolics-	P	0.0261	mg/l	8/20/2025 14:19:44	
Q2893-08	S	Phenolics-	P	0.05	mg/l	8/20/2025 14:19:45	
CCV2	S	Phenolics-	P	0.986	mg/l	8/20/2025 14:24:29	
CCB2	S	Phenolics-	P	0.0016	mg/l	8/20/2025 14:24:32	

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

8/20/2025 13:44

Test Phenolics-


Accepted 8/20/2025 13:44

Factor 10.07

Bias 0.008

Coeff. of det. 0.999887

Errors

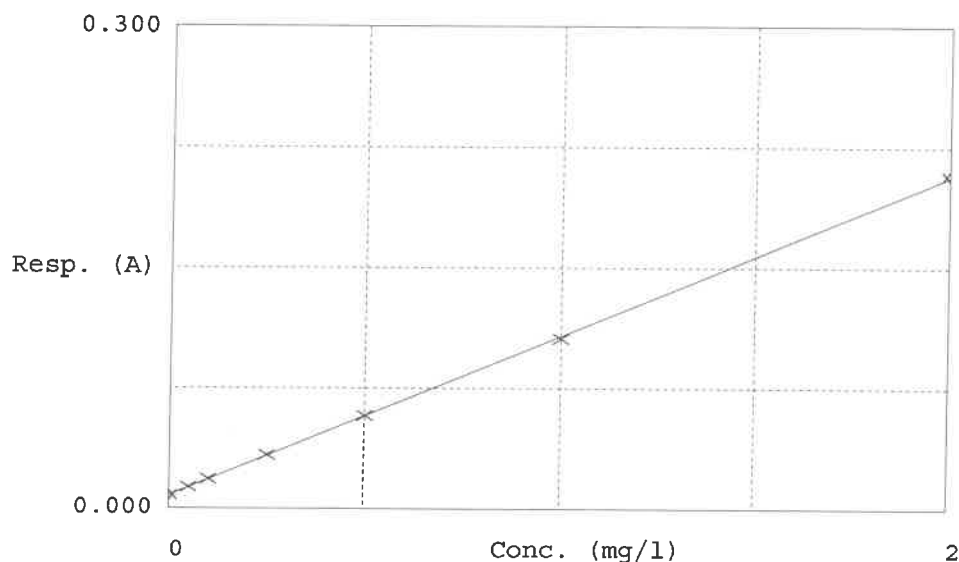

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.00PPM	0.008	-0.0004	0.0000	-
2	Phenol-2	0.013	0.0524	0.0500	4.8
3	Phenol-2	0.018	0.1032	0.1000	3.2
4	Phenol-2	0.033	0.2535	0.2500	1.4
5	Phenol-2	0.058	0.5003	0.5000	0.1
6	Phenol-2	0.106	0.9835	1.0000	-1.7
7	Phenol-2	0.208	2.0075	2.0000	0.4

08/20/2025
RM