


LB137049 INSTRUMENT ID :CV1

Method: 7470A		Operator: Admin		Date of Analysis: 03 Sep 2025 10:12:44					
Type	Sample ID	Extended ID	Conc.	µ Abs.	Units	Type	Std Conc	Method	Date
S	0.0 - 1	5.0	-	-192	PPB	Std	0.0000	7470A	03 Sep 2025 10:24:33
S	0.2 - 1	5.0.2	-	717	PPB	Std	0.2000	7470A	03 Sep 2025 10:26:51
S	2.5 - 1	5.2.5	-	11263	PPB	Std	2.5000	7470A	03 Sep 2025 10:29:08
S	5.0 - 1	5.5.0	-	21510	PPB	Std	5.0000	7470A	03 Sep 2025 10:31:25
S	7.5 - 1	5.7.5	-	33940	PPB	Std	7.5000	7470A	03 Sep 2025 10:33:41
S	10.0 - 1	5.10.0	-	43857	PPB	Std	10.0000	7470A	03 Sep 2025 10:35:57
U	ICV18 - 1	ICV18	3.7573	16551	PPB	SMPL	-7470A		03 Sep 2025 10:39:01
U	ICB18 - 1	ICB18	0.0098	-83	PPB	SMPL	-7470A		03 Sep 2025 10:41:16
U	CCV52 - 1	CCV52	4.8948	21600	PPB	SMPL	-7470A		03 Sep 2025 10:43:31
U	CCB52 - 1	CCB52	0.0071	-95	PPB	SMPL	-7470A		03 Sep 2025 10:45:45
U	CRA - 1	CRA	0.2249	872	PPB	SMPL	-7470A		03 Sep 2025 10:53:50
U	HighStd - 1	HighStd	9.8529	43607	PPB	SMPL	-7470A		03 Sep 2025 10:56:05
U	ChkStd - 1	ChkStd	7.4538	32958	PPB	SMPL	-7470A		03 Sep 2025 10:58:20
U	PB169512BL - 1	PBW	0.0445	71	PPB	SMPL	-7470A		03 Sep 2025 11:00:37
U	PB169512BS - 1	LCSW	4.4938	19820	PPB	SMPL	-7470A		03 Sep 2025 11:02:55
U	Q2991-02 - 1	309	0.0460	78	PPB	SMPL	-7470A		03 Sep 2025 11:05:11
U	Q2995-02 - 1	RT5427	0.0990	313	PPB	SMPL	-7470A		03 Sep 2025 11:07:28
U	Q2996-02 - 1	CONTAINMENT-A	0.1062	345	PPB	SMPL	-7470A		03 Sep 2025 11:09:45
U	Q2996-04 - 1	CONTAINMENT-B	0.1308	454	PPB	SMPL	-7470A		03 Sep 2025 11:12:11
U	Q2996-06 - 1	CONTAINMENT-C	0.1513	545	PPB	SMPL	-7470A		03 Sep 2025 11:14:34
U	CCV53 - 1	CCV53	4.7741	21064	PPB	SMPL	-7470A		03 Sep 2025 11:16:50
U	CCB53 - 1	CCB53	0.0093	-85	PPB	SMPL	-7470A		03 Sep 2025 11:19:05
U	Q2996-06DUP - 1	CONTAINMENT-CDUP	0.1407	498	PPB	SMPL	-7470A		03 Sep 2025 11:21:21
U	Q2996-06MS - 1	CONTAINMENT-CMS	4.4305	19539	PPB	SMPL	-7470A		03 Sep 2025 11:23:37
U	Q2996-06MSD - 1	CONTAINMENT-CMSD	3.9675	17484	PPB	SMPL	-7470A		03 Sep 2025 11:25:53
U	PB169513BL - 1	PBW	0.0749	206	PPB	SMPL	-7470A		03 Sep 2025 11:28:09
U	PB169513BS - 1	LCSW	4.6396	20467	PPB	SMPL	-7470A		03 Sep 2025 11:30:25
U	Q2990-01 - 1	310	0.3060	1232	PPB	SMPL	-7470A		03 Sep 2025 11:32:41
U	Q2990-02 - 1	308	0.3750	1538	PPB	SMPL	-7470A		03 Sep 2025 11:34:58
U	Q2990-02DUP - 1	308DUP	0.4198	1737	PPB	SMPL	-7470A		03 Sep 2025 11:37:15
U	Q2990-02MS - 1	308MS	3.9689	17490	PPB	SMPL	-7470A		03 Sep 2025 11:39:33
U	Q2990-02MSD - 1	308MSD	3.8981	17176	PPB	SMPL	-7470A		03 Sep 2025 11:44:42
U	CCV54 - 1	CCV54	4.6574	20546	PPB	SMPL	-7470A		03 Sep 2025 11:53:16
U	CCB54 - 1	CCB54	-0.0175	-204	PPB	SMPL	-7470A		03 Sep 2025 11:55:31
U	Q2996-06LX5 - 1		0.0733	199	PPB	SMPL	-7470A		03 Sep 2025 11:57:54
U	Q2996-06A - 1		3.5280	15533	PPB	SMPL	-7470A		03 Sep 2025 12:00:09
U	Q2990-02LX5 - 1		0.0780	220	PPB	SMPL	-7470A		03 Sep 2025 12:12:47
U	Q2990-02A - 1		3.1889	14028	PPB	SMPL	-7470A		03 Sep 2025 12:17:44
U	PB169428TB - 1	PB169428TB	-0.0010	-131	PPB	SMPL	-7470A		03 Sep 2025 12:22:46
U	CCV55 - 1	CCV55	4.6443	20488	PPB	SMPL	-7470A		03 Sep 2025 12:25:02
U	CCB55 - 1	CCB55	-0.0360	-286	PPB	SMPL	-7470A		03 Sep 2025 12:27:18

LB137049
INSTRUMENT ID: CV1

7470A

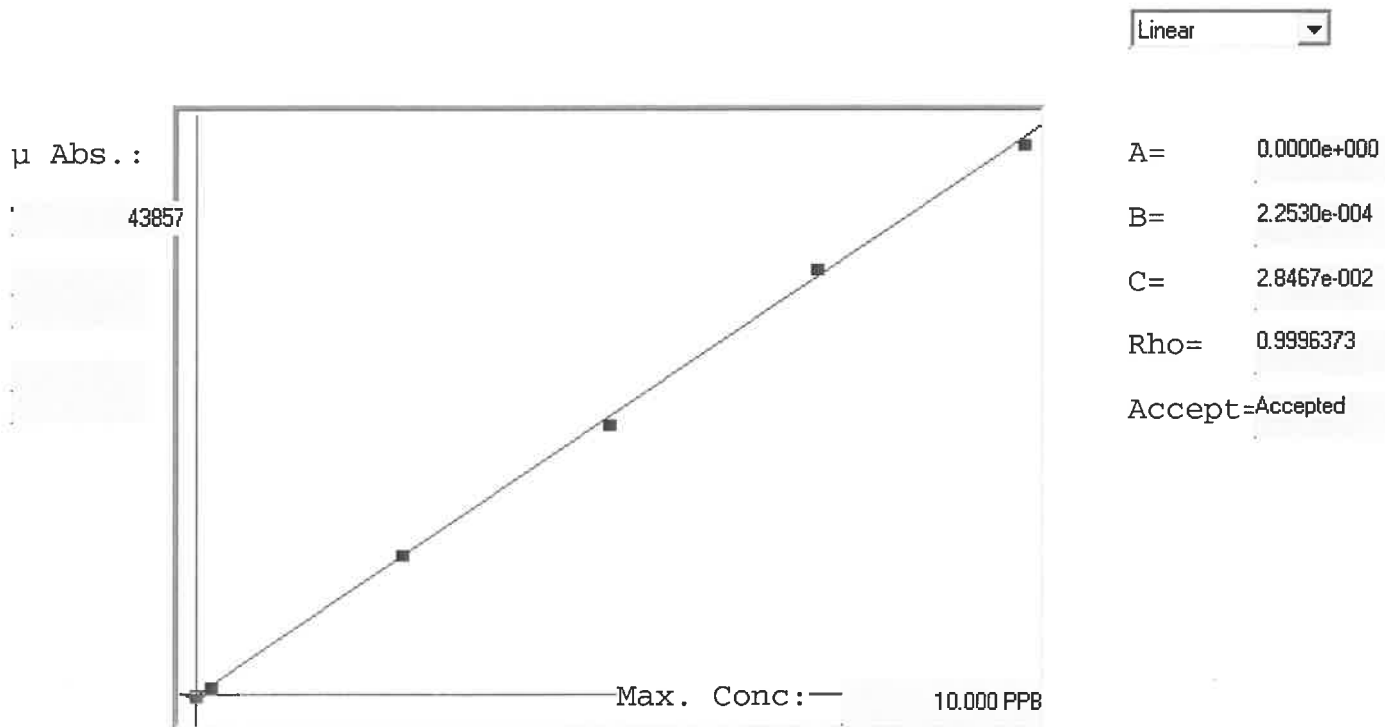

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.0	0.000	-0.015	-0.015	-192	0.000	-192	0				-5
0.2	0.200	0.190	-0.010	717	0.0 %	717	0				3
2.5	2.500	2.566	0.066	11263	0.0 %	11263	0				-3
5.0	5.000	4.875	-0.125	21510	0.0 %	21510					2
7.5	7.500	7.675	0.175	33940	0.0 %	33940					-1
10.0	10.000	9.909	-0.091	43857	0.0 %	43857					