

LB137054 INSTRUMENT ID :CV1

Method: 7471B

Operator: Admin

Date of Analysis: 03 Sep 2025 12:52:44


Type	Sample ID	Extended ID	Conc.	µ Abs.	Units	Type	Std Conc	Method	Date
S	0.0 - 1	50	-	125	PPB	Std	0.0000	7471B	03 Sep 2025 13:02:11
S	0.2 - 1	50.2	-	1109	PPB	Std	0.2000	7471B	03 Sep 2025 13:04:37
S	2.5 - 1	52.5	-	11749	PPB	Std	2.5000	7471B	03 Sep 2025 13:06:55
S	5.0 - 1	550	-	25690	PPB	Std	5.0000	7471B	03 Sep 2025 13:09:12
S	7.5 - 1	57.5	-	37561	PPB	Std	7.5000	7471B	03 Sep 2025 13:11:29
S	10.0 - 1	510.0	-	49787	PPB	Std	10.0000	7471B	03 Sep 2025 13:13:47
U	ICV19 - 1	ICV19	3.9165	19586	PPB	SMPL	-7471B		03 Sep 2025 13:16:35
U	ICB19 - 1	ICB19	-0.0163	-81	PPB	SMPL	-7471B		03 Sep 2025 13:18:52
U	CCV55 - 1	CCV55	5.1730	25869	PPB	SMPL	-7471B		03 Sep 2025 13:21:09
U	CCB55 - 1	CCB55	-0.0121	-60	PPB	SMPL	-7471B		03 Sep 2025 13:23:24
U	CRA - 1	CRA	0.2167	1084	PPB	SMPL	-7471B		03 Sep 2025 13:25:41
U	HighStd - 1	HighStd	10.1425	50720	PPB	SMPL	-7471B		03 Sep 2025 13:27:57
U	ChkStd - 1	ChkStd	7.4778	37395	PPB	SMPL	-7471B		03 Sep 2025 13:30:12
U	PB169525BL - 1	PB169525BL	-0.0847	-423	PPB	SMPL	-7471B		03 Sep 2025 13:32:31
U	PB169525BS - 1	PB169525BS	4.6976	23492	PPB	SMPL	-7471B		03 Sep 2025 13:40:12
U	Q2989-01 - 1	SOUTH-TP-5	0.2970	1486	PPB	SMPL	-7471B		03 Sep 2025 13:42:28
U	Q2989-03 - 1	SOUTH-TP-6	0.2680	1341	PPB	SMPL	-7471B		03 Sep 2025 13:44:47
U	Q2991-01 - 1	309	0.0897	449	PPB	SMPL	-7471B		03 Sep 2025 13:47:05
U	Q2994-01 - 1	PAULDING-WC1	11.6305	58161	PPB	SMPL	-7471B		03 Sep 2025 13:49:24
U	Q2995-01 - 1	RT5427	0.0401	201	PPB	SMPL	-7471B		03 Sep 2025 13:51:39
U	CCV56 - 1	CCV56	5.0288	25148	PPB	SMPL	-7471B		03 Sep 2025 13:53:57
U	CCB56 - 1	CCB56	-0.0377	-188	PPB	SMPL	-7471B		03 Sep 2025 13:56:12
U	Q2995-01DUP - 1	RT5427DUP	0.1069	535	PPB	SMPL	-7471B		03 Sep 2025 13:58:29
U	Q2995-01MS - 1	RT5427MS	4.7268	23638	PPB	SMPL	-7471B		03 Sep 2025 14:00:44
U	Q2995-01MSD - 1	RT5427MSD	4.7562	23785	PPB	SMPL	-7471B		03 Sep 2025 14:03:00
U	Q2996-01 - 1	CONTAINMENT-A	-0.0291	-145	PPB	SMPL	-7471B		03 Sep 2025 14:05:18
U	Q2996-03 - 1	CONTAINMENT-B	0.0527	264	PPB	SMPL	-7471B		03 Sep 2025 14:07:36
U	Q2996-05 - 1	CONTAINMENT-C	0.0275	138	PPB	SMPL	-7471B		03 Sep 2025 14:09:53
U	Q2997-01 - 1	EO-01-082925	0.3802	1902	PPB	SMPL	-7471B		03 Sep 2025 14:12:09
U	Q2998-01 - 1	AU-05-082925	1.2783	6393	PPB	SMPL	-7471B		03 Sep 2025 14:14:26
U	Q3003-01 - 1	VNJ-231	0.5516	2759	PPB	SMPL	-7471B		03 Sep 2025 14:16:44
U	Q2995-01LX5 - 1		-0.0007	-3	PPB	SMPL	-7471B		03 Sep 2025 14:19:00
U	CCV57 - 1	CCV57	5.1026	25517	PPB	SMPL	-7471B		03 Sep 2025 14:21:16
U	CCB57 - 1	CCB57	-0.0353	-176	PPB	SMPL	-7471B		03 Sep 2025 14:23:31
U	Q2995-01A - 1		4.0013	20010	PPB	SMPL	-7471B		03 Sep 2025 14:25:48
U	Q2994-01DLX5 - 1		6.0162	30086	PPB	SMPL	-7471B		03 Sep 2025 14:28:03
U	CCV58 - 1	CCV58	5.0974	25491	PPB	SMPL	-7471B		03 Sep 2025 14:30:54
U	CCB58 - 1	CCB58	-0.0289	-144	PPB	SMPL	-7471B		03 Sep 2025 14:33:11

LB137054
INSTRUMENT ID: CV1

7471B

μ Abs. :

49787

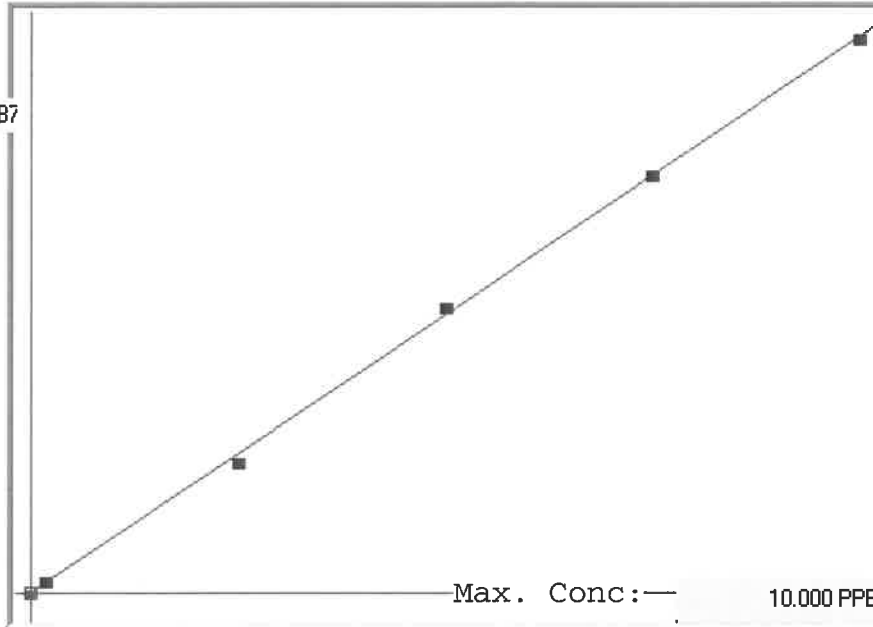

Linear

A= 0.0000e+000

B= 1.9997e-004

C= -1.1447e-004

Rho= 0.9997266

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	% D
0.0	0.000	0.025	0.025	125	0.000	125					
0.2	0.200	0.222	0.022	1109	0.0 %	1109					
2.5	2.500	2.349	-0.151	11749	0.0 %	11749					
5.0	5.000	5.137	0.137	25690	0.0 %	25690					
7.5	7.500	7.511	0.011	37561	0.0 %	37561					
10.0	10.000	9.956	-0.044	49787	0.0 %	49787					

0.0000