

66137059

Test results

Aquakem 7.2AQ1

Page: 1

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

9/3/2025 13:53

Reviewed by : RM

Instrument ID : Konelab

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	96.092	0.0	0.090	
ICB001 ICB001	1.447	0.0	0.001	
CCV001 CCV001	243.037	0.0	0.227	
CCB001 CCB001	1.674	0.0	0.002	
PB169536BL PBW536	1.576	0.0	0.002	
02099-01-MDL-WATER-QT3-2025-05	5.243	0.0	0.005	
PB169535BL PBS535	1.138	0.0	0.001	
02099-03-MDL-SOIL-QT3-2025-05	5.206	0.0	0.005	
CCV002 CCV002	246.409	0.0	0.231	
09/03/2025 RM CCB002 CCB002	1.321	0.0	0.001	
N	10			
Mean	60.314			
SD	101.4915			
CV%	168.27			

Aquakem v. 7.2AQ1

Results from time period:

Wed Sep 03 13:06:53 2025

Wed Sep 03 13:47:38 2025

Sample Id	Sam	Test short r	Test Result	Result unit	Result date and time
S0.0	A	CNEPA-NE\ P	1.0219	µg/l	9/3/2025 13:06:53
S5.0	A	CNEPA-NE\ P	5.1709	µg/l	9/3/2025 13:06:54
S10.0	A	CNEPA-NE\ P	10.2732	µg/l	9/3/2025 13:06:55
S100.0	A	CNEPA-NE\ P	98.7936	µg/l	9/3/2025 13:06:56
S250.0	A	CNEPA-NE\ P	249.0126	µg/l	9/3/2025 13:06:57
S500.0	A	CNEPA-NE\ P	500.7278	µg/l	9/3/2025 13:06:58
ICV001 ICV001	S	CNEPA-NE\ P	96.0917	µg/l	9/3/2025 13:40:52
ICB001 ICB001	S	CNEPA-NE\ P	1.4474	µg/l	9/3/2025 13:40:53
CCV001 CCV001	S	CNEPA-NE\ P	243.0368	µg/l	9/3/2025 13:40:55
CCB001 CCB001	S	CNEPA-NE\ P	1.6738	µg/l	9/3/2025 13:40:58
PB169536BL PBW536	S	CNEPA-NE\ P	1.5759	µg/l	9/3/2025 13:41:00
Q2899-01-MDL-WATER-QT3-2025-05	S	CNEPA-NE\ P	5.2427	µg/l	9/3/2025 13:41:01
PB169535BL PBS535	S	CNEPA-NE\ P	1.138	µg/l	9/3/2025 13:47:31
Q2899-03-MDL-SOIL-QT3-2025-05	S	CNEPA-NE\ P	5.2062	µg/l	9/3/2025 13:47:33
CCV002 CCV002	S	CNEPA-NE\ P	246.4088	µg/l	9/3/2025 13:47:36
CCB002 CCB002	S	CNEPA-NE\ P	1.3215	µg/l	9/3/2025 13:47:38

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RH

Instrument ID : Konelab

9/3/2025 13:07

Test CNEPA-NEW

Accepted

9/3/2025 13:07

~~Factor~~ Slope

10690.000936

Bias y-intercept.


0

09/04/2025
RM

Coeff. of det.

0.999979

Errors

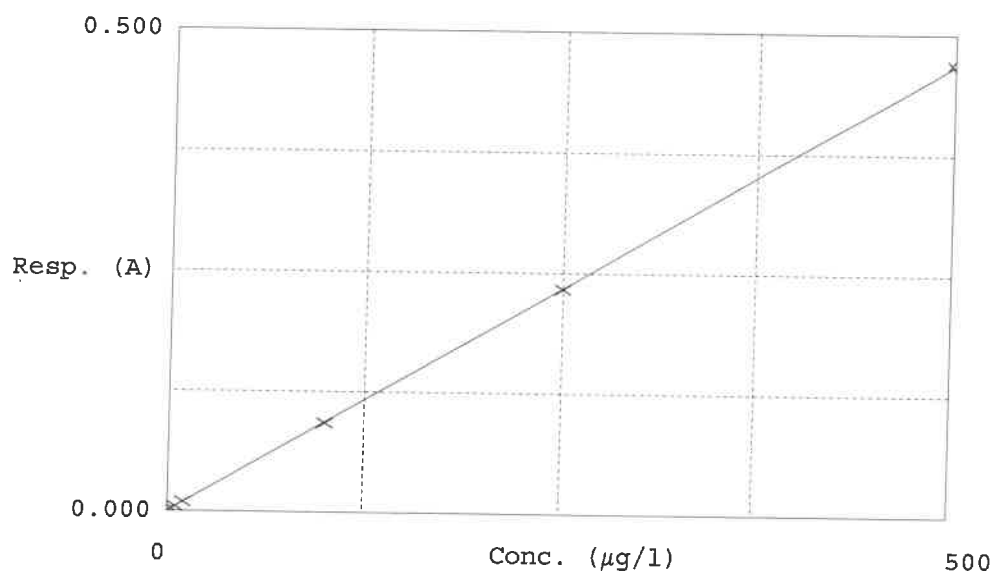

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCNS0.0	0.001	1.0219	0.0000	-
2	5.0PPBCNS5.0	0.005	5.1709	5.0000	3.4
3	10PPBCNS10.0	0.010	10.2732	10.0000	2.7
4	100PPBCNS100.0	0.092	98.7936	100.0000	-1.2
5	250PPBCNS250.0	0.233	249.0126	250.0000	-0.4
6	500PPBCNS500.0	0.469	500.7278	500.0000	0.1

09/03/2025
RM