


Ident	Instrument IC-1			Analyst: RM		Method: 300.0 / 9056A		Initial w Analyst		
	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4			
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/6/2025 10:18	10 RM/IZ
STD2	0.413	0.620	0.623	2.052	0.515	1.033	3.185	IC1-080625	8/6/2025 10:40	10 RM/IZ
STD3	0.794	1.184	1.185	3.953	0.990	2.067	5.931	IC1-080625	8/6/2025 11:01	10 RM/IZ
STD4	1.023	1.524	1.519	5.070	1.270	2.633	7.597	IC1-080625	8/6/2025 11:23	10 RM/IZ
STD5	1.972	2.981	2.982	9.960	2.483	4.695	14.838	IC1-080625	8/6/2025 11:44	10 RM/IZ
STD6	3.956	5.938	5.934	19.801	4.945	9.953	29.505	IC1-080625	8/6/2025 12:06	10 RM/IZ
STD7	5.041	7.553	7.556	25.165	6.298	12.620	37.443	IC1-080625	8/6/2025 12:27	10 RM/IZ
ICV	2.038	3.184	3.095	10.343	2.641	4.970	15.425	IC1-080625	8/6/2025 12:48	10 RM/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	8/6/2025 13:10	10 RM/IZ
CCV	2.033	3.069	3.047	10.273	2.565	5.096	15.084	IC1-080625	9/4/2025 11:23	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	9/4/2025 11:45	10 RM/IZ
LB137075BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	9/4/2025 12:06	10 RM/IZ
LB137075BSW	2.040	3.069	3.052	10.274	2.570	5.215	15.236	IC1-080625	9/4/2025 12:28	10 RM/IZ
Q3022-01	0.289	286.053	0.000	0.200	0.000	0.443	43.366	IC1-080625	9/4/2025 14:57	10 RM/IZ
Q3022-01MS	2.329	275.661	3.109	11.180	2.620	4.706	58.107	IC1-080625	9/4/2025 15:18	10 RM/IZ
Q3022-01MSD	2.269	275.412	2.979	10.719	2.511	5.521	57.613	IC1-080625	9/4/2025 15:40	10 RM/IZ
CCV	2.026	3.071	3.064	10.823	2.565	5.279	15.247	IC1-080625	9/4/2025 16:01	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-080625	9/4/2025 16:23	10 RM/IZ

Clear table

Instrument ID: IC-2 Analyst: IZ Method: 300.0 / 9056A											
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentratio n HPO4	concentrati on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	IC1-080625	8/6/2025 10:18	10	RM/Z
STD2	0.4130	0.6200	0.6230	2.0520	0.5150	1.0330	3.1850	IC1-080625	8/6/2025 10:40	10	RM/Z
STD3	0.7940	1.1840	1.1850	3.9530	0.9900	2.0670	5.9310	IC1-080625	8/6/2025 11:01	10	RM/Z
STD4	1.0230	1.5240	1.5190	5.0700	1.2700	2.6330	7.5970	IC1-080625	8/6/2025 11:23	10	RM/Z
STD5	1.9720	2.9810	2.9820	9.9600	2.4830	4.6950	14.8380	IC1-080625	8/6/2025 11:44	10	RM/Z
STD6	3.9560	5.9380	5.9340	19.8010	4.9450	9.9530	29.5050	IC1-080625	8/6/2025 12:06	10	RM/Z
STD7	5.0410	7.5530	7.5560	25.1650	6.2980	12.6200	37.4430	IC1-080625	8/6/2025 12:27	10	RM/Z
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1											
STD2	3.2500	3.3333	3.8333	2.6000	3.0000	3.3000	6.1667				
STD3	-0.7500	-1.3333	-1.2500	-1.1750	-1.0000	3.3500	-1.1500				
STD4	2.3000	1.6000	1.2667	1.4000	1.6000	5.3200	1.2933				
STD5	-1.4000	-0.6333	-0.6000	-0.4000	-0.6800	-6.1000	-1.0800				
STD6	-1.1000	-1.0333	-1.1000	-0.9950	-1.1000	-0.4700	-1.6500				
STD7	0.8200	0.7067	0.7467	0.6600	0.7680	0.9600	1.1973				

Fluoride (Anions)

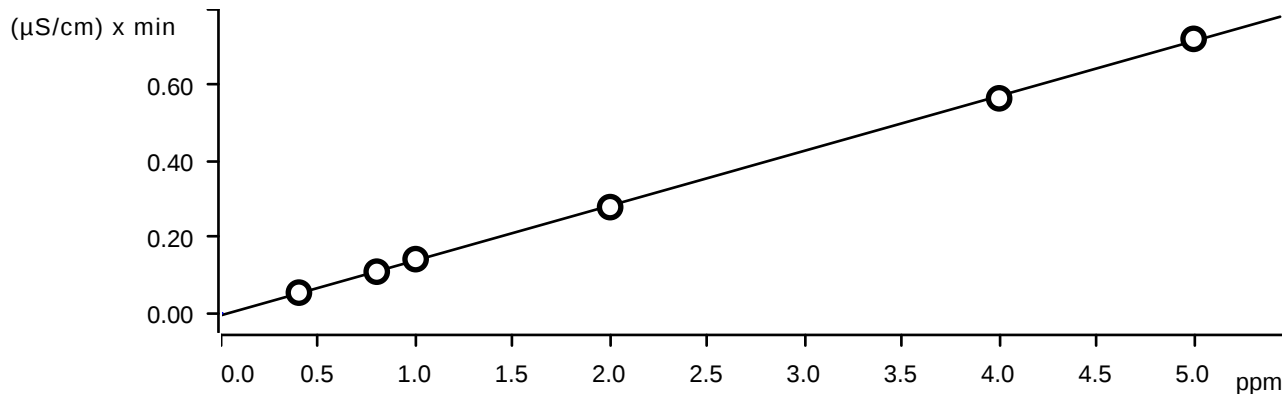


Function: $A = -5.18233\text{E-}3 + 0.0144368 \times Q$

Relative standard deviation 1.650446 %

Correlation coefficient 0.999856

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.400	10.0	1.0	1.0	0.054	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	0.800	10.0	1.0	1.0	0.110	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.000	10.0	1.0	1.0	0.143	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	2.000	10.0	1.0	1.0	0.280	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	4.000	10.0	1.0	1.0	0.566	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	5.000	10.0	1.0	1.0	0.723	STD7	2025-08-06 12:27:27 UTC-4	used

Chloride (Anions)

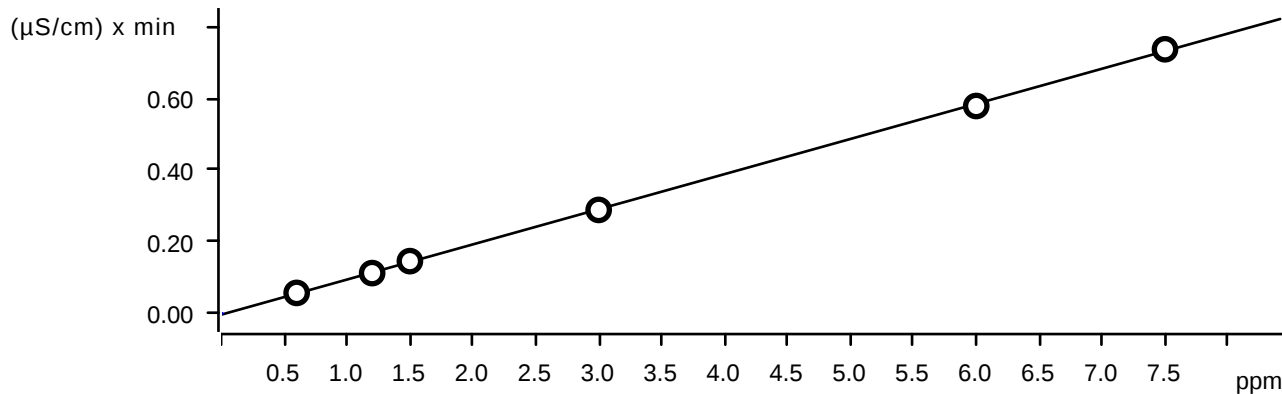

Function: $A = -3.45407\text{E-}3 + 9.79772\text{E-}3 \times Q$


Relative standard deviation 1.384132 %

Correlation coefficient 0.999898

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.057	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.113	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.146	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.289	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	0.578	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	0.737	STD7	2025-08-06 12:27:27 UTC-4	used

Nitrite (Anions)

(μS/cm) x min

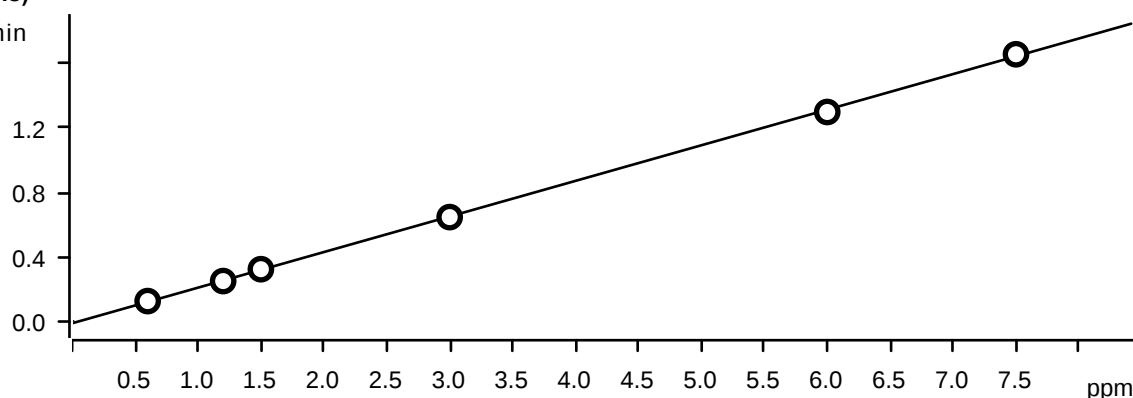
Function: $A = -0.0116303 + 0.0220561 \times Q$

Relative standard deviation 1.449488 %

Correlation coefficient 0.999889

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.600	10.0	1.0	1.0	0.126	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	1.200	10.0	1.0	1.0	0.250	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.500	10.0	1.0	1.0	0.323	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	3.000	10.0	1.0	1.0	0.646	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	6.000	10.0	1.0	1.0	1.297	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	7.500	10.0	1.0	1.0	1.655	STD7	2025-08-06 12:27:27 UTC-4	used


Bromide (Anions)

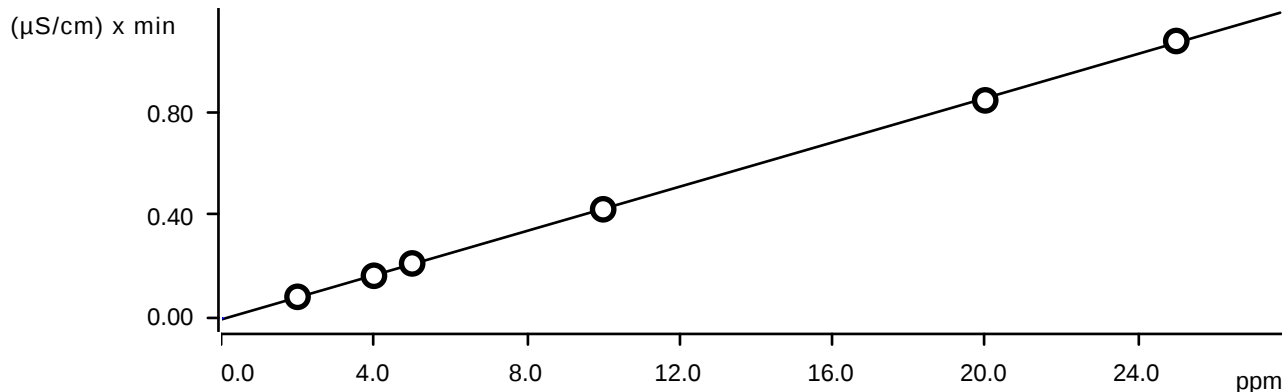

Function: $A = -4.59233\text{E-}3 + 4.28617\text{E-}3 \times Q$
 Relative standard deviation 1.283698 %
 Correlation coefficient 0.999912

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	2.000	10.0	1.0	1.0	0.083	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	4.000	10.0	1.0	1.0	0.165	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	5.000	10.0	1.0	1.0	0.213	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	10.000	10.0	1.0	1.0	0.422	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	20.000	10.0	1.0	1.0	0.844	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	25.000	10.0	1.0	1.0	1.074	STD7	2025-08-06 12:27:27 UTC-4	used


Nitrate (Anions)

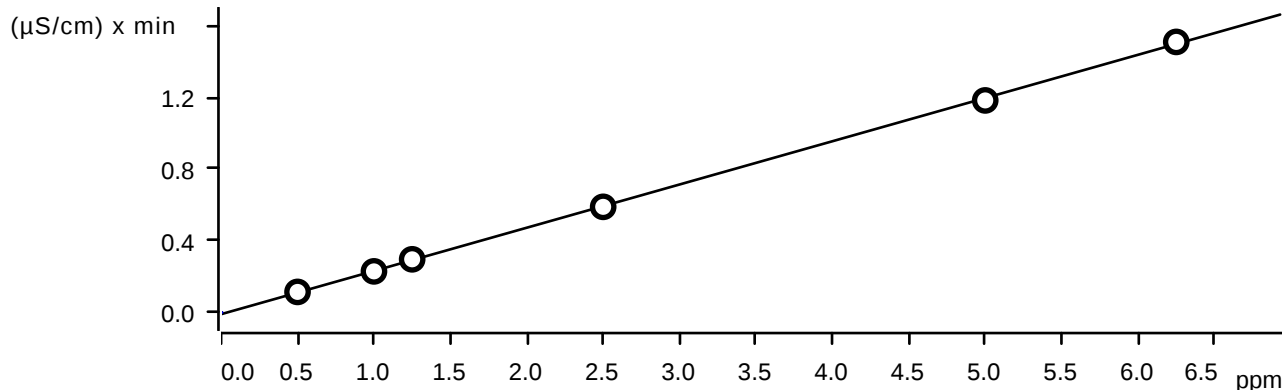

Function: $A = -9.68516\text{E-}3 + 0.0241085 \times Q$
 Relative standard deviation 1.469135 %

Correlation coefficient 0.999886


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	0.500	10.0	1.0	1.0	0.115	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	1.000	10.0	1.0	1.0	0.229	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	1.250	10.0	1.0	1.0	0.296	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	2.500	10.0	1.0	1.0	0.589	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	5.000	10.0	1.0	1.0	1.182	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	6.250	10.0	1.0	1.0	1.509	STD7	2025-08-06 12:27:27 UTC-4	used

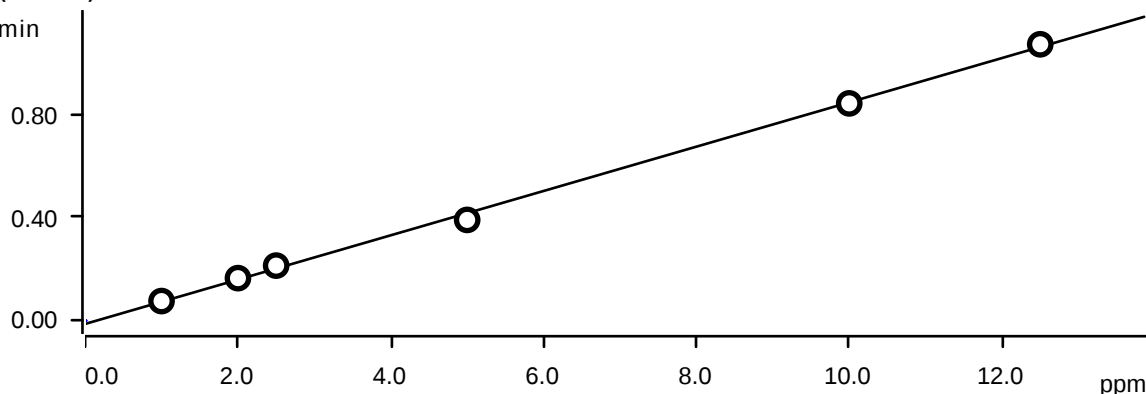Phosphate (Anions) $(\mu\text{S/cm}) \times \text{min}$ Function: $A = -0.0128563 + 8.58091E-3 \times Q$

Relative standard deviation 3.406332 %

Correlation coefficient 0.999402

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	1.000	10.0	1.0	1.0	0.076	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	2.000	10.0	1.0	1.0	0.164	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	2.500	10.0	1.0	1.0	0.213	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	5.000	10.0	1.0	1.0	0.390	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	10.000	10.0	1.0	1.0	0.841	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	12.500	10.0	1.0	1.0	1.070	STD7	2025-08-06 12:27:27 UTC-4	used

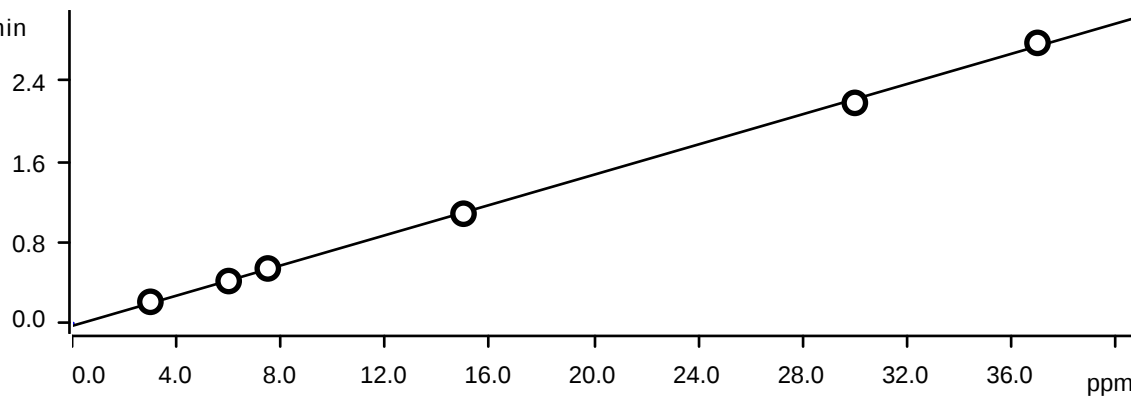Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0267558 + 7.49232E-3 \times Q$

Relative standard deviation 2.236460 %

Correlation coefficient 0.999736

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-08-06 10:18:54 UTC-4	used
Standard 2	1	3.000	10.0	1.0	1.0	0.212	STD2	2025-08-06 10:40:18 UTC-4	used
Standard 3	1	6.000	10.0	1.0	1.0	0.418	STD3	2025-08-06 11:01:42 UTC-4	used
Standard 4	1	7.500	10.0	1.0	1.0	0.542	STD4	2025-08-06 11:23:08 UTC-4	used
Standard 5	1	15.000	10.0	1.0	1.0	1.085	STD5	2025-08-06 11:44:33 UTC-4	used
Standard 6	1	30.000	10.0	1.0	1.0	2.184	STD6	2025-08-06 12:06:00 UTC-4	used
Standard 7	1	37.000	10.0	1.0	1.0	2.779	STD7	2025-08-06 12:27:27 UTC-4	used


Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-08-06 10:18:54 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.73 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

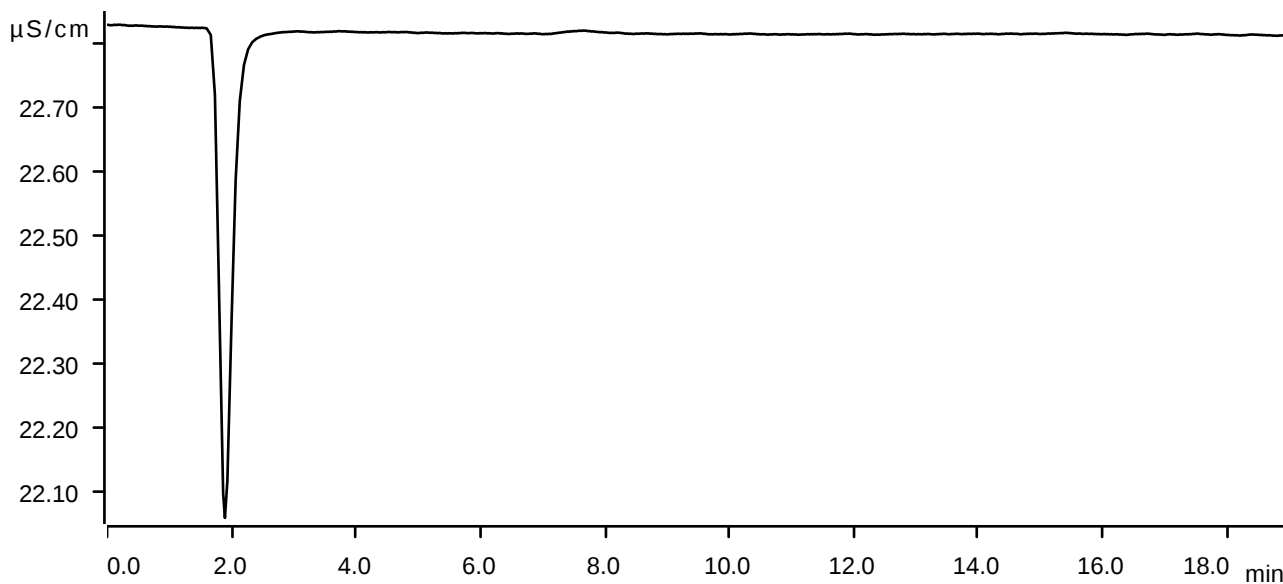


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-08-06 10:40:18 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.61 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

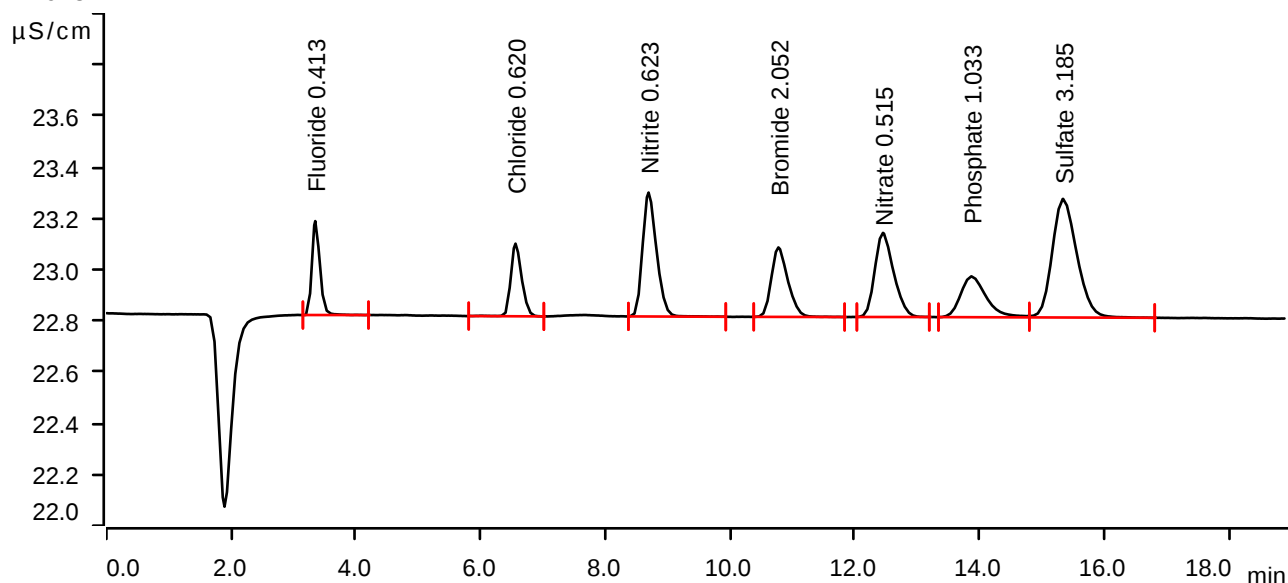

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.350	0.0544	0.367	0.413	Fluoride
2	6.560	0.0573	0.284	0.620	Chloride
3	8.693	0.1258	0.484	0.623	Nitrite
4	10.775	0.0833	0.271	2.052	Bromide
5	12.452	0.1145	0.328	0.515	Nitrate
6	13.870	0.0758	0.159	1.033	Phosphate
7	15.340	0.2119	0.463	3.185	Sulfate


Sample data

Ident STD3
 Sample type Standard 3
 Determination start 2025-08-06 11:01:42 UTC-4
 Method IC1-080625
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 12.61 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

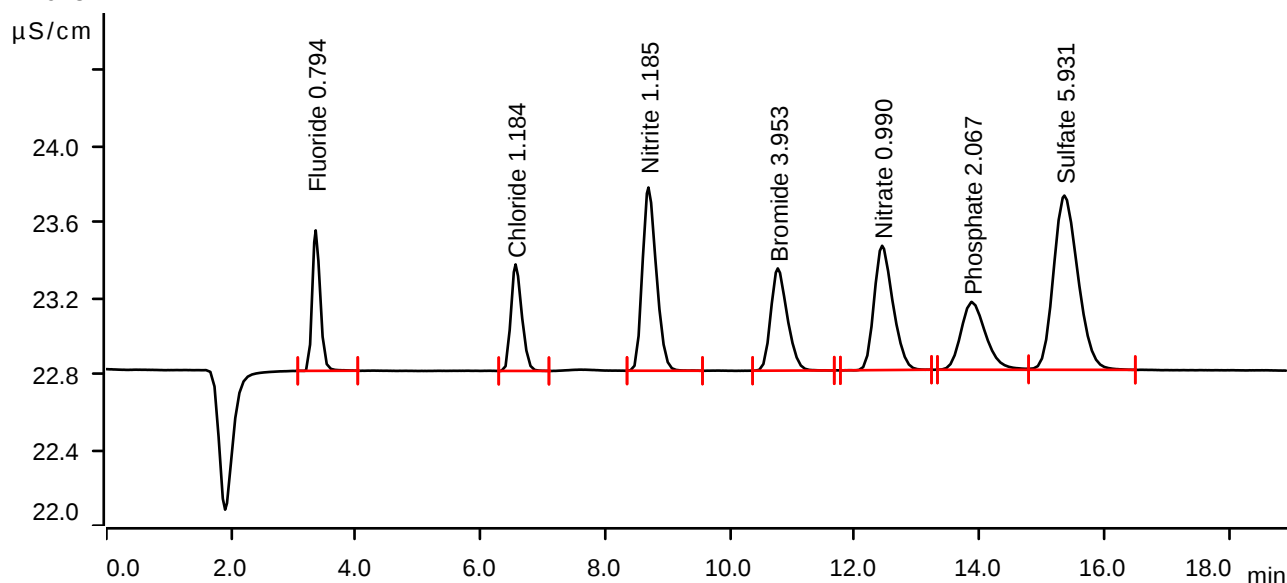

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.357	0.1095	0.740	0.794	Fluoride
2	6.562	0.1125	0.561	1.184	Chloride
3	8.692	0.2498	0.966	1.185	Nitrite
4	10.765	0.1649	0.539	3.953	Bromide
5	12.438	0.2291	0.655	0.990	Nitrate
6	13.875	0.1645	0.358	2.067	Phosphate
7	15.360	0.4176	0.918	5.931	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-08-06 11:23:08 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

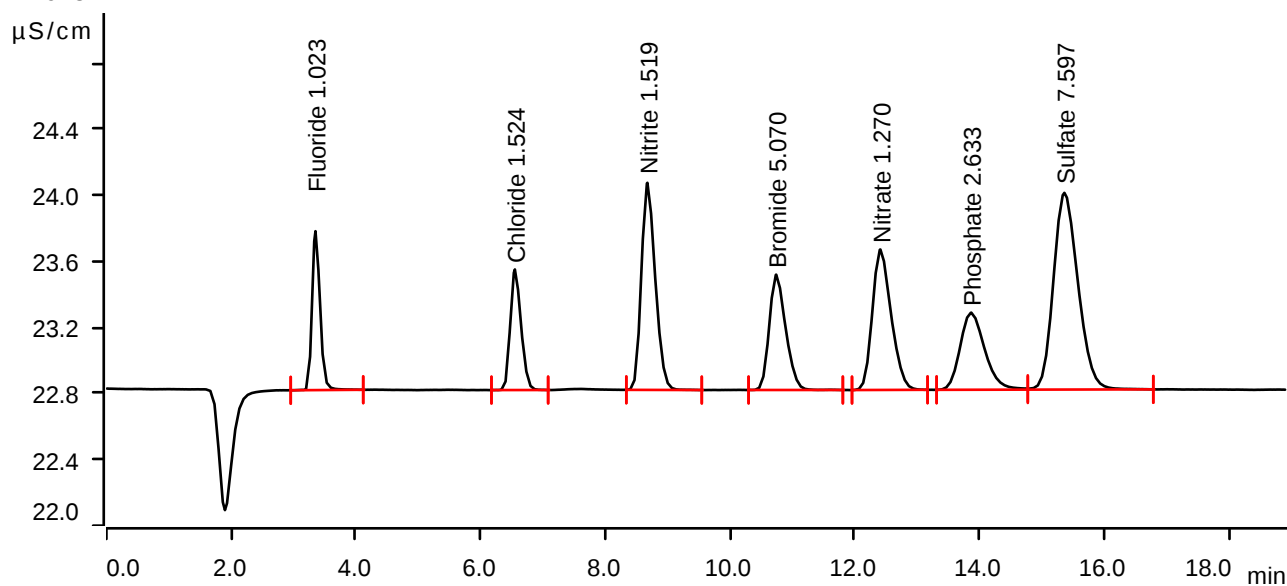

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.1425	0.962	1.023	Fluoride
2	6.552	0.1459	0.730	1.524	Chloride
3	8.675	0.3233	1.254	1.519	Nitrite
4	10.740	0.2127	0.698	5.070	Bromide
5	12.410	0.2964	0.850	1.270	Nitrate
6	13.862	0.2131	0.467	2.633	Phosphate
7	15.360	0.5424	1.191	7.597	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-08-06 11:44:33 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

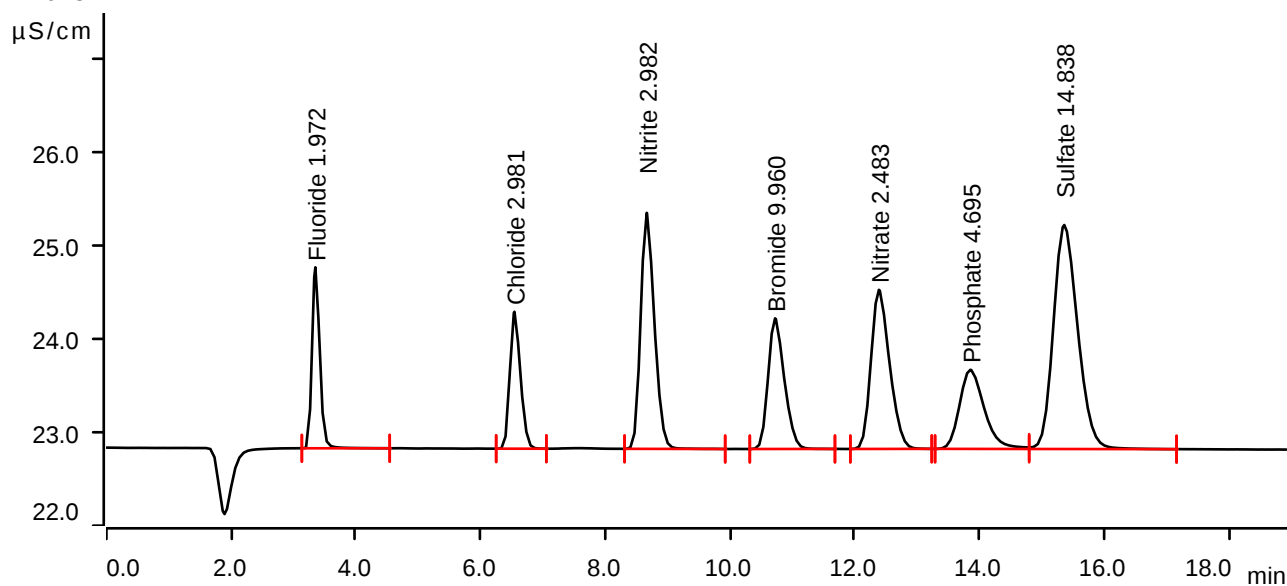

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.352	0.2796	1.943	1.972	Fluoride
2	6.543	0.2887	1.470	2.981	Chloride
3	8.663	0.6461	2.534	2.982	Nitrite
4	10.722	0.4223	1.403	9.960	Bromide
5	12.387	0.5889	1.709	2.483	Nitrate
6	13.853	0.3900	0.850	4.695	Phosphate
7	15.358	1.0850	2.405	14.838	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-08-06 12:06:00 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

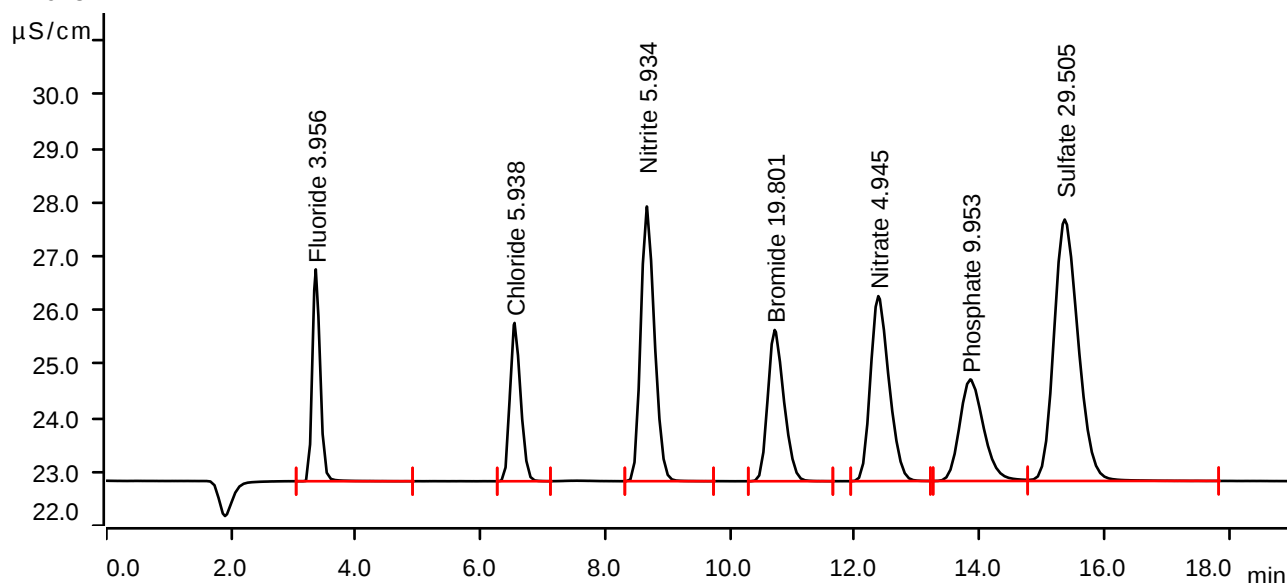

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.5660	3.928	3.956	Fluoride
2	6.545	0.5784	2.936	5.938	Chloride
3	8.665	1.2973	5.095	5.934	Nitrite
4	10.715	0.8441	2.805	19.801	Bromide
5	12.377	1.1824	3.431	4.945	Nitrate
6	13.852	0.8412	1.884	9.953	Phosphate
7	15.365	2.1839	4.849	29.505	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-08-06 12:27:27 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

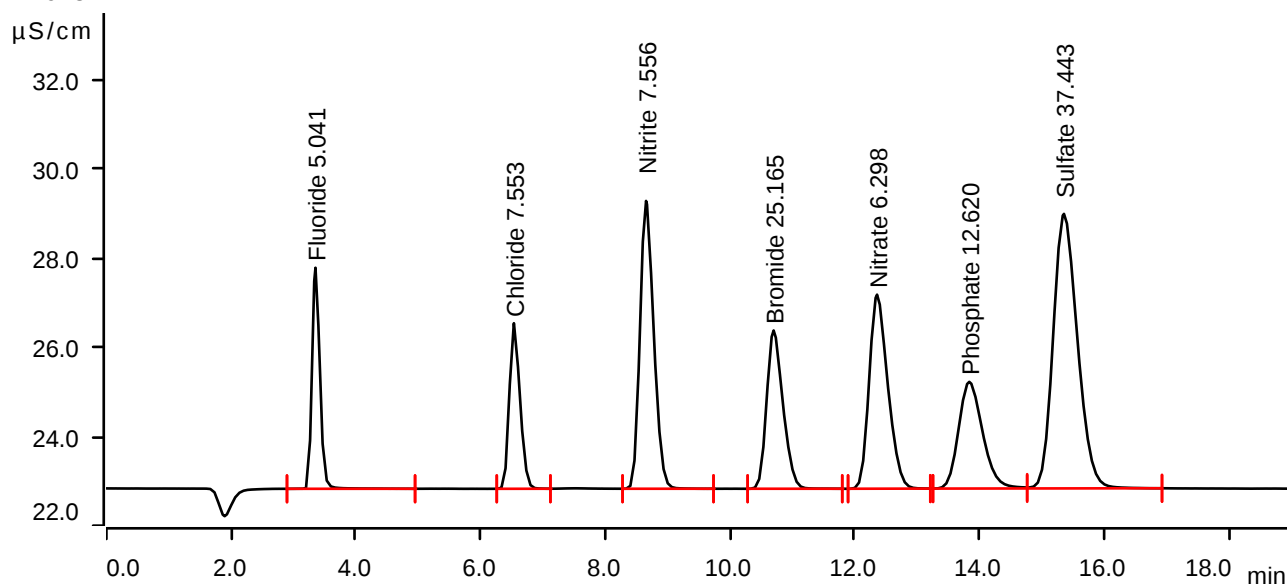

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.353	0.7226	4.963	5.041	Fluoride
2	6.535	0.7366	3.716	7.553	Chloride
3	8.653	1.6550	6.462	7.556	Nitrite
4	10.698	1.0740	3.554	25.165	Bromide
5	12.357	1.5086	4.357	6.298	Nitrate
6	13.835	1.0700	2.396	12.620	Phosphate
7	15.353	2.7786	6.163	37.443	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-08-06 12:48:56 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

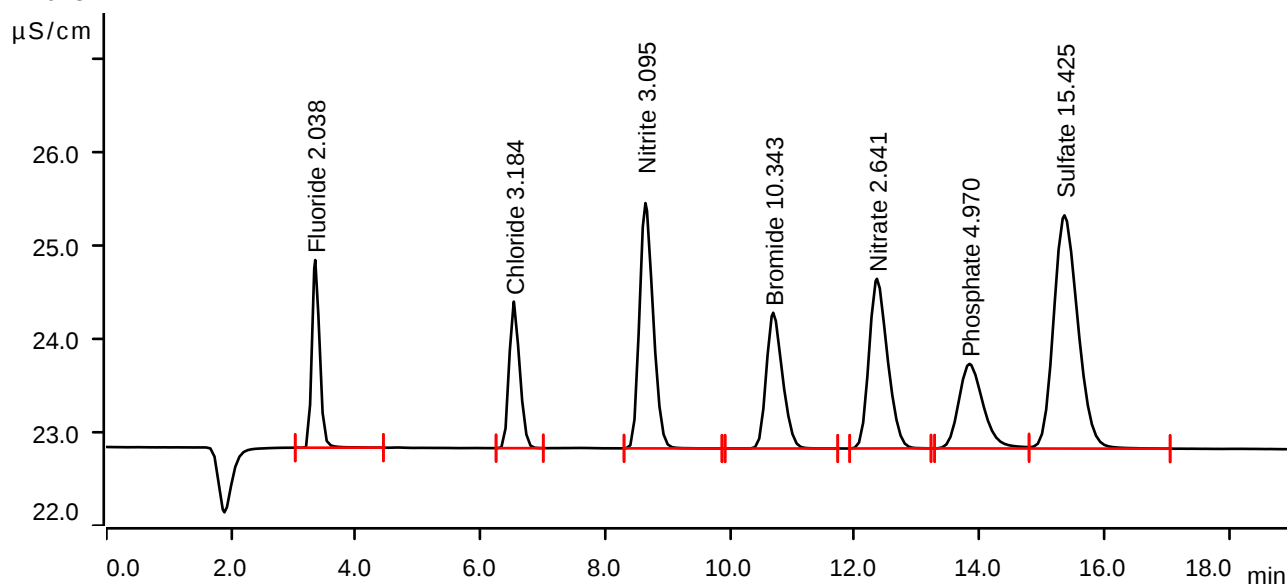


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.350	0.2890	2.015	2.038	Fluoride
2	6.532	0.3085	1.574	3.184	Chloride
3	8.643	0.6711	2.634	3.095	Nitrite
4	10.692	0.4387	1.458	10.343	Bromide
5	12.355	0.6270	1.822	2.641	Nitrate
6	13.838	0.4136	0.908	4.970	Phosphate
7	15.362	1.1289	2.504	15.425	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2025-08-06 13:10:25 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

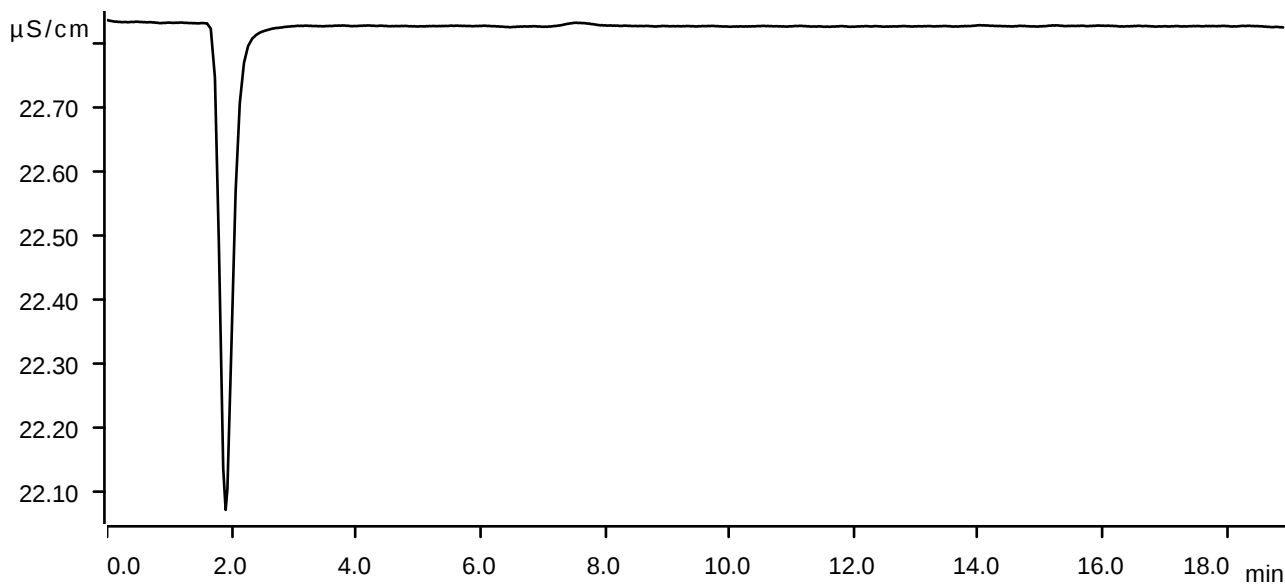Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-09-04 11:23:52 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.33 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

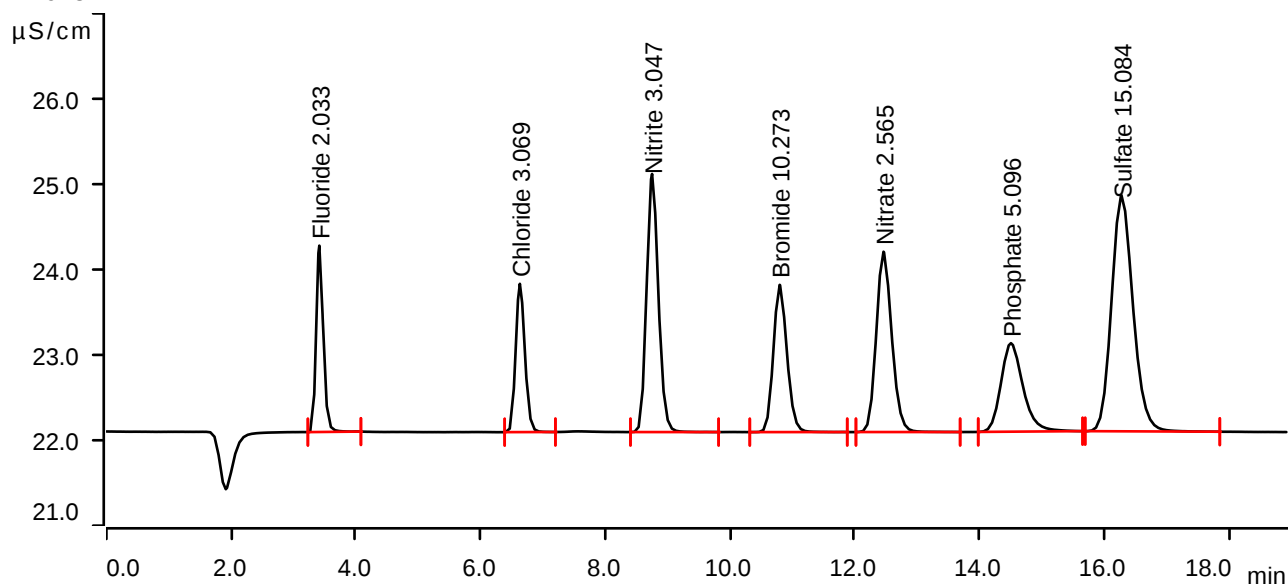


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.415	0.2883	2.183	2.033	Fluoride
2	6.630	0.2973	1.737	3.069	Chloride
3	8.750	0.6604	3.023	3.047	Nitrite
4	10.795	0.4357	1.725	10.273	Bromide
5	12.460	0.6087	2.112	2.565	Nitrate
6	14.503	0.4244	1.037	5.096	Phosphate
7	16.275	1.1034	2.765	15.084	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-09-04 11:45:22 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

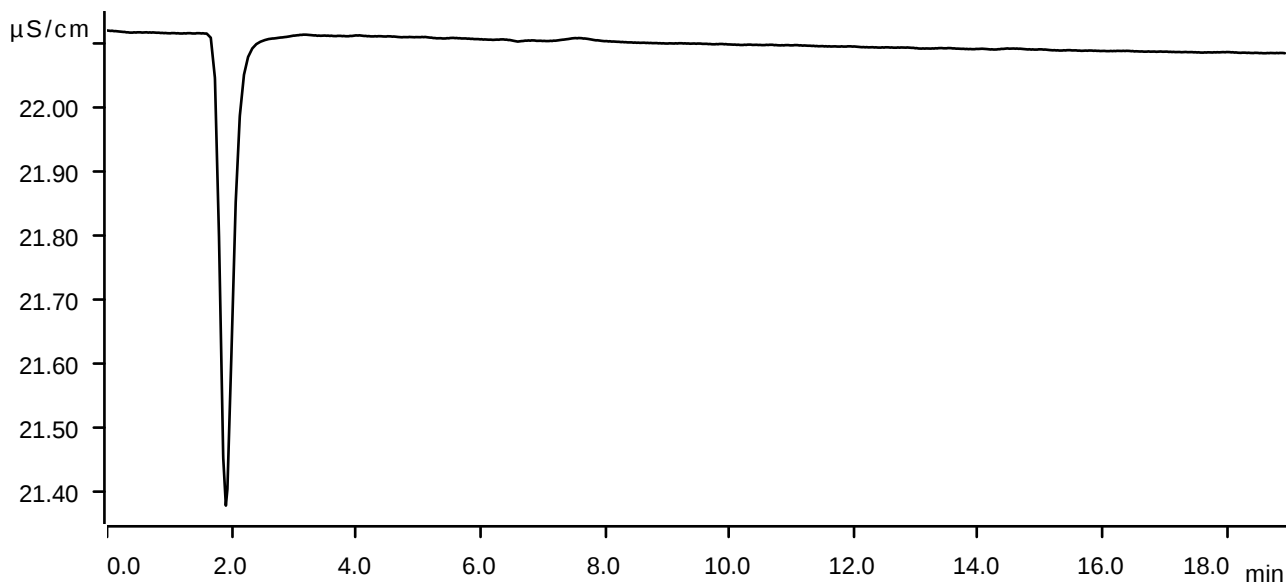
Anions

Sample data

Ident LB137075BLW
Sample type Sample
Determination start 2025-09-04 12:06:53 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

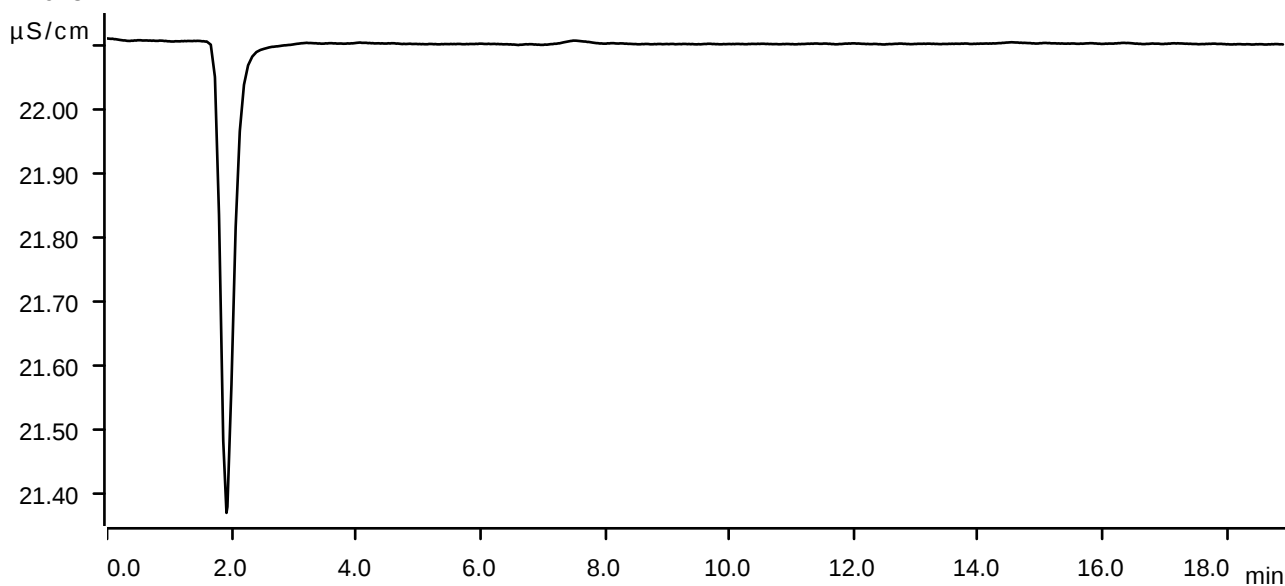Anions


Sample data

Ident LB137075BSW
 Sample type Check standard 1
 Determination start 2025-09-04 12:28:25 UTC-4
 Method IC1-080625
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 12.05 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

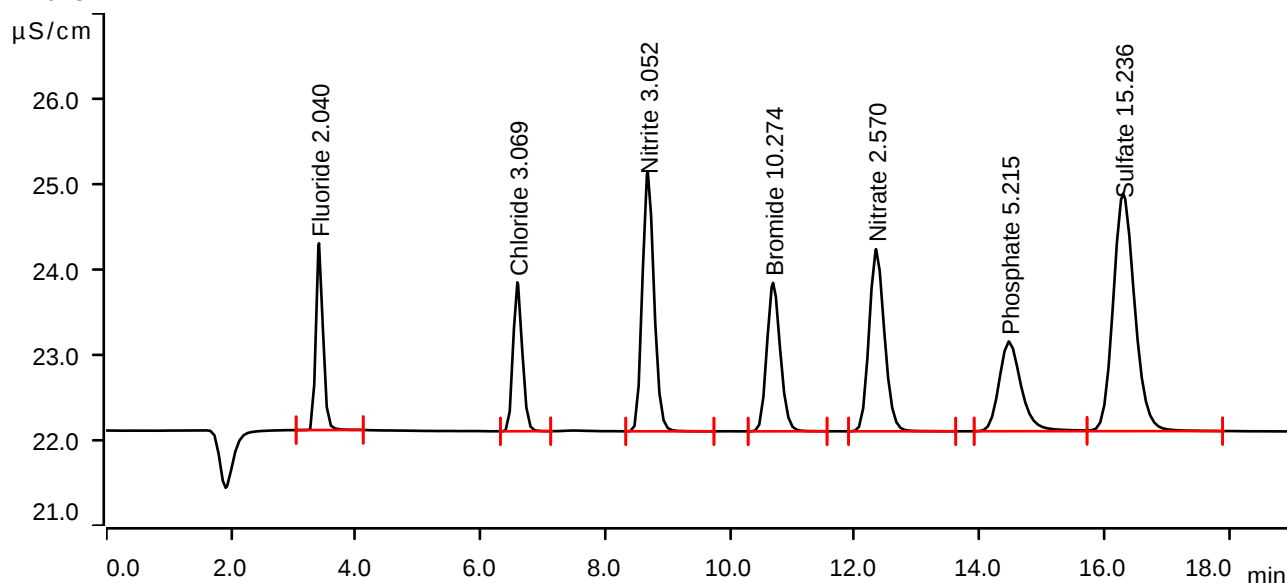

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.410	0.2893	2.187	2.040	Fluoride
2	6.590	0.2972	1.743	3.069	Chloride
3	8.680	0.6615	3.047	3.052	Nitrite
4	10.690	0.4358	1.739	10.274	Bromide
5	12.342	0.6099	2.133	2.570	Nitrate
6	14.472	0.4346	1.051	5.215	Phosphate
7	16.303	1.1148	2.782	15.236	Sulfate


Sample data

Ident Q3022-01
Sample type Sample
Determination start 2025-09-04 14:57:00 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

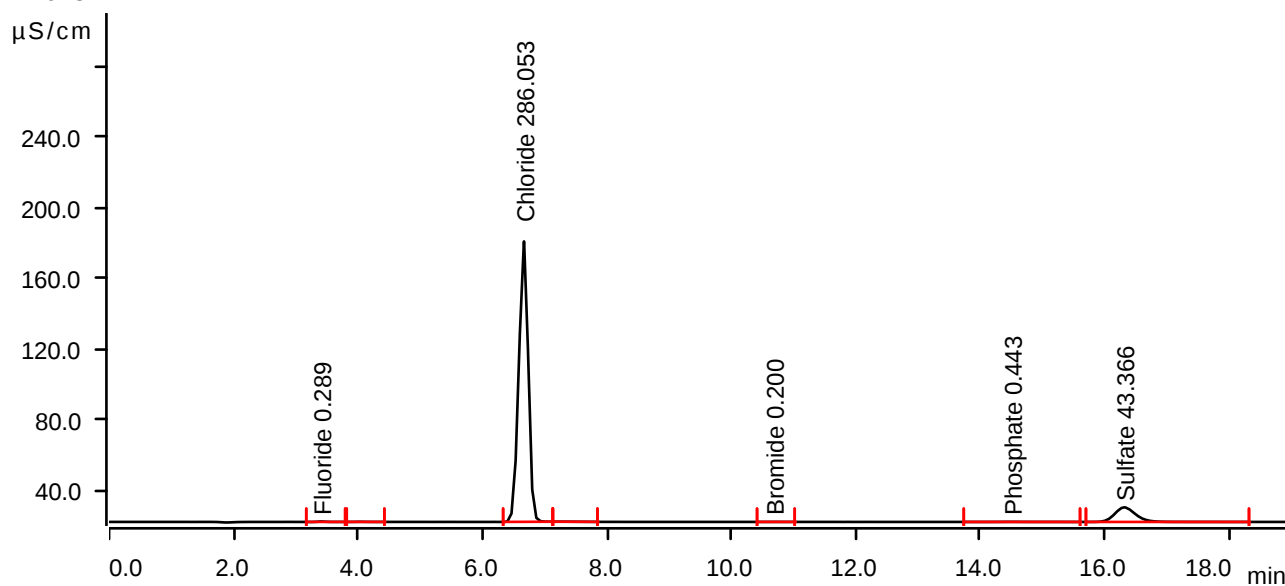

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.408	0.0366	0.267	0.289	Fluoride
2	4.032	0.0166	0.085	invalid	
3	6.670	28.0232	158.775	286.053	Chloride
4	7.313	0.0182	0.052	invalid	
5	10.685	0.0040	0.016	0.200	Bromide
6	14.507	0.0252	0.051	0.443	Phosphate
7	16.313	3.2223	8.265	43.366	Sulfate


Sample data

Ident Q3022-01MS
Sample type Sample
Determination start 2025-09-04 15:18:38 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

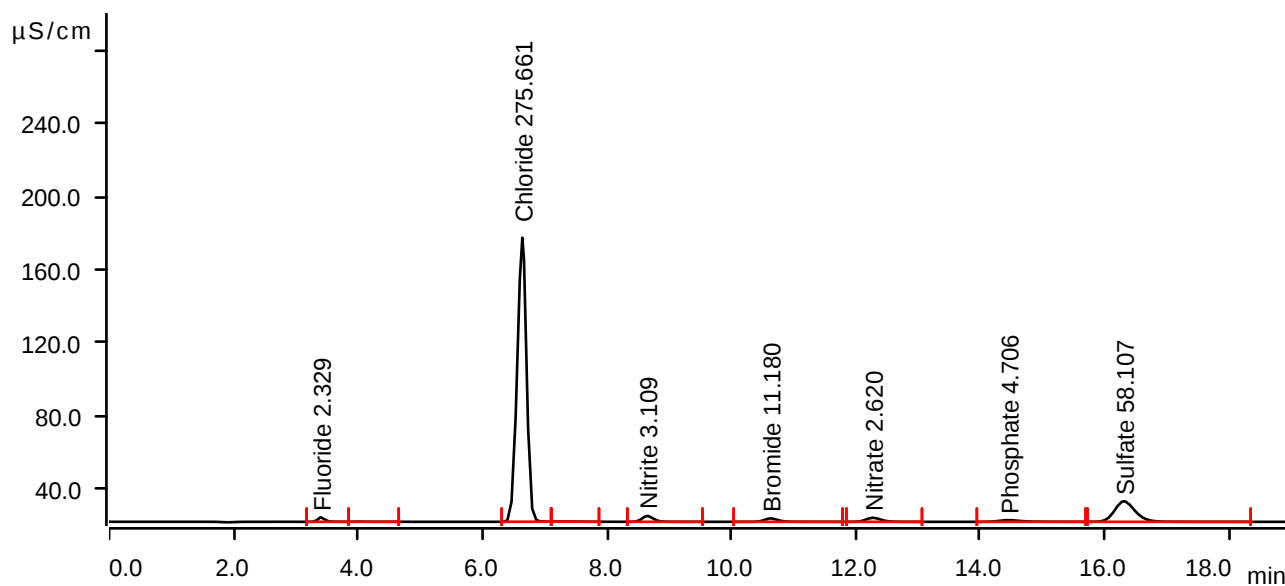

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.403	0.3310	2.507	2.329	Fluoride
2	4.030	0.0205	0.087	invalid	
3	6.642	27.0051	155.224	275.661	Chloride
4	7.302	0.0194	0.053	invalid	
5	8.650	0.6741	3.189	3.109	Nitrite
6	10.630	0.4746	1.858	11.180	Bromide
7	12.273	0.6219	2.220	2.620	Nitrate
8	14.452	0.3909	0.911	4.706	Phosphate
9	16.308	4.3268	11.241	58.107	Sulfate


Sample data

Ident Q3022-01MSD
Sample type Sample
Determination start 2025-09-04 15:40:15 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

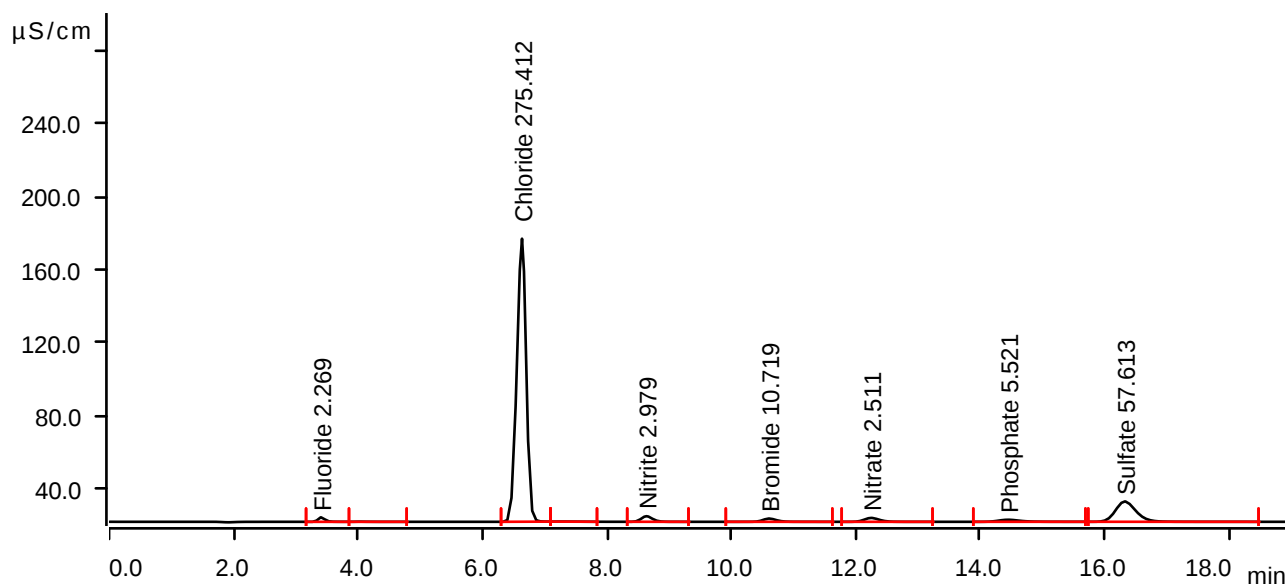

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	3.408	0.3224	2.436	2.269	Fluoride
2	4.040	0.0208	0.087	invalid	
3	6.637	26.9807	154.717	275.412	Chloride
4	7.292	0.0192	0.054	invalid	
5	8.637	0.6453	3.058	2.979	Nitrite
6	10.607	0.4548	1.787	10.719	Bromide
7	12.248	0.5956	2.127	2.511	Nitrate
8	14.447	0.4609	1.125	5.521	Phosphate
9	16.323	4.2898	11.117	57.613	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-09-04 16:01:50 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

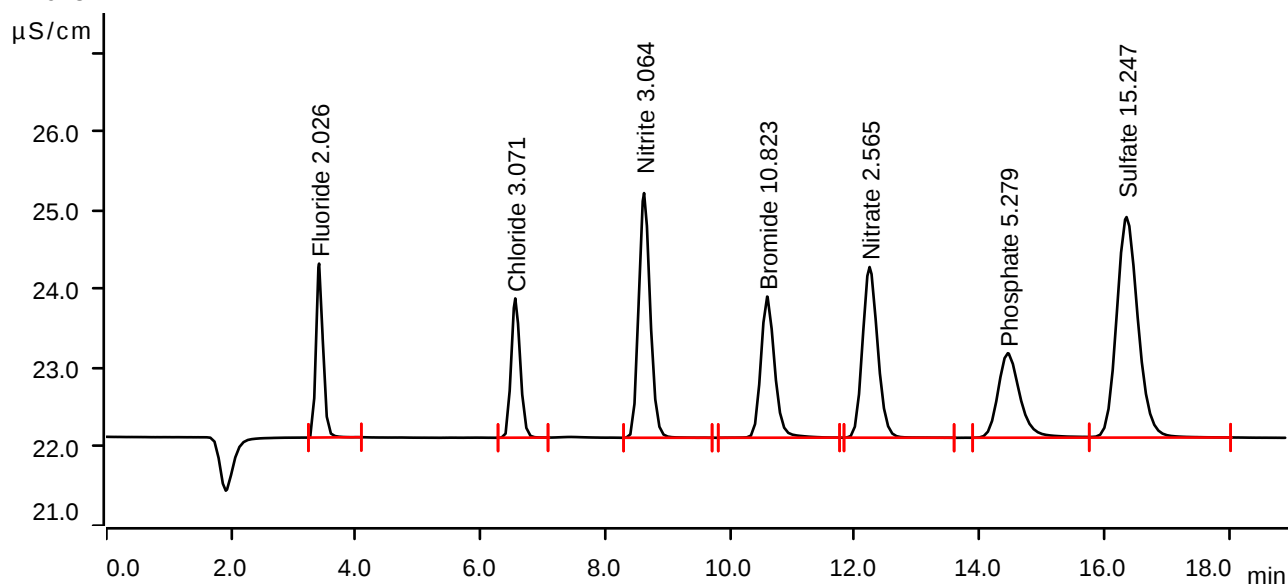

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.412	0.2873	2.206	2.026	Fluoride
2	6.557	0.2974	1.767	3.071	Chloride
3	8.622	0.6641	3.105	3.064	Nitrite
4	10.595	0.4593	1.791	10.823	Bromide
5	12.237	0.6088	2.166	2.565	Nitrate
6	14.453	0.4401	1.073	5.279	Phosphate
7	16.357	1.1156	2.799	15.247	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-09-04 16:23:20 UTC-4
Method IC1-080625
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions