

LB137189 INSTRUMENT ID: CV1

Method: 245.1

Operator: Admin

Date of Analysis: 15 Sep 2025 11:14:31

Type	Sample ID	Extended ID	Conc.	μ Abs	Units	Type	Std Conc	Method	Date
S	0.0 - 1	SO	-	-11	PPB	Std	0.0000	245.1	15 Sep 2025 11:31:39
S	0.05 - 1	SO.05	-	127	PPB	Std	0.0500	245.1	15 Sep 2025 11:42:08
S	0.2 - 1	SO.2	-	521	PPB	Std	0.2000	245.1	15 Sep 2025 11:44:25
S	2.5 - 1	SO.2	-	8734	PPB	Std	2.5000	245.1	15 Sep 2025 11:46:42
S	5.0 - 1	SO.5	-	16963	PPB	Std	5.0000	245.1	15 Sep 2025 11:48:58
S	7.5 - 1	SO	-	25420	PPB	Std	7.5000	245.1	15 Sep 2025 11:54:05
S	10.0 - 1	SO	-	34458	PPB	Std	10.0000	245.1	15 Sep 2025 12:01:59
U	ICV28 - 1	ICV28	4.1503	14180	PPB	SMPL	-245.1		15 Sep 2025 12:04:50
U	ICB28 - 1	ICB28	-0.0542	-250	PPB	SMPL	-245.1		15 Sep 2025 12:07:06
U	CCV85 - 1	CCV85	5.0436	17246	PPB	SMPL	-245.1		15 Sep 2025 12:09:24
U	CCB85 - 1	CCB85	-0.0452	-219	PPB	SMPL	-245.1		15 Sep 2025 12:11:38
U	CRA - 1	CRA	0.0591	139	PPB	SMPL	-245.1		15 Sep 2025 12:13:56
U	HighStd - 1	HighStd	10.2171	35002	PPB	SMPL	-245.1		15 Sep 2025 12:16:11
U	ChkStd - 1	ChkStd	6.7216	23005	PPB	SMPL	-245.1		15 Sep 2025 12:18:27
U	PB169688BL - 1	PBW	-0.0667	-293	PPB	SMPL	-245.1		15 Sep 2025 12:20:49
U	PB169688BS - 1	LCSW	4.2534	14534	PPB	SMPL	-245.1		15 Sep 2025 12:23:09
U	Q2893-10 - 1	LOD-MDL-WATER-04-QT3-2025	0.0422	81	PPB	SMPL	-245.1		15 Sep 2025 12:47:43
U	Q2893-11 - 1	LOQ-WATER-05-QT3-2025	0.2072	647	PPB	SMPL	-245.1		15 Sep 2025 12:49:59
U	Q3063-02 - 1	FALL-2025	0.0111	-26	PPB	SMPL	-245.1		15 Sep 2025 12:52:16
U	Q3063-02DUP - 1	FALL-2025DUP	0.1512	455	PPB	SMPL	-245.1		15 Sep 2025 13:03:17
U	Q3063-02MS - 1	FALL-2025MS	4.0226	13742	PPB	SMPL	-245.1		15 Sep 2025 13:05:32
U	CCV86 - 1	CCV86	4.8903	16720	PPB	SMPL	-245.1		15 Sep 2025 13:07:47
U	CCB86 - 1	CCB86	-0.0524	-244	PPB	SMPL	-245.1		15 Sep 2025 13:10:06
U	Q3063-02MSD - 1	FALL-2025MSD	4.0797	13938	PPB	SMPL	-245.1		15 Sep 2025 13:12:25
U	Q3063-02LX5 - 1		-0.0245	-146	PPB	SMPL	-245.1		15 Sep 2025 13:14:40
U	Q3063-02A - 1		4.1587	14209	PPB	SMPL	-245.1		15 Sep 2025 13:16:59
U	CCV87 - 1	CCV87	4.9658	16979	PPB	SMPL	-245.1		15 Sep 2025 13:19:15
U	CCB87 - 1	CCB87	-0.0434	-213	PPB	SMPL	-245.1		15 Sep 2025 13:21:34

LB137189


245.1

INSTRUMENT ID: CV1

Linear

μ Abs.:

34458

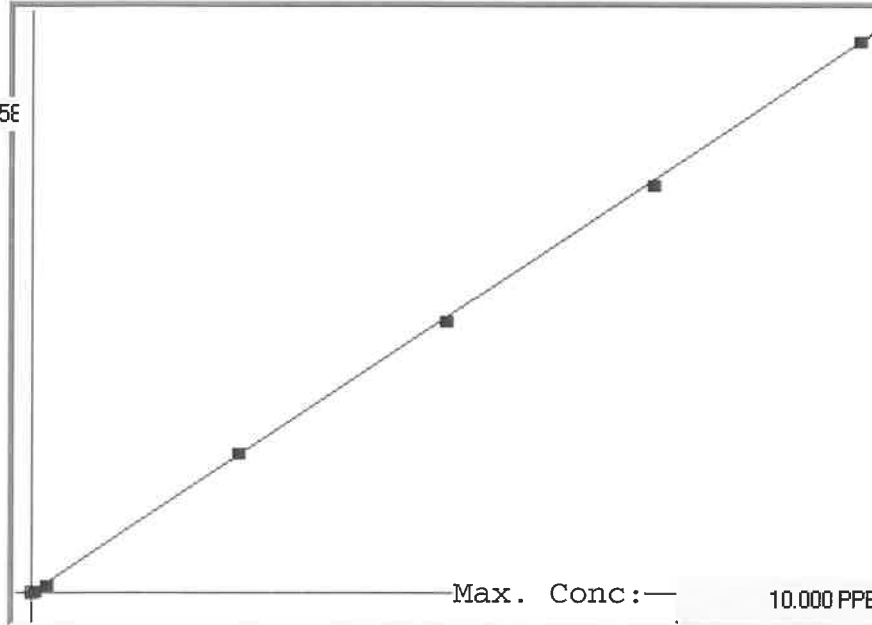

A= 0.0000e+000

B= 2.9137e-004

C= 1.8645e-002

Rho= 0.9999186

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	1/1
0.0	0.000	0.015	0.015	-11	0.000	-11					12
0.05	0.050	0.056	0.006	127	0.0 %	127					-15
0.2	0.200	0.170	-0.030	521	0.0 %	521					3
2.5	2.500	2.563	0.063	8734	0.0 %	8734					-1
5.0	5.000	4.961	-0.039	16963	0.0 %	16963					-1
7.5	7.500	7.425	-0.075	25420	0.0 %	25420					-1
10.0	10.000	10.059	0.059	34458	0.0 %	34458					1

Max. Conc.: 10.000 PPB