

LB137193 INSTRUMENT ID:CV1

Method: 7471B


Operator: Admin

Date of Analysis: 15 Sep 2025 13:38:21

Type	Sample ID	Extended ID	Conc.	μ Abs.	Units	Type	Std Conc	Method	Date
S	0.0 - 1	5.0	-	0	PPB	Std	0.0000	7471B	15 Sep 2025 13:38:41
S	0.2 - 1	50.2	-	839	PPB	Std	0.2000	7471B	15 Sep 2025 13:40:58
S	2.5 - 1	52.5	-	11006	PPB	Std	2.5000	7471B	15 Sep 2025 13:43:15
S	5.0 - 1	55.0	-	21462	PPB	Std	5.0000	7471B	15 Sep 2025 13:45:32
S	7.5 - 1	57.5	-	33038	PPB	Std	7.5000	7471B	15 Sep 2025 13:48:02
S	10.0 - 1	510.0	-	44498	PPB	Std	10.0000	7471B	15 Sep 2025 13:56:19
U	ICV29 - 1	ICV29	4.2266	18592	PPB	SMPL	-7471B		15 Sep 2025 13:59:14
U	ICB29 - 1	ICB29	-0.0347	-306	PPB	SMPL	-7471B		15 Sep 2025 14:01:47
U	CCV88 - 1	CCV88	4.8740	21463	PPB	SMPL	-7471B		15 Sep 2025 14:04:24
U	CCB88 - 1	CCB88	-0.0374	-318	PPB	SMPL	-7471B		15 Sep 2025 14:06:39
U	CRA - 1	CRA	0.1955	715	PPB	SMPL	-7471B		15 Sep 2025 14:09:17
U	HighStd - 1	HighStd	9.9627	44030	PPB	SMPL	-7471B		15 Sep 2025 14:11:32
U	ChkStd - 1	ChkStd	7.4410	32847	PPB	SMPL	-7471B		15 Sep 2025 14:13:47
U	PB169695BL - 1	PB169695BL	-0.0237	-257	PPB	SMPL	-7471B		15 Sep 2025 14:16:37
U	PB169695BS - 1	PB169695BS	4.7033	20706	PPB	SMPL	-7471B		15 Sep 2025 14:19:21
U	Q3082-01 - 1	WC-29	26.1418	115780	PPB	SMPL	-7471B		15 Sep 2025 14:21:37
U	Q3082-03 - 1	WC-30	9.0042	39779	PPB	SMPL	-7471B		15 Sep 2025 14:24:17
U	Q3082-05 - 1	WC-31	5.6964	25110	PPB	SMPL	-7471B		15 Sep 2025 14:27:12
U	Q3082-07 - 1	WC-32	27.8321	123276	PPB	SMPL	-7471B		15 Sep 2025 14:29:55
U	Q3082-09 - 1	WC-33	3.6180	15893	PPB	SMPL	-7471B		15 Sep 2025 14:32:37
U	CCV89 - 1	CCV89	4.9284	21704	PPB	SMPL	-7471B		15 Sep 2025 14:35:29
U	CCB89 - 1	CCB89	-0.0514	-380	PPB	SMPL	-7471B		15 Sep 2025 14:38:04
U	Q3091-01 - 1	12/9C-COMP	0.0663	142	PPB	SMPL	-7471B		15 Sep 2025 14:40:41
U	Q3091-01DUP - 1	12/9C-COMPDUP	0.0474	58	PPB	SMPL	-7471B		15 Sep 2025 14:43:13
U	Q3091-01MS - 1	12/9C-COMPMS	4.0573	17841	PPB	SMPL	-7471B		15 Sep 2025 14:45:28
U	Q3091-01MSD - 1	12/9C-COMPMSD	3.8203	16790	PPB	SMPL	-7471B		15 Sep 2025 14:47:44
U	Q3091-08 - 1	12/9B-COMP	0.0187	-69	PPB	SMPL	-7471B		15 Sep 2025 14:50:21
U	Q3091-01LX5 - 1		0.0142	-89	PPB	SMPL	-7471B		15 Sep 2025 14:52:59
U	Q3091-01A - 1		4.2052	18497	PPB	SMPL	-7471B		15 Sep 2025 14:55:15
U	Q3082-01DLX5 - 1		4.6652	20537	PPB	SMPL	-7471B		15 Sep 2025 14:57:32
U	Q3082-07DLX5 - 1		5.4871	24182	PPB	SMPL	-7471B		15 Sep 2025 15:00:09
U	CCV90 - 1	CCV90	4.9300	21711	PPB	SMPL	-7471B		15 Sep 2025 15:02:46
U	CCB90 - 1	CCB90	-0.0381	-321	PPB	SMPL	-7471B		15 Sep 2025 15:05:23

LB137193
INSTRUMENT ID : CV1

7471B

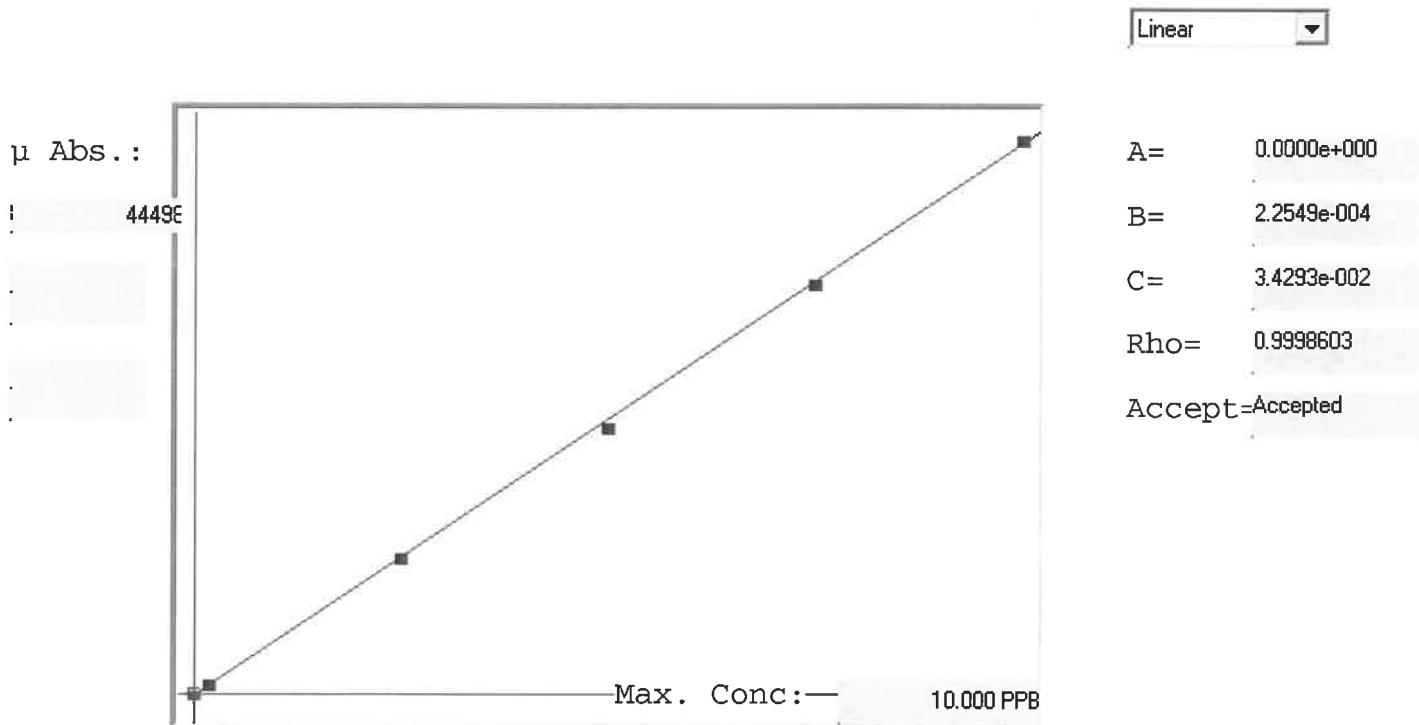

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.034	0.034	0	0.000	0					1
0.2	0.200	0.223	0.023	839	0.0 %	839					12
2.5	2.500	2.516	0.016	11006	0.0 %	11006					0
5.0	5.000	4.874	-0.126	21462	0.0 %	21462					-3
7.5	7.500	7.484	-0.016	33038	0.0 %	33038					0
10.0	10.000	10.068	0.068	44498	0.0 %	44498					0