

LB137304 INSTRUMENT ID:CV1

Method: 7470A


Operator: Admin

Date of Analysis: 25 Sep 2025 10:01:31

Type	Sample ID	Extended ID	Conc.	μ Abs.	Units	Type	Std ConcMethod	Date
S	0.0 - 1	50	-	-66	PPB	Std	0.00007470A	25 Sep 2025 10:17:53
S	0.2 - 1	50.2	-	498	PPB	Std	0.20007470A	25 Sep 2025 10:20:10
S	2.5 - 1	52.5	-	6691	PPB	Std	2.50007470A	25 Sep 2025 10:22:28
S	5.0 - 1	55.0	-	17074	PPB	Std	5.00007470A	25 Sep 2025 10:24:45
S	7.5 - 1	57.5	-	25912	PPB	Std	7.50007470A	25 Sep 2025 10:27:04
S	10.0 - 1	5100	-	31257	PPB	Std	10.00007470A	25 Sep 2025 10:43:02
U	ICV45 - 1	ICV45	4.2631	13769	PPB	SMPL	-7470A	25 Sep 2025 10:45:58
U	ICB45 - 1	ICB45	0.0143	-240	PPB	SMPL	-7470A	25 Sep 2025 10:48:12
U	CCV36 - 1	CCV36	4.6662	15098	PPB	SMPL	-7470A	25 Sep 2025 10:50:30
U	CCB36 - 1	CCB36	0.0177	-229	PPB	SMPL	-7470A	25 Sep 2025 10:52:46
U	CRA - 1	CRA	0.2485	532	PPB	SMPL	-7470A	25 Sep 2025 10:55:04
U	HighStd - 1	HighStd	9.4323	30813	PPB	SMPL	-7470A	25 Sep 2025 10:57:19
U	ChkStd - 1	ChkStd	7.0430	22935	PPB	SMPL	-7470A	25 Sep 2025 10:59:34
U	PB169815BL - 1	PBW	-0.0099	-320	PPB	SMPL	-7470A	25 Sep 2025 11:01:58
U	PB169815BS - 1	LCSW	4.5497	14714	PPB	SMPL	-7470A	25 Sep 2025 11:04:19
U	Q3159-02 - 1	VNJ-245	0.0228	-212	PPB	SMPL	-7470A	25 Sep 2025 11:06:35
U	Q3159-04 - 1	VNJ-255	0.0829	-14	PPB	SMPL	-7470A	25 Sep 2025 11:08:54
U	Q3167-02 - 1	RT4784	0.0944	24	PPB	SMPL	-7470A	25 Sep 2025 11:11:11
U	Q3167-02DUP - 1	RT4784DUP	0.0914	14	PPB	SMPL	-7470A	25 Sep 2025 11:13:28
U	Q3167-02MS - 1	RT4784MS	4.3410	14026	PPB	SMPL	-7470A	25 Sep 2025 11:18:47
U	CCV37 - 1	CCV37	4.6555	15063	PPB	SMPL	-7470A	25 Sep 2025 11:21:02
U	CCB37 - 1	CCB37	0.0171	-231	PPB	SMPL	-7470A	25 Sep 2025 11:23:20
U	Q3167-02MSD - 1	RT4784MSD	4.4047	14236	PPB	SMPL	-7470A	25 Sep 2025 11:28:12
U	PB169791TB - 1	PB169791TB	0.0249	-205	PPB	SMPL	-7470A	25 Sep 2025 11:30:28
U	Q3167-02LX5 - 1		0.1096	74	PPB	SMPL	-7470A	25 Sep 2025 11:32:46
U	Q3167-02A - 1		4.3104	13925	PPB	SMPL	-7470A	25 Sep 2025 11:35:02
U	CCV38 - 1	CCV38	4.6771	15134	PPB	SMPL	-7470A	25 Sep 2025 11:39:50
U	CCB38 - 1	CCB38	0.0240	-208	PPB	SMPL	-7470A	25 Sep 2025 11:42:08

LB137304
INSTRUMENT ID: CV1

7470A

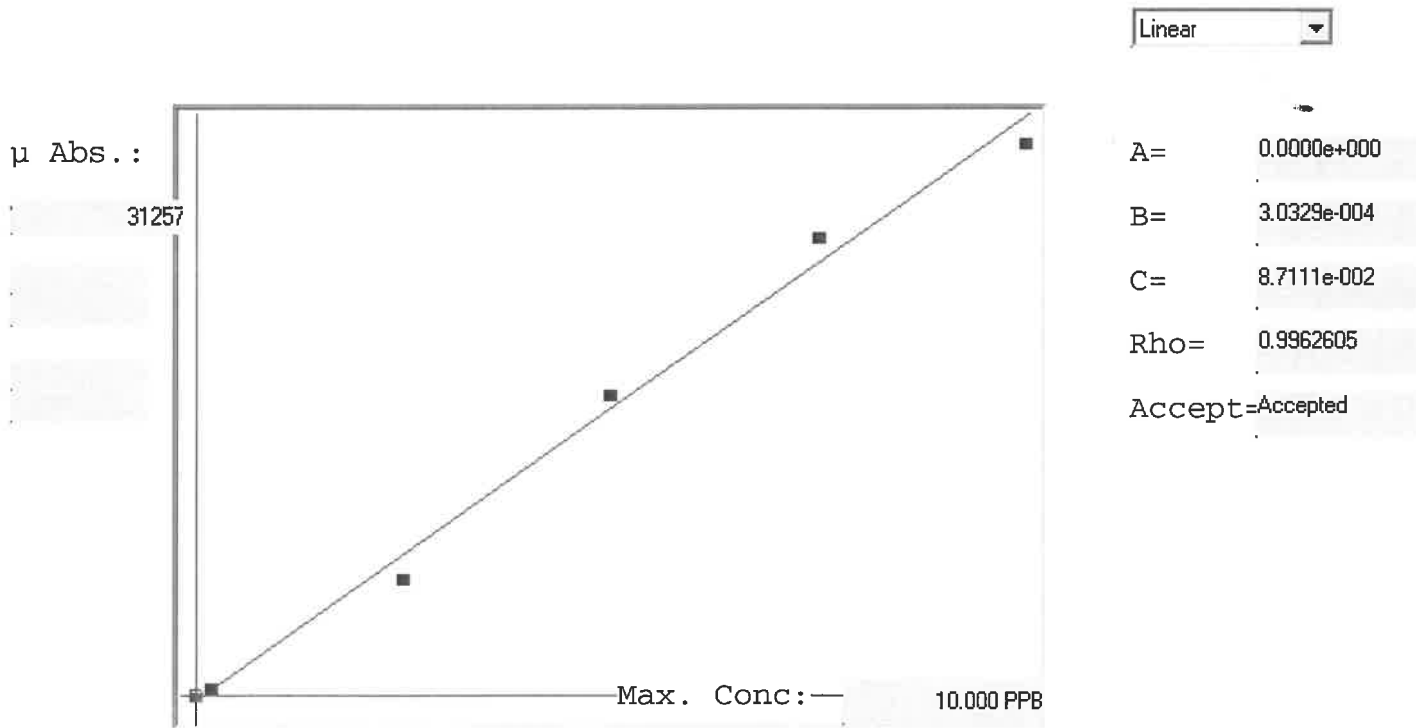

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	0.067	0.067	-66	0.000	-66	0				
0.2	0.200	0.238	0.038	498	0.0 %	498	0				
2.5	2.500	2.116	-0.384	6691	0.0 %	6691	0				
5.0	5.000	5.265	0.265	17074	0.0 %	17074					
7.5	7.500	7.946	0.446	25912	0.0 %	25912					
10.0	10.000	9.567	-0.433	31257	0.0 %	31257					

19
505
6
0