

06137647

=====

Test results	Aquakem 7.2AQ1	Page: 1
--------------	----------------	---------

Alliance Technical Group
284 Sheffield Street, Mountainside, NJ 07092

10/24/2025 16:26	Reviewed by : <u>RM</u>	Instrument ID : Konelab
------------------	-------------------------	-------------------------

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	1.004	0.0	0.109	
ICB1	0.001	0.0	0.008	
CCV1	0.980	0.0	0.106	
CCB1	0.000	0.0	0.008	
PB170233BL	0.002	0.0	0.009	
PB170233BS	1.001	0.0	0.109	
Q3448-03	-0.068	0.0	0.001	
Q3448-03DUP	0.018	0.0	0.010	
Q3448-03MS	1.006	0.0	0.109	
Q3448-03MSD	0.996	0.0	0.108	
CCV2	0.973	0.0	0.106	
CCB2	0.000	0.0	0.008	

N	12
Mean	0.493
SD	0.5233
CV%	106.20

Aquakem v. 7.2AQ1

Results from time period:

Fri Oct 24 15:28:42 2025

Fri Oct 24 16:24:25 2025

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	0	mg/l	10/24/2025 15:28:42	
0.05PPM	A	Phenolics-	P	0.0531	mg/l	10/24/2025 15:28:43	
0.1PPM	A	Phenolics-	P	0.1023	mg/l	10/24/2025 15:28:44	
0.25PPM	A	Phenolics-	P	0.2481	mg/l	10/24/2025 15:28:45	
0.50PPM	A	Phenolics-	P	0.4991	mg/l	10/24/2025 15:28:46	
1.0PPM	A	Phenolics-	P	0.9943	mg/l	10/24/2025 15:28:47	
2.0PPM	A	Phenolics-	P	2.0031	mg/l	10/24/2025 15:28:48	
ICV1	S	Phenolics-	P	1.0041	mg/l	10/24/2025 15:57:26	
ICB1	S	Phenolics-	P	0.0011	mg/l	10/24/2025 15:57:28	
CCV1	S	Phenolics-	P	0.9799	mg/l	10/24/2025 15:57:30	
CCB1	S	Phenolics-	P	0.0005	mg/l	10/24/2025 15:57:32	
PB170233BL	S	Phenolics-	P	0.0022	mg/l	10/24/2025 15:57:33	
PB170233BS	S	Phenolics-	P	1.0012	mg/l	10/24/2025 15:57:36	
Q3448-03	S	Phenolics-	P	-0.0683	mg/l	10/24/2025 16:07:28	
Q3448-03DUP	S	Phenolics-	P	0.0175	mg/l	10/24/2025 16:07:30	
Q3448-03MS	S	Phenolics-	P	1.0058	mg/l	10/24/2025 16:07:33	
Q3448-03MSD	S	Phenolics-	P	0.9962	mg/l	10/24/2025 16:07:34	
CCV2	S	Phenolics-	P	0.973	mg/l	10/24/2025 16:07:35	
CCB2	S	Phenolics-	P	0.0001	mg/l	10/24/2025 16:07:37	

Alliance Technical Group
284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM Instrument ID : Konelab

10/24/2025 15:35


Test Phenolics-

Accepted 10/24/2025 15:35

Factor 9.994
Bias 0.008

Coeff. of det. 0.999981

Errors

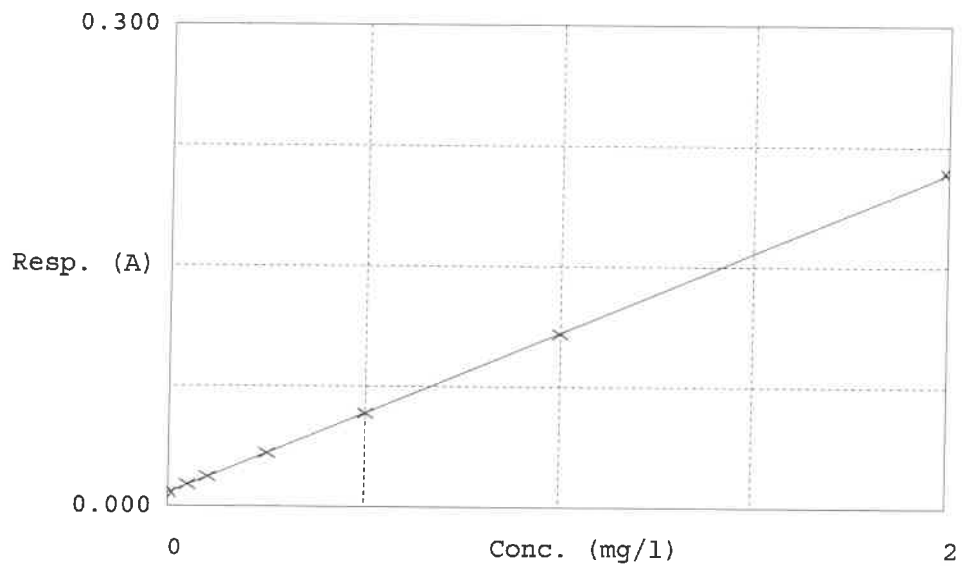

	Calibrator	Response	Calc. con.	Conc.	^{Re} Errors
1	0.00PPM	0.008	-0.0000	0.0000	-
2	Phenol-2	0.014	0.0531	0.0500	6.2
3	Phenol-2	0.019	0.1023	0.1000	2.3
4	Phenol-2	0.033	0.2481	0.2500	-0.8
5	Phenol-2	0.058	0.4991	0.5000	-0.2
6	Phenol-2	0.108	0.9943	1.0000	0.6
7	Phenol-2	0.209	2.0031	2.0000	0.2

10/24/2025
RM