


Instrument IC-1			Analyst : RM		Method: 300.0 / 9056A					
Ident	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4	Method name	date time	Initial w Analyst
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/3/2025 15:58	10 RM/IZ
STD2	0.417	0.655	0.659	2.182	0.549	0.953	3.345	IC1-110325	11/3/2025 16:22	10 RM/IZ
STD3	0.813	1.228	1.228	4.086	1.024	2.097	6.147	IC1-110325	11/3/2025 17:04	10 RM/IZ
STD4	1.014	1.491	1.496	4.984	1.245	2.506	7.444	IC1-110325	11/3/2025 17:47	10 RM/IZ
STD5	1.966	2.918	2.907	9.724	2.426	5.166	14.580	IC1-110325	11/3/2025 18:08	10 RM/IZ
STD6	3.912	5.914	5.907	19.694	4.918	9.286	29.234	IC1-110325	11/3/2025 18:30	10 RM/IZ
STD7	5.078	7.595	7.603	25.330	6.339	12.992	37.751	IC1-110325	11/3/2025 18:51	10 RM/IZ
ICV	1.960	2.885	2.908	9.698	2.364	5.176	14.547	IC1-110325	11/3/2025 19:13	10 RM/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/3/2025 19:34	10 RM/IZ
CCV	2.019	3.032	3.015	10.073	2.512	5.081	14.900	IC1-110325	11/5/2025 13:47	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/5/2025 14:08	10 RM/IZ
LB137815BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/5/2025 14:30	10 RM/IZ
LB137815BSW	2.041	3.059	3.032	10.148	2.531	5.150	15.044	IC1-110325	11/5/2025 14:51	10 RM/IZ
Q3552-01	0.321	0.000	0.106	10.529	0.115	0.057	1.113	IC1-110325	11/5/2025 15:47	10 RM/IZ
Q3552-02	0.140	0.000	0.000	31.375	0.108	0.000	6.874	IC1-110325	11/5/2025 16:08	10 RM/IZ
Q3552-03	0.308	416.101	0.180	2.189	3.915	0.000	10.132	IC1-110325	11/5/2025 16:30	10 RM/IZ
Q3552-04	0.222	0.000	0.000	28.383	0.104	0.000	1254.705	IC1-110325	11/5/2025 16:51	10 RM/IZ
Q3552-04MS	2.146	0.000	2.941	37.492	2.470	1.322	1208.840	IC1-110325	11/5/2025 17:13	10 RM/IZ
Q3552-04MSD	2.087	0.000	2.846	37.215	2.387	1.053	1211.533	IC1-110325	11/5/2025 17:35	10 RM/IZ
Q3552-05	0.208	509.854	0.000	3.747	0.000	0.109	1.302	IC1-110325	11/5/2025 17:56	10 RM/IZ
CCV	1.987	3.079	3.141	10.140	2.530	4.965	15.195	IC1-110325	11/5/2025 19:01	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-110325	11/5/2025 19:22	10 RM/IZ

Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A											
ident	concentra tion F-	concentratio n CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time	Initial wt/ Final	Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000 IC1-110325	11/3/2025 15:58	10	RM/IZ
STD2	0.4170	0.6550	0.6590	2.1820	0.5490	0.9530	3.3450	IC1-110325	11/3/2025 16:22	10	RM/IZ
STD3	0.8130	1.2280	1.2280	4.0860	1.0240	2.0970	6.1470	IC1-110325	11/3/2025 17:04	10	RM/IZ
STD4	1.0140	1.4910	1.4960	4.9840	1.2450	2.5060	7.4440	IC1-110325	11/3/2025 17:47	10	RM/IZ
STD5	1.9660	2.9180	2.9070	9.7240	2.4260	5.1660	14.5800	IC1-110325	11/3/2025 18:08	10	RM/IZ
STD6	3.9120	5.9140	5.9070	19.6940	4.9180	9.2860	29.2340	IC1-110325	11/3/2025 18:30	10	RM/IZ
STD7	5.0780	7.5950	7.6030	25.3300	6.3390	12.9920	37.7510	IC1-110325	11/3/2025 18:51	10	RM/IZ
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4				
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000				
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000				
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000				
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000				
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000				
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000				
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000				
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4				
STD1	4.2500	9.1667	9.8333	9.1000	9.8000	-4.7000	11.5000				
STD2	1.6250	2.3333	2.3333	2.1500	2.4000	4.8500	2.4500				
STD3	1.4000	-0.6000	-0.2667	-0.3200	-0.4000	0.2400	-0.7467				
STD4	-1.7000	-2.7333	-3.1000	-2.7600	-2.9600	3.3200	-2.8000				
STD5	-2.2000	-1.4333	-1.5500	-1.5300	-1.6400	-7.1400	-2.5533				
STD6	1.5600	1.2667	1.3733	1.3200	1.4240	3.9360	2.0297				

Fluoride (Anions)

($\mu\text{S}/\text{cm}$) x min

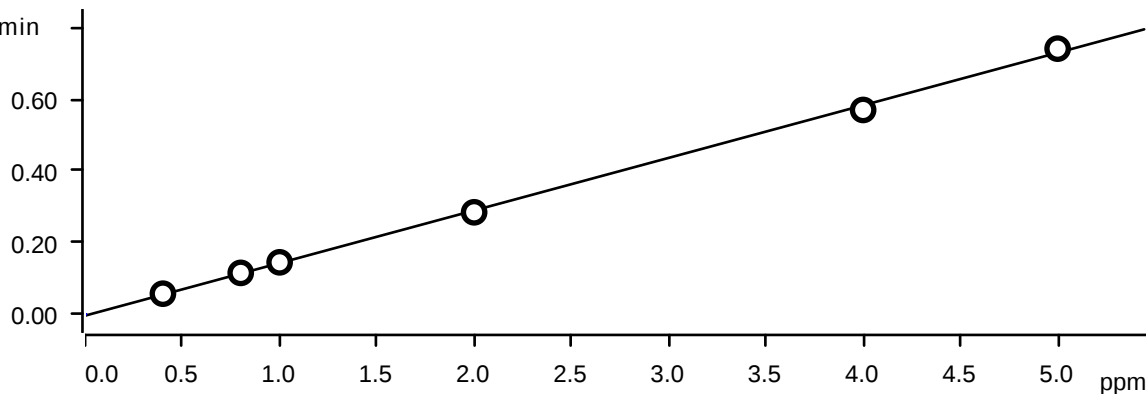

Function: $A = -3.63197\text{E-}3 + 0.0146595 \times Q$


Relative standard deviation 2.880512 %

Correlation coefficient 0.999558

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	0.400	10.0	1.0	1.0	0.058	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.116	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.145	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.285	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.570	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.741	STD7	2025-11-03 18:51:52 UTC-5	used

Chloride (Anions)


($\mu\text{S}/\text{cm}$) x min

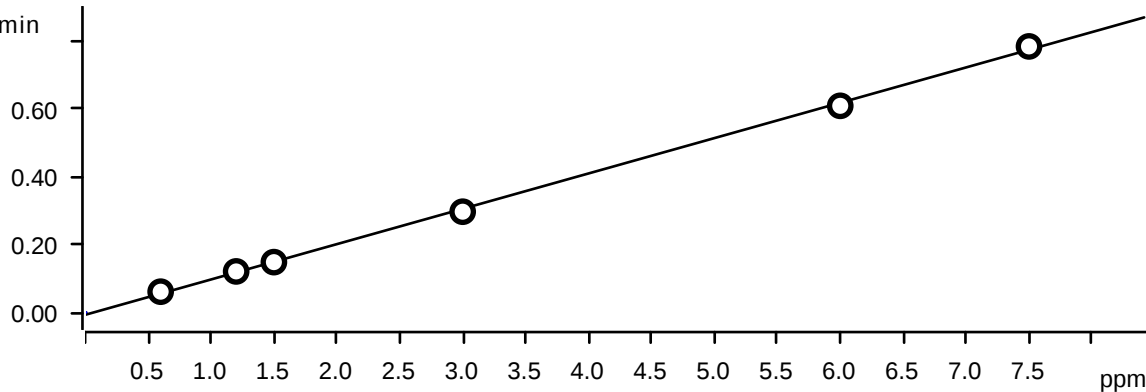

Function: $A = -7.14286\text{E-}3 + 0.0104011 \times Q$

Relative standard deviation 2.544562 %
Correlation coefficient 0.999662


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.061	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.121	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.148	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.296	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.608	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.783	STD7	2025-11-03 18:51:52 UTC-5	used

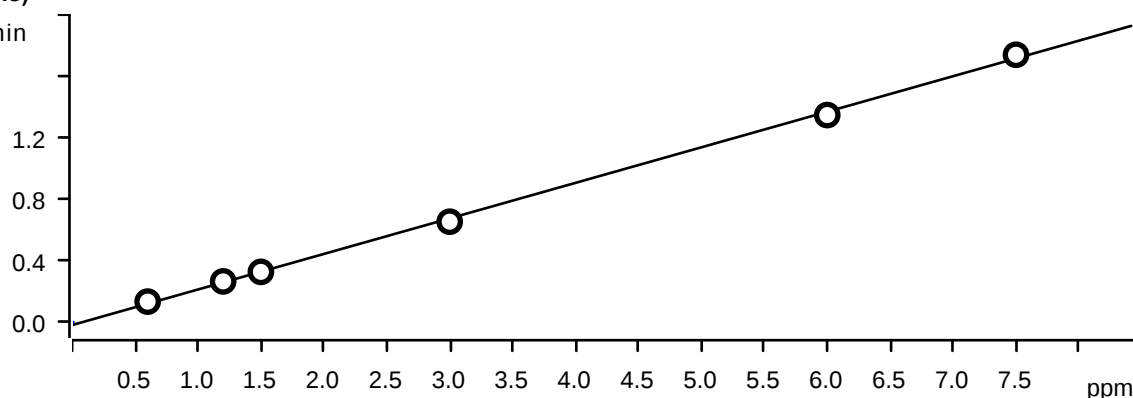Nitrite (Anions) $(\mu\text{S/cm}) \times \text{min}$ 

Function: $A = -0.0188106 + 0.0231263 \times Q$
Relative standard deviation 2.785229 %
Correlation coefficient 0.999598

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.134	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.265	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.327	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.654	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.347	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.740	STD7	2025-11-03 18:51:52 UTC-5	used

Bromide (Anions)

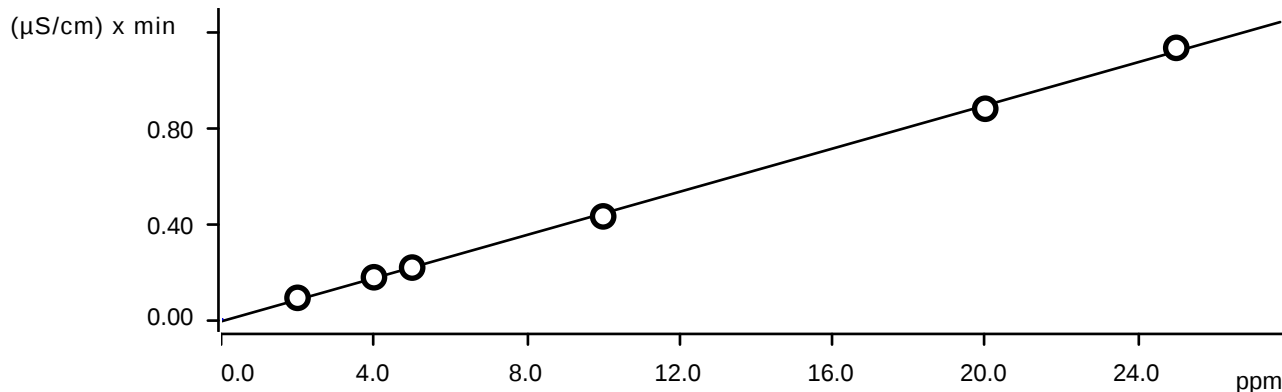


Function: $A = -8.73633E-3 + 4.51609E-3 \times Q$

Relative standard deviation: 2.618377 %

Correlation coefficient: 0.999640

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	2.000	10.0	1.0	1.0	0.090	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.176	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.216	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.430	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.881	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.135	STD7	2025-11-03 18:51:52 UTC-5	used

Nitrate (Anions)

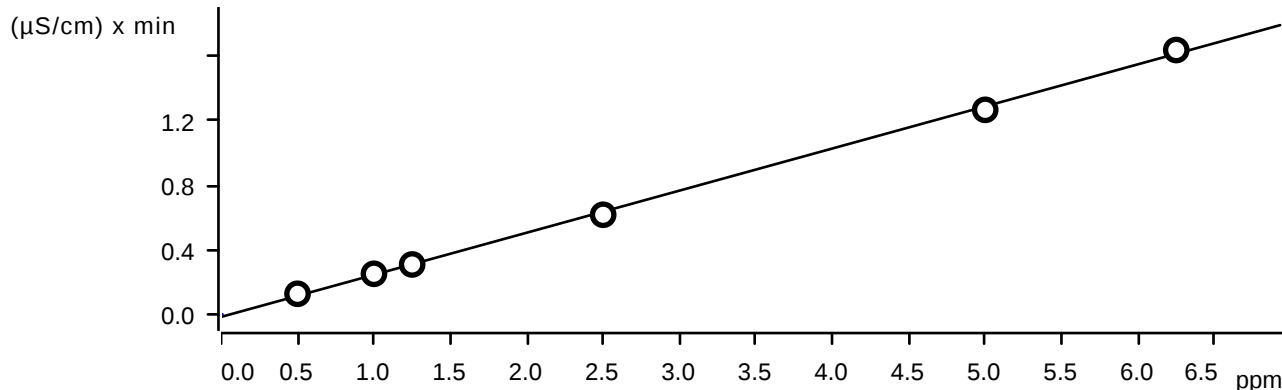

Function: $A = -0.0164240 + 0.0260850 \times Q$


Relative standard deviation: 2.824357 %

Correlation coefficient 0.999585

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	0.500	10.0	1.0	1.0	0.127	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	1.000	10.0	1.0	1.0	0.251	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.308	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.616	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.266	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.637	STD7	2025-11-03 18:51:52 UTC-5	used

Phosphate (Anions)


(μS/cm) x min

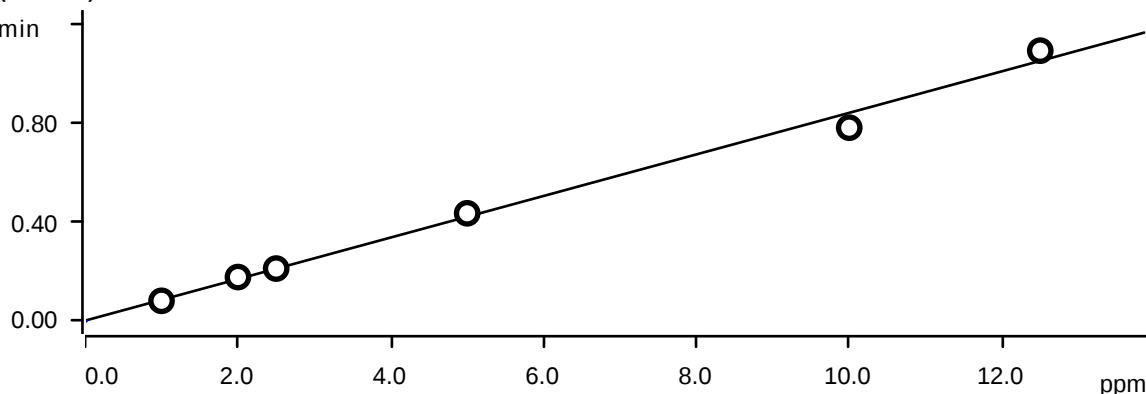Function: $A = 1.95294E-3 + 8.36815E-3 \times Q$

Relative standard deviation 8.053642 %

Correlation coefficient 0.996454

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	1.000	10.0	1.0	1.0	0.082	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.177	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.212	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.434	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.779	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	1.089	STD7	2025-11-03 18:51:52 UTC-5	used

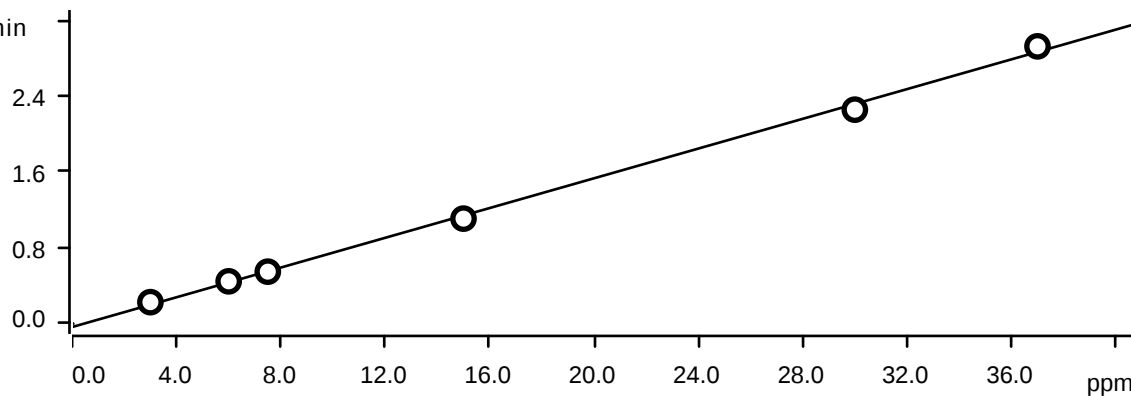Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0341972 + 7.83080E-3 \times Q$

Relative standard deviation 3.795793 %

Correlation coefficient 0.999249


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-11-03 15:58:57 UTC-5	used
Standard 2	1	3.000	10.0	1.0	1.0	0.228	STD2	2025-11-03 16:22:03 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.447	STD3	2025-11-03 17:04:52 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.549	STD4	2025-11-03 17:47:32 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.108	STD5	2025-11-03 18:08:59 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.255	STD6	2025-11-03 18:30:25 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.922	STD7	2025-11-03 18:51:52 UTC-5	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-11-03 15:58:57 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

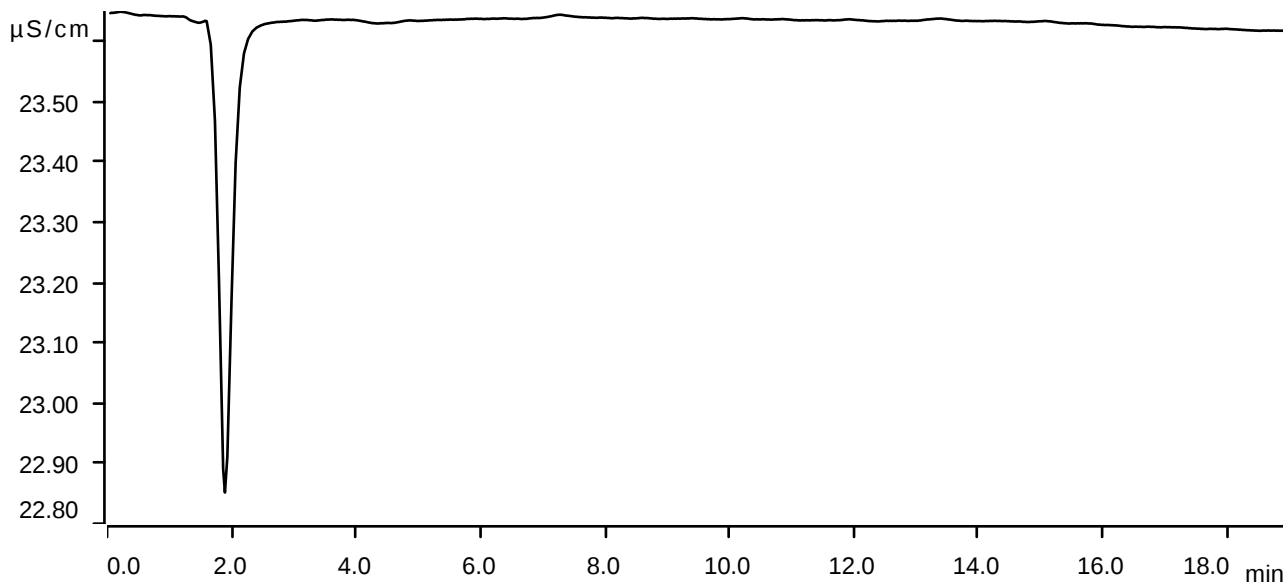Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-11-03 16:22:03 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

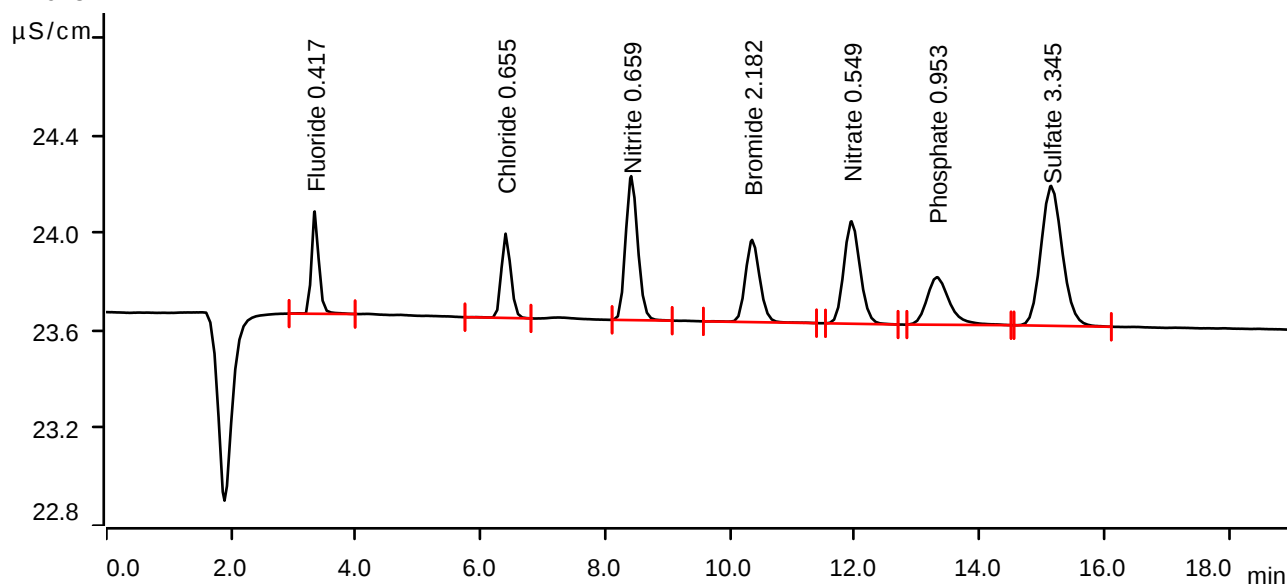

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.340	0.0576	0.420	0.417	Fluoride
2	6.402	0.0609	0.345	0.655	Chloride
3	8.415	0.1336	0.590	0.659	Nitrite
4	10.353	0.0898	0.337	2.182	Bromide
5	11.947	0.1268	0.420	0.549	Nitrate
6	13.317	0.0817	0.195	0.953	Phosphate
7	15.147	0.2277	0.574	3.345	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-11-03 17:04:52 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.27 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

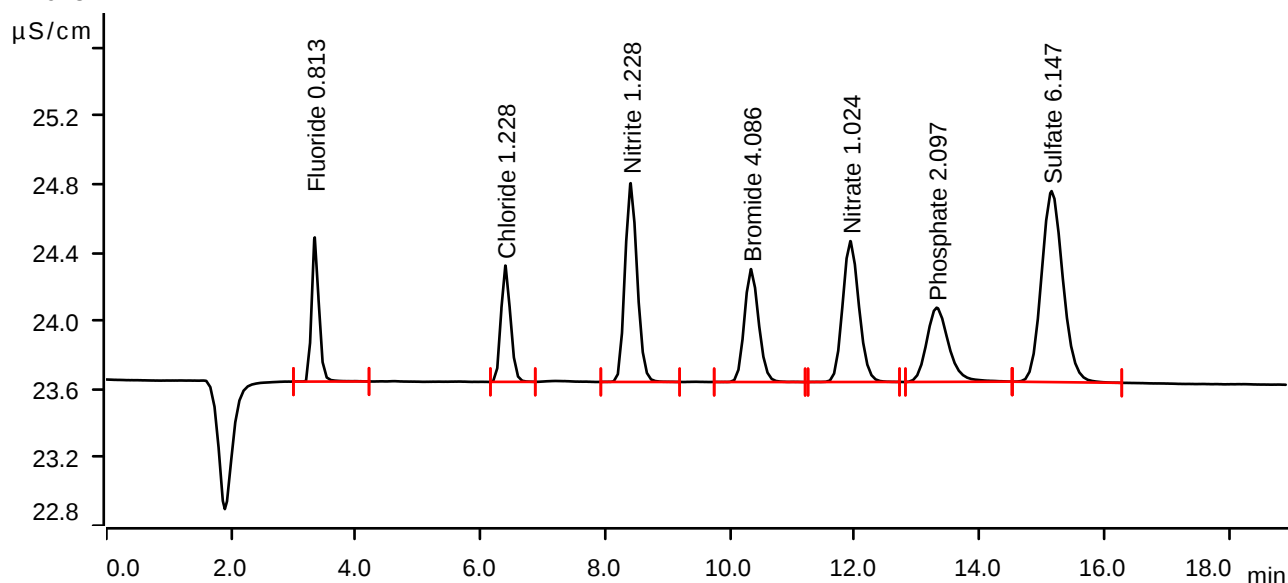

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.342	0.1156	0.844	0.813	Fluoride
2	6.397	0.1206	0.681	1.228	Chloride
3	8.407	0.2651	1.164	1.228	Nitrite
4	10.337	0.1758	0.661	4.086	Bromide
5	11.928	0.2506	0.825	1.024	Nitrate
6	13.312	0.1774	0.435	2.097	Phosphate
7	15.155	0.4471	1.119	6.147	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-11-03 17:47:32 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

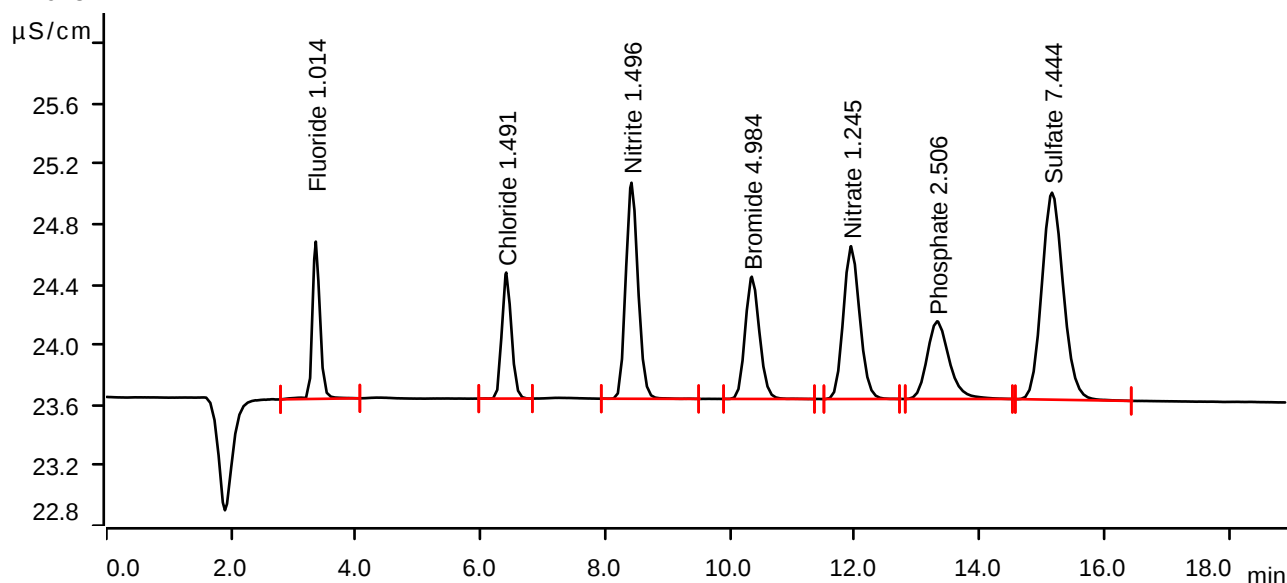

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.358	0.1450	1.044	1.014	Fluoride
2	6.412	0.1479	0.837	1.491	Chloride
3	8.420	0.3271	1.434	1.496	Nitrite
4	10.348	0.2164	0.811	4.984	Bromide
5	11.940	0.3084	1.014	1.245	Nitrate
6	13.320	0.2117	0.516	2.506	Phosphate
7	15.162	0.5487	1.374	7.444	Sulfate


Sample data

Ident STD5
Sample type Standard 5
Determination start 2025-11-03 18:08:59 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.44 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

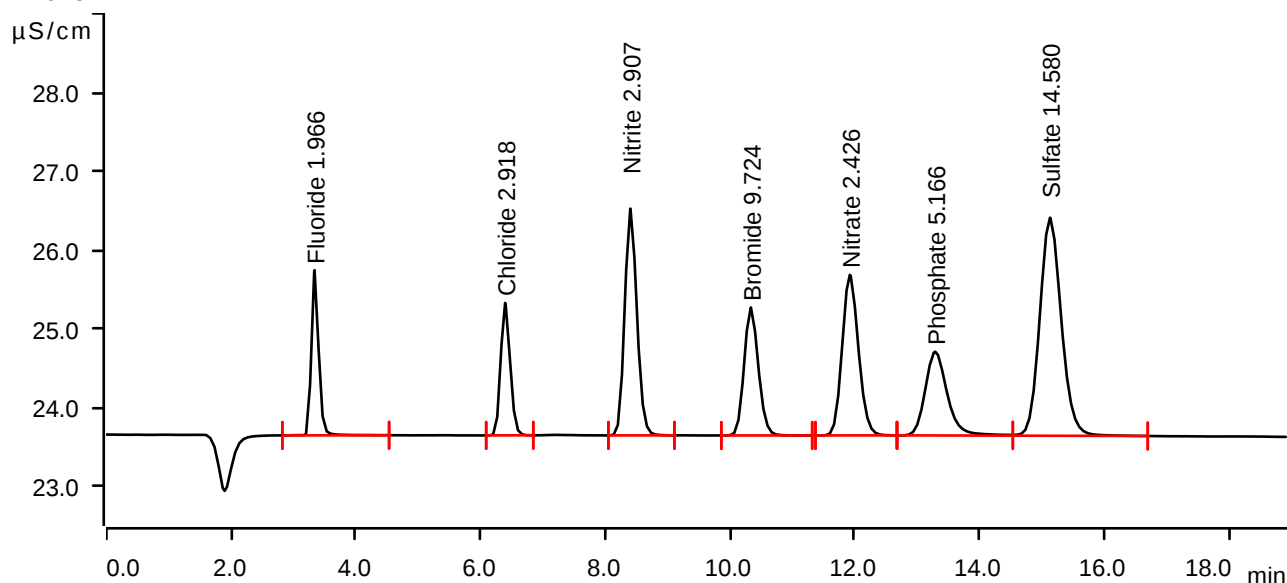

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.338	0.2845	2.095	1.966	Fluoride
2	6.393	0.2963	1.681	2.918	Chloride
3	8.403	0.6535	2.878	2.907	Nitrite
4	10.332	0.4304	1.624	9.724	Bromide
5	11.920	0.6163	2.038	2.426	Nitrate
6	13.290	0.4342	1.063	5.166	Phosphate
7	15.128	1.1075	2.767	14.580	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-11-03 18:30:25 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

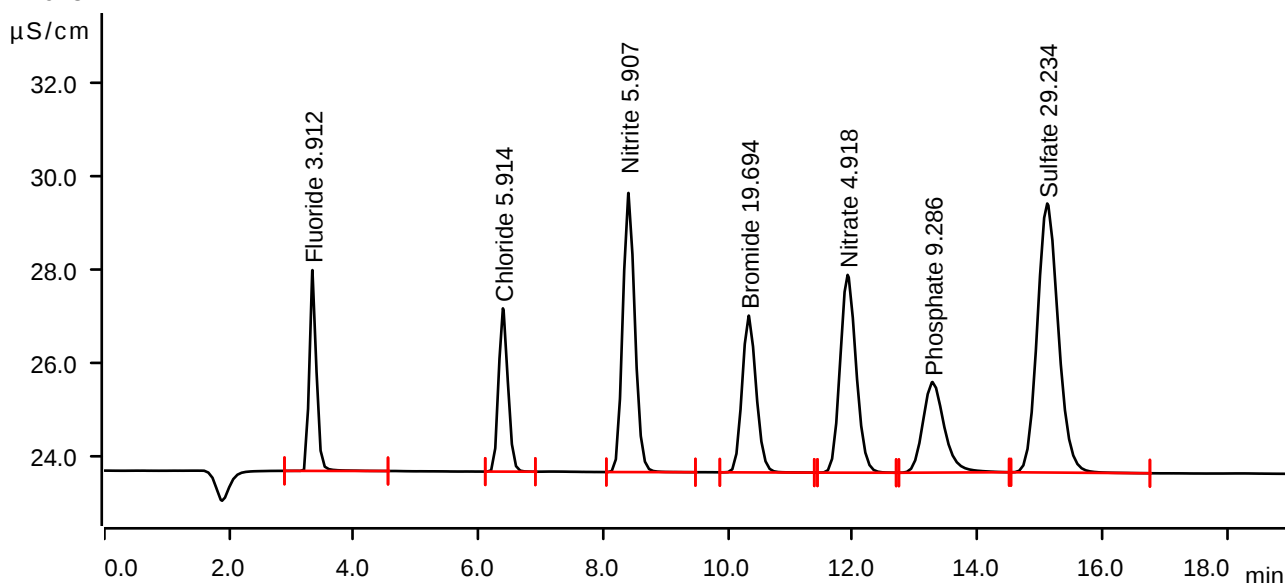

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.337	0.5698	4.312	3.912	Fluoride
2	6.390	0.6080	3.506	5.914	Chloride
3	8.403	1.3473	5.995	5.907	Nitrite
4	10.330	0.8806	3.367	19.694	Bromide
5	11.917	1.2665	4.248	4.918	Nitrate
6	13.278	0.7790	1.945	9.286	Phosphate
7	15.117	2.2550	5.777	29.234	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-11-03 18:51:52 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.50 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

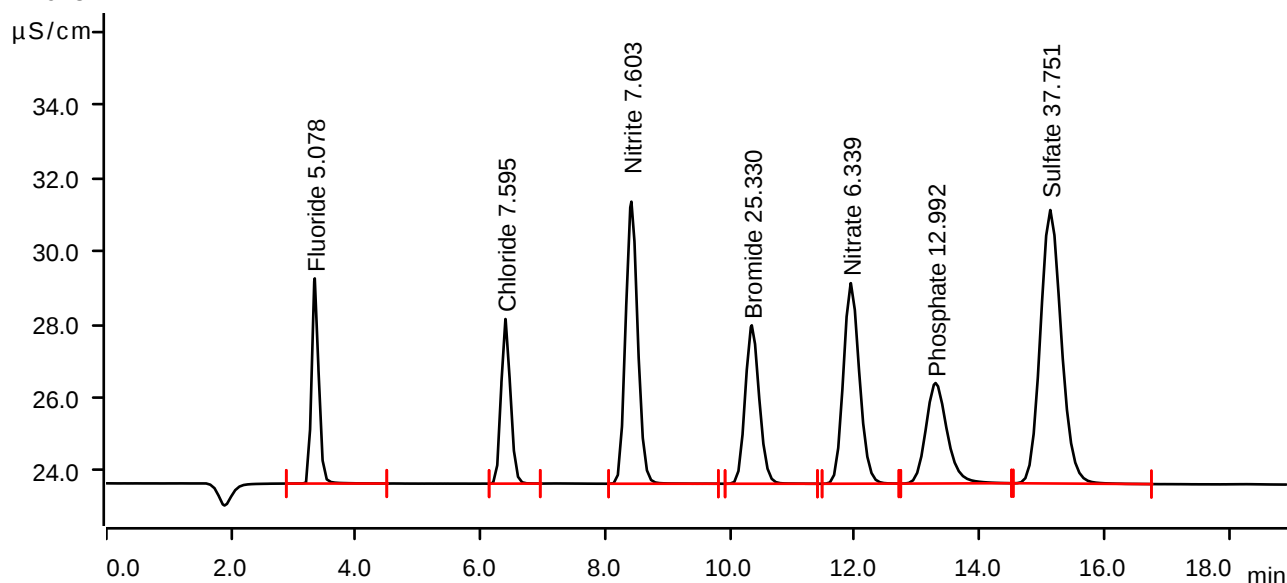

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.342	0.7408	5.606	5.078	Fluoride
2	6.398	0.7828	4.499	7.595	Chloride
3	8.418	1.7395	7.709	7.603	Nitrite
4	10.348	1.1352	4.330	25.330	Bromide
5	11.937	1.6370	5.482	6.339	Nitrate
6	13.295	1.0891	2.746	12.992	Phosphate
7	15.133	2.9220	7.473	37.751	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-11-03 19:13:20 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

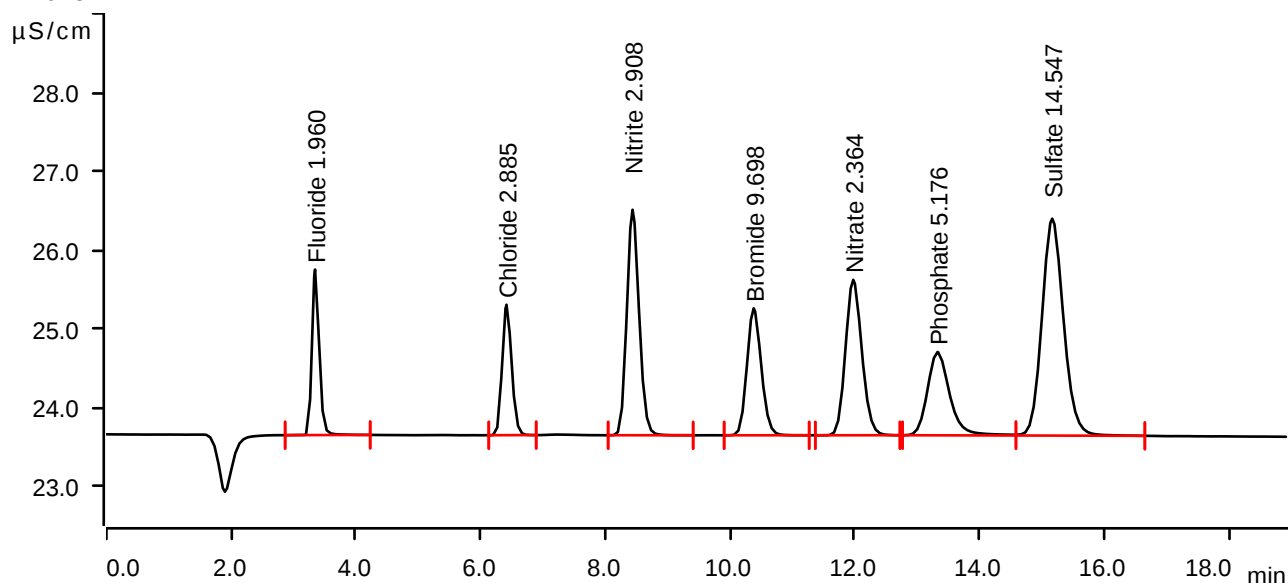


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.347	0.2837	2.100	1.960	Fluoride
2	6.417	0.2929	1.656	2.885	Chloride
3	8.437	0.6536	2.862	2.908	Nitrite
4	10.378	0.4292	1.611	9.698	Bromide
5	11.975	0.6003	1.973	2.364	Nitrate
6	13.327	0.4351	1.058	5.176	Phosphate
7	15.165	1.1050	2.753	14.547	Sulfate

Sample data

Ident ICB
Sample type Sample
Determination start 2025-11-03 19:34:48 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

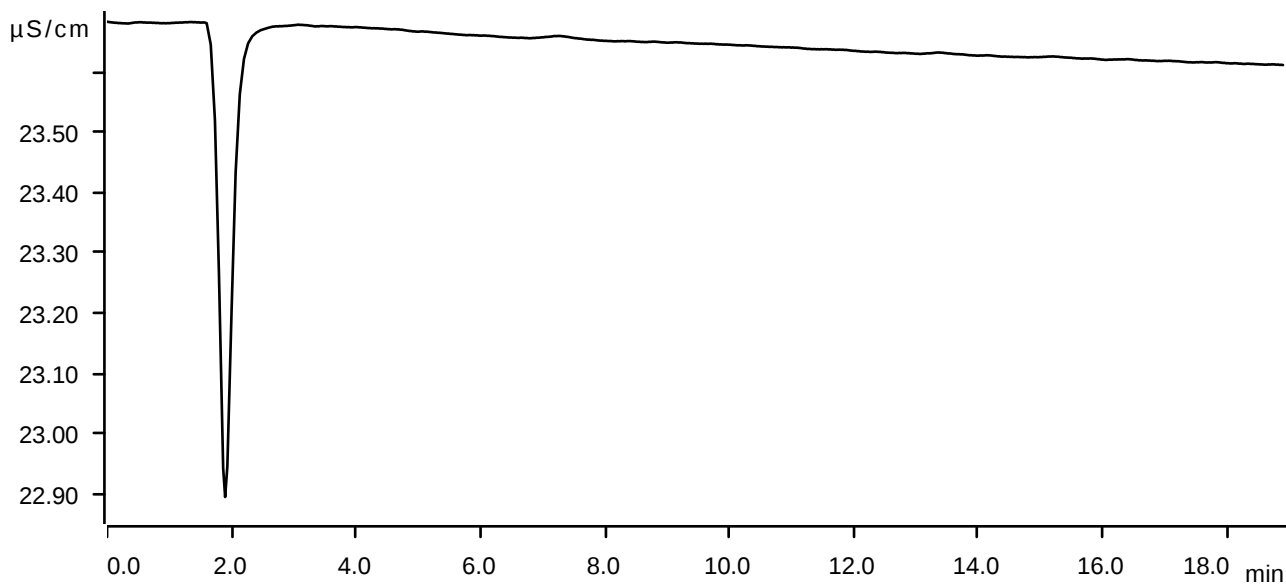Anions


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-11-05 13:47:07 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

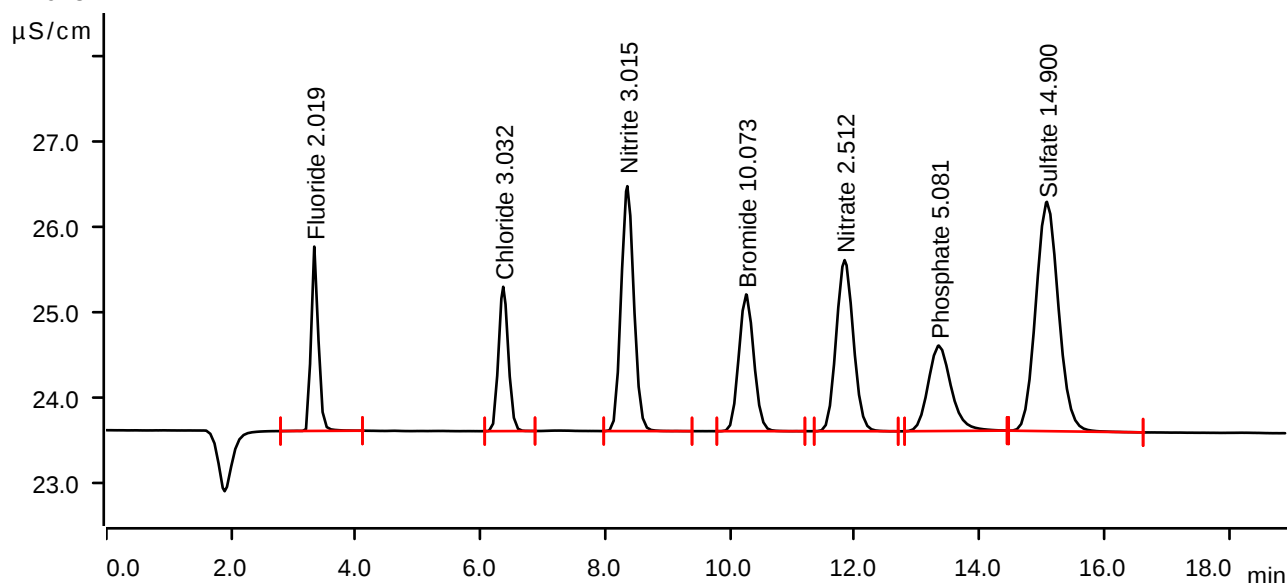

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.335	0.2924	2.158	2.019	Fluoride
2	6.363	0.3082	1.690	3.032	Chloride
3	8.353	0.6783	2.869	3.015	Nitrite
4	10.258	0.4462	1.602	10.073	Bromide
5	11.837	0.6389	2.005	2.512	Nitrate
6	13.347	0.4271	1.001	5.081	Phosphate
7	15.080	1.1326	2.686	14.900	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2025-11-05 14:08:40 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.39 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

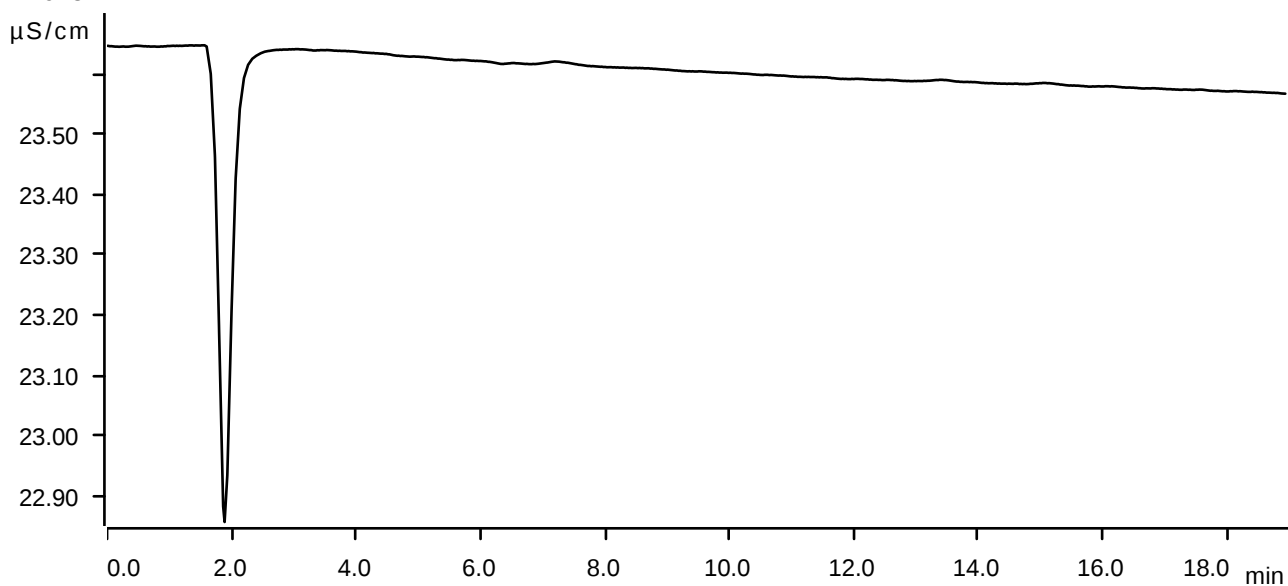


Sample data

Ident LB137815BLW
Sample type Sample
Determination start 2025-11-05 14:30:11 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.16 MPa
Maximum pressure monitored yes
Temperature ---- °C

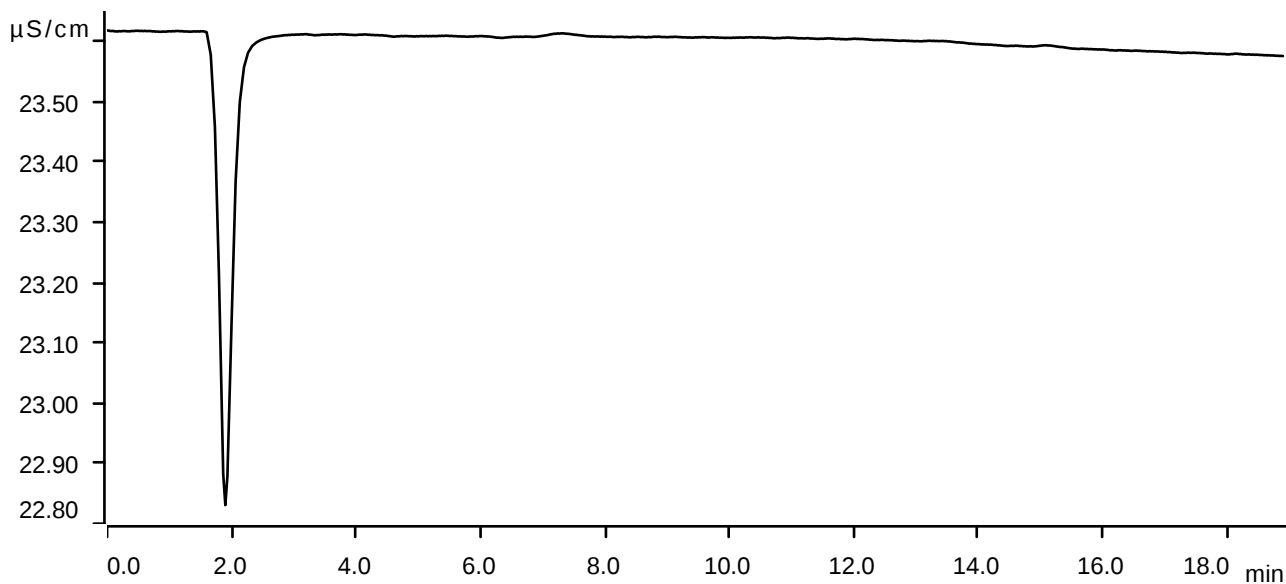Anions


Sample data

Ident LB137815BSW
Sample type Sample
Determination start 2025-11-05 14:51:43 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

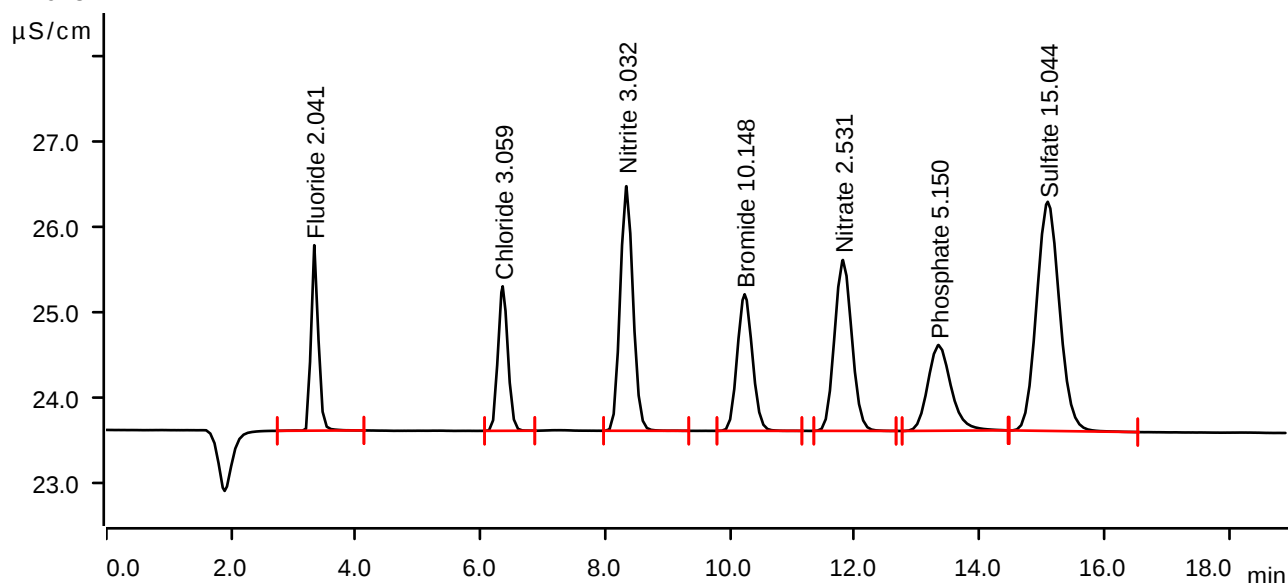

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.333	0.2956	2.172	2.041	Fluoride
2	6.355	0.3111	1.693	3.059	Chloride
3	8.338	0.6825	2.865	3.032	Nitrite
4	10.233	0.4495	1.600	10.148	Bromide
5	11.810	0.6438	2.002	2.531	Nitrate
6	13.343	0.4329	1.004	5.150	Phosphate
7	15.093	1.1439	2.684	15.044	Sulfate


Sample data

Ident Q3552-01
Sample type Sample
Determination start 2025-11-05 15:47:11 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

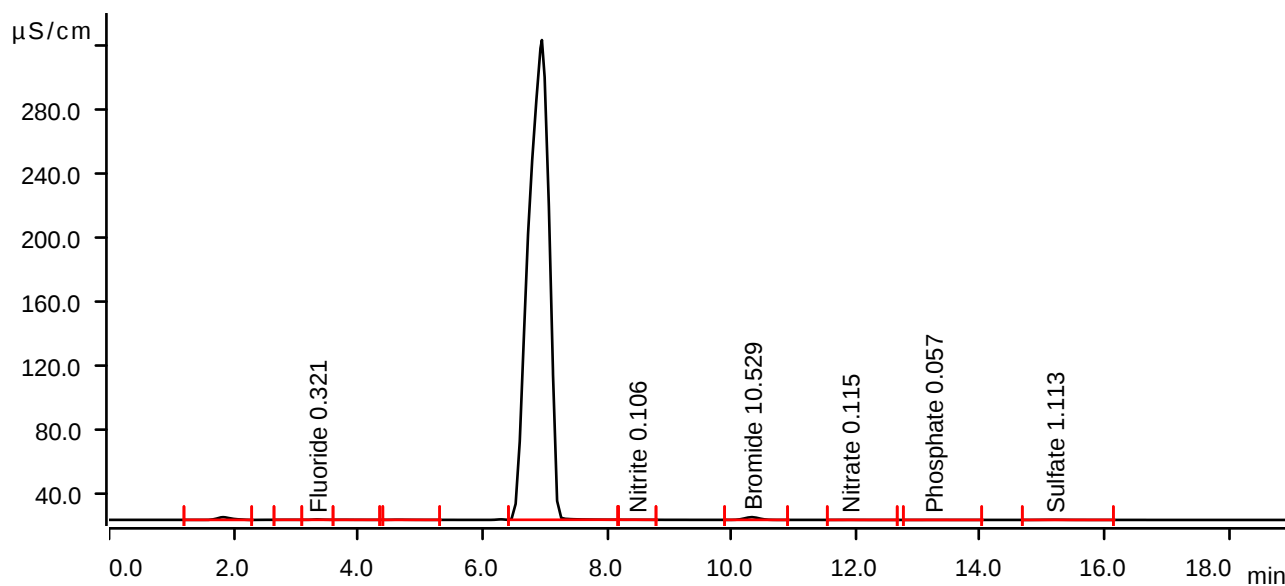

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.833	0.4631	1.708	invalid	
2	2.940	0.0045	0.019	invalid	
3	3.340	0.0434	0.231	0.321	Fluoride
4	3.767	0.0142	0.043	invalid	
5	4.638	0.0255	0.097	invalid	
6	6.957	114.3983	299.700	invalid	
7	8.455	0.0057	0.023	0.106	Nitrite
8	10.328	0.4668	1.706	10.529	Bromide
9	11.895	0.0135	0.042	0.115	Nitrate
10	13.238	0.0067	0.013	0.057	Phosphate
11	15.190	0.0529	0.113	1.113	Sulfate


Sample data

Ident Q3552-02
Sample type Sample
Determination start 2025-11-05 16:08:49 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

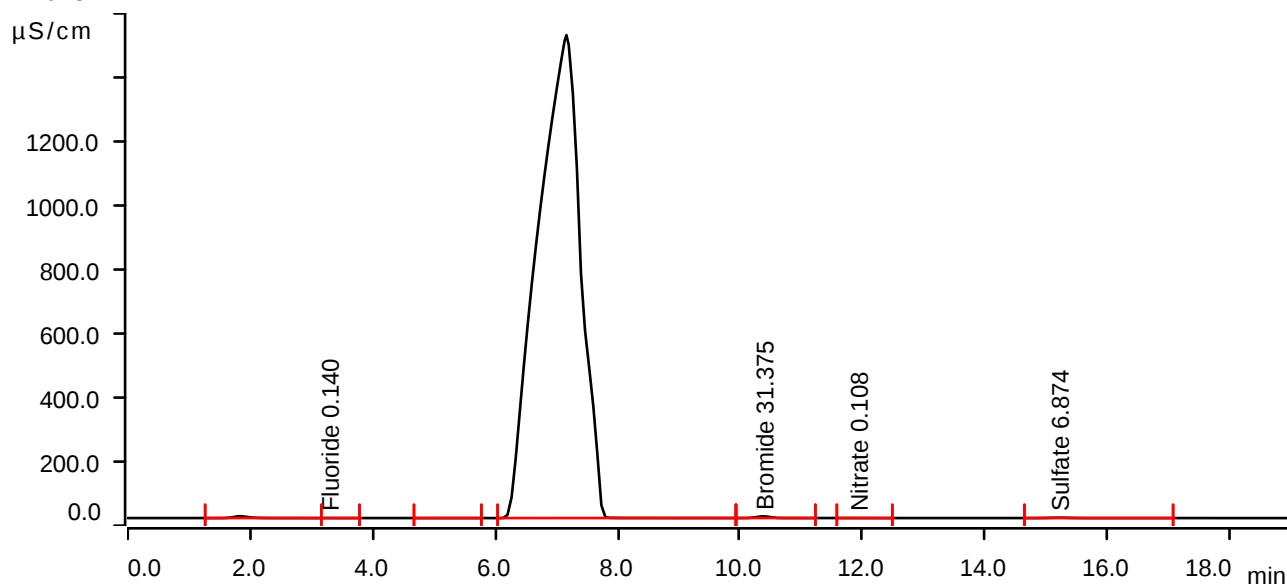

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.835	1.7634	5.946	invalid	
2	3.287	0.0168	0.053	0.140	Fluoride
3	5.007	0.0332	0.055	invalid	
4	7.163	1217.9805	1508.517	invalid	
5	10.378	1.4082	5.354	31.375	Bromide
6	11.918	0.0117	0.038	0.108	Nitrate
7	15.205	0.5041	1.174	6.874	Sulfate


Sample data

Ident Q3552-03
Sample type Sample
Determination start 2025-11-05 16:30:23 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

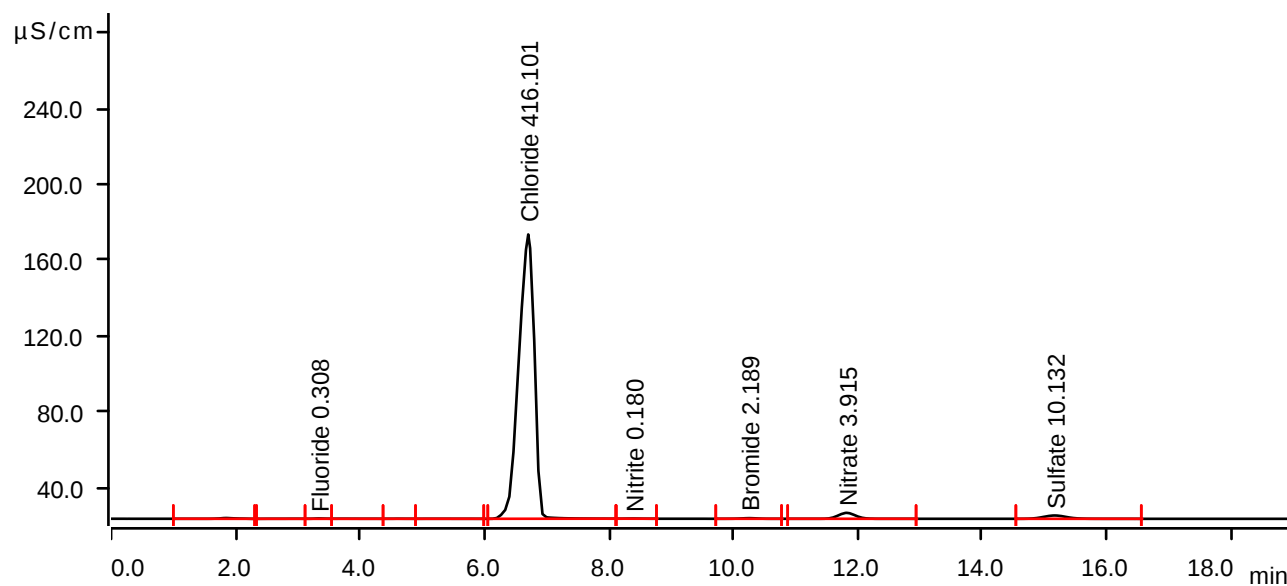

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.848	0.1283	0.424	invalid	
2	2.948	0.0307	0.051	invalid	
3	3.340	0.0415	0.194	0.308	Fluoride
4	3.775	0.0378	0.063	invalid	
5	4.608	0.0172	0.054	invalid	
6	5.263	0.0181	0.026	invalid	
7	6.705	43.2718	149.870	416.101	Chloride
8	8.388	0.0229	0.097	0.180	Nitrite
9	10.253	0.0901	0.317	2.189	Bromide
10	11.822	1.0049	3.124	3.915	Nitrate
11	15.165	0.7592	1.747	10.132	Sulfate


Sample data

Ident Q3552-04
Sample type Sample
Determination start 2025-11-05 16:51:58 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.37 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

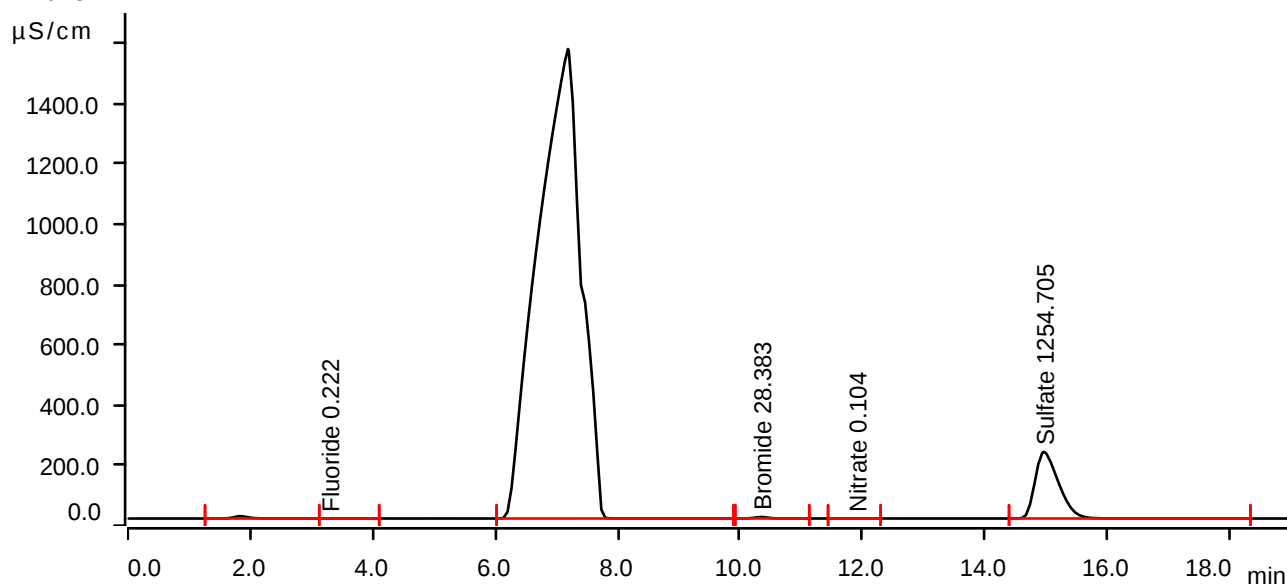

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.835	2.2969	7.898	invalid	
2	3.290	0.0289	0.066	0.222	Fluoride
3	7.188	1277.1984	1558.170	invalid	
4	10.345	1.2731	4.832	28.383	Bromide
5	11.878	0.0108	0.035	0.104	Nitrate
6	14.958	98.2193	221.381	1254.705	Sulfate


Sample data

Ident Q3552-04MS
Sample type Sample
Determination start 2025-11-05 17:13:33 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

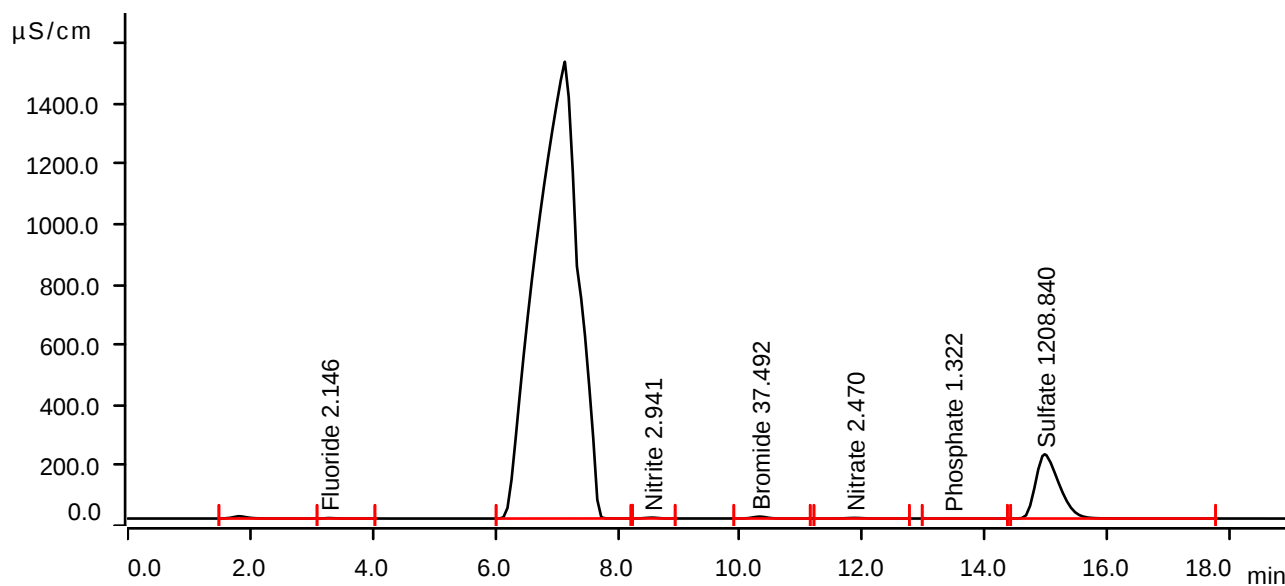

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.820	2.2009	7.551	invalid	
2	3.285	0.3109	1.583	2.146	Fluoride
3	7.138	1214.4626	1515.802	invalid	
4	8.563	0.6613	2.742	2.941	Nitrite
5	10.320	1.6844	6.223	37.492	Bromide
6	11.867	0.6279	2.002	2.470	Nitrate
7	13.470	0.1126	0.204	1.322	Phosphate
8	14.972	94.6277	213.173	1208.840	Sulfate


Sample data

Ident Q3552-04MSD
Sample type Sample
Determination start 2025-11-05 17:35:09 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

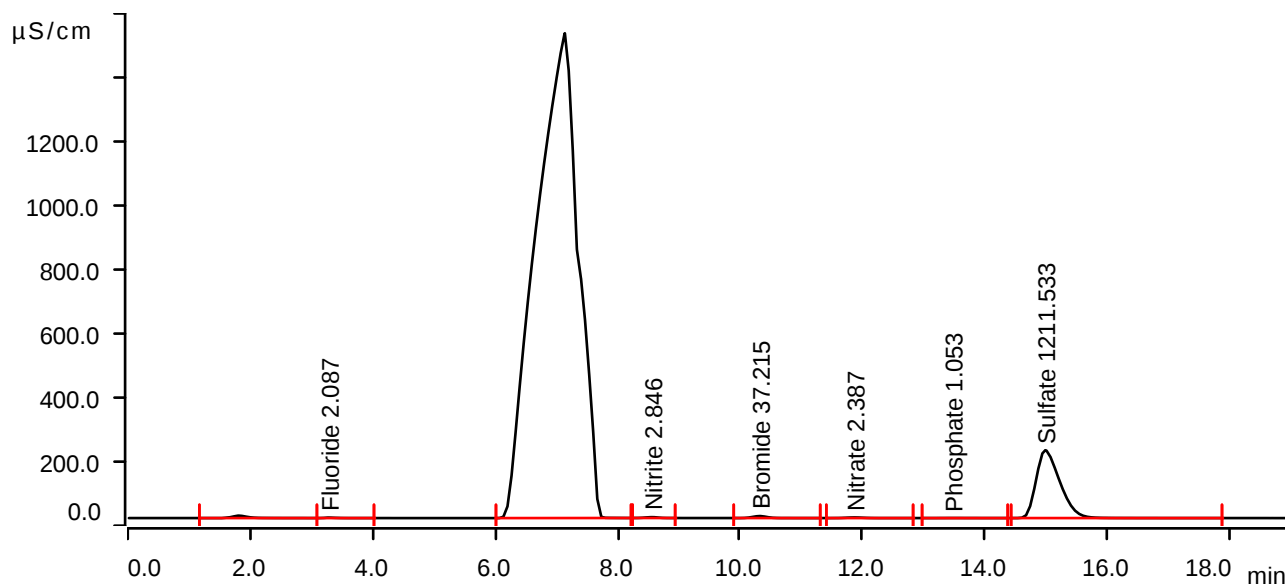

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.815	2.2469	7.588	invalid	
2	3.285	0.3024	1.528	2.087	Fluoride
3	7.138	1217.8740	1514.215	invalid	
4	8.562	0.6393	2.659	2.846	Nitrite
5	10.318	1.6719	6.154	37.215	Bromide
6	11.865	0.6063	1.925	2.387	Nitrate
7	13.483	0.0901	0.164	1.053	Phosphate
8	14.982	94.8386	212.003	1211.533	Sulfate


Sample data

Ident Q3552-05
Sample type Sample
Determination start 2025-11-05 17:56:43 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

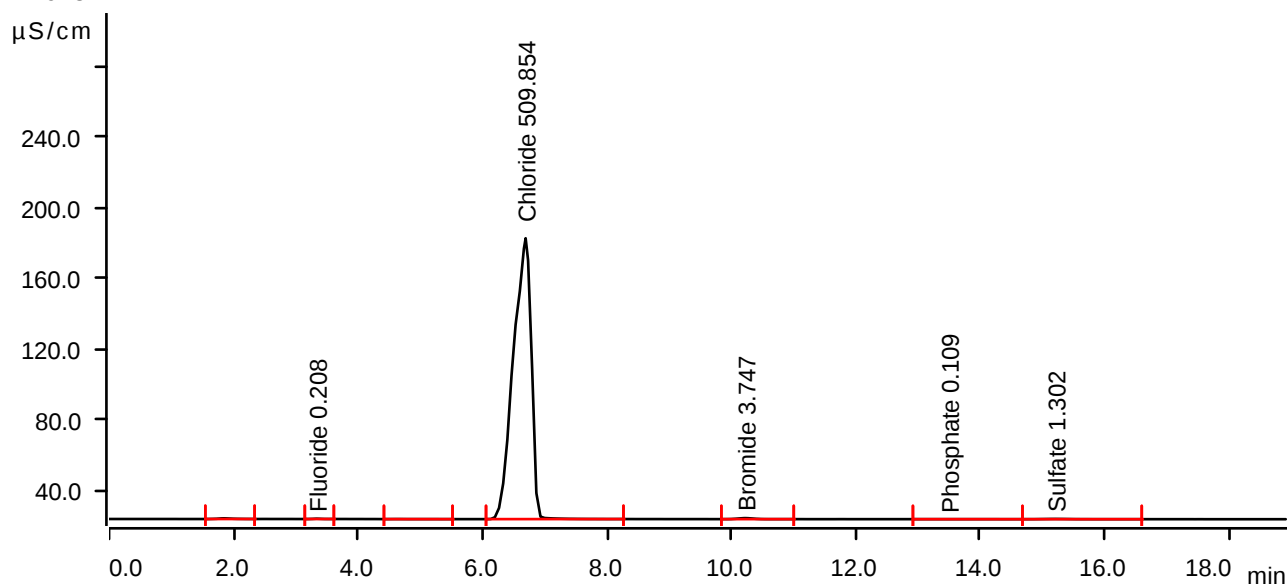

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.845	0.1001	0.381	invalid	
2	3.338	0.0269	0.190	0.208	Fluoride
3	4.617	0.0074	0.033	invalid	
4	6.695	53.0231	159.004	509.854	Chloride
5	10.225	0.1605	0.565	3.747	Bromide
6	13.492	0.0111	0.014	0.109	Phosphate
7	15.210	0.0677	0.143	1.302	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-11-05 19:01:01 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

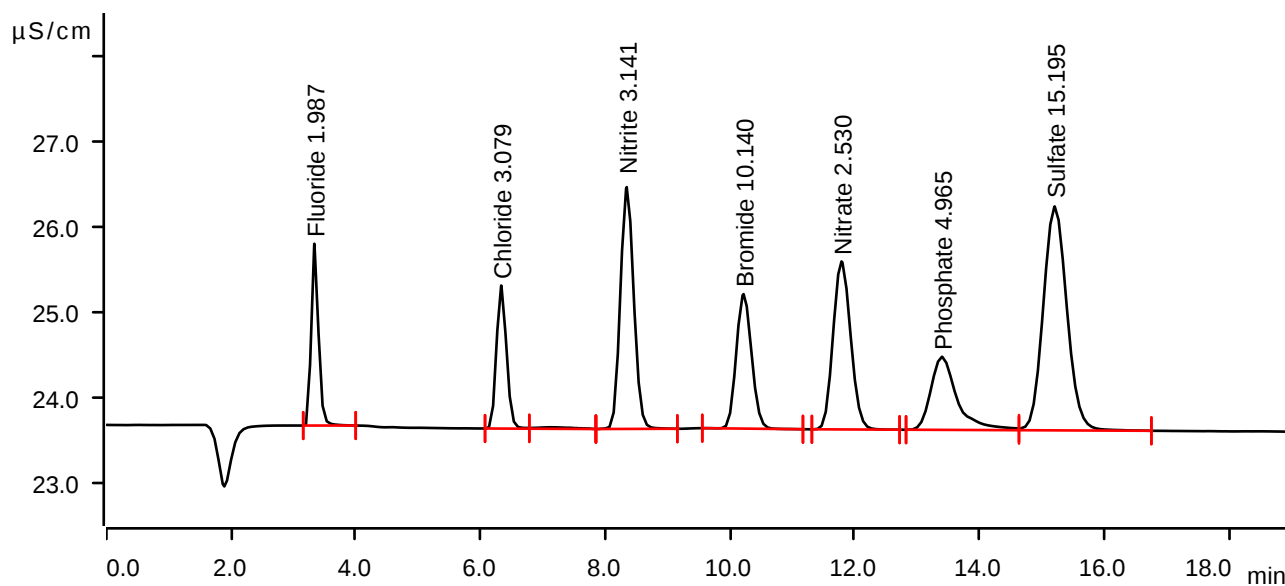

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.337	0.2877	2.129	1.987	Fluoride
2	6.330	0.3131	1.676	3.079	Chloride
3	7.108	0.0124	0.018	invalid	
4	8.343	0.7075	2.833	3.141	Nitrite
5	10.217	0.4492	1.576	10.140	Bromide
6	11.787	0.6435	1.967	2.530	Nitrate
7	13.397	0.4174	0.856	4.965	Phosphate
8	15.205	1.1557	2.623	15.195	Sulfate


Sample data

Ident CCB
Sample type Sample
Determination start 2025-11-05 19:22:32 UTC-5
Method IC1-110325
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

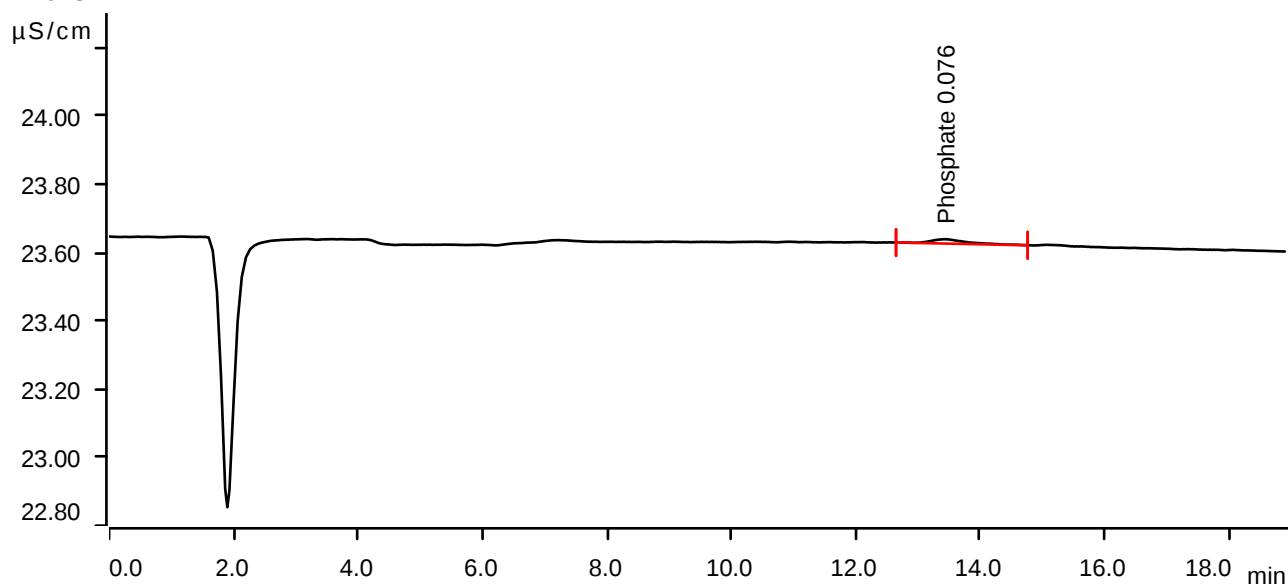

Peak number	Retention time	Area	Height	Concentration	Component name
	min	($\mu\text{S/cm}$) x min	$\mu\text{S/cm}$	ppm	
1	13.425	0.0083	0.013	0.076	Phosphate