

66137910

Test results

Aquakem 7.2AQ1

Page: 1

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

11/14/2025 16:20

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.732	0.0	0.084	
ICB1	0.704	0.0	0.001	
CCV1	239.127	0.0	0.214	
CCB1	1.138	0.0	0.002	
PB170559BL	1.134	0.0	0.002	
Q3628-04	0.553	0.0	0.001	
Q3628-04DUP	0.774	0.0	0.001	
Q3638-02	0.725	0.0	0.001	
Q3638-04	0.633	0.0	0.001	
Q3640-02	0.716	0.0	0.001	
Q3640-03	0.725	0.0	0.001	
Q3647-02	0.890	0.0	0.001	
CCV2	237.303	0.0	0.212	
CCB2	0.679	0.0	0.001	
PB170564BL	0.658	0.0	0.001	
Q3640-04	0.688	0.0	0.001	
Q3640-04DUP	0.733	0.0	0.001	
CCV3	242.318	0.0	0.217	
CCB3	1.067	0.0	0.002	
N	19			
Mean	43.384			
SD	89.8291			
CV%	207.05			

Aquakem v. 7.2AQ1

Results from time period:

Fri Nov 14 16:04:33 2025

Fri Nov 14 16:19:21 2025

Sample Id	Sam/Ctr/c#	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	-0.022	µg/l	11/14/2025 9:19:45	
5.0PPBCN	A	Total CN	P	5.343	µg/l	11/14/2025 9:19:46	
10PPBCN	A	Total CN	P	10.4033	µg/l	11/14/2025 9:19:47	
50PPBCN	A	Total CN	P	49.6432	µg/l	11/14/2025 9:19:48	
100PPBCN	A	Total CN	P	99.0638	µg/l	11/14/2025 9:19:49	
250PPBCN	A	Total CN	P	250.7143	µg/l	11/14/2025 9:19:50	
500PPBCN	A	Total CN	P	499.8543	µg/l	11/14/2025 9:19:51	
ICV1	S	Total CN	P	93.7322	µg/l	11/14/2025 16:04:34	
ICB1	S	Total CN	P	0.7044	µg/l	11/14/2025 16:04:35	
CCV1	S	Total CN	P	239.1275	µg/l	11/14/2025 16:04:38	
CCB1	S	Total CN	P	1.1377	µg/l	11/14/2025 16:04:40	
PB170559BL	S	Total CN	P	1.1343	µg/l	11/14/2025 16:04:41	
Q3628-04	S	Total CN	P	0.5529	µg/l	11/14/2025 16:12:05	
Q3628-04DUP	S	Total CN	P	0.7742	µg/l	11/14/2025 16:12:07	
Q3638-02	S	Total CN	P	0.7254	µg/l	11/14/2025 16:12:08	
Q3638-04	S	Total CN	P	0.6329	µg/l	11/14/2025 16:12:09	
Q3640-02	S	Total CN	P	0.7162	µg/l	11/14/2025 16:12:10	
Q3640-03	S	Total CN	P	0.7252	µg/l	11/14/2025 16:12:11	
Q3647-02	S	Total CN	P	0.8899	µg/l	11/14/2025 16:12:12	
CCV2	S	Total CN	P	237.3029	µg/l	11/14/2025 16:12:15	
CCB2	S	Total CN	P	0.6794	µg/l	11/14/2025 16:19:12	
PB170564BL	S	Total CN	P	0.6584	µg/l	11/14/2025 16:19:13	
Q3640-04	S	Total CN	P	0.6883	µg/l	11/14/2025 16:19:14	
Q3640-04DUP	S	Total CN	P	0.7331	µg/l	11/14/2025 16:19:15	
CCV3	S	Total CN	P	242.3183	µg/l	11/14/2025 16:19:20	
CCB3	S	Total CN	P	1.0667	µg/l	11/14/2025 16:19:21	

Alliance Technical Group
 284 Sheffield Street, Mountainside, NJ 07092

11/14/2025 9:20 Reviewed by : RM Instrument ID : Konelab


Test Total CN

Accepted 11/14/2025 9:20

Factor 1122
 Bias 0.001

Coeff. of det. 0.999991

Errors

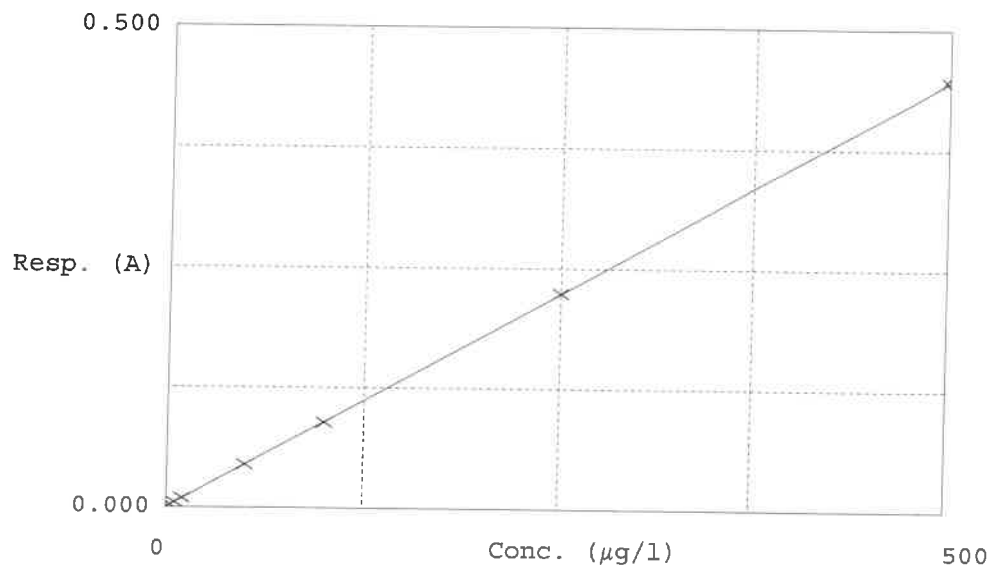

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.001	-0.0220	0.0000	-
2	5.0PPBCN	0.005	5.3430	5.0000	6.9
3	10PPBCN	0.010	10.4033	10.0000	4.0
4	50PPBCN	0.045	49.6432	50.0000	-0.7
5	100PPBCN	0.089	99.0638	100.0000	-0.9
6	250PPBCN	0.224	250.7143	250.0000	0.3
7	500PPBCN	0.446	499.8543	500.0000	0.0

11/14/2025
 RM