

66138003

Test results

Aquakem 7.2AQ1

Page: 1

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

11/21/2025 10:40

Test: CNEPA-NEW

Sample Id	Result	Dil. 1 +	Response	Errors
ICV001 ICV001	93.497	0.0	0.095	
ICB001 ICB001	0.630	0.0	0.007	
CCV001 CCV001	236.140	0.0	0.229	
CCB001 CCB001	1.088	0.0	0.008	
PB170669BL PBS669	0.913	0.0	0.007	
Q3589-04- MDL-SOIL-QT4-2025-08	4.813	0.0	0.011	
PB170670BL PBW670	0.233	0.0	0.007	
Q3589-02-MIX-WATER-QT4-2025-08	4.946	0.0	0.011	
CCV002 CCV002	244.843	0.0	0.237	
CCB002 CCB002	0.164	0.0	0.007	

N 10
Mean 58.727
SD 100.0076
CV% 170.29

Aquakem v. 7.2AQ1

Results from time period:

Fri Nov 21 09:55:09 2025

Fri Nov 21 10:39:31 2025

Sample Id	Sam	Test short r	Te	Result	Resul	Result date and time	Stat
S0.0	A	CNEPA-NE\ P		0.6462 µg/l		11/21/2025 9:55:09	
S5.0	A	CNEPA-NE\ P		5.043 µg/l		11/21/2025 9:55:10	
S10.0	A	CNEPA-NE\ P		10.0734 µg/l		11/21/2025 9:55:11	
S100.0	A	CNEPA-NE\ P		99.4278 µg/l		11/21/2025 9:55:12	
S250.0	A	CNEPA-NE\ P		249.3942 µg/l		11/21/2025 9:55:13	
S500.0	A	CNEPA-NE\ P		500.4154 µg/l		11/21/2025 9:55:14	
ICV001 ICB001	S	CNEPA-NE\ P		93.4975 µg/l		11/21/2025 10:32:45	
ICB001 ICB001	S	CNEPA-NE\ P		0.6299 µg/l		11/21/2025 10:32:46	
CCV001 CCV001	S	CNEPA-NE\ P		236.14 µg/l		11/21/2025 10:32:49	
CCB001 CCB001	S	CNEPA-NE\ P		1.088 µg/l		11/21/2025 10:32:51	
PB170669BL PBS669	S	CNEPA-NE\ P		0.9134 µg/l		11/21/2025 10:32:52	
Q3589-04-MDL-SOIL-QT4-2025-08	S	CNEPA-NE\ P		4.8128 µg/l		11/21/2025 10:32:54	
PB170670BL PBW670	S	CNEPA-NE\ P		0.2331 µg/l		11/21/2025 10:39:24	
Q3589-02-MDL-WATER-QT4-2025-08	S	CNEPA-NE\ P		4.9456 µg/l		11/21/2025 10:39:27	
CCV002 CCV002	S	CNEPA-NE\ P		244.8428 µg/l		11/21/2025 10:39:29	
CCB002 CCB002	S	CNEPA-NE\ P		0.1641 µg/l		11/21/2025 10:39:31	

Calibration results

Aquakem 7.2AQ1

Page: 1

Alliance Technical Group
284 Sheffield Street, Mountainside, NJ 07092

11/21/2025 10:07

Reviewed by : RM

Instrument ID : Konelab


Test CNEPA-NEW

Accepted 11/21/2025 10:07

Factor slope 1063 0.000941
Bias Intercept 0.007 11/25/2025
RM

Coeff. of det. 0.999994

Errors

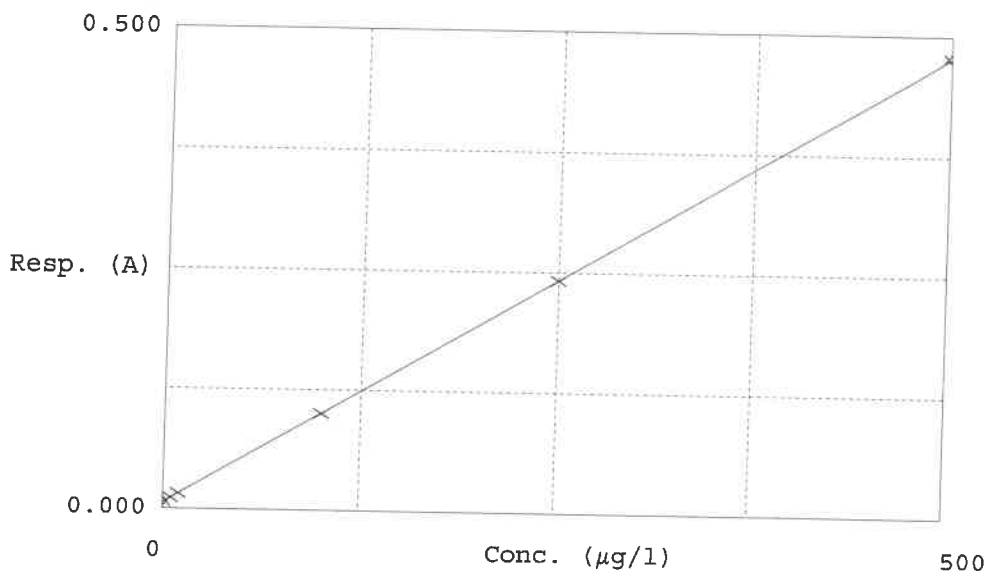

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN50.0	0.007	0.6462	0.0000	-
2	5.0PPBCN55.0	0.011	5.0430	5.0000	0.9
3	10PPBCN510.0	0.016	10.0734	10.0000	0.7
4	100PPBCN5100.0	0.100	99.4278	100.0000	-0.6
5	250PPBCN5250.0	0.241	249.3942	250.0000	-0.2
6	500PPBCN5500.0	0.478	500.4154	500.0000	0.1

11/21/2025
RM