

16138010

Test results

Aquakem 7.2AQ1

Page: 1

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

11/21/2025 15:27

Reviewed by : RM

Instrument ID : Konelab

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.993	0.0	0.105	
ICB1	-0.009	0.0	0.008	
CCV1	0.998	0.0	0.106	
CCB1	-0.006	0.0	0.008	
PB170666BL	-0.006	0.0	0.008	
PB170666BS	0.987	0.0	0.105	
Q3530-03	0.020	0.0	0.011	
PB170668BL	-0.008	0.0	0.008	
PB170668BS	0.991	0.0	0.105	
Q3530-09	0.020	0.0	0.011	
CCV2	0.987	0.0	0.105	
CCB2	-0.007	0.0	0.008	

N 12
Mean 0.413
SD 0.5103
CV% 123.42

Aquakem v. 7.2AQ1

Results from time period:

Fri Nov 21 12:49:48 2025

Fri Nov 21 15:23:32 2025

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.00PPM	A	Phenolics-	P	-0.0018	mg/l	11/21/2025 12:49:48	
0.05PPM	A	Phenolics-	P	0.0476	mg/l	11/21/2025 12:49:49	
0.1PPM	A	Phenolics-	P	0.0997	mg/l	11/21/2025 12:49:50	
0.25PPM	A	Phenolics-	P	0.2592	mg/l	11/21/2025 12:49:51	
0.50PPM	A	Phenolics-	P	0.4992	mg/l	11/21/2025 12:49:52	
1.0PPM	A	Phenolics-	P	0.9941	mg/l	11/21/2025 12:49:53	
2.0PPM	A	Phenolics-	P	2.0021	mg/l	11/21/2025 12:49:54	
ICV1	S	Phenolics-	P	0.993	mg/l	11/21/2025 15:23:21	
ICB1	S	Phenolics-	P	-0.0087	mg/l	11/21/2025 15:23:22	
CCV1	S	Phenolics-	P	0.9982	mg/l	11/21/2025 15:23:23	
CCB1	S	Phenolics-	P	-0.0063	mg/l	11/21/2025 15:23:24	
PB170666BL	S	Phenolics-	P	-0.0064	mg/l	11/21/2025 15:23:25	
PB170666BS	S	Phenolics-	P	0.9874	mg/l	11/21/2025 15:23:26	
Q3530-03	S	Phenolics-	P	0.0203	mg/l	11/21/2025 15:23:27	
PB170668BL	S	Phenolics-	P	-0.0079	mg/l	11/21/2025 15:23:28	
PB170668BS	S	Phenolics-	P	0.9914	mg/l	11/21/2025 15:23:29	
Q3530-09	S	Phenolics-	P	0.02	mg/l	11/21/2025 15:23:30	
CCV2	S	Phenolics-	P	0.9869	mg/l	11/21/2025 15:23:31	
CCB2	S	Phenolics-	P	-0.0066	mg/l	11/21/2025 15:23:32	

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

11/21/2025 12:56

Reviewed by : RM

Instrument ID : Konelab


Test Phenolics-

Accepted 11/21/2025 12:56

Factor 10.28
Bias 0.009

Coeff. of det. 0.999958

Errors

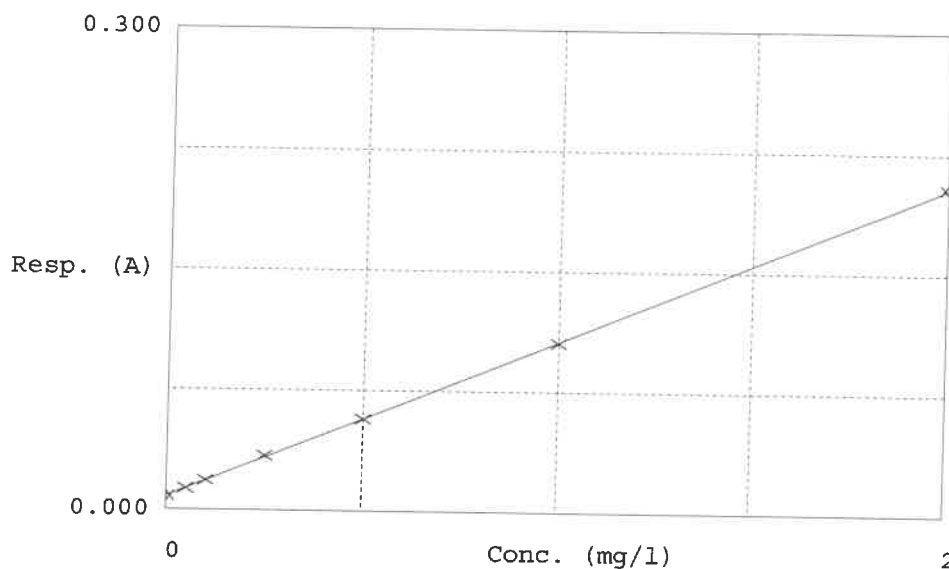

	Calibrator	Response	Calc. con.	Conc.	Re Errors
1	0.00PPM	0.008	-0.0018	0.0000	-
2	Phenol-2	0.013	0.0476	0.0500	-4.8
3	Phenol-2	0.018	0.0997	0.1000	-0.3
4	Phenol-2	0.034	0.2592	0.2500	3.7
5	Phenol-2	0.057	0.4992	0.5000	-0.2
6	Phenol-2	0.105	0.9941	1.0000	-0.6
7	Phenol-2	0.203	2.0021	2.0000	0.1

11/21/2025

RM