

65138031

=====

Test results

Aquakem 7.2AQ1

Page: 1

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

11/24/2025 14:40

Reviewed by : RM

Instrument ID : Konelab

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.832	0.0	0.082	
ICB1	0.709	0.0	0.001	
CCV1	244.464	0.0	0.204	
CCB1	0.740	0.0	0.001	
PB170698BL	0.618	0.0	0.001	
Q3697-04	0.554	0.0	0.001	
Q3697-04DUP	0.514	0.0	0.001	
PB170699BL	0.620	0.0	0.001	
Q3697-01	0.572	0.0	0.001	
Q3697-01DUP	0.517	0.0	0.001	
Q3697-02	0.363	0.0	0.001	
Q3697-03	0.615	0.0	0.001	
Q3707-03	0.738	0.0	0.001	
Q3710-02	0.798	0.0	0.002	
CCV2	243.195	0.0	0.203	
CCB2	0.874	0.0	0.002	
Q3710-04	0.510	0.0	0.001	
Q3710-06	0.611	0.0	0.001	
Q3711-02	0.759	0.0	0.001	
Q3711-04	0.748	0.0	0.001	
CCV3	246.335	0.0	0.205	
CCB3	0.820	0.0	0.002	

N	22
Mean	38.341
SD	86.4168
CV%	225.39

Aquakem v. 7.2AQ1

Results from time period:

Mon Nov 24 14:16:41 2025

Mon Nov 24 14:39:33 2025

Sample Id	Sam/Ctr/c/	Test short r	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.8561	µg/l	11/24/2025 10:00:18	
5.0PPBCN	A	Total CN	P	5.4993	µg/l	11/24/2025 10:00:19	
10PPBCN	A	Total CN	P	10.1742	µg/l	11/24/2025 10:00:20	
50PPBCN	A	Total CN	P	47.955	µg/l	11/24/2025 10:00:21	
100PPBCN	A	Total CN	P	100.4082	µg/l	11/24/2025 10:00:22	
250PPBCN	A	Total CN	P	249.9857	µg/l	11/24/2025 10:00:23	
500PPBCN	A	Total CN	P	500.1216	µg/l	11/24/2025 10:00:24	
ICV1	S	Total CN	P	97.832	µg/l	11/24/2025 14:16:41	
ICB1	S	Total CN	P	0.7091	µg/l	11/24/2025 14:16:43	
CCV1	S	Total CN	P	244.4643	µg/l	11/24/2025 14:16:45	
CCB1	S	Total CN	P	0.7399	µg/l	11/24/2025 14:16:48	
PB170698BL	S	Total CN	P	0.6185	µg/l	11/24/2025 14:16:50	
Q3697-04	S	Total CN	P	0.5541	µg/l	11/24/2025 14:24:18	
Q3697-04DUP	S	Total CN	P	0.5144	µg/l	11/24/2025 14:24:19	
PB170699BL	S	Total CN	P	0.6204	µg/l	11/24/2025 14:24:22	
Q3697-01	S	Total CN	P	0.5721	µg/l	11/24/2025 14:24:23	
Q3697-01DUP	S	Total CN	P	0.5174	µg/l	11/24/2025 14:24:26	
Q3697-02	S	Total CN	P	0.363	µg/l	11/24/2025 14:31:48	
Q3697-03	S	Total CN	P	0.615	µg/l	11/24/2025 14:31:49	
Q3707-03	S	Total CN	P	0.7383	µg/l	11/24/2025 14:31:50	
Q3710-02	S	Total CN	P	0.7982	µg/l	11/24/2025 14:31:51	
CCV2	S	Total CN	P	243.1948	µg/l	11/24/2025 14:31:55	
CCB2	S	Total CN	P	0.8742	µg/l	11/24/2025 14:31:58	
Q3710-04	S	Total CN	P	0.51	µg/l	11/24/2025 14:39:23	
Q3710-06	S	Total CN	P	0.6109	µg/l	11/24/2025 14:39:24	
Q3711-02	S	Total CN	P	0.7592	µg/l	11/24/2025 14:39:25	
Q3711-04	S	Total CN	P	0.7482	µg/l	11/24/2025 14:39:26	
CCV3	S	Total CN	P	246.3345	µg/l	11/24/2025 14:39:30	
CCB3	S	Total CN	P	0.8199	µg/l	11/24/2025 14:39:33	

Alliance Technical Group

284 Sheffield Street, Mountainside, NJ 07092

Reviewed by : RM

Instrument ID : Konelab

11/24/2025 10:01


Test Total CN

Accepted 11/24/2025 10:01

Factor 1206
Bias 0.001

Coeff. of det. 0.999974

Errors

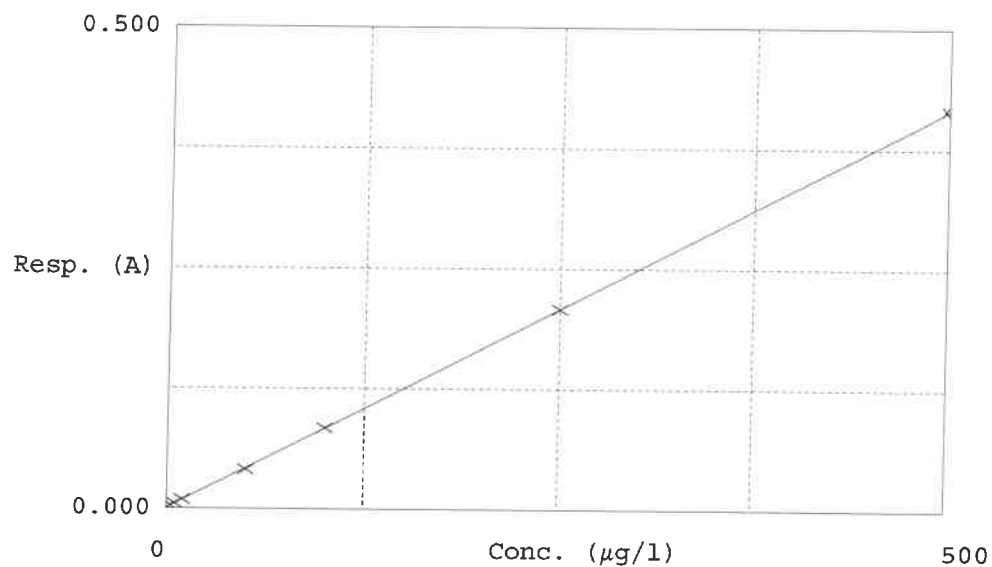

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.002	0.8561	0.0000	-
2	5.0PPBCN	0.005	5.4993	5.0000	10.0
3	10PPBCN	0.009	10.1742	10.0000	1.7
4	50PPBCN	0.041	47.9550	50.0000	-4.1
5	100PPBCN	0.084	100.4082	100.0000	0.4
6	250PPBCN	0.208	249.9857	250.0000	0.0
7	500PPBCN	0.416	500.1216	500.0000	0.0

11/24/2025
RM