


Ident	Instrument IC-1			Analyst: RM		Method: 300.0 / 9056A		Method name date time	Initial w/ Analyst	
	Con F-	Con CL-	Con NO2	Con BR-	Con NO3	Con HPO4	Con SO4			
STD1	0.000	0.000	0.000	0.000	0.000	0.000	0.000	0.000 IC1-120125	12/1/2025 11:48	10 RM/IZ
STD2	0.412	0.635	0.639	2.103	0.536	0.913	3.265	IC1-120125	12/1/2025 12:09	10 RM/IZ
STD3	0.798	1.201	1.199	4.008	0.999	2.097	5.981	IC1-120125	12/1/2025 12:52	10 RM/IZ
STD4	0.975	1.481	1.479	4.937	1.234	2.295	7.437	IC1-120125	12/1/2025 13:13	10 RM/IZ
STD5	2.015	2.982	2.983	9.952	2.481	5.096	14.845	IC1-120125	12/1/2025 13:35	10 RM/IZ
STD6	4.009	5.961	5.958	19.885	4.959	10.523	29.548	IC1-120125	12/1/2025 13:57	10 RM/IZ
STD7	4.991	7.539	7.542	25.114	6.291	12.075	37.424	IC1-120125	12/1/2025 14:18	10 RM/IZ
ICV	2.032	2.991	2.998	10.111	2.458	5.430	14.904	IC1-120125	12/1/2025 14:40	10 RM/IZ
ICB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-120125	12/1/2025 14:58	10 RM/IZ
CCV	2.101	3.131	3.137	10.450	2.593	5.064	15.536	IC1-120125	12/2/2025 11:05	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-120125	12/2/2025 11:26	10 RM/IZ
LB138084BLW	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-120125	12/2/2025 11:48	10 RM/IZ
LB138084BSW	2.148	3.195	3.180	10.677	2.664	5.450	16.057	IC1-120125	12/2/2025 12:09	10 RM/IZ
Q3737-01	0.207	38.229	0.098	0.000	1.506	0.494	127.879	IC1-120125	12/2/2025 12:31	10 RM/IZ
Q3737-02	0.078	15.776	411.917	0.402	1.193	0.072	1206.334	IC1-120125	12/2/2025 12:58	10 RM/IZ
Q3737-02MS	2.251	19.602	3.393	10.878	3.765	5.437	1176.116	IC1-120125	12/2/2025 13:21	10 RM/IZ
Q3737-02MSD	2.256	19.529	3.288	10.522	3.670	5.671	1161.278	IC1-120125	12/2/2025 13:43	10 RM/IZ
Q3737-01DLX10	0.036	3.199	0.000	0.000	0.190	0.112	10.980	IC1-120125	12/2/2025 14:05	10 RM/IZ
Q3737-02DLX50	0.000	0.326	0.000	0.000	0.077	0.000	16.487	IC1-120125	12/2/2025 14:26	10 RM/IZ
CCV	2.111	3.155	3.164	10.566	2.623	5.818	15.507	IC1-120125	12/2/2025 14:48	10 RM/IZ
CCB	0.000	0.000	0.000	0.000	0.000	0.000	0.000	IC1-120125	12/2/2025 15:09	10 RM/IZ

Clear table

Instrument ID: IC-2 Analyst : IZ Method: 300.0 / 9056A										
ident	concentra tion F-	concentratio n CL-	concentratio on NO2	concentratio on BR-	concentratio on NO3	concentratio on HPO4	concentratio on SO4	file name	date time	Initial wt/ Final Analyst
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000 IC1-120125	12/1/2025 11:48	10 RM/IZ
STD2	0.4120	0.6350	0.6390	2.1030	0.5360	0.9130	3.2650	IC1-120125	12/1/2025 12:09	10 RM/IZ
STD3	0.7980	1.2010	1.1990	4.0080	0.9990	2.0970	5.9810	IC1-120125	12/1/2025 12:52	10 RM/IZ
STD4	0.9750	1.4810	1.4790	4.9370	1.2340	2.2950	7.4370	IC1-120125	12/1/2025 13:13	10 RM/IZ
STD5	2.0150	2.9820	2.9830	9.9520	2.4810	5.0960	14.8450	IC1-120125	12/1/2025 13:35	10 RM/IZ
STD6	4.0090	5.9610	5.9580	19.8850	4.9590	10.5230	29.5480	IC1-120125	12/1/2025 13:57	10 RM/IZ
STD7	4.9910	7.5390	7.5420	25.1140	6.2910	12.0750	37.4240	IC1-120125	12/1/2025 14:18	10 RM/IZ
True Value										
ident	True Value F-	True Value CL-	True Value NO2	True Value BR-	True Value NO3	True Value HPO4	True Value SO4			
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000			
STD2	0.4000	0.6000	0.6000	2.0000	0.5000	1.0000	3.0000			
STD3	0.8000	1.2000	1.2000	4.0000	1.0000	2.0000	6.0000			
STD4	1.0000	1.5000	1.5000	5.0000	1.2500	2.5000	7.5000			
STD5	2.0000	3.0000	3.0000	10.0000	2.5000	5.0000	15.0000			
STD6	4.0000	6.0000	6.0000	20.0000	5.0000	10.0000	30.0000			
STD7	5.0000	7.5000	7.5000	25.0000	6.2500	12.5000	37.0000			
Relative Error										
ident	Relative Error F-	Relative Error CL-	Relative Error NO2	Relative Error BR-	Relative Error NO3	Relative Error HPO4	Relative Error SO4			
STD1										
STD2	3.0000	5.8333	6.5000	5.1500	7.2000	-8.7000	8.8333			
STD3	-0.2500	0.0833	-0.0833	0.2000	-0.1000	4.8500	-0.3167			
STD4	-2.5000	-1.2667	-1.4000	-1.2600	-1.2800	-8.2000	-0.8400			
STD5	0.7500	-0.6000	-0.5667	-0.4800	-0.7600	1.9200	-1.0333			
STD6	0.2250	-0.6500	-0.7000	-0.5750	-0.8200	5.2300	-1.5067			
STD7	-0.1800	0.5200	0.5600	0.4560	0.6560	-3.4000	1.1459			

Fluoride (Anions)

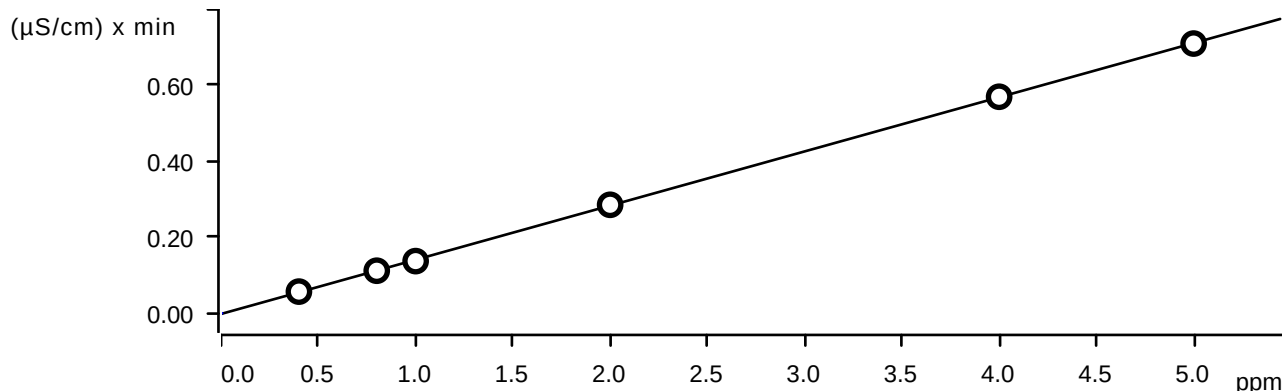


Function: $A = -1.71119\text{E-}3 + 0.0142641 \times Q$

Relative standard deviation 0.777267 %

Correlation coefficient 0.999967

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-12-01 11:48:15 UTC-5	used
Standard 2	1	0.400	10.0	1.0	1.0	0.057	STD2	2025-12-01 12:09:37 UTC-5	used
Standard 3	1	0.800	10.0	1.0	1.0	0.112	STD3	2025-12-01 12:52:25 UTC-5	used
Standard 4	1	1.000	10.0	1.0	1.0	0.137	STD4	2025-12-01 13:13:50 UTC-5	used
Standard 5	1	2.000	10.0	1.0	1.0	0.286	STD5	2025-12-01 13:35:52 UTC-5	used
Standard 6	1	4.000	10.0	1.0	1.0	0.570	STD6	2025-12-01 13:57:13 UTC-5	used
Standard 7	1	5.000	10.0	1.0	1.0	0.710	STD7	2025-12-01 14:18:41 UTC-5	used

Chloride (Anions)

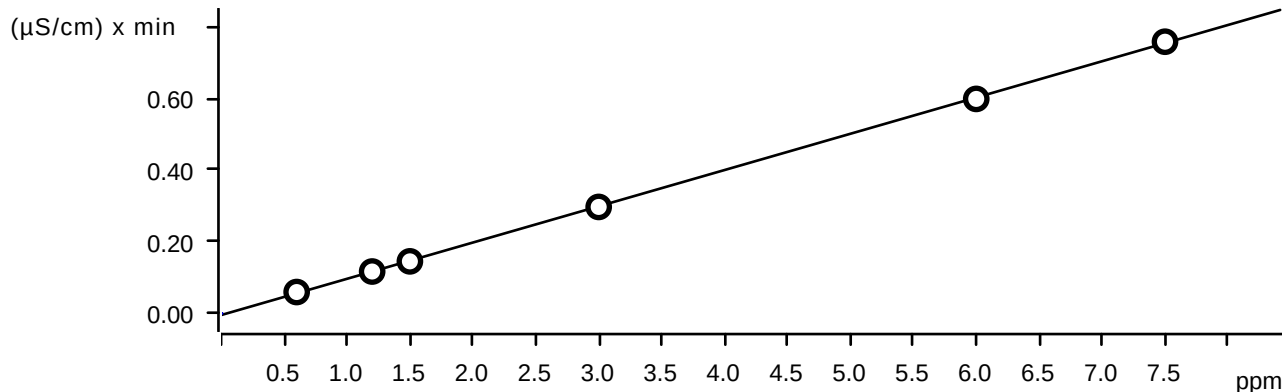


Function: $A = -4.50795\text{E-}3 + 0.0101091 \times Q$

Relative standard deviation 1.077238 %
 Correlation coefficient 0.999938

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-12-01 11:48:15 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.060	STD2	2025-12-01 12:09:37 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.117	STD3	2025-12-01 12:52:25 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.145	STD4	2025-12-01 13:13:50 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.297	STD5	2025-12-01 13:35:52 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	0.598	STD6	2025-12-01 13:57:13 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	0.758	STD7	2025-12-01 14:18:41 UTC-5	used

Nitrite (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

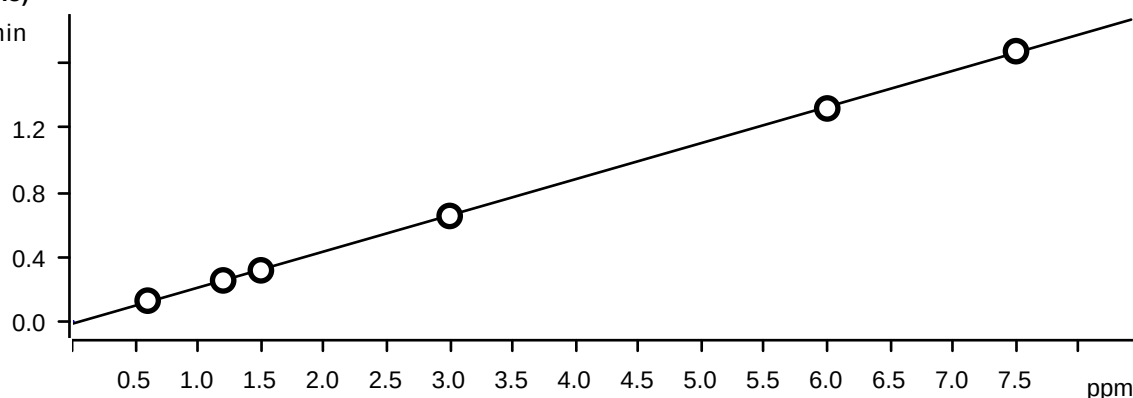


Function: $A = -0.0147505 + 0.0223943 \times Q$
 Relative standard deviation 1.183356 %
 Correlation coefficient 0.999927

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-12-01 11:48:15 UTC-5	used
Standard 2	1	0.600	10.0	1.0	1.0	0.128	STD2	2025-12-01 12:09:37 UTC-5	used
Standard 3	1	1.200	10.0	1.0	1.0	0.254	STD3	2025-12-01 12:52:25 UTC-5	used
Standard 4	1	1.500	10.0	1.0	1.0	0.316	STD4	2025-12-01 13:13:50 UTC-5	used
Standard 5	1	3.000	10.0	1.0	1.0	0.653	STD5	2025-12-01 13:35:52 UTC-5	used
Standard 6	1	6.000	10.0	1.0	1.0	1.319	STD6	2025-12-01 13:57:13 UTC-5	used
Standard 7	1	7.500	10.0	1.0	1.0	1.674	STD7	2025-12-01 14:18:41 UTC-5	used

Bromide (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

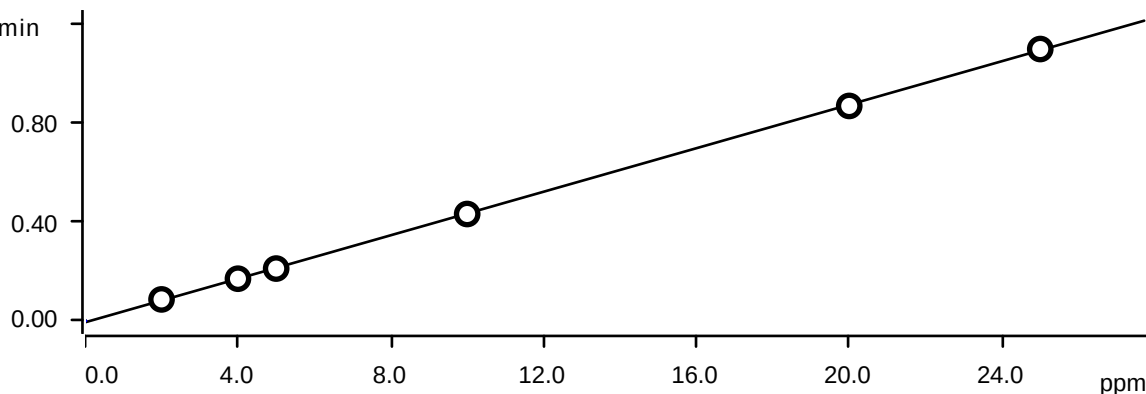

Function: $A = -5.85906E-3 + 4.38185E-3 \times Q$


Relative standard deviation 0.955560 %

Correlation coefficient 0.999951

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-12-01 11:48:15 UTC-5	used
Standard 2	1	2.000	10.0	1.0	1.0	0.086	STD2	2025-12-01 12:09:37 UTC-5	used
Standard 3	1	4.000	10.0	1.0	1.0	0.170	STD3	2025-12-01 12:52:25 UTC-5	used
Standard 4	1	5.000	10.0	1.0	1.0	0.210	STD4	2025-12-01 13:13:50 UTC-5	used
Standard 5	1	10.000	10.0	1.0	1.0	0.430	STD5	2025-12-01 13:35:52 UTC-5	used
Standard 6	1	20.000	10.0	1.0	1.0	0.865	STD6	2025-12-01 13:57:13 UTC-5	used
Standard 7	1	25.000	10.0	1.0	1.0	1.095	STD7	2025-12-01 14:18:41 UTC-5	used

Nitrate (Anions)

($\mu\text{S}/\text{cm}$) $\times$ min

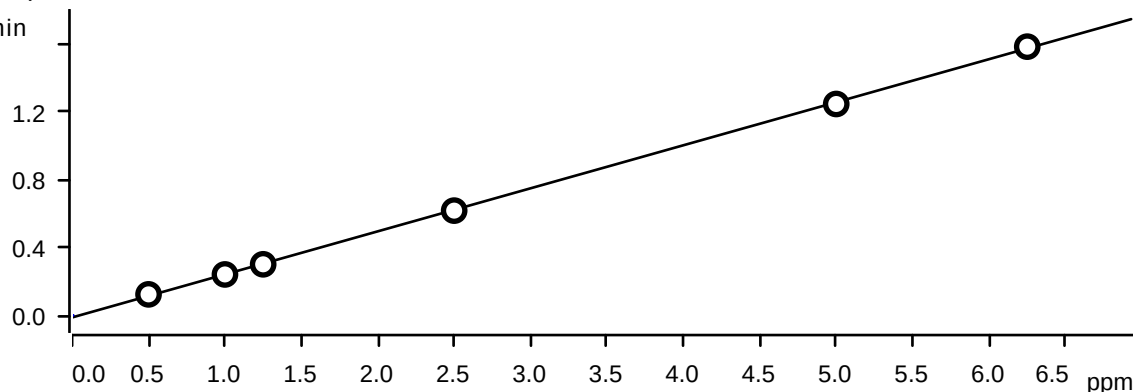

Function: $A = -0.0119899 + 0.0253343 \times Q$


Relative standard deviation 1.343370 %

Correlation coefficient 0.999905

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-12-01 11:48:15 UTC-5	used
Standard 2	1	0.500	10.0	1.0	1.0	0.124	STD2	2025-12-01 12:09:37 UTC-5	used
Standard 3	1	1.000	10.0	1.0	1.0	0.241	STD3	2025-12-01 12:52:25 UTC-5	used
Standard 4	1	1.250	10.0	1.0	1.0	0.301	STD4	2025-12-01 13:13:50 UTC-5	used
Standard 5	1	2.500	10.0	1.0	1.0	0.617	STD5	2025-12-01 13:35:52 UTC-5	used
Standard 6	1	5.000	10.0	1.0	1.0	1.244	STD6	2025-12-01 13:57:13 UTC-5	used
Standard 7	1	6.250	10.0	1.0	1.0	1.582	STD7	2025-12-01 14:18:41 UTC-5	used

Phosphate (Anions)


(μS/cm) x min

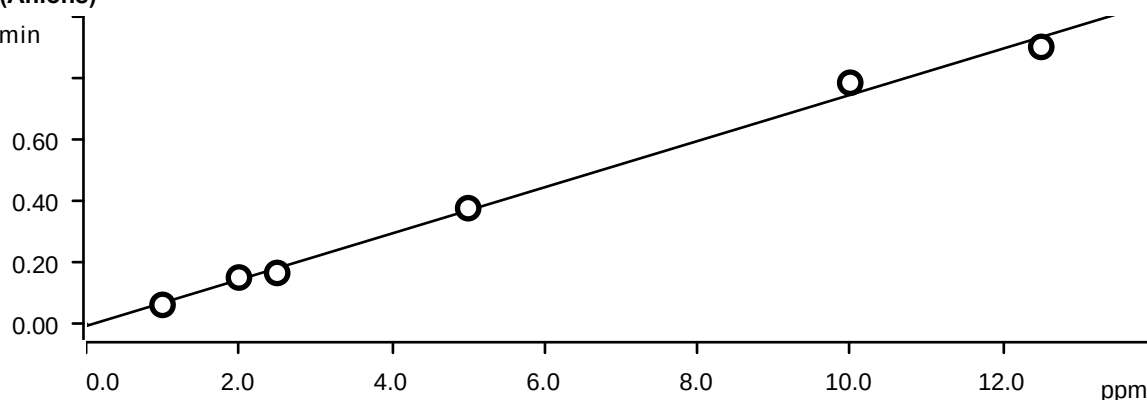Function: $A = -5.90721E-3 + 7.51764E-3 \times Q$

Relative standard deviation 6.666731 %

Correlation coefficient 0.997655

Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-12-01 11:48:15 UTC-5	used
Standard 2	1	1.000	10.0	1.0	1.0	0.063	STD2	2025-12-01 12:09:37 UTC-5	used
Standard 3	1	2.000	10.0	1.0	1.0	0.152	STD3	2025-12-01 12:52:25 UTC-5	used
Standard 4	1	2.500	10.0	1.0	1.0	0.167	STD4	2025-12-01 13:13:50 UTC-5	used
Standard 5	1	5.000	10.0	1.0	1.0	0.377	STD5	2025-12-01 13:35:52 UTC-5	used
Standard 6	1	10.000	10.0	1.0	1.0	0.785	STD6	2025-12-01 13:57:13 UTC-5	used
Standard 7	1	12.500	10.0	1.0	1.0	0.902	STD7	2025-12-01 14:18:41 UTC-5	used

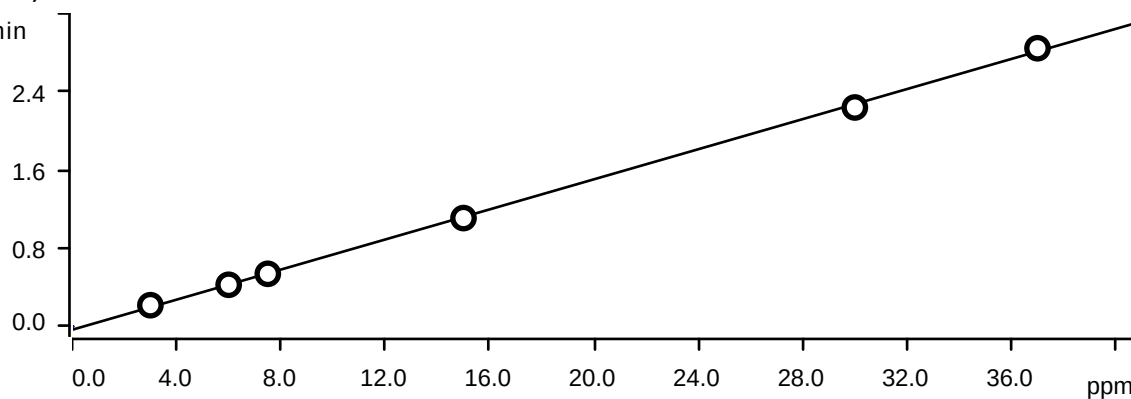Sulfate (Anions) $(\mu\text{S}/\text{cm}) \times \text{min}$ Function: $A = -0.0335409 + 7.69031E-3 \times Q$

Relative standard deviation 2.174138 %

Correlation coefficient 0.999753


Sample type	Index	Conc.	Volume	Dilution	Sample amount	Area	Ident	Date	Used
Standard 1	1	0.000	10.0	1.0	1.0	n. d.	STD1	2025-12-01 11:48:15 UTC-5	used
Standard 2	1	3.000	10.0	1.0	1.0	0.218	STD2	2025-12-01 12:09:37 UTC-5	used
Standard 3	1	6.000	10.0	1.0	1.0	0.426	STD3	2025-12-01 12:52:25 UTC-5	used
Standard 4	1	7.500	10.0	1.0	1.0	0.538	STD4	2025-12-01 13:13:50 UTC-5	used
Standard 5	1	15.000	10.0	1.0	1.0	1.108	STD5	2025-12-01 13:35:52 UTC-5	used
Standard 6	1	30.000	10.0	1.0	1.0	2.239	STD6	2025-12-01 13:57:13 UTC-5	used
Standard 7	1	37.000	10.0	1.0	1.0	2.844	STD7	2025-12-01 14:18:41 UTC-5	used

Sample data

Ident STD1
Sample type Standard 1
Determination start 2025-12-01 11:48:15 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

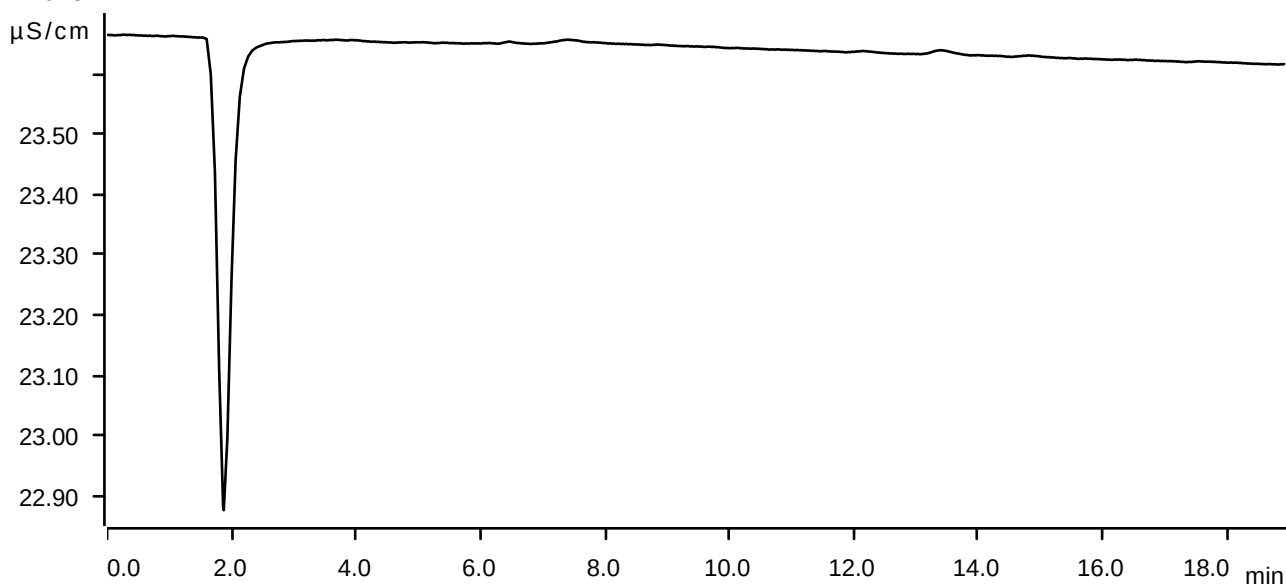Anions


Sample data

Ident STD2
Sample type Standard 2
Determination start 2025-12-01 12:09:37 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

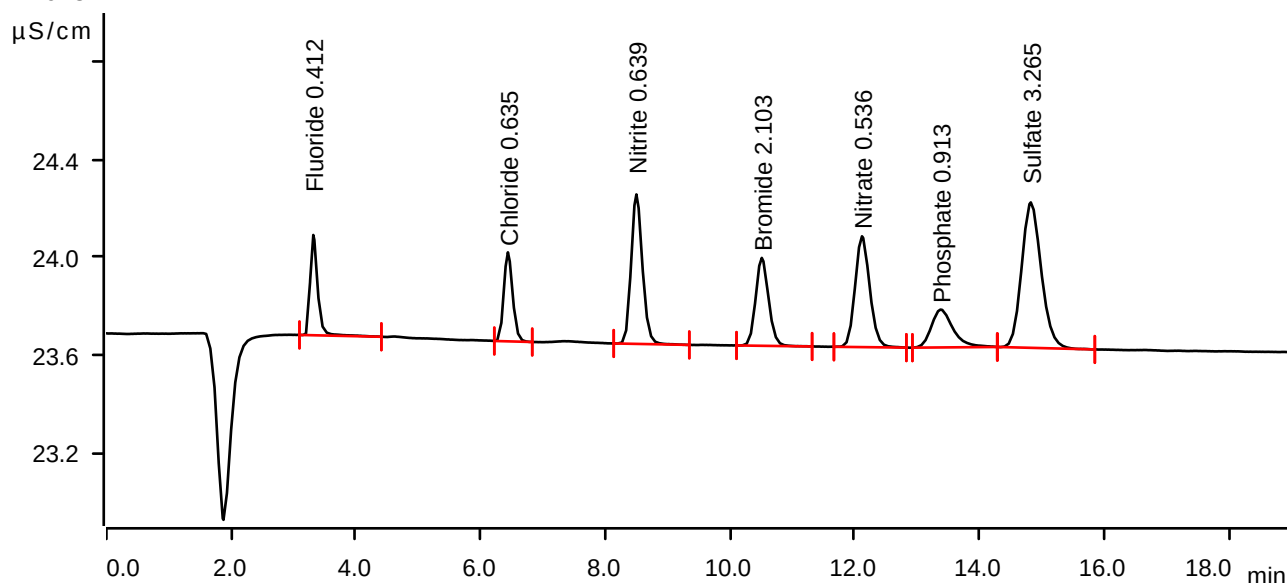

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.318	0.0571	0.411	0.412	Fluoride
2	6.438	0.0597	0.365	0.635	Chloride
3	8.498	0.1284	0.613	0.639	Nitrite
4	10.508	0.0863	0.360	2.103	Bromide
5	12.115	0.1238	0.454	0.536	Nitrate
6	13.373	0.0628	0.155	0.913	Phosphate
7	14.822	0.2176	0.596	3.265	Sulfate


Sample data

Ident STD3
Sample type Standard 3
Determination start 2025-12-01 12:52:25 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

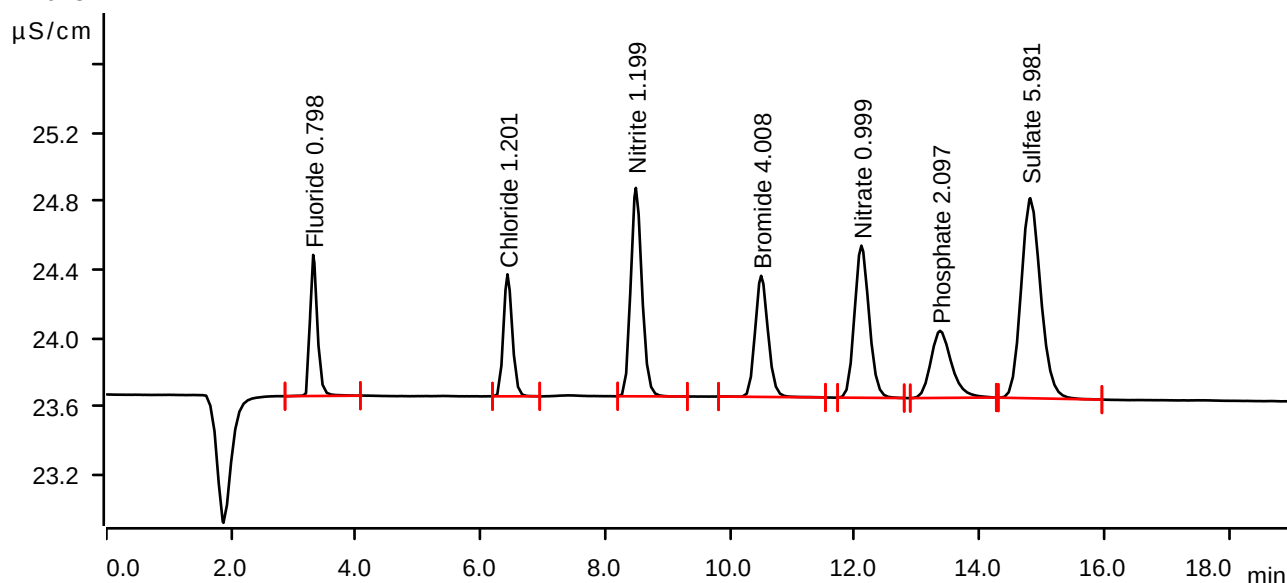

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.317	0.1121	0.826	0.798	Fluoride
2	6.432	0.1169	0.714	1.201	Chloride
3	8.490	0.2538	1.221	1.199	Nitrite
4	10.498	0.1698	0.710	4.008	Bromide
5	12.105	0.2411	0.891	0.999	Nitrate
6	13.367	0.1518	0.393	2.097	Phosphate
7	14.813	0.4264	1.172	5.981	Sulfate


Sample data

Ident STD4
Sample type Standard 4
Determination start 2025-12-01 13:13:50 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

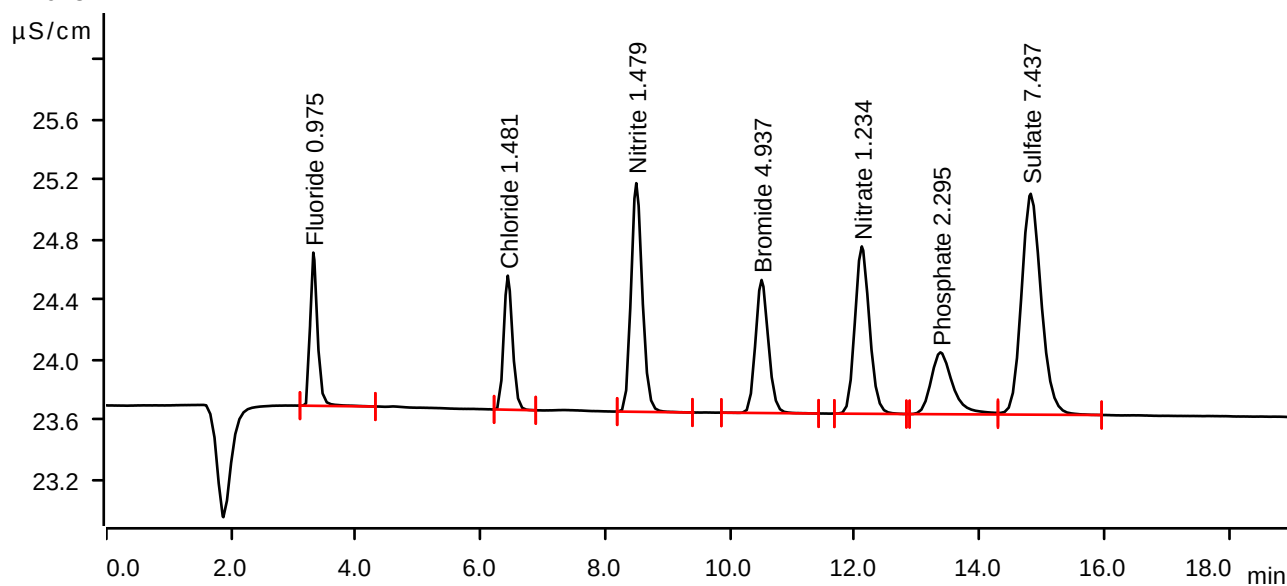

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.318	0.1374	1.017	0.975	Fluoride
2	6.437	0.1452	0.890	1.481	Chloride
3	8.497	0.3164	1.518	1.479	Nitrite
4	10.505	0.2105	0.883	4.937	Bromide
5	12.112	0.3007	1.111	1.234	Nitrate
6	13.372	0.1666	0.410	2.295	Phosphate
7	14.820	0.5384	1.466	7.437	Sulfate


Sample data

Ident STD5
 Sample type Standard 5
 Determination start 2025-12-01 13:35:52 UTC-5
 Method IC1-120125
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.94 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

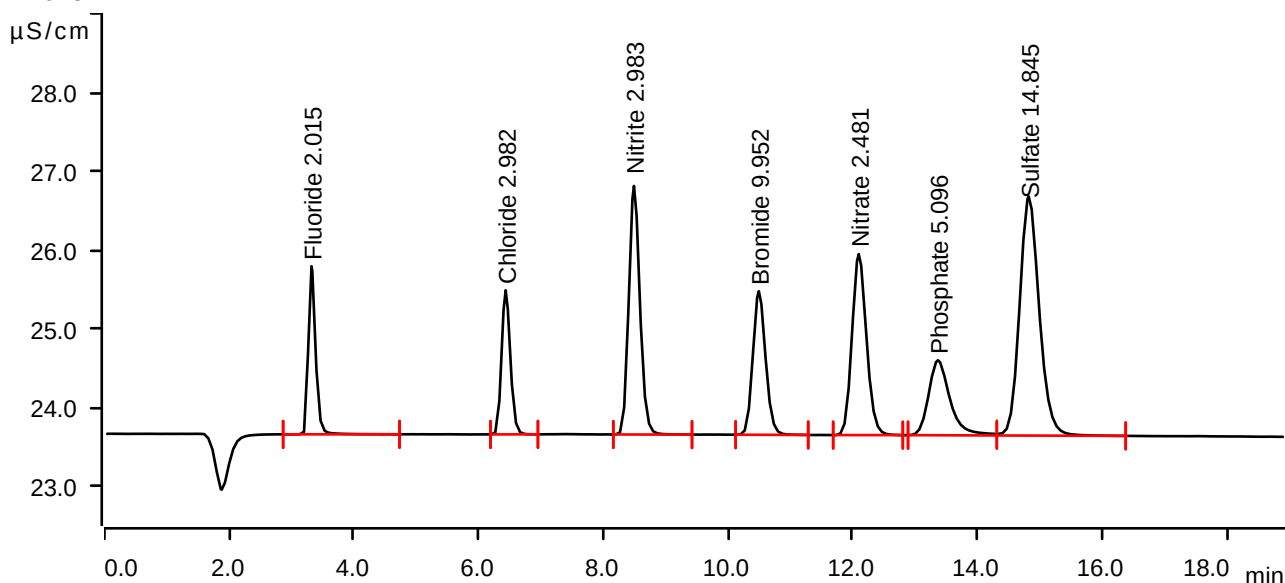

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.322	0.2857	2.133	2.015	Fluoride
2	6.435	0.2970	1.828	2.982	Chloride
3	8.492	0.6533	3.155	2.983	Nitrite
4	10.493	0.4302	1.822	9.952	Bromide
5	12.095	0.6166	2.297	2.481	Nitrate
6	13.365	0.3772	0.952	5.096	Phosphate
7	14.820	1.1081	3.035	14.845	Sulfate


Sample data

Ident STD6
Sample type Standard 6
Determination start 2025-12-01 13:57:13 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.88 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

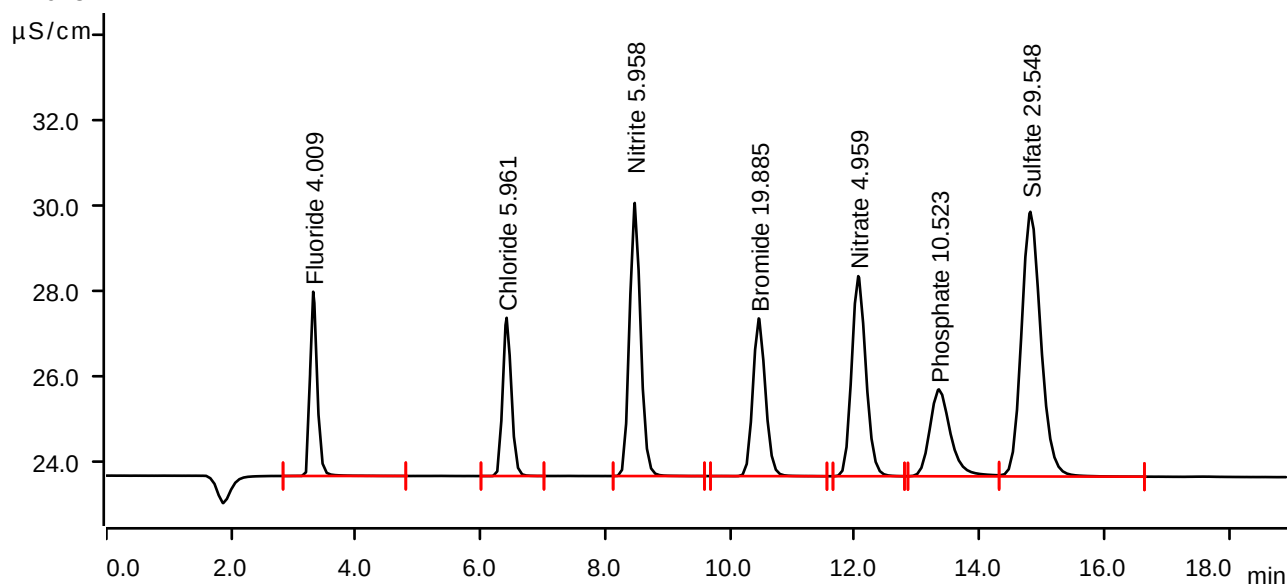

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.317	0.5701	4.316	4.009	Fluoride
2	6.418	0.5981	3.707	5.961	Chloride
3	8.472	1.3194	6.398	5.958	Nitrite
4	10.460	0.8655	3.695	19.885	Bromide
5	12.055	1.2443	4.688	4.959	Nitrate
6	13.348	0.7852	2.036	10.523	Phosphate
7	14.815	2.2388	6.200	29.548	Sulfate


Sample data

Ident STD7
Sample type Standard 7
Determination start 2025-12-01 14:18:41 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.77 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

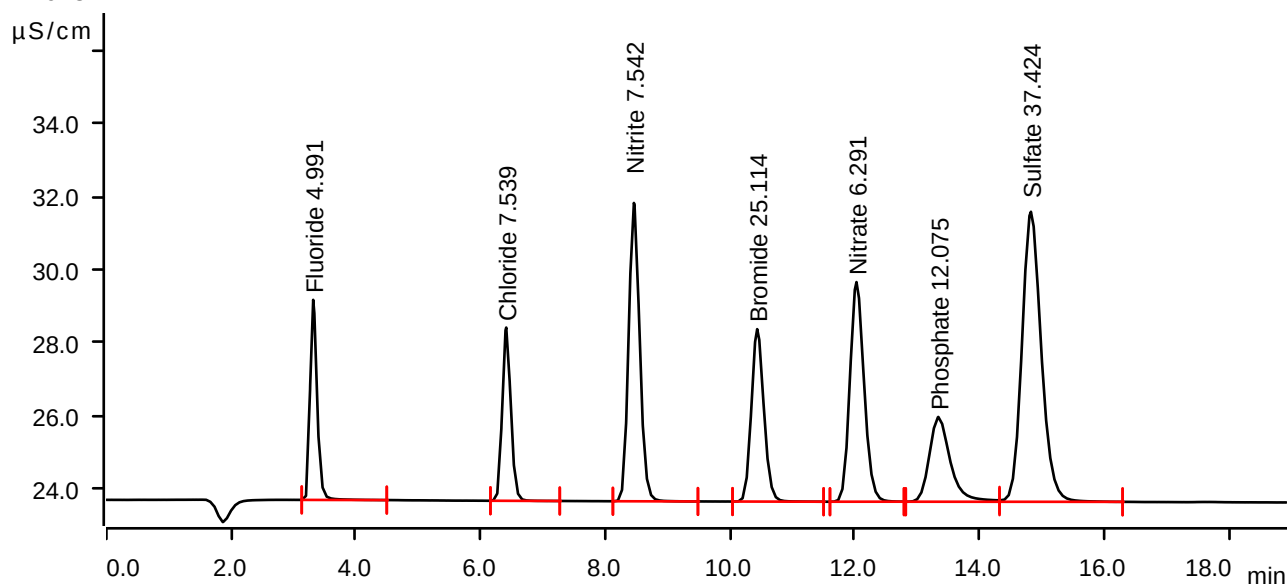

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.317	0.7102	5.467	4.991	Fluoride
2	6.412	0.7576	4.735	7.539	Chloride
3	8.458	1.6742	8.154	7.542	Nitrite
4	10.435	1.0946	4.713	25.114	Bromide
5	12.027	1.5818	6.003	6.291	Nitrate
6	13.340	0.9019	2.316	12.075	Phosphate
7	14.823	2.8445	7.927	37.424	Sulfate


Sample data

Ident ICV
Sample type Check standard 1
Determination start 2025-12-01 14:40:08 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 15.9 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.82 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

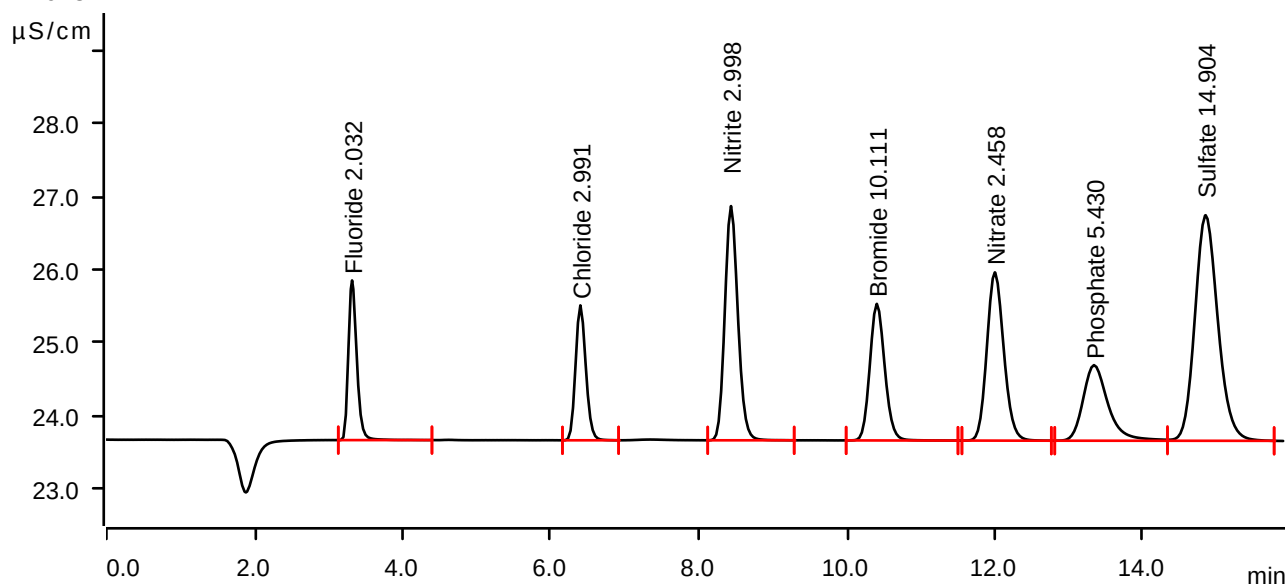

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.318	0.2884	2.182	2.032	Fluoride
2	6.400	0.2984	1.844	2.991	Chloride
3	8.433	0.6564	3.200	2.998	Nitrite
4	10.403	0.4372	1.866	10.111	Bromide
5	11.995	0.6105	2.299	2.458	Nitrate
6	13.335	0.4042	1.033	5.430	Phosphate
7	14.842	1.1126	3.083	14.904	Sulfate


Sample data

Ident ICB
Sample type Sample
Determination start 2025-12-01 14:58:59 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 18.1 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.60 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

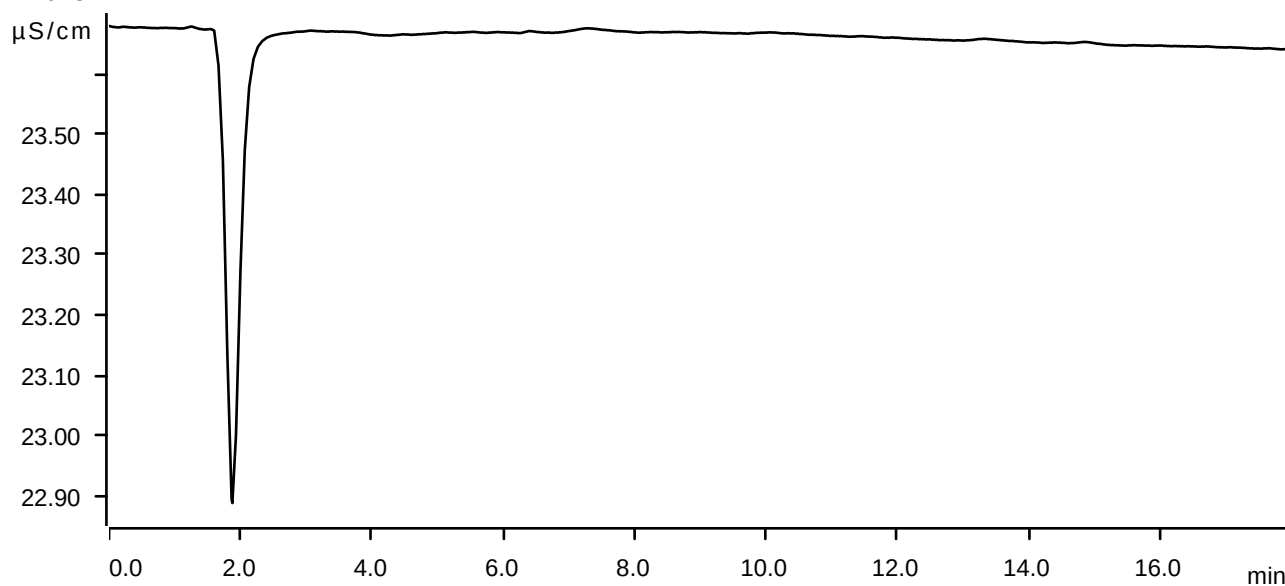


Sample data

Ident CCV
 Sample type Check standard 1
 Determination start 2025-12-02 11:05:10 UTC-5
 Method IC1-120125
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 12.33 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

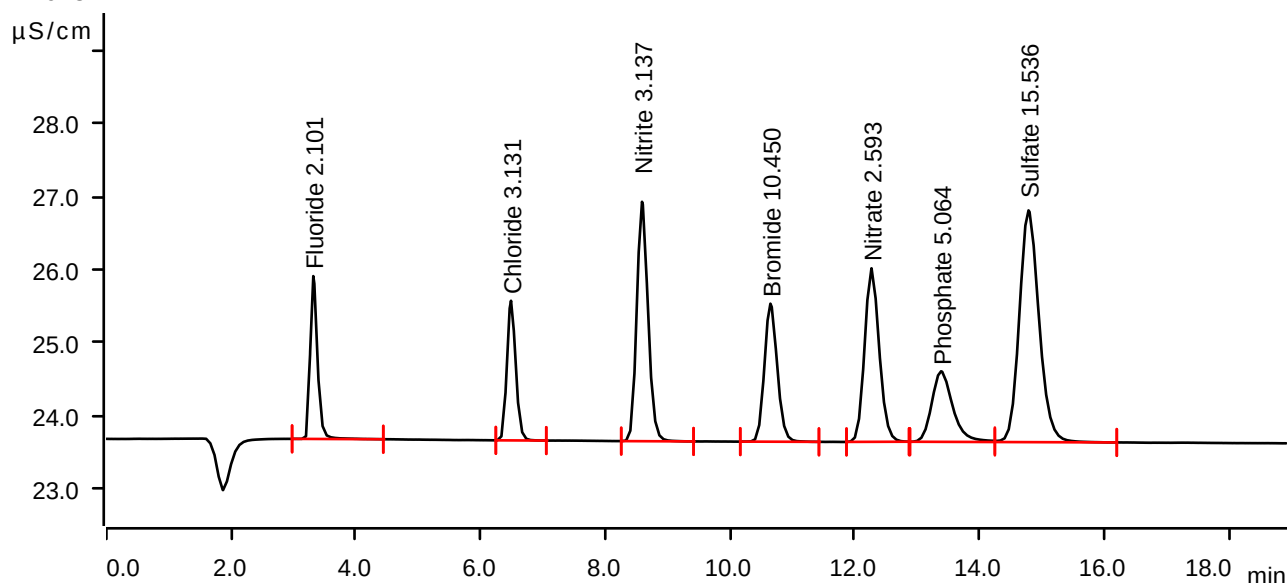


Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.318	0.2982	2.225	2.101	Fluoride
2	6.488	0.3126	1.908	3.131	Chloride
3	8.588	0.6876	3.272	3.137	Nitrite
4	10.647	0.4520	1.886	10.450	Bromide
5	12.267	0.6448	2.371	2.593	Nitrate
6	13.383	0.3769	0.964	5.064	Phosphate
7	14.785	1.1613	3.167	15.536	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-12-02 11:26:41 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

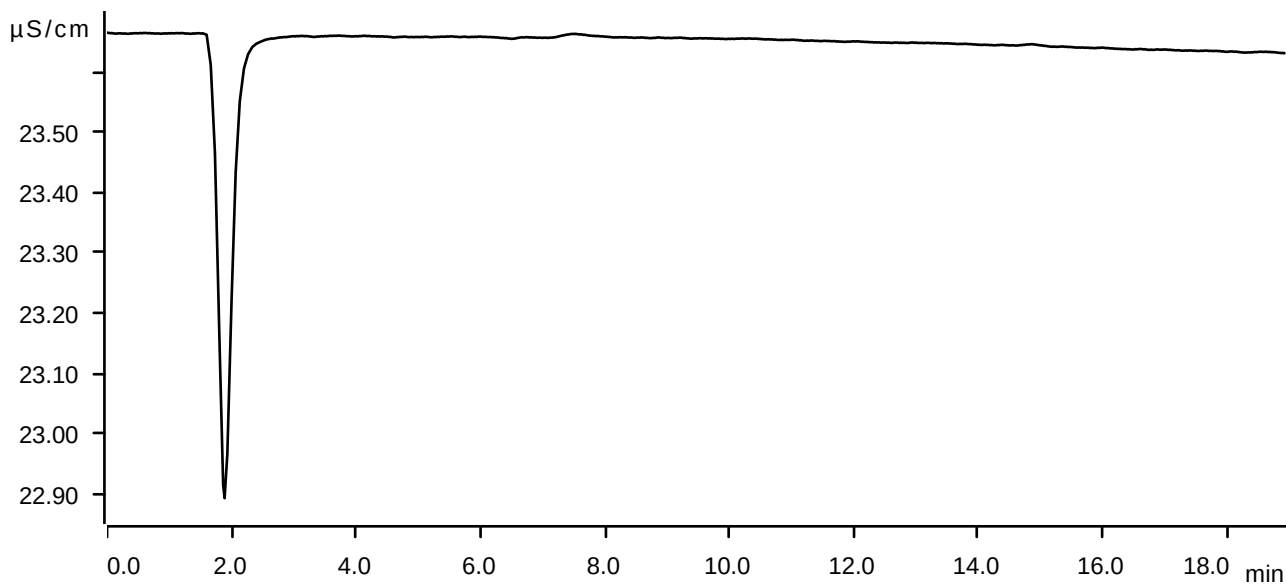Anions


Sample data

Ident LB138084BLW
Sample type Sample
Determination start 2025-12-02 11:48:11 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.22 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

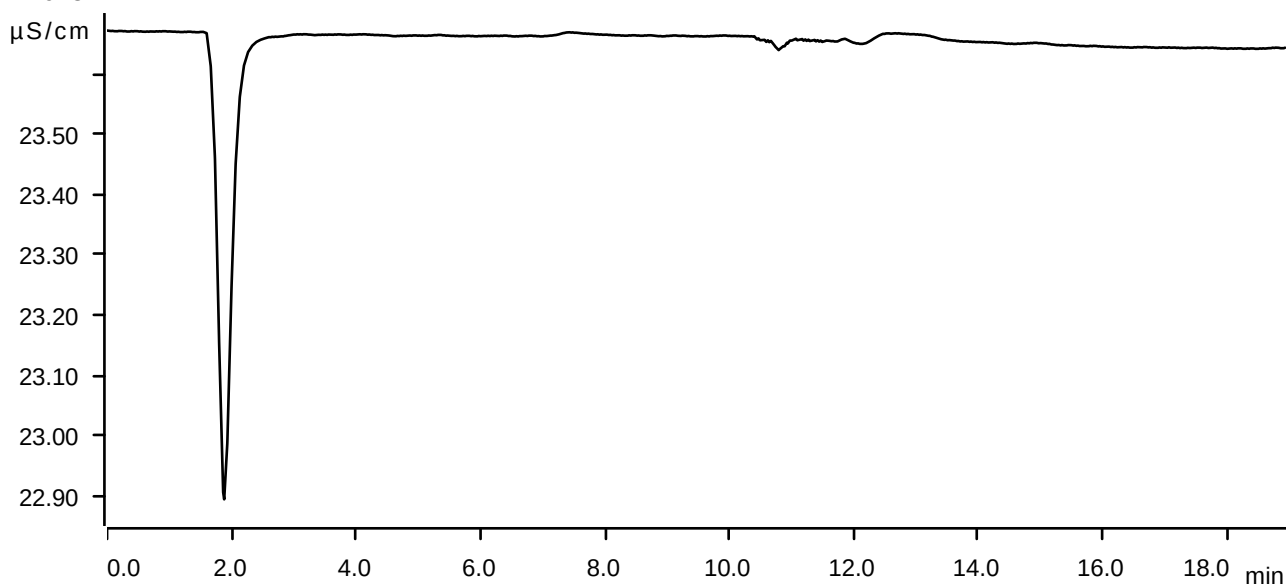


Sample data

Ident LB138084BSW
Sample type Check standard 1
Determination start 2025-12-02 12:09:42 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.11 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

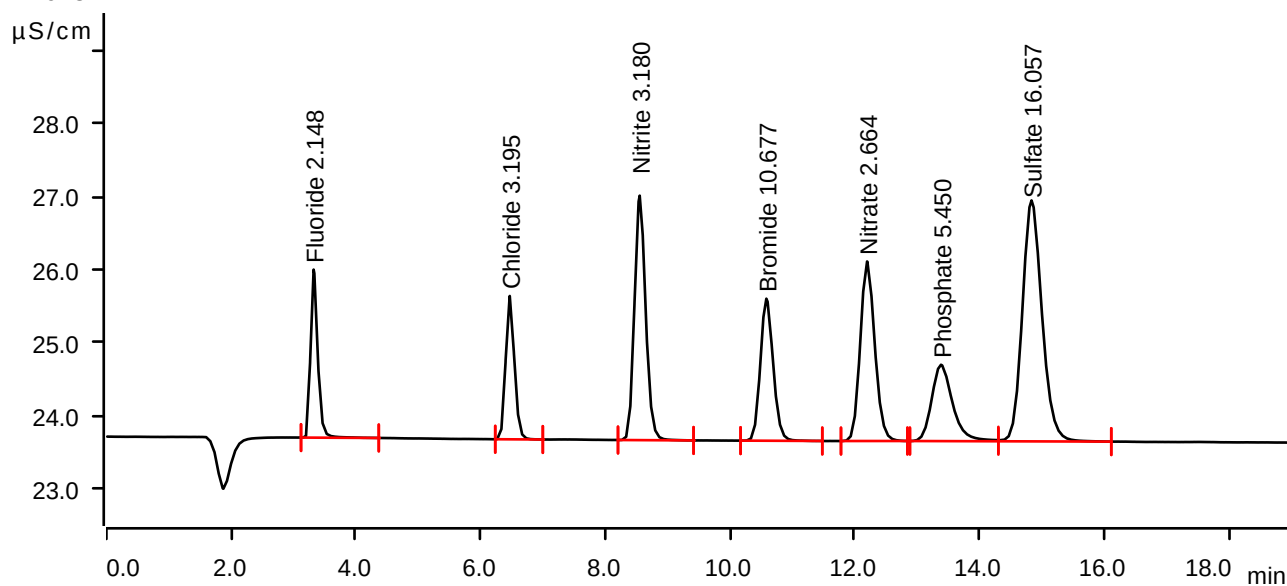

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.323	0.3049	2.296	2.148	Fluoride
2	6.467	0.3189	1.958	3.195	Chloride
3	8.552	0.6973	3.341	3.180	Nitrite
4	10.582	0.4620	1.942	10.677	Bromide
5	12.197	0.6627	2.454	2.664	Nitrate
6	13.382	0.4057	1.044	5.450	Phosphate
7	14.833	1.2013	3.293	16.057	Sulfate


Sample data

Ident Q3737-01
Sample type Sample
Determination start 2025-12-02 12:31:15 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

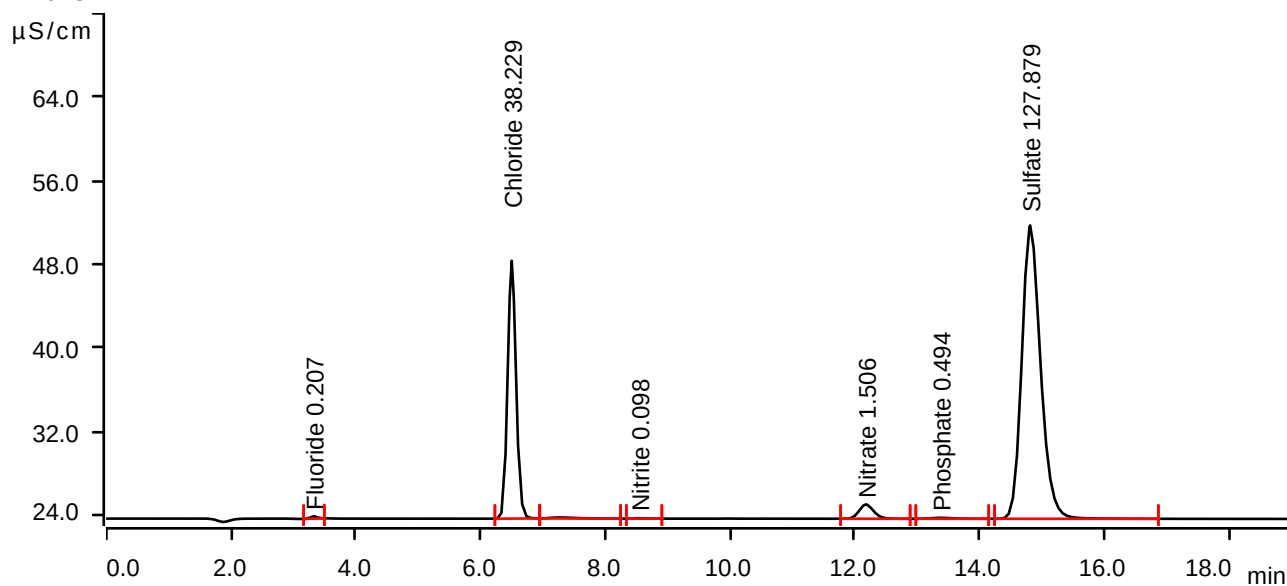

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.323	0.0283	0.225	0.207	Fluoride
2	6.500	3.8536	24.659	38.229	Chloride
3	7.267	0.0458	0.095	invalid	
4	8.540	0.0067	0.033	0.098	Nitrite
5	12.178	0.3694	1.367	1.506	Nitrate
6	13.373	0.0354	0.091	0.494	Phosphate
7	14.812	9.8007	28.063	127.879	Sulfate


Sample data

Ident Q3737-02
Sample type Sample
Determination start 2025-12-02 12:58:24 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 12.05 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

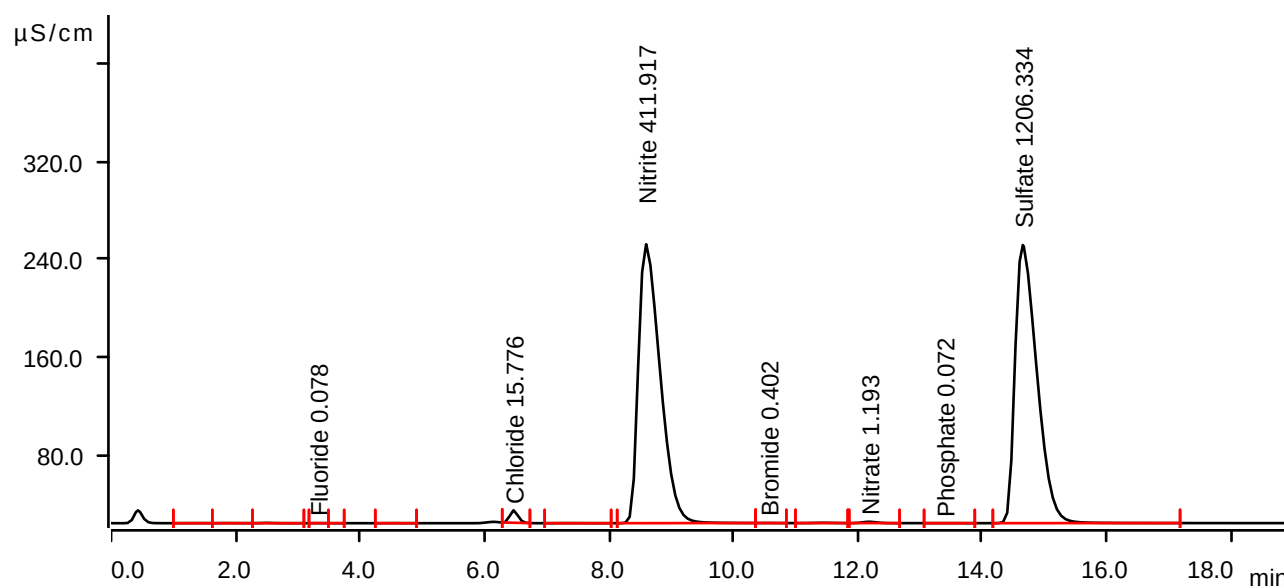

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.292	0.0187	0.043	invalid	
2	1.870	0.0345	0.097	invalid	
3	2.503	0.0563	0.250	invalid	
4	3.323	0.0099	0.072	0.078	Fluoride
5	3.533	0.0013	0.009	invalid	
6	4.527	0.0160	0.067	invalid	
7	6.470	1.5883	10.207	15.776	Chloride
8	7.312	0.0270	0.056	invalid	
9	8.598	92.2691	228.705	411.917	Nitrite
10	10.553	0.0117	0.054	0.402	Bromide
11	11.445	0.0978	0.270	invalid	
12	12.180	0.2901	1.094	1.193	Nitrate
13	13.393	0.0039	0.011	0.072	Phosphate
14	14.652	92.7370	228.037	1206.334	Sulfate


Sample data

Ident Q3737-02MS
Sample type Sample
Determination start 2025-12-02 13:21:49 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

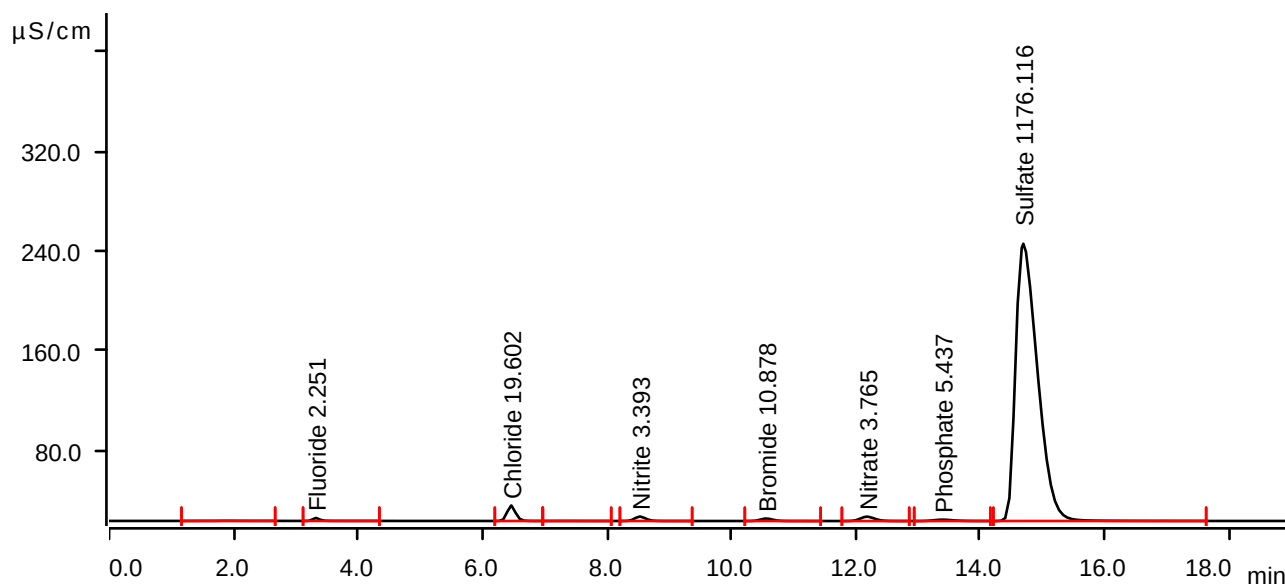

Peak number	Retention time min	Area ($\mu\text{S/cm}$) x min	Height $\mu\text{S/cm}$	Concentration ppm	Component name
1	1.890	0.0390	0.106	invalid	
2	3.322	0.3195	2.330	2.251	Fluoride
3	6.462	1.9743	12.361	19.602	Chloride
4	7.332	0.0194	0.039	invalid	
5	8.530	0.7450	3.571	3.393	Nitrite
6	10.560	0.4708	1.979	10.878	Bromide
7	12.180	0.9417	3.504	3.765	Nitrate
8	13.392	0.4047	1.076	5.437	Phosphate
9	14.692	90.4131	221.918	1176.116	Sulfate


Sample data

Ident Q3737-02MSD
Sample type Sample
Determination start 2025-12-02 13:43:24 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.94 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

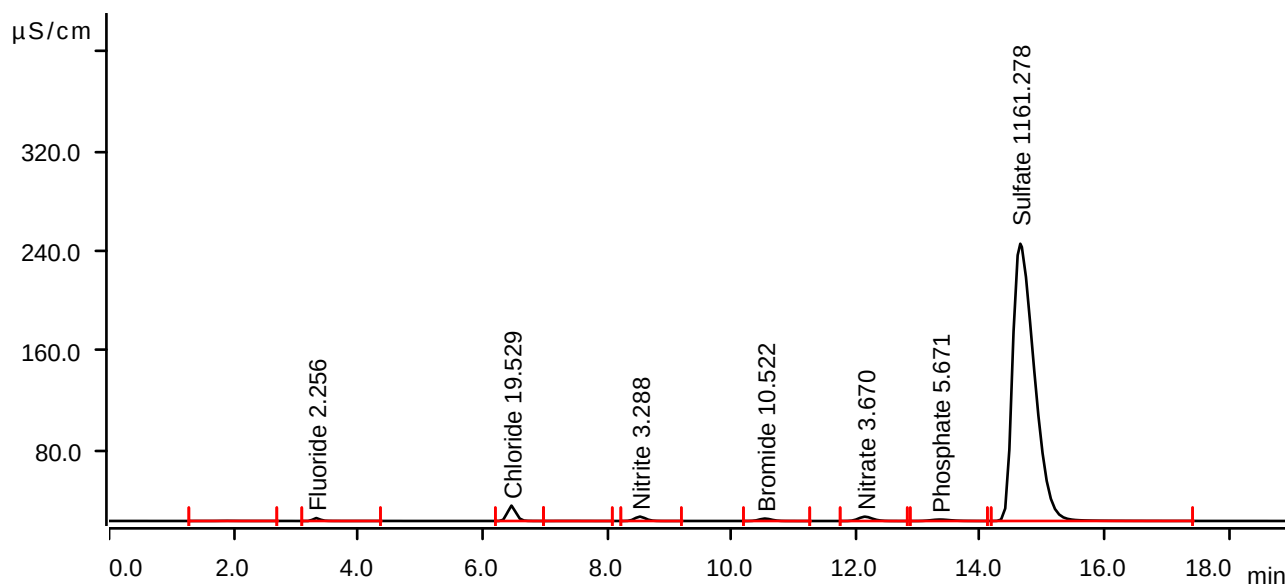

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	1.903	0.0381	0.105	invalid	
2	3.328	0.3203	2.298	2.256	Fluoride
3	6.467	1.9670	12.303	19.529	Chloride
4	7.348	0.0194	0.039	invalid	
5	8.530	0.7214	3.490	3.288	Nitrite
6	10.542	0.4552	1.933	10.522	Bromide
7	12.148	0.9178	3.449	3.670	Nitrate
8	13.352	0.4223	1.139	5.671	Phosphate
9	14.643	89.2720	221.931	1161.278	Sulfate


Sample data

Ident Q3737-01DLX10
 Sample type Sample
 Determination start 2025-12-02 14:05:00 UTC-5
 Method IC1-120125
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 12.11 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

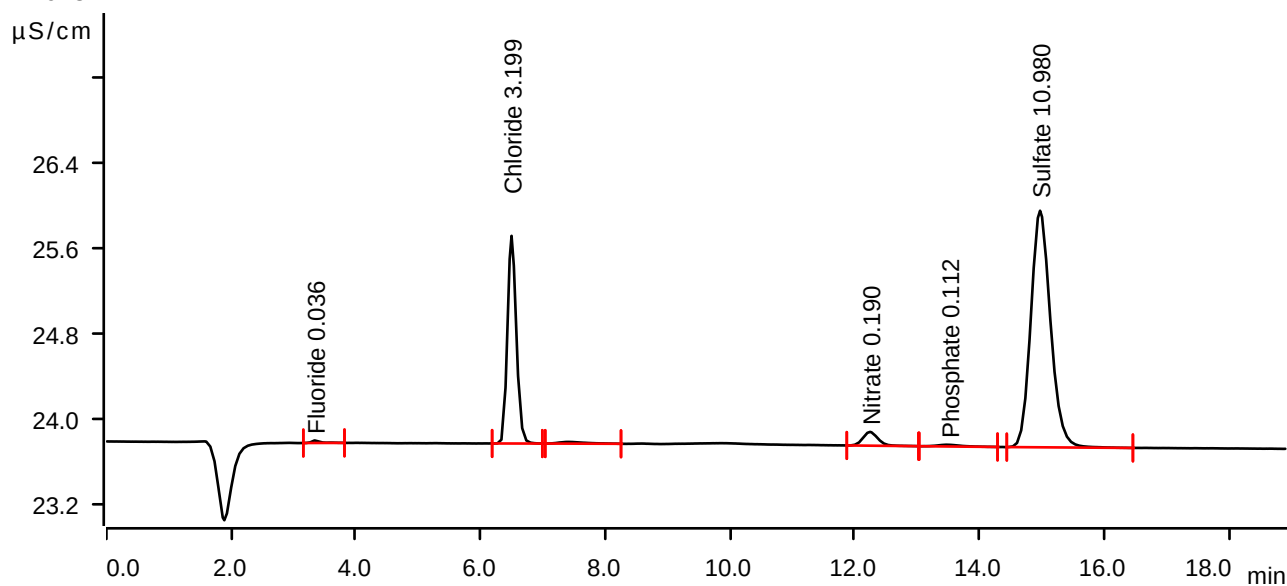

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.342	0.0039	0.023	0.036	Fluoride
2	6.497	0.3194	1.946	3.199	Chloride
3	7.418	0.0080	0.016	invalid	
4	12.245	0.0360	0.129	0.190	Nitrate
5	13.463	0.0068	0.016	0.112	Phosphate
6	14.970	0.8109	2.217	10.980	Sulfate


Sample data

Ident Q3737-02DLX50
 Sample type Sample
 Determination start 2025-12-02 14:26:34 UTC-5
 Method IC1-120125
 Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
 Channel Conductivity
 Recording time 19.0 min
 Integration Automatically
 Column type Metrosep A Supp 19 - 150/4.0
 Eluent composition not defined
 Flow 0.700 mL/min
 Maximum flow monitored yes
 Pressure 11.88 MPa
 Maximum pressure monitored yes
 Temperature ---- °C

Anions

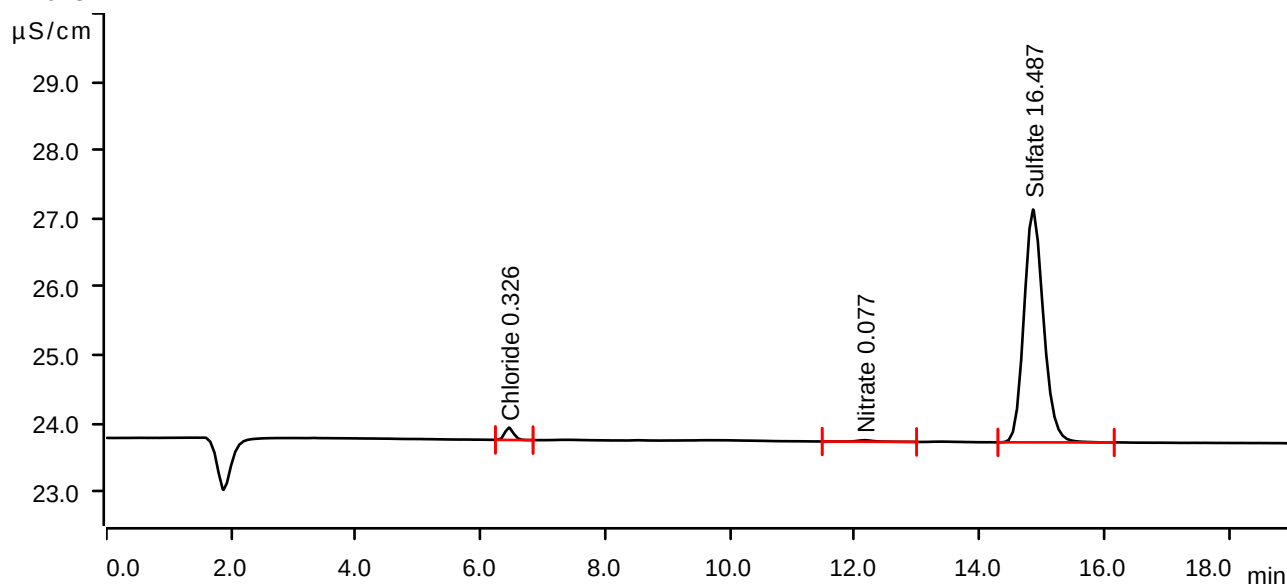

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	6.455	0.0295	0.181	0.326	Chloride
2	12.153	0.0073	0.022	0.077	Nitrate
3	14.857	1.2344	3.409	16.487	Sulfate


Sample data

Ident CCV
Sample type Check standard 1
Determination start 2025-12-02 14:48:08 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.99 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

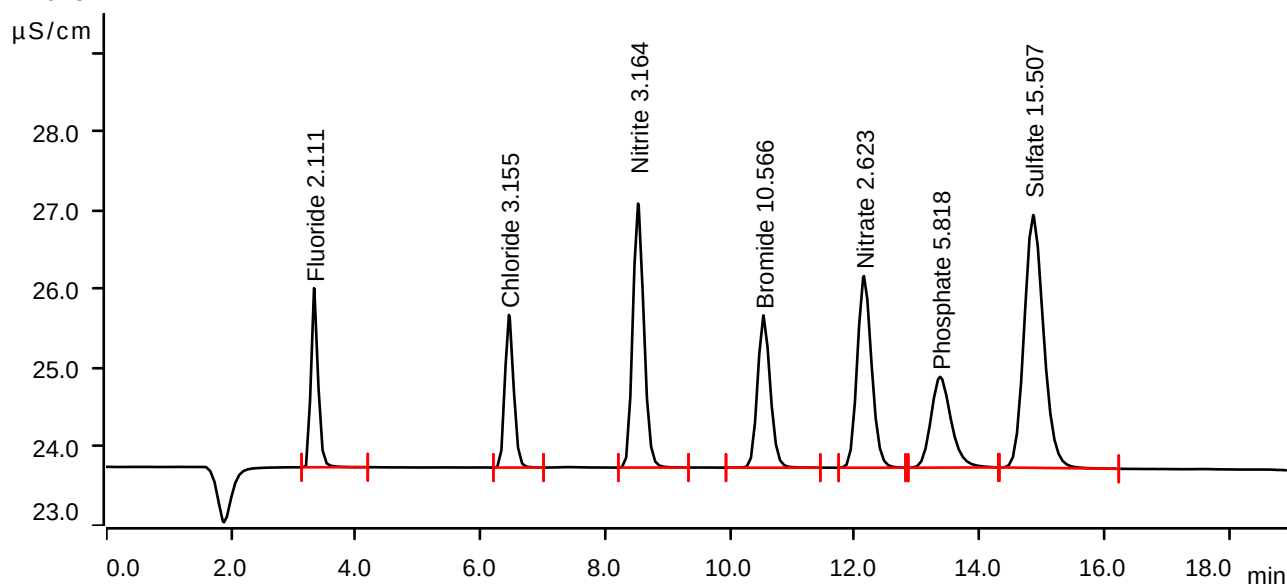

Peak number	Retention time min	Area (µS/cm) x min	Height µS/cm	Concentration ppm	Component name
1	3.330	0.2996	2.272	2.111	Fluoride
2	6.455	0.3150	1.937	3.155	Chloride
3	8.525	0.6936	3.350	3.164	Nitrite
4	10.537	0.4571	1.932	10.566	Bromide
5	12.147	0.6524	2.433	2.623	Nitrate
6	13.368	0.4332	1.152	5.818	Phosphate
7	14.860	1.1590	3.208	15.507	Sulfate

Sample data

Ident CCB
Sample type Sample
Determination start 2025-12-02 15:09:38 UTC-5
Method IC1-120125
Operator

Anions

Data source Conductivity detector 1 (Eco IC 1)
Channel Conductivity
Recording time 19.0 min
Integration Automatically
Column type Metrosep A Supp 19 - 150/4.0
Eluent composition not defined
Flow 0.700 mL/min
Maximum flow monitored yes
Pressure 11.26 MPa
Maximum pressure monitored yes
Temperature ---- °C

Anions

