


LB 193392

7470A

INSTRUMENT ID: CV1

 μ Abs.:

32934

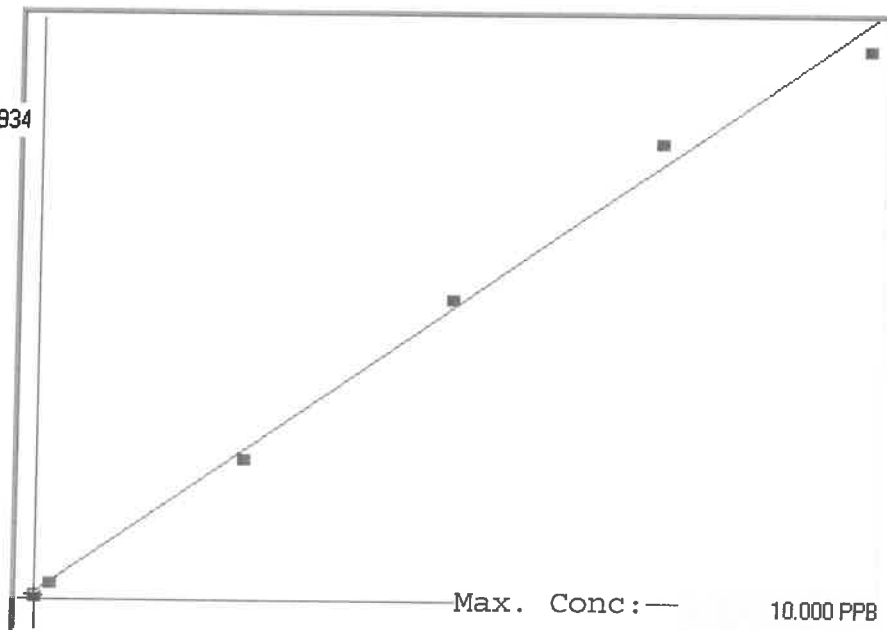

Linear

A= 0.0000e+000

B= 2.9413e-004

C= -1.1964e-001

Rho= 0.9973132

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.0	0.000	-0.050	-0.050	237	0.000	237	0				=
0.2	0.200	0.196	-0.004	1072	0.0 %	1072					-2
2.5	2.500	2.363	-0.137	8439	0.0 %	8439					-5
5.0	5.000	5.180	0.180	18018	0.0 %	18018					4
7.5	7.500	7.944	0.444	27416	0.0 %	27416					6
10.0	10.000	9.567	-0.433	32934	0.0 %	32934					-4

L133392 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 11 Nov 2024 13:25:25

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	237	-	0.0000	7470A	PPB	11 Nov 2024 13:36:48	S	Std
0.2 - 1	50-2	1072	-	0.2000	7470A	PPB	11 Nov 2024 13:41:52	S	Std
2.5 - 1	52.5	8439	-	2.5000	7470A	PPB	11 Nov 2024 13:44:09	S	Std
5.0 - 1	55	18018	-	5.0000	7470A	PPB	11 Nov 2024 13:46:26	S	Std
7.5 - 1	57.5	27416	-	7.5000	7470A	PPB	11 Nov 2024 13:53:38	S	Std
10.0 - 1	50	32934	-	10.0000	7470A	PPB	11 Nov 2024 13:55:55	S	Std
ICV80 - 1	ICV80	14302	4.0871	-	7470A	PPB	11 Nov 2024 13:58:50	U	SMPL
ICB80 - 1	ICB80	282	-0.0367	-	7470A	PPB	11 Nov 2024 14:01:05	U	SMPL
CCV64 - 1	CCV64	17943	5.1580	-	7470A	PPB	11 Nov 2024 14:03:21	U	SMPL
CCB64 - 1	CCB64	250	-0.0461	-	7470A	PPB	11 Nov 2024 14:05:36	U	SMPL
CRA - 1	CRA	1106	0.2057	-	7470A	PPB	11 Nov 2024 14:10:47	U	SMPL
HighStd - 1	HighStd	32302	9.3815	-	7470A	PPB	11 Nov 2024 14:13:01	U	SMPL
ChkStd - 1	ChkStd	24651	7.1310	-	7470A	PPB	11 Nov 2024 14:15:16	U	SMPL
PB164872BL - 1	PBW	275	-0.0388	-	7470A	PPB	11 Nov 2024 14:20:09	U	SMPL
PB164872BS - 1	LCSW	12697	3.6150	-	7470A	PPB	11 Nov 2024 14:22:24	U	SMPL
P4718-04 - 1	WB-307-SW	-57	-0.1364	-	7470A	PPB	11 Nov 2024 14:24:40	U	SMPL
P4736-02 - 1	COMP	295	-0.0329	-	7470A	PPB	11 Nov 2024 14:26:58	U	SMPL
P4791-02 - 1	HINCHMAN-OILY-WATER	-25	-0.1270	-	7470A	PPB	11 Nov 2024 14:29:14	U	SMPL
P4791-02DUP - 1	HINCHMAN-OILY-WATERDUP	15	-0.1152	-	7470A	PPB	11 Nov 2024 14:31:31	U	SMPL
P4791-02MS - 1	HINCHMAN-OILY-WATERMS	10827	3.0649	-	7470A	PPB	11 Nov 2024 14:33:45	U	SMPL
CCV65 - 1	CCV65	16902	4.8518	-	7470A	PPB	11 Nov 2024 14:36:01	U	SMPL
CCB65 - 1	CCB65	265	-0.0417	-	7470A	PPB	11 Nov 2024 14:41:02	U	SMPL
P4791-02MSD - 1	HINCHMAN-OILY-WATERMSD	11003	3.1167	-	7470A	PPB	11 Nov 2024 14:43:16	U	SMPL
P4792-04 - 1	MANHOLE-WASTE-DRUMS	2123	0.5048	-	7470A	PPB	11 Nov 2024 14:45:31	U	SMPL
P4797-01 - 1	2885	7550	2.1011	-	7470A	PPB	11 Nov 2024 14:47:49	U	SMPL
P4791-02LX5 - 1		-612	-0.2997	-	7470A	PPB	11 Nov 2024 14:50:07	U	SMPL
P4791-02A - 1		14217	4.0621	-	7470A	PPB	11 Nov 2024 14:52:26	U	SMPL
CCV66 - 1	CCV66	17178	4.9330	-	7470A	PPB	11 Nov 2024 14:54:42	U	SMPL
CCB66 - 1	CCB66	192	-0.0632	-	7470A	PPB	11 Nov 2024 14:57:00	U	SMPL