


7471A

LB 85328
INSTRUMENT ID: CV1

 μ Abs.:

42281

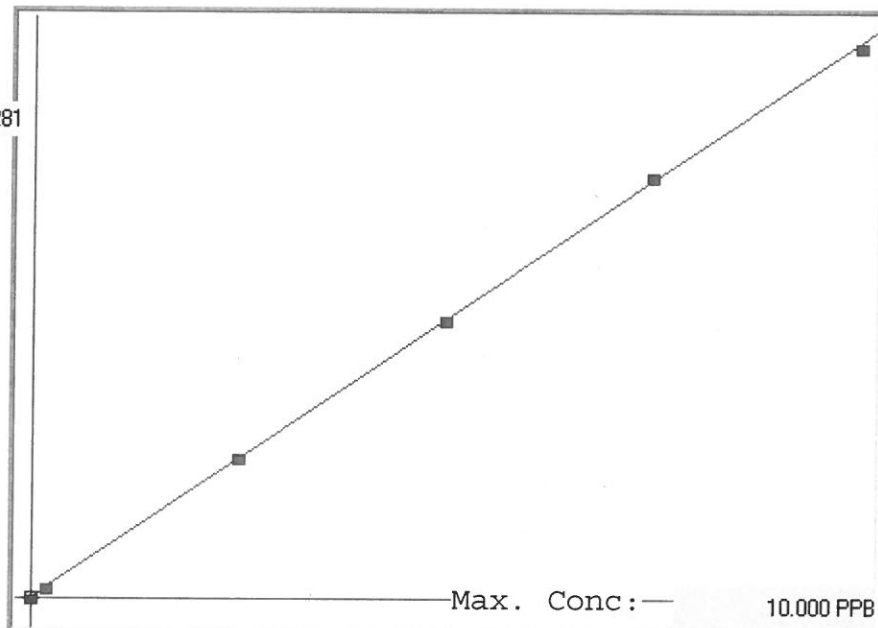

Linear

A= 0.0000e+000

B= 2.3501e-004

C= -9.8449e-003

Rho= 0.9999199

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.027	-0.027	-71	0.000	-71				
0.2	0.200	0.187	-0.013	837	0.0 %	837				
2.5	2.500	2.516	0.016	10748	0.0 %	10748				
5.0	5.000	5.018	0.018	21393	0.0 %	21393				
7.5	7.500	7.579	0.079	32292	0.0 %	32292				
10.0	10.000	9.927	-0.073	42281	0.0 %	42281				

LB85328 INSTRUMENT ID : CV1

Method: 7471A

Operator: Admin

Date of Analysis: 13 Jan 2017 10:41:33

Sample ID	Extended ID	μ Abs.	Conc.	Std CondMethod	Units	Date	Type	Type
0.0 - 1	50	-71	-	0.00007471A	PPB	13 Jan 2017 11:04:45	S	Std
0.2 - 1	50.2	837	-	0.20007471A	PPB	13 Jan 2017 11:07:03	S	Std
2.5 - 1	52.5	10748	-	2.50007471A	PPB	13 Jan 2017 11:09:21	S	Std
5.0 - 1	55	21393	-	5.00007471A	PPB	13 Jan 2017 11:11:38	S	Std
7.5 - 1	57.5	32292	-	7.50007471A	PPB	13 Jan 2017 11:16:36	S	Std
10.0 - 1	510	42281	-	10.00007471A	PPB	13 Jan 2017 11:21:28	S	Std
ICV96 - 1	ICV96	15770	3.6963	-7471A	PPB	13 Jan 2017 11:24:39	U	SMPL
ICB96 - 1	ICB96	-33	-0.0176	-7471A	PPB	13 Jan 2017 11:26:54	U	SMPL
CCV54 - 1	CCV54	21581	5.0619	-7471A	PPB	13 Jan 2017 11:29:10	U	SMPL
CCB54 - 1	CCB54	-13	-0.0129	-7471A	PPB	13 Jan 2017 11:31:26	U	SMPL
CRA - 1	CRA	844	0.1885	-7471A	PPB	13 Jan 2017 11:33:42	U	SMPL
HighStd - 1	HighStd	42920	10.0769	-7471A	PPB	13 Jan 2017 11:35:58	U	SMPL
ChkStd - 1	ChkStd	30197	7.0868	-7471A	PPB	13 Jan 2017 11:38:14	U	SMPL
PB95960BL - 1	PBS	-31	-0.0171	-7471A	PPB	13 Jan 2017 11:40:30	U	SMPL
PB95960BS - 1	LCSS	15624	3.6620	-7471A	PPB	13 Jan 2017 11:42:47	U	SMPL
I1029-01 - 1	COMP-001	2008	0.4621	-7471A	PPB	13 Jan 2017 11:45:04	U	SMPL
I1029-01DUP - 1	COMP-001DUP	2010	0.4625	-7471A	PPB	13 Jan 2017 11:47:21	U	SMPL
I1029-01MS - 1	COMP-001MS	18208	4.2693	-7471A	PPB	13 Jan 2017 11:49:38	U	SMPL
I1029-01MSD - 1	COMP-001MSD	17880	4.1922	-7471A	PPB	13 Jan 2017 11:51:56	U	SMPL
I1029-03 - 1	COMP-002	1110	0.2510	-7471A	PPB	13 Jan 2017 11:54:13	U	SMPL
CCV55 - 1	CCV55	20705	4.8561	-7471A	PPB	13 Jan 2017 11:56:29	U	SMPL
CCB55 - 1	CCB55	-48	-0.0211	-7471A	PPB	13 Jan 2017 11:58:45	U	SMPL
I1029-05 - 1	COMP-003	2194	0.5058	-7471A	PPB	13 Jan 2017 12:01:01	U	SMPL
I1029-07 - 1	COMP-004	1886	0.4334	-7471A	PPB	13 Jan 2017 12:03:17	U	SMPL
I1029-09 - 1	COMP-005	1699	0.3894	-7471A	PPB	13 Jan 2017 12:05:33	U	SMPL
I1029-11 - 1	COMP-006	3229	0.7490	-7471A	PPB	13 Jan 2017 12:07:49	U	SMPL
I1029-13 - 1	COMP-007	3535	0.8209	-7471A	PPB	13 Jan 2017 12:10:06	U	SMPL
I1029-15 - 1	COMP-008	3209	0.7443	-7471A	PPB	13 Jan 2017 12:12:23	U	SMPL
I1029-17 - 1	COMP-009	3512	0.8155	-7471A	PPB	13 Jan 2017 12:14:40	U	SMPL
I1029-19 - 1	COMP-0010	3425	0.7951	-7471A	PPB	13 Jan 2017 12:16:58	U	SMPL
I1030-01 - 1	COMP-0011	3338	0.7746	-7471A	PPB	13 Jan 2017 12:19:16	U	SMPL
I1030-03 - 1	COMP-0012	2378	0.5490	-7471A	PPB	13 Jan 2017 12:21:32	U	SMPL
CCV56 - 1	CCV56	21710	5.0923	-7471A	PPB	13 Jan 2017 12:23:49	U	SMPL
CCB56 - 1	CCB56	-24	-0.0155	-7471A	PPB	13 Jan 2017 12:26:05	U	SMPL
I1030-05 - 1	COMP-0013	2045	0.4708	-7471A	PPB	13 Jan 2017 12:28:21	U	SMPL
I1030-07 - 1	COMP-0014	2205	0.5084	-7471A	PPB	13 Jan 2017 12:30:38	U	SMPL
I1030-09 - 1	COMP-0015	2051	0.4722	-7471A	PPB	13 Jan 2017 12:32:54	U	SMPL
I1030-11 - 1	COMP-0016	4282	0.9965	-7471A	PPB	13 Jan 2017 12:35:11	U	SMPL
I1030-13 - 1	COMP-0017	5300	1.2357	-7471A	PPB	13 Jan 2017 12:37:28	U	SMPL
I1030-15 - 1	COMP-0018	2518	0.5819	-7471A	PPB	13 Jan 2017 12:39:44	U	SMPL
I1030-17 - 1	COMP-0019	2119	0.4881	-7471A	PPB	13 Jan 2017 12:42:02	U	SMPL
I1030-19 - 1	COMP-0020	1111	0.2513	-7471A	PPB	13 Jan 2017 12:44:19	U	SMPL
PB95961BL - 1	PBS	19	-0.0054	-7471A	PPB	13 Jan 2017 12:46:37	U	SMPL
PB95961BS - 1	LCSS	15970	3.7433	-7471A	PPB	13 Jan 2017 12:48:53	U	SMPL
CCV57 - 1	CCV57	21512	5.0457	-7471A	PPB	13 Jan 2017 12:51:10	U	SMPL
CCB57 - 1	CCB57	-27	-0.0162	-7471A	PPB	13 Jan 2017 12:53:26	U	SMPL
I1031-01 - 1	COMP-0021	4111	0.9563	-7471A	PPB	13 Jan 2017 12:55:43	U	SMPL
I1031-03 - 1	COMP-0022	2757	0.6381	-7471A	PPB	13 Jan 2017 12:57:59	U	SMPL
I1031-05 - 1	COMP-0023	3518	0.8169	-7471A	PPB	13 Jan 2017 13:00:15	U	SMPL
I1031-07 - 1	COMP-0024	4369	1.0169	-7471A	PPB	13 Jan 2017 13:02:32	U	SMPL
I1031-09 - 1	COMP-0025	2339	0.5398	-7471A	PPB	13 Jan 2017 13:04:48	U	SMPL
I1031-11 - 1	COMP-0026	3203	0.7429	-7471A	PPB	13 Jan 2017 13:07:05	U	SMPL
I1031-13 - 1	COMP-0027	3365	0.7810	-7471A	PPB	13 Jan 2017 13:09:22	U	SMPL
I1031-15 - 1	COMP-0028	4218	0.9814	-7471A	PPB	13 Jan 2017 13:11:40	U	SMPL
I1031-17 - 1	COMP-0029	4761	1.1090	-7471A	PPB	13 Jan 2017 13:13:58	U	SMPL
I1031-19 - 1	COMP-0030	3335	0.7739	-7471A	PPB	13 Jan 2017 13:16:14	U	SMPL
CCV58 - 1	CCV58	21240	4.9818	-7471A	PPB	13 Jan 2017 13:18:30	U	SMPL
CCB58 - 1	CCB58	-17	-0.0138	-7471A	PPB	13 Jan 2017 13:20:47	U	SMPL
I1147-01 - 1	TOD-SB-01-0-2	11319	2.6503	-7471A	PPB	13 Jan 2017 13:23:03	U	SMPL
I1147-01DUP - 1	TOD-SB-01-0-2DUP	10869	2.5445	-7471A	PPB	13 Jan 2017 13:25:19	U	SMPL
I1147-02 - 1	I1147-01MS	27996	6.5695	-7471A	PPB	13 Jan 2017 13:27:36	U	SMPL
I1147-03 - 1	I1147-01MSD	27214	6.3858	-7471A	PPB	13 Jan 2017 13:29:52	U	SMPL
I1147-04 - 1	TOD-SB-101-0-2	8829	2.0651	-7471A	PPB	13 Jan 2017 13:32:09	U	SMPL
I029-01LX5 - 1		375	0.0783	-7471A	PPB	13 Jan 2017 13:34:26	U	SMPL
I029-01A - 1		20807	4.8800	-7471A	PPB	13 Jan 2017 13:36:43	U	SMPL
I1147-01LX5 - 1		1944	0.4470	-7471A	PPB	13 Jan 2017 13:39:01	U	SMPL
I1147-01A - 1		28785	6.7550	-7471A	PPB	13 Jan 2017 13:41:18	U	SMPL
CCV59 - 1	CCV59	21346	5.0067	-7471A	PPB	13 Jan 2017 13:43:35	U	SMPL
CCB59 - 1	CCB59	-26	-0.0160	-7471A	PPB	13 Jan 2017 13:45:52	U	SMPL