

7470A


LB 85488

INSTRUMENT ID: CX1

Linear

 μ Abs.:

38819

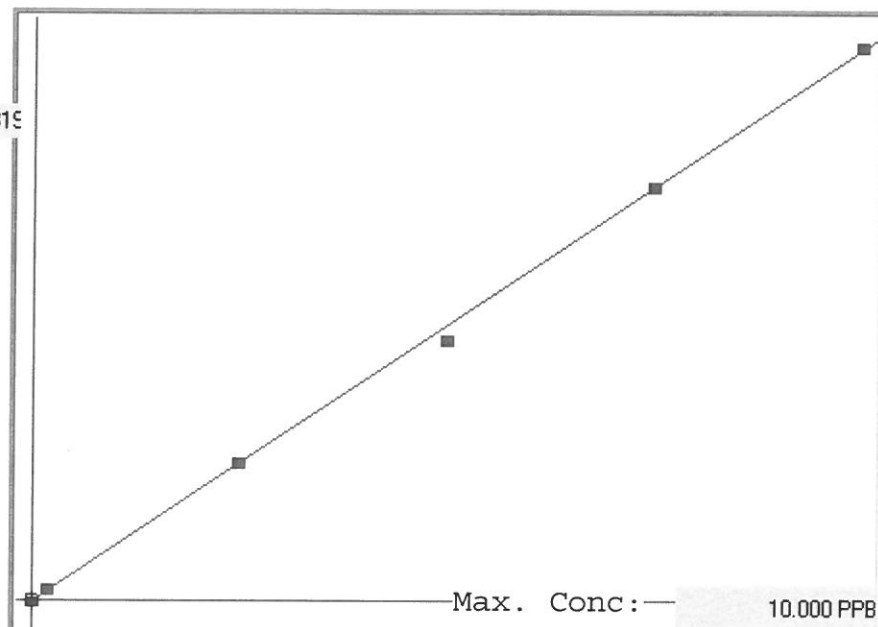

A= 0.0000e+000

B= 2.5856e-004

C= 3.0381e-002

Rho= 0.9996609

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.035	0.035	17	0.000	17				
0.2	0.200	0.244	0.044	828	0.0 %	828				
2.5	2.500	2.534	0.034	9684	0.0 %	9684				
5.0	5.000	4.787	-0.213	18396	0.0 %	18396				
7.5	7.500	7.532	0.032	29015	0.0 %	29015				
10.0	10.000	10.067	0.067	38819	0.0 %	38819				

LB85488 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 25 Jan 2017 10:56:51

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	17	-	0.00007470A	PPB		25 Jan 2017 11:35:03	S	Std
0.2 - 1	50.2	828	-	0.20007470A	PPB		25 Jan 2017 11:37:11	S	Std
2.5 - 1	52.5	9684	-	2.50007470A	PPB		25 Jan 2017 11:39:20	S	Std
5.0 - 1	55	18396	-	5.00007470A	PPB		25 Jan 2017 11:41:28	S	Std
7.5 - 1	57.5	29015	-	7.50007470A	PPB		25 Jan 2017 11:43:36	S	Std
10.0 - 1	510	38819	-	10.00007470A	PPB		25 Jan 2017 11:45:43	S	Std
ICV08 - 1	ICV08	14800	3.8570	-7470A	PPB		25 Jan 2017 11:51:28	U	SMPL
ICB08 - 1	ICB08	-7	0.0286	-7470A	PPB		25 Jan 2017 11:53:34	U	SMPL
CCV17 - 1	CCV17	18393	4.7860	-7470A	PPB		25 Jan 2017 11:55:40	U	SMPL
CCB17 - 1	CCB17	-15	0.0265	-7470A	PPB		25 Jan 2017 11:57:47	U	SMPL
CRA - 1	CRA	825	0.2437	-7470A	PPB		25 Jan 2017 11:59:54	U	SMPL
HighStd - 1	HighStd	38370	9.9512	-7470A	PPB		25 Jan 2017 12:02:00	U	SMPL
ChkStd - 1	ChkStd	27393	7.1130	-7470A	PPB		25 Jan 2017 12:04:07	U	SMPL
PB96300BL - 1	PBW	-42	0.0195	-7470A	PPB		25 Jan 2017 12:06:14	U	SMPL
PB96300BS - 1	LCSW	14012	3.6533	-7470A	PPB		25 Jan 2017 12:08:22	U	SMPL
PB96300TB - 1	PB96191TB	-20	0.0252	-7470A	PPB		25 Jan 2017 12:10:29	U	SMPL
I1351-01 - 1	CAS-WCS-011917(0-15)	61	0.0462	-7470A	PPB		25 Jan 2017 12:12:38	U	SMPL
I1351-02 - 1	CAS-WCS-011917(15-70)	0	0.0304	-7470A	PPB		25 Jan 2017 12:14:46	U	SMPL
I1363-02 - 1	BLDG-3-FLOOR-COMP	2	0.0309	-7470A	PPB		25 Jan 2017 12:16:55	U	SMPL
I1363-05 - 1	BLDG-3-BLOCK-WALL-COMP	0	0.0304	-7470A	PPB		25 Jan 2017 12:19:02	U	SMPL
CCV18 - 1	CCV18	18277	4.7560	-7470A	PPB		25 Jan 2017 12:21:08	U	SMPL
CCB18 - 1	CCB18	-19	0.0255	-7470A	PPB		25 Jan 2017 12:23:15	U	SMPL
I1363-08 - 1	BLDG-1-FLOOR-COMP	5	0.0317	-7470A	PPB		25 Jan 2017 12:25:22	U	SMPL
I1363-08DUP - 1	BLDG-1-FLOOR-COMPDUP	9	0.0327	-7470A	PPB		25 Jan 2017 12:27:29	U	SMPL
I1363-08MS - 1	BLDG-1-FLOOR-COMPMS	14454	3.7676	-7470A	PPB		25 Jan 2017 12:29:36	U	SMPL
I1379-06 - 1	WC-COMPOSITE	-14	0.0268	-7470A	PPB		25 Jan 2017 12:33:51	U	SMPL
I1363-08LX5 - 1		-12	0.0273	-7470A	PPB		25 Jan 2017 12:35:58	U	SMPL
I1363-08A - 1		14635	3.8144	-7470A	PPB		25 Jan 2017 12:38:07	U	SMPL
I1363-08MSD - 1	BLDG-1-FLOOR-COMPMSD	14287	3.7244	-7470A	PPB		25 Jan 2017 12:45:12	U	SMPL
CCV19 - 1	CCV19	18256	4.7506	-7470A	PPB		25 Jan 2017 12:47:20	U	SMPL
CCB19 - 1	CCB19	-19	0.0255	-7470A	PPB		25 Jan 2017 12:49:27	U	SMPL