


ISM02.3

LB85776
INSTRUMENT ID: CV1

Linear

 μ Abs.:

4222E

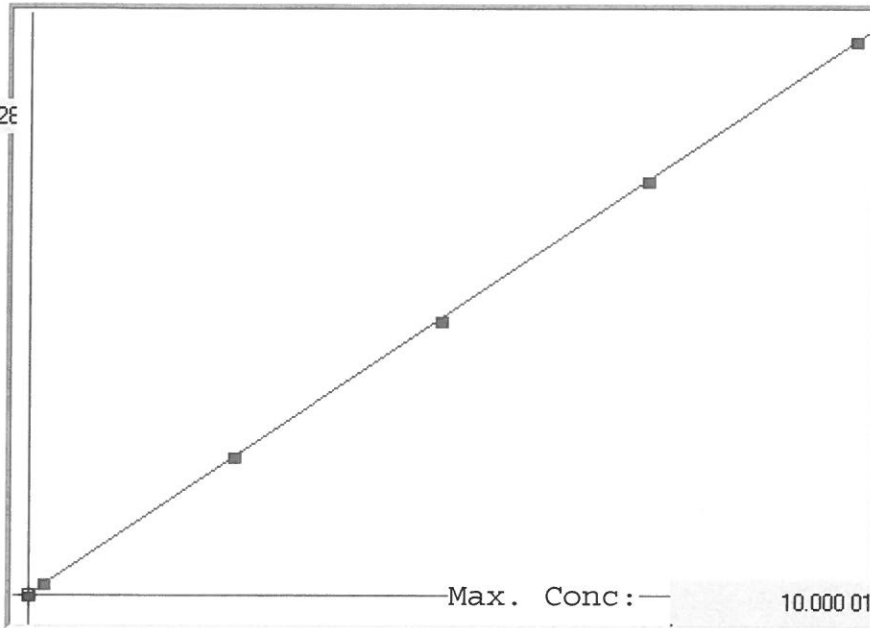

A= 0.0000e+000

B= 2.3712e-004

C= -4.1480e-003

Rho= 0.9999924

Accept=Accepted

slope
y = 1.21e5 x

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5	%D
0.00	0.000	0.000	0.000	18	0.000	18					1
0.2	0.200	0.211	0.011	906	0.0 %	906					5
2.5	2.500	2.505	0.005	10580	0.0 %	10580					0
5.0	5.000	4.969	-0.031	20972	0.0 %	20972					-1
7.5	7.500	7.507	0.007	31676	0.0 %	31676					0
10.0	10.000	10.009	0.009	42228	0.0 %	42228					0

MB
2/10/17

INSTRUMENT ID : CV1

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type
	0 S0	18	-		0 ISM02.3	1	2/10/2017 16:05	Std
	0.2 S0.2	906	-		0.2 ISM02.3	1	2/10/2017 16:07	Std
	2.5 S2.5	10580	-		2.5 ISM02.3	1	2/10/2017 16:09	Std
	5 S5	20972	-		5 ISM02.3	1	2/10/2017 16:11	Std
	7.5 S7.5	31676	-		7.5 ISM02.3	1	2/10/2017 16:13	Std
	10 S10	42228	-		10 ISM02.3	1	2/10/2017 16:15	Std
ICV	ICV	15942	3.776 -		ISM02.3	1	2/10/2017 16:18	SMPL
ICB	ICB	15	-0.0006 -		ISM02.3	1	2/10/2017 16:20	SMPL
CCV001	CCV001	21042	4.9853 -		ISM02.3	1	2/10/2017 16:22	SMPL
CCB001	CCB001	15	-0.0006 -		ISM02.3	1	2/10/2017 16:24	SMPL
PB96837BL	PBW003	-3	-0.0049 -		ISM02.3	1	2/10/2017 16:26	SMPL
I1680-01	MCOAA9	-5	-0.0053 -		ISM02.3	1	2/10/2017 16:29	SMPL
I1680-02	MCOAB1	-9	-0.0063 -		ISM02.3	1	2/10/2017 16:31	SMPL
I1680-03	MCOAA8	14	-0.0008 -		ISM02.3	1	2/10/2017 16:33	SMPL
I1680-04	MCOAA8D	-3	-0.0049 -		ISM02.3	1	2/10/2017 16:37	SMPL
I1680-05	MCOAA8S	4077	0.9626 -		ISM02.3	1	2/10/2017 16:39	SMPL
CCV002	CCV002	21225	5.0287 -		ISM02.3	1	2/10/2017 16:42	SMPL
CCB002	CCB002	16	-0.0004 -		ISM02.3	1	2/10/2017 16:44	SMPL