

LB 85810

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

2/14/2017 11:45

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	93.459	0.0	0.093	
ICB1	0.958	0.0	0.005	
CCV1	240.269	0.0	0.231	
CCB1	1.331	0.0	0.006	
PB96905BLW	1.403	0.0	0.006	
PB96905BSW	96.744	0.0	0.096	
MIDPB96905	243.813	0.0	0.235	
I1789-01	1.709	0.0	0.006	
I1789-01D	1.377	0.0	0.006	
I1789-01S	35.388	0.0	0.038	
I1789-01SD	34.956	0.0	0.037	
CCV2	255.658	0.0	0.246	
CCB2	1.199	0.0	0.006	

N	13
Mean	77.559
SD	102.0272
CV%	131.55

LB85810

AK

Aquakem v. 7.2AQ1

Results from time period:

Tue Feb 14 11:36:28 2017

Tue Feb 14 11:39:52 2017

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Total CN	P	0.9853	µg/l	2/14/2017 9:36:18	
5.0PPBCN	A	Total CN	P	5.5592	µg/l	2/14/2017 9:36:19	
10PPBCN	A	Total CN	P	10.4879	µg/l	2/14/2017 9:36:20	
50PPBCN	A	Total CN	P	47.7403	µg/l	2/14/2017 9:36:21	
100PPBCN	A	Total CN	P	100.145	µg/l	2/14/2017 9:36:22	
250PPBCN	A	Total CN	P	249.8013	µg/l	2/14/2017 9:36:23	
500PPBCN	A	Total CN	P	500.2809	µg/l	2/14/2017 9:36:24	
ICV1	S	Total CN	P	93.4586	µg/l	2/14/2017 11:36:28	
ICB1	S	Total CN	P	0.9579	µg/l	2/14/2017 11:36:29	
CCV1	S	Total CN	P	240.2691	µg/l	2/14/2017 11:36:30	
CCB1	S	Total CN	P	1.3308	µg/l	2/14/2017 11:36:31	
PB96905BLW	S	Total CN	P	1.4031	µg/l	2/14/2017 11:36:32	
PB96905BSW	S	Total CN	P	96.7443	µg/l	2/14/2017 11:36:33	
MIDPB96905	S	Total CN	P	243.813	µg/l	2/14/2017 11:36:34	
I1789-01	S	Total CN	P	1.7086	µg/l	2/14/2017 11:36:35	
I1789-01D	S	Total CN	P	1.3775	µg/l	2/14/2017 11:36:36	
I1789-01S	S	Total CN	P	35.3884	µg/l	2/14/2017 11:36:37	
I1789-01SD	S	Total CN	P	34.9564	µg/l	2/14/2017 11:36:38	
CCV2	S	Total CN	P	255.6585	µg/l	2/14/2017 11:39:51	
CCB2	S	Total CN	P	1.1987	µg/l	2/14/2017 11:39:52	

LB7580

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

2/14/2017 9:40


Test Total CN

Accepted 2/14/2017 9:40

Factor 1060
Bias 0.004

Coeff. of det. 0.999967

Errors

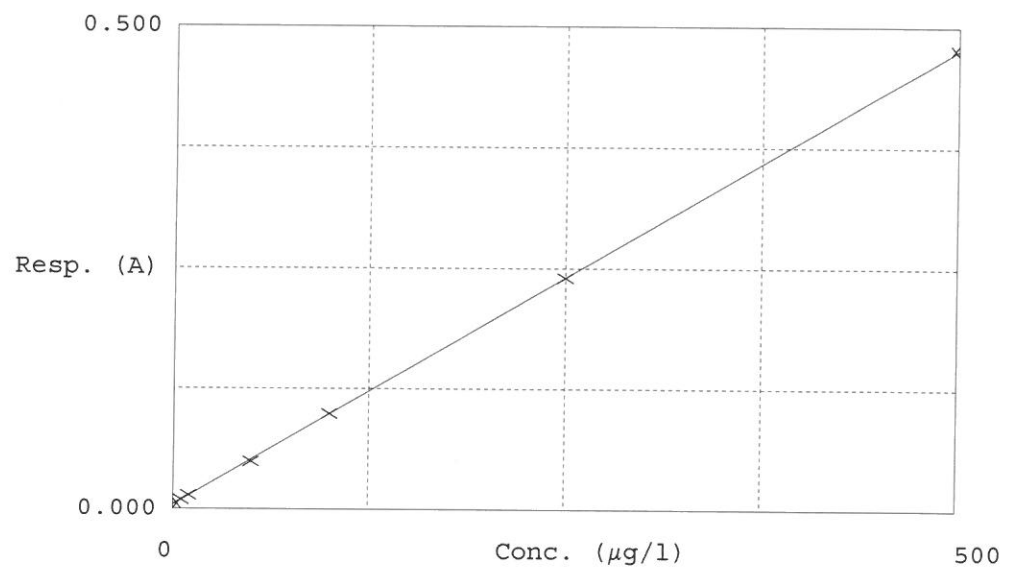

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.005	0.9853	0.0000	
2	5.0PPBCN	0.010	5.5592	5.0000	
3	10PPBCN	0.014	10.4879	10.0000	
4	50PPBCN	0.049	47.7403	50.0000	
5	100PPBCN	0.099	100.1450	100.0000	
6	250PPBCN	0.240	249.8013	250.0000	
7	500PPBCN	0.477	500.2809	500.0000	