

245.1


LB86037

INSTRUMENT ID: CV1

Linear

 μ Abs.:

35651

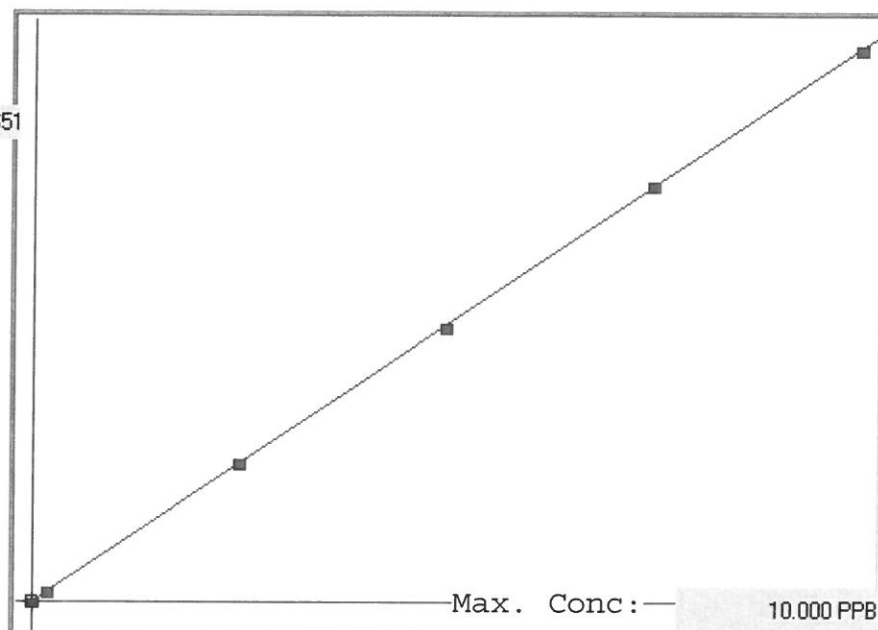

A= 0.0000e+000

B= 2.8028e-004

C= 6.6585e-003

Rho= 0.9999951

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.004	0.004	-11	0.000	-11				
0.2	0.200	0.197	-0.003	680	0.0 %	680				
2.5	2.500	2.510	0.010	8930	0.0 %	8930				
5.0	5.000	4.977	-0.023	17735	0.0 %	17735				
7.5	7.500	7.513	0.013	26782	0.0 %	26782				
10.0	10.000	9.999	-0.001	35651	0.0 %	35651				

LB86037 INSTRUMENT ID : CV1

Method: 245.1

Operator: Admin

Date of Analysis: 27 Feb 2017 11:19:39

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	-11	-	0.0000	245.1	PPB	27 Feb 2017 11:24:15	S	Std
0.2 - 1	50.2	680	-	0.2000	245.1	PPB	27 Feb 2017 11:26:23	S	Std
2.5 - 1	52.5	8930	-	2.5000	245.1	PPB	27 Feb 2017 11:28:31	S	Std
5.0 - 1	55	17735	-	5.0000	245.1	PPB	27 Feb 2017 11:30:39	S	Std
7.5 - 1	57.5	26782	-	7.5000	245.1	PPB	27 Feb 2017 11:32:47	S	Std
10.0 - 1	510	35651	-	10.0000	245.1	PPB	27 Feb 2017 11:34:54	S	Std
ICV48 - 1	ICV48	14154	3.9738	-245.1		PPB	27 Feb 2017 11:38:44	U	SMPL
ICB48 - 1	ICB48	-23	0.0002	-245.1		PPB	27 Feb 2017 11:40:50	U	SMPL
CCV80 - 1	CCV80	17812	4.9990	-245.1		PPB	27 Feb 2017 11:42:57	U	SMPL
CCB80 - 1	CCB80	-32	-0.0023	-245.1		PPB	27 Feb 2017 11:45:03	U	SMPL
CRA - 1	CRA	683	0.1981	-245.1		PPB	27 Feb 2017 11:47:10	U	SMPL
HighStd - 1	HighStd	36401	10.2092	-245.1		PPB	27 Feb 2017 11:49:17	U	SMPL
ChkStd - 1	ChkStd	24623	6.9080	-245.1		PPB	27 Feb 2017 11:51:24	U	SMPL
PB97191BL - 1	PBW	-39	-0.0043	-245.1		PPB	27 Feb 2017 11:53:30	U	SMPL
PB97191BS - 1	LCSW	13877	3.8961	-245.1		PPB	27 Feb 2017 11:55:38	U	SMPL
I1965-02 - 1	EFFLUENTMETALS	474	0.1395	-245.1		PPB	27 Feb 2017 11:57:45	U	SMPL
I1965-02DUP - 1	EFFLUENTMETALSDUP	375	0.1118	-245.1		PPB	27 Feb 2017 12:02:25	U	SMPL
I1965-02MS - 1	EFFLUENTMETALSMS	12088	3.3947	-245.1		PPB	27 Feb 2017 12:04:32	U	SMPL
I1965-02MSD - 1	EFFLUENTMETALSMSD	12644	3.5505	-245.1		PPB	27 Feb 2017 12:06:41	U	SMPL
I1979-01 - 1	2AVE-02	224	0.0694	-245.1		PPB	27 Feb 2017 12:08:48	U	SMPL
CCV81 - 1	CCV81	17221	4.8334	-245.1		PPB	27 Feb 2017 12:10:55	U	SMPL
CCB81 - 1	CCB81	-99	-0.0211	-245.1		PPB	27 Feb 2017 12:13:01	U	SMPL
I1965-02LX5 - 1		148	0.0481	-245.1		PPB	27 Feb 2017 12:15:08	U	SMPL
I1965-02A - 1		13604	3.8196	-245.1		PPB	27 Feb 2017 12:17:15	U	SMPL
CCV82 - 1	CCV82	17296	4.8544	-245.1		PPB	27 Feb 2017 12:19:22	U	SMPL
CCB82 - 1	CCB82	-98	-0.0208	-245.1		PPB	27 Feb 2017 12:21:28	U	SMPL