


7470A

LB86102
INSTRUMENT ID: CV1

Linear

 μ Abs.:

3742E

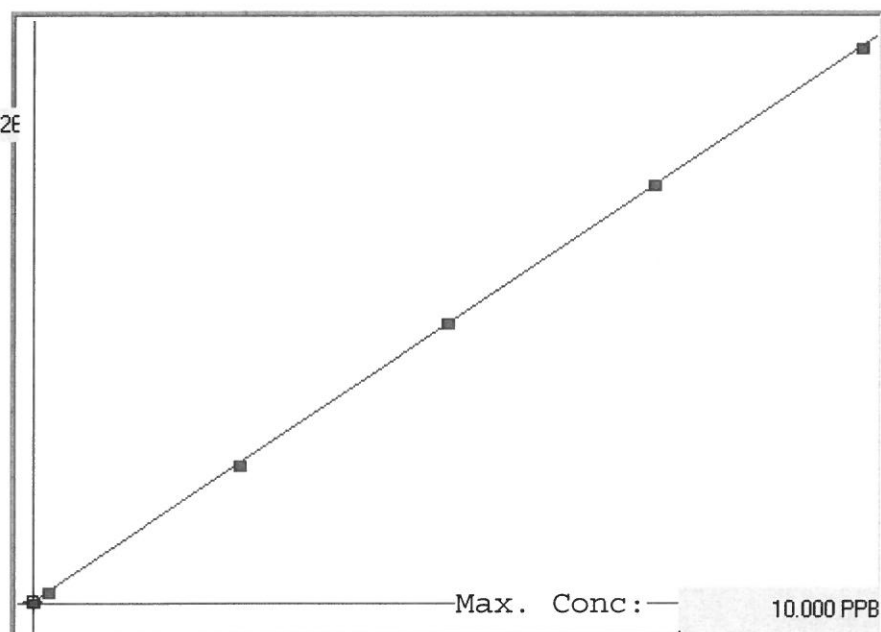

A= 0.0000e+000

B= 2.6712e-004

C= -2.9600e-002

Rho= 0.9999706

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.013	0.013	159	0.000	159				
0.2	0.200	0.190	-0.010	823	0.0 %	823				
2.5	2.500	2.464	-0.036	9334	0.0 %	9334				
5.0	5.000	5.032	0.032	18949	0.0 %	18949				
7.5	7.500	7.534	0.034	28315	0.0 %	28315				
10.0	10.000	9.967	-0.033	37426	0.0 %	37426				

LB86102 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 01 Mar 2017 14:09:07

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	159	-	0.0000	7470A	PPB	01 Mar 2017 14:13:41	S	Std
0.2 - 1	50.2	823	-	0.2000	7470A	PPB	01 Mar 2017 14:15:49	S	Std
2.5 - 1	52.5	9334	-	2.5000	7470A	PPB	01 Mar 2017 14:17:57	S	Std
5.0 - 1	55	18949	-	5.0000	7470A	PPB	01 Mar 2017 14:20:05	S	Std
7.5 - 1	57.5	28315	-	7.5000	7470A	PPB	01 Mar 2017 14:22:14	S	Std
10.0 - 1	59.0	37426	-	10.0000	7470A	PPB	01 Mar 2017 14:24:21	S	Std
ICV53 - 1	ICV53	14218	3.7683	-	7470A	PPB	01 Mar 2017 14:27:03	U	SMPL
ICB53 - 1	ICB53	64	-0.0125	-	7470A	PPB	01 Mar 2017 14:29:09	U	SMPL
CCV15 - 1	CCV15	18779	4.9866	-	7470A	PPB	01 Mar 2017 14:31:16	U	SMPL
CCB15 - 1	CCB15	60	-0.0136	-	7470A	PPB	01 Mar 2017 14:33:22	U	SMPL
CRA - 1	CRA	812	0.1873	-	7470A	PPB	01 Mar 2017 14:35:29	U	SMPL
HighStd - 1	HighStd	36636	9.7565	-	7470A	PPB	01 Mar 2017 14:37:35	U	SMPL
ChkStd - 1	ChkStd	25921	6.8943	-	7470A	PPB	01 Mar 2017 14:39:42	U	SMPL
PB97250BL - 1	PBW	25	-0.0229	-	7470A	PPB	01 Mar 2017 14:41:50	U	SMPL
PB97250BS - 1	LCSW	13867	3.6745	-	7470A	PPB	01 Mar 2017 14:43:58	U	SMPL
PB97250TB - 1	PB97219TB	74	-0.0098	-	7470A	PPB	01 Mar 2017 14:46:05	U	SMPL
I2011-02 - 1	FRAC-TANK-A155	112	0.0003	-	7470A	PPB	01 Mar 2017 14:48:14	U	SMPL
I2011-02DUP - 1	FRAC-TANK-A155DUP	128	0.0046	-	7470A	PPB	01 Mar 2017 14:50:22	U	SMPL
I2011-02MS - 1	FRAC-TANK-A155MS	14616	3.8746	-	7470A	PPB	01 Mar 2017 14:52:31	U	SMPL
I2011-02MSD - 1	FRAC-TANK-A155MSD	14339	3.8006	-	7470A	PPB	01 Mar 2017 14:54:37	U	SMPL
CCV16 - 1	CCV16	18689	4.9625	-	7470A	PPB	01 Mar 2017 14:56:44	U	SMPL
CCB16 - 1	CCB16	45	-0.0176	-	7470A	PPB	01 Mar 2017 14:58:51	U	SMPL
I2014-01 - 1	PRESS-WASTE-WATER-CAKE	174	0.0169	-	7470A	PPB	01 Mar 2017 15:00:57	U	SMPL
I2011-02LX5 - 1		110	-0.0002	-	7470A	PPB	01 Mar 2017 15:03:04	U	SMPL
I2011-02A - 1		14119	3.7418	-	7470A	PPB	01 Mar 2017 15:05:11	U	SMPL
CCV17 - 1	CCV17	18906	5.0205	-	7470A	PPB	01 Mar 2017 15:07:18	U	SMPL
CCB17 - 1	CCB17	30	-0.0216	-	7470A	PPB	01 Mar 2017 15:09:26	U	SMPL