


7471A

LB 86269
INSTRUMENT ID: CV1

Linear

 μ Abs.:

48063

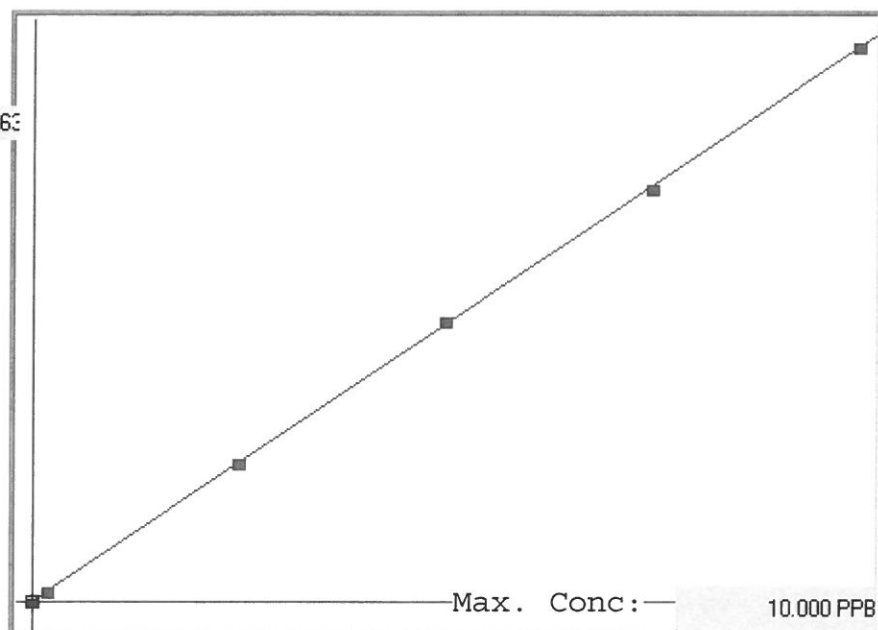

A= 0.0000e+000

B= 2.0815e-004

C= -6.4920e-003

Rho= 0.9999647

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	-0.001	-0.001	24	0.000	24				
0.2	0.200	0.179	-0.021	890	0.0 %	890				
2.5	2.500	2.503	0.003	12054	0.0 %	12054				
5.0	5.000	5.061	0.061	24348	0.0 %	24348				
7.5	7.500	7.461	-0.039	35876	0.0 %	35876				
10.0	10.000	9.998	-0.002	48063	0.0 %	48063				

LB86269 INSTRUMENT ID : CV1

Method: 7471A

Operator: Admin

Date of Analysis: 09 Mar 2017 16:49:31

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	24	-	0.0000	7471A	PPB	09 Mar 2017 16:52:04	S	Std
0.2 - 1	50.2	890	-	0.2000	7471A	PPB	09 Mar 2017 16:54:21	S	Std
2.5 - 1	52.5	12054	-	2.5000	7471A	PPB	09 Mar 2017 16:56:39	S	Std
5.0 - 1	55	24348	-	5.0000	7471A	PPB	09 Mar 2017 16:58:56	S	Std
7.5 - 1	57.5	35876	-	7.5000	7471A	PPB	09 Mar 2017 17:03:49	S	Std
10.0 - 1	510	48063	-	10.0000	7471A	PPB	09 Mar 2017 17:18:29	S	Std
ICV64 - 1	ICV64	17688	3.6752	-	7471A	PPB	09 Mar 2017 17:23:40	U	SMPL
ICB64 - 1	ICB64	-17	-0.0100	-	7471A	PPB	09 Mar 2017 17:25:55	U	SMPL
CCV71 - 1	CCV71	23071	4.7957	-	7471A	PPB	09 Mar 2017 17:28:11	U	SMPL
CCB71 - 1	CCB71	-41	-0.0150	-	7471A	PPB	09 Mar 2017 17:30:27	U	SMPL
CRA - 1	CRA	855	0.1715	-	7471A	PPB	09 Mar 2017 17:32:43	U	SMPL
HighStd - 1	HighStd	47884	9.9605	-	7471A	PPB	09 Mar 2017 17:34:58	U	SMPL
ChkStd - 1	ChkStd	31302	6.5089	-	7471A	PPB	09 Mar 2017 17:37:15	U	SMPL
PB97457BL - 1	PBS	-61	-0.0192	-	7471A	PPB	09 Mar 2017 17:39:32	U	SMPL
PB97457BS - 1	LCSS	17475	3.6309	-	7471A	PPB	09 Mar 2017 17:44:23	U	SMPL
I2010-04 - 1	HY-SB428	2704	0.5563	-	7471A	PPB	09 Mar 2017 17:46:39	U	SMPL
I2010-04DUP - 1	HY-SB428DUP	3209	0.6615	-	7471A	PPB	09 Mar 2017 17:48:56	U	SMPL
I2010-04MS - 1	HY-SB428MS	19344	4.0199	-	7471A	PPB	09 Mar 2017 17:51:14	U	SMPL
I2010-04MSD - 1	HY-SB428MSD	18744	3.8950	-	7471A	PPB	09 Mar 2017 17:53:32	U	SMPL
I2154-01 - 1	EME-BLEND8-1	656	0.1301	-	7471A	PPB	09 Mar 2017 17:55:47	U	SMPL
CCV72 - 1	CCV72	23471	4.8789	-	7471A	PPB	09 Mar 2017 17:58:04	U	SMPL
CCB72 - 1	CCB72	-34	-0.0136	-	7471A	PPB	09 Mar 2017 18:00:20	U	SMPL
I2155-01 - 1	EME-BLEND8-01	1107	0.2239	-	7471A	PPB	09 Mar 2017 18:02:36	U	SMPL
I2156-01 - 1	EME-BLEND008-1	817	0.1636	-	7471A	PPB	09 Mar 2017 18:04:52	U	SMPL
I2157-01 - 1	EME-BLEND008-01	784	0.1567	-	7471A	PPB	09 Mar 2017 18:07:08	U	SMPL
I2188-02 - 1	RU-BUBBLE-01	3597	0.7422	-	7471A	PPB	09 Mar 2017 18:09:24	U	SMPL
I2010-04LX5 - 1		553	0.1086	-	7471A	PPB	09 Mar 2017 18:11:41	U	SMPL
I2010-04A - 1		19095	3.9681	-	7471A	PPB	09 Mar 2017 18:13:58	U	SMPL
CCV73 - 1	CCV73	23750	4.9370	-	7471A	PPB	09 Mar 2017 18:16:15	U	SMPL
CCB73 - 1	CCB73	-19	-0.0104	-	7471A	PPB	09 Mar 2017 18:18:33	U	SMPL