

7470A


~~LD 86365~~ LB 86360
INSTRUMENT ID: CV2

23
3/16/17

Linear

 μ Abs.:

37056

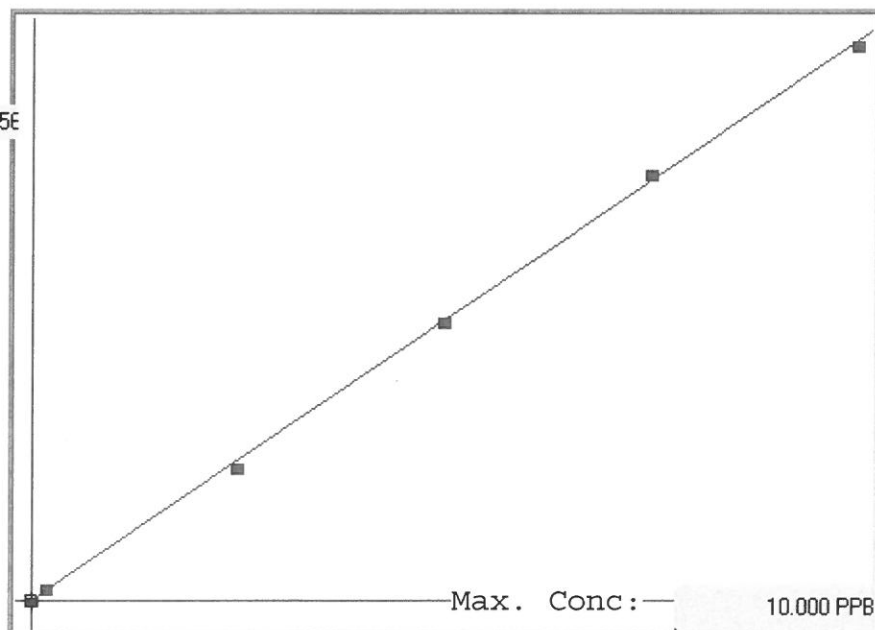

A= 0.0000e+000

B= 2.6731e-004

C= 4.6661e-003

Rho= 0.9997606

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.021	0.021	62	0.000	62				
0.2	0.200	0.219	0.019	800	0.0 %	800				
2.5	2.500	2.401	-0.099	8963	0.0 %	8963				
5.0	5.000	5.007	0.007	18713	0.0 %	18713				
7.5	7.500	7.643	0.143	28573	0.0 %	28573				
10.0	10.000	9.910	-0.090	37056	0.0 %	37056				

LB86360 INSTRUMENT ID : CV1

Method: 7470A		Operator: Admin		Date of Analysis: 15 Mar 2017 08:45:21				
Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type
0.0 - 1	50.2	62	-	0.0000	7470A	PPB	15 Mar 2017 09:07:14	S Std
0.2 - 1	52.5	800	-	0.2000	7470A	PPB	15 Mar 2017 09:09:23	S Std
2.5 - 1	55	8963	-	2.5000	7470A	PPB	15 Mar 2017 09:11:31	S Std
5.0 - 1	57.3	18713	-	5.0000	7470A	PPB	15 Mar 2017 09:13:39	S Std
7.5 - 1	510	28573	-	7.5000	7470A	PPB	15 Mar 2017 09:15:47	S Std
10.0 - 1		37056	-	10.0000	7470A	PPB	15 Mar 2017 09:24:42	S Std
ICV70 - 1	ICV70	13755	3.6815	-	7470A	PPB	15 Mar 2017 09:27:17	U SMPL
ICB70 - 1	ICB70	-43	-0.0068	-	7470A	PPB	15 Mar 2017 09:29:23	U SMPL
CCV96 - 1	CCV96	17724	4.7425	-	7470A	PPB	15 Mar 2017 09:31:30	U SMPL
CCB96 - 1	CCB96	-34	-0.0044	-	7470A	PPB	15 Mar 2017 09:33:36	U SMPL
CRA - 1	CRA	768	0.2100	-	7470A	PPB	15 Mar 2017 09:35:43	U SMPL
HighStd - 1	HighStd	36831	9.8500	-	7470A	PPB	15 Mar 2017 09:37:49	U SMPL
ChkStd - 1	ChkStd	26816	7.1729	-	7470A	PPB	15 Mar 2017 09:39:56	U SMPL
PB97579BL - 1	PBW	-75	-0.0154	-	7470A	PPB	15 Mar 2017 09:42:04	U SMPL
PB97579BS - 1	LCSW	13185	3.5292	-	7470A	PPB	15 Mar 2017 09:44:12	U SMPL
PB97579TB - 1	PB97496TB	-23	-0.0015	-	7470A	PPB	15 Mar 2017 09:46:20	U SMPL
I2199-21 - 1	D-87	128	0.0389	-	7470A	PPB	15 Mar 2017 09:48:28	U SMPL
I2199-22 - 1	D-89	65	0.0220	-	7470A	PPB	15 Mar 2017 09:50:37	U SMPL
I2199-23 - 1	D-93	3	0.0055	-	7470A	PPB	15 Mar 2017 09:52:45	U SMPL
I2199-24 - 1	D-97	15	0.0087	-	7470A	PPB	15 Mar 2017 09:54:51	U SMPL
CCV97 - 1	CCV97	17793	4.7610	-	7470A	PPB	15 Mar 2017 09:56:58	U SMPL
CCB97 - 1	CCB97	-21	-0.0009	-	7470A	PPB	15 Mar 2017 09:59:04	U SMPL
I2199-25 - 1	D-101	0	0.0047	-	7470A	PPB	15 Mar 2017 10:01:11	U SMPL
I2199-26 - 1	D-103	8	0.0068	-	7470A	PPB	15 Mar 2017 10:03:18	U SMPL
I2199-27 - 1	D-105	339	0.0953	-	7470A	PPB	15 Mar 2017 10:05:24	U SMPL
I2199-28 - 1	D-107	76	0.0250	-	7470A	PPB	15 Mar 2017 10:07:31	U SMPL
I2199-29 - 1	D-110	-17	0.0001	-	7470A	PPB	15 Mar 2017 10:09:39	U SMPL
I2199-30 - 1	D-111	63	0.0215	-	7470A	PPB	15 Mar 2017 10:11:46	U SMPL
I2201-17 - 1	D-112	9	0.0071	-	7470A	PPB	15 Mar 2017 10:13:54	U SMPL
I2201-18 - 1	D-117	25	0.0113	-	7470A	PPB	15 Mar 2017 10:16:03	U SMPL
I2201-19 - 1	D-119	67	0.0226	-	7470A	PPB	15 Mar 2017 10:18:12	U SMPL
I2201-20 - 1	D-120	0	0.0047	-	7470A	PPB	15 Mar 2017 10:20:19	U SMPL
CCV98 - 1	CCV98	18210	4.8724	-	7470A	PPB	15 Mar 2017 10:22:25	U SMPL
CCB98 - 1	CCB98	-9	0.0023	-	7470A	PPB	15 Mar 2017 10:24:32	U SMPL
I2201-21 - 1	D-121	-11	0.0017	-	7470A	PPB	15 Mar 2017 10:26:39	U SMPL
I2201-22 - 1	D-123	133	0.0402	-	7470A	PPB	15 Mar 2017 10:28:45	U SMPL
I2201-23 - 1	D-126	24	0.0111	-	7470A	PPB	15 Mar 2017 10:30:52	U SMPL
I2201-24 - 1	D-127	41	0.0156	-	7470A	PPB	15 Mar 2017 10:32:59	U SMPL
I2201-24DUP - 1	D-127DUP	50	0.0180	-	7470A	PPB	15 Mar 2017 10:35:06	U SMPL
I2201-24MS - 1	D-127MS	13639	3.6505	-	7470A	PPB	15 Mar 2017 10:37:14	U SMPL
I2201-24MSD - 1	D-127MSD	13252	3.5471	-	7470A	PPB	15 Mar 2017 10:39:22	U SMPL
PB97580BL - 1	PB97580BL	19	0.0097	-	7470A	PPB	15 Mar 2017 10:41:30	U SMPL
PB97580BS - 1	PB97580BS	14127	3.7810	-	7470A	PPB	15 Mar 2017 10:43:38	U SMPL
PB97580TB - 1	PB97533TB	12	0.0079	-	7470A	PPB	15 Mar 2017 10:45:45	U SMPL
CCV99 - 1	CCV99	18540	4.9606	-	7470A	PPB	15 Mar 2017 10:47:52	U SMPL
CCB99 - 1	CCB99	0	0.0047	-	7470A	PPB	15 Mar 2017 10:49:59	U SMPL
I2230-02 - 1	COMPOSITE-1-CHAR	45	0.0167	-	7470A	PPB	15 Mar 2017 10:52:07	U SMPL
I2230-04 - 1	COMPOSITE-2-CHAR	48	0.0175	-	7470A	PPB	15 Mar 2017 10:54:14	U SMPL
I2230-06 - 1	COMPOSITE-3-CHAR	61	0.0210	-	7470A	PPB	15 Mar 2017 10:56:21	U SMPL
I2230-08 - 1	COMPOSITE-4-CHAR	45	0.0167	-	7470A	PPB	15 Mar 2017 10:58:28	U SMPL
I2233-02 - 1	FRAC-TANK-BOTTOM	69	0.0231	-	7470A	PPB	15 Mar 2017 11:00:36	U SMPL
I2233-02DUP - 1	FRAC-TANK-BOTTOMDUP	55	0.0194	-	7470A	PPB	15 Mar 2017 11:02:43	U SMPL
I2233-02MS - 1	FRAC-TANK-BOTTOMMS	13305	3.5613	-	7470A	PPB	15 Mar 2017 11:04:51	U SMPL
I2233-02MSD - 1	FRAC-TANK-BOTTOMMSD	13302	3.5605	-	7470A	PPB	15 Mar 2017 11:06:59	U SMPL
PB97581BL - 1	PBW	-44	-0.0071	-	7470A	PPB	15 Mar 2017 11:09:07	U SMPL
PB97581BS - 1	LCSW	13443	3.5981	-	7470A	PPB	15 Mar 2017 11:11:14	U SMPL
CCV01 - 1	CCV01	18562	4.9665	-	7470A	PPB	15 Mar 2017 11:13:22	U SMPL
CCB01 - 1	CCB01	-30	-0.0034	-	7470A	PPB	15 Mar 2017 11:15:29	U SMPL
PB97581TB - 1	PB97531TB	1	0.0049	-	7470A	PPB	15 Mar 2017 11:17:36	U SMPL
2137-06 - 1	38D-9-11	244	0.0699	-	7470A	PPB	15 Mar 2017 11:24:18	U SMPL
2137-06DUP - 1	38D-9-11DUP	244	0.0699	-	7470A	PPB	15 Mar 2017 11:28:06	U SMPL
2137-06MS - 1	38D-9-11MS	16274	4.3549	-	7470A	PPB	15 Mar 2017 11:30:12	U SMPL
2137-06MSD - 1	38D-9-11MSD	16159	4.3242	-	7470A	PPB	15 Mar 2017 11:32:19	U SMPL
CCV02 - 1	CCV02	17956	4.8045	-	7470A	PPB	15 Mar 2017 11:34:27	U SMPL
CCB02 - 1	CCB02	16	0.0089	-	7470A	PPB	15 Mar 2017 11:36:35	U SMPL
2201-24LX5 - 1		108	0.0335	-	7470A	PPB	15 Mar 2017 11:38:43	U SMPL
2201-24A - 1		15429	4.1290	-	7470A	PPB	15 Mar 2017 11:40:52	U SMPL
2233-02LX5 - 1		-7	0.0028	-	7470A	PPB	15 Mar 2017 11:42:59	U SMPL
2233-02A - 1		15510	4.1507	-	7470A	PPB	15 Mar 2017 11:45:07	U SMPL
2137-06LX5 - 1		107	0.0333	-	7470A	PPB	15 Mar 2017 11:47:14	U SMPL
2137-06A - 1		17769	4.7545	-	7470A	PPB	15 Mar 2017 11:49:21	U SMPL
CCV03 - 1	CCV03	18158	4.8585	-	7470A	PPB	15 Mar 2017 11:51:28	U SMPL
CCB03 - 1	CCB03	21	0.0103	-	7470A	PPB	15 Mar 2017 11:53:36	U SMPL