

LB86472

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

3/21/2017 11:53

Test: Phenolics-

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	0.986	0.0	0.114	
ICB1	-0.003	0.0	0.007	
CCV1	0.987	0.0	0.114	
CCB1	-0.005	0.0	0.007	
PB97664BL	-0.003	0.0	0.007	
PB97664BS	0.988	0.0	0.114	
I2212-26	0.687	0.0	0.082	
CCV2	0.989	0.0	0.114	
CCB2	-0.002	0.0	0.007	

N	9
Mean	0.514
SD	0.4997
CV%	97.22

LB 86472

Ak

Aquakem v. 7.2AQ1

Results from time period:

Tue Mar 21 11:50:18 2017

Tue Mar 21 11:50:27 2017

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.05PPM	A	Phenolics-	P	0.0519	mg/l	3/21/2017 9:47:48	
0.1PPM	A	Phenolics-	P	0.1005	mg/l	3/21/2017 9:47:49	
0.25PPM	A	Phenolics-	P	0.2517	mg/l	3/21/2017 9:47:50	
0.50PPM	A	Phenolics-	P	0.4999	mg/l	3/21/2017 9:47:51	
1.0PPM	A	Phenolics-	P	0.9925	mg/l	3/21/2017 9:47:52	
2.0PPM	A	Phenolics-	P	2.0035	mg/l	3/21/2017 9:47:53	
ICV1	S	Phenolics-	P	0.9862	mg/l	3/21/2017 11:50:18	
ICB1	S	Phenolics-	P	-0.0033	mg/l	3/21/2017 11:50:19	
CCV1	S	Phenolics-	P	0.9872	mg/l	3/21/2017 11:50:20	
CCB1	S	Phenolics-	P	-0.0046	mg/l	3/21/2017 11:50:21	
PB97664BL	S	Phenolics-	P	-0.003	mg/l	3/21/2017 11:50:22	
PB97664BS	S	Phenolics-	P	0.9883	mg/l	3/21/2017 11:50:23	
I2212-26	S	Phenolics-	P	0.6872	mg/l	3/21/2017 11:50:24	
CCV2	S	Phenolics-	P	0.989	mg/l	3/21/2017 11:50:26	
CCB2	S	Phenolics-	P	-0.0016	mg/l	3/21/2017 11:50:27	

LB86472

Calibration results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

3/21/2017 10:02


Test Phenolics-

Accepted 3/21/2017 10:02

Factor 9.224
Bias 0.007

Coeff. of det. 0.999973

Errors

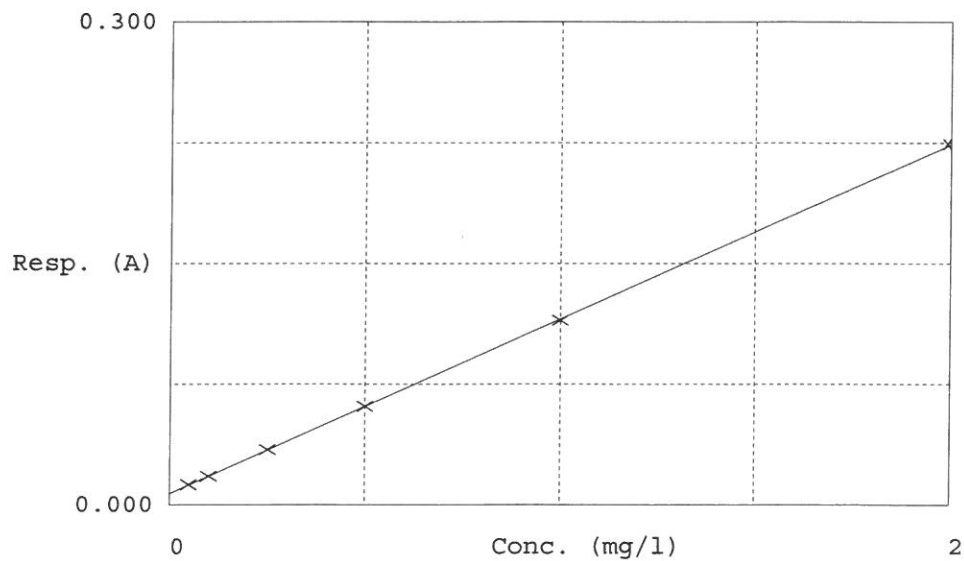

	Calibrator	Response	Calc. con.	Conc.	Errors
1	Phenol-2	0.013	0.0519	0.0500	
2	Phenol-2	0.018	0.1005	0.1000	
3	Phenol-2	0.034	0.2517	0.2500	
4	Phenol-2	0.061	0.4999	0.5000	
5	Phenol-2	0.115	0.9925	1.0000	
6	Phenol-2	0.224	2.0035	2.0000	