


7471A

LB 86651
INSTRUMENT ID: CV1

Linear

 μ Abs.:

45582

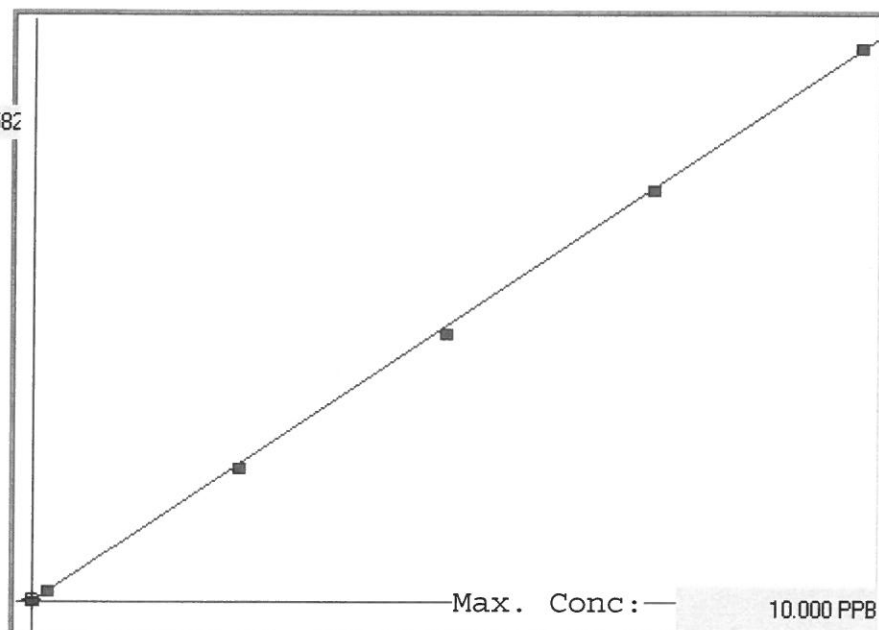

A= 0.0000e+000

B= 2.2029e-004

C= 1.0938e-002

Rho= 0.9998858

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.056	0.056	204	0.000	204				
0.2	0.200	0.224	0.024	967	0.0 %	967				
2.5	2.500	2.463	-0.037	11131	0.0 %	11131				
5.0	5.000	4.896	-0.104	22176	0.0 %	22176				
7.5	7.500	7.509	0.009	34035	0.0 %	34035				
10.0	10.000	10.052	0.052	45582	0.0 %	45582				

LB86651 INSTRUMENT ID : CV1

Method: 7471A

Operator: Admin

Date of Analysis: 31 Mar 2017 12:54:32

Sample ID	Extended ID	µ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	204	-	0.0000	7471A	PPB	31 Mar 2017 13:06:11	S	Std
0.2 - 1	50.2	967	-	0.2000	7471A	PPB	31 Mar 2017 13:08:28	S	Std
2.5 - 1	52.5	11131	-	2.5000	7471A	PPB	31 Mar 2017 13:10:46	S	Std
5.0 - 1	55	22176	-	5.0000	7471A	PPB	31 Mar 2017 13:13:04	S	Std
7.5 - 1	57.5	34035	-	7.5000	7471A	PPB	31 Mar 2017 13:15:21	S	Std
10.0 - 1	58	45582	-	10.0000	7471A	PPB	31 Mar 2017 13:17:37	S	Std
ICV99 - 1	ICV99	17331	3.8288	-	7471A	PPB	31 Mar 2017 13:20:24	U	SMPL
ICB99 - 1	ICB99	59	0.0239	-	7471A	PPB	31 Mar 2017 13:22:40	U	SMPL
CCV20 - 1	CCV20	21815	4.8166	-	7471A	PPB	31 Mar 2017 13:24:55	U	SMPL
CCB20 - 1	CCB20	78	0.0281	-	7471A	PPB	31 Mar 2017 13:27:11	U	SMPL
CRA - 1	CRA	982	0.2273	-	7471A	PPB	31 Mar 2017 13:29:27	U	SMPL
HighStd - 1	HighStd	45462	10.0259	-	7471A	PPB	31 Mar 2017 13:31:43	U	SMPL
ChkStd - 1	ChkStd	31639	6.9808	-	7471A	PPB	31 Mar 2017 13:33:59	U	SMPL
PB97947BL - 1	PBS	113	0.0358	-	7471A	PPB	31 Mar 2017 13:38:50	U	SMPL
PB97947BS - 1	LCSS	14945	3.3032	-	7471A	PPB	31 Mar 2017 13:41:06	U	SMPL
I2416-07 - 1	TP-4(1.5-2)	4922	1.0952	-	7471A	PPB	31 Mar 2017 13:43:24	U	SMPL
I2416-10 - 1	TP-6(1.5-2)	2489	0.5592	-	7471A	PPB	31 Mar 2017 13:45:41	U	SMPL
I2416-11 - 1	TP-6(9.5-10)	1842	0.4167	-	7471A	PPB	31 Mar 2017 13:47:58	U	SMPL
I2416-16 - 1	TP-9(1.5-2)	2269	0.5108	-	7471A	PPB	31 Mar 2017 13:50:16	U	SMPL
I2416-17 - 1	TP-9(7.5-8)	2127	0.4795	-	7471A	PPB	31 Mar 2017 13:52:32	U	SMPL
CCV21 - 1	CCV21	22037	4.8655	-	7471A	PPB	31 Mar 2017 13:54:48	U	SMPL
CCB21 - 1	CCB21	128	0.0391	-	7471A	PPB	31 Mar 2017 13:57:04	U	SMPL
I2417-04 - 1	SW-1(1.5-2)	7898	1.7508	-	7471A	PPB	31 Mar 2017 13:59:20	U	SMPL
I2417-05 - 1	SW-1(8.0-8.5)	519	0.1253	-	7471A	PPB	31 Mar 2017 14:01:36	U	SMPL
I2417-05DUP - 1	SW-1(8.0-8.5)DUP	494	0.1198	-	7471A	PPB	31 Mar 2017 14:03:52	U	SMPL
I2417-05MS - 1	SW-1(8.0-8.5)MS	16494	3.6445	-	7471A	PPB	31 Mar 2017 14:06:08	U	SMPL
I2417-05MSD - 1	SW-1(8.0-8.5)MSD	16755	3.7020	-	7471A	PPB	31 Mar 2017 14:08:25	U	SMPL
I2417-06 - 1	SW-2(1.5-2)	1020	0.2356	-	7471A	PPB	31 Mar 2017 14:10:42	U	SMPL
I2417-07 - 1	SW-2(3.5-4)	1866	0.4220	-	7471A	PPB	31 Mar 2017 14:12:59	U	SMPL
I2417-08 - 1	SW-3(1.5-2)	1422	0.3242	-	7471A	PPB	31 Mar 2017 14:15:16	U	SMPL
I2417-09 - 1	SW-3(6.5-7)	1483	0.3376	-	7471A	PPB	31 Mar 2017 14:17:34	U	SMPL
I2417-10 - 1	SW-4(1.5-2)	947	0.2196	-	7471A	PPB	31 Mar 2017 14:19:50	U	SMPL
CCV22 - 1	CCV22	22243	4.9109	-	7471A	PPB	31 Mar 2017 14:22:06	U	SMPL
CCB22 - 1	CCB22	124	0.0383	-	7471A	PPB	31 Mar 2017 14:24:22	U	SMPL
I2417-11 - 1	SW-4(8.8-5)	3445	0.7698	-	7471A	PPB	31 Mar 2017 14:26:38	U	SMPL
I2417-12 - 1	SW-5(1.5-2)	1751	0.3967	-	7471A	PPB	31 Mar 2017 14:28:54	U	SMPL
I2417-13 - 1	SW-6(1.5-2)	1783	0.4037	-	7471A	PPB	31 Mar 2017 14:31:11	U	SMPL
PB97948BL - 1	PBS	78	0.0281	-	7471A	PPB	31 Mar 2017 14:33:27	U	SMPL
PB97948BS - 1	LCSS	15740	3.4784	-	7471A	PPB	31 Mar 2017 14:35:44	U	SMPL
I2457-01 - 1	S-1	1119	0.2574	-	7471A	PPB	31 Mar 2017 14:38:00	U	SMPL
I2458-01 - 1	B-4-S1(1.5-2)	1432	0.3264	-	7471A	PPB	31 Mar 2017 14:40:17	U	SMPL
I2458-02 - 1	B-4-S2(5.5-6)	384	0.0955	-	7471A	PPB	31 Mar 2017 14:42:34	U	SMPL
I2458-03 - 1	B-42-S1(1.0-1.5)	24200	5.3420	-	7471A	PPB	31 Mar 2017 14:44:53	U	SMPL
I2458-04 - 1	B-42-S2(2.0-2.5)	1632	0.3705	-	7471A	PPB	31 Mar 2017 14:47:08	U	SMPL
CCV23 - 1	CCV23	22222	4.9063	-	7471A	PPB	31 Mar 2017 14:49:25	U	SMPL
CCB23 - 1	CCB23	172	0.0488	-	7471A	PPB	31 Mar 2017 14:51:41	U	SMPL
I2458-05 - 1	B-6-S1(1.0-1.5)	4057	0.9047	-	7471A	PPB	31 Mar 2017 14:53:57	U	SMPL
I2458-05DUP - 1	B-6-S1(1.0-1.5)DUP	3959	0.8831	-	7471A	PPB	31 Mar 2017 14:56:13	U	SMPL
I2458-05MS - 1	B-6-S1(1.0-1.5)MS	19531	4.3135	-	7471A	PPB	31 Mar 2017 14:58:30	U	SMPL
I2458-05MSD - 1	B-6-S1(1.0-1.5)MSD	19280	4.2582	-	7471A	PPB	31 Mar 2017 15:00:46	U	SMPL
I2458-06 - 1	B-6-S2(2.5-3.0)	2386	0.5366	-	7471A	PPB	31 Mar 2017 15:03:03	U	SMPL
I2463-01 - 1	E2-R11-BASE	4670	1.0397	-	7471A	PPB	31 Mar 2017 15:05:20	U	SMPL
I2463-02 - 1	E2-Q11-BASE	31459	6.9411	-	7471A	PPB	31 Mar 2017 15:07:37	U	SMPL
I2463-03 - 1	E2-Q12-BASE	5418	1.2045	-	7471A	PPB	31 Mar 2017 15:09:55	U	SMPL
I2463-04 - 1	E2-R12-BASE	9303	2.0603	-	7471A	PPB	31 Mar 2017 15:12:12	U	SMPL
I2463-05 - 1	E2-R-Q-11-12-BASE	21506	4.7486	-	7471A	PPB	31 Mar 2017 15:14:28	U	SMPL
CCV24 - 1	CCV24	22857	5.0462	-	7471A	PPB	31 Mar 2017 15:16:44	U	SMPL
CCB24 - 1	CCB24	161	0.0464	-	7471A	PPB	31 Mar 2017 15:19:01	U	SMPL
I2463-06 - 1	E2-S-R-11-12-BASE	18701	4.1306	-	7471A	PPB	31 Mar 2017 15:21:17	U	SMPL
I2463-07 - 1	E2-R-Q-12-13-BASE	5438	1.2089	-	7471A	PPB	31 Mar 2017 15:23:33	U	SMPL
I2463-08 - 1	E2-Q-P-12-13-BASE	65771	14.4999	-	7471A	PPB	31 Mar 2017 15:25:50	U	SMPL
I2463-09 - 1	E2-BB-8-9-SSW	4738	1.0547	-	7471A	PPB	31 Mar 2017 15:28:06	U	SMPL
I2463-10 - 1	E2-BB-7-8-SSW	30003	6.6204	-	7471A	PPB	31 Mar 2017 15:30:24	U	SMPL
I2463-11 - 1	E2-BB-8-9-ESW	1862	0.4211	-	7471A	PPB	31 Mar 2017 15:32:40	U	SMPL
I2474-01 - 1	49B-9-11	576	0.1378	-	7471A	PPB	31 Mar 2017 15:34:57	U	SMPL
CCV25 - 1	CCV25	22769	5.0268	-	7471A	PPB	31 Mar 2017 15:37:15	U	SMPL
CCB25 - 1	CCB25	171	0.0486	-	7471A	PPB	31 Mar 2017 15:39:33	U	SMPL
I2417-05LX5 - 1		315	0.0803	-	7471A	PPB	31 Mar 2017 15:41:48	U	SMPL
I2417-05A - 1		18611	4.1108	-	7471A	PPB	31 Mar 2017 15:44:05	U	SMPL
I2458-05LX5 - 1		941	0.2182	-	7471A	PPB	31 Mar 2017 15:46:21	U	SMPL
I2458-05A - 1		22067	4.8722	-	7471A	PPB	31 Mar 2017 15:48:38	U	SMPL
I2463-08DLX5 - 1		13990	3.0928	-	7471A	PPB	31 Mar 2017 15:50:54	U	SMPL
CCV26 - 1	CCV26	22742	5.0208	-	7471A	PPB	31 Mar 2017 15:53:11	U	SMPL
CCB26 - 1	CCB26	58	0.0237	-	7471A	PPB	31 Mar 2017 15:55:28	U	SMPL