


7471A

LB 86944
INSTRUMENT ID: CV1

Linear

 μ Abs.:

45046

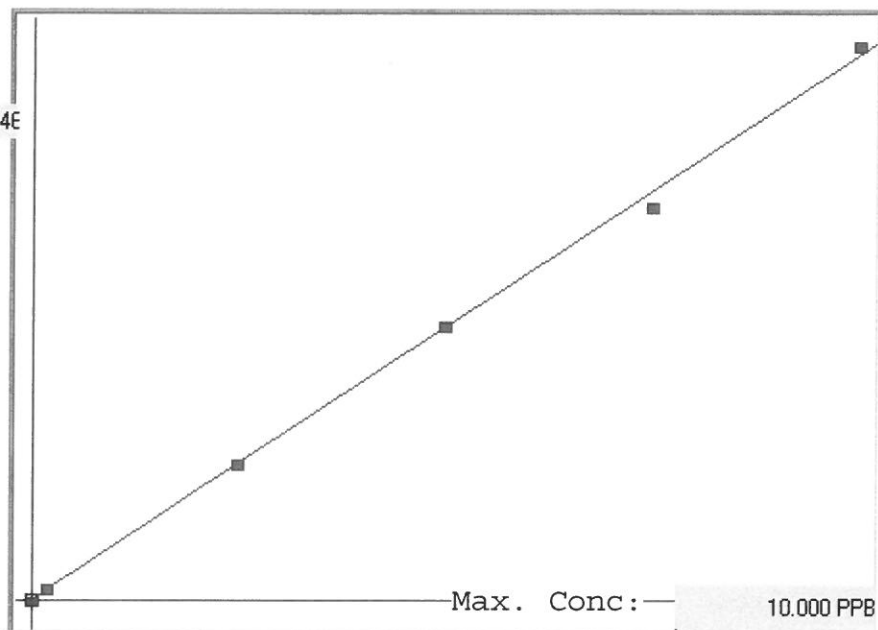

A= 0.0000e+000

B= 2.2595e-004

C= -6.7177e-003

Rho= 0.9992978

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.019	0.019	113	0.000	113				
0.2	0.200	0.221	0.021	1010	0.0 %	1010				
2.5	2.500	2.524	0.024	11201	0.0 %	11201				
5.0	5.000	5.050	0.050	22379	0.0 %	22379				
7.5	7.500	7.215	-0.285	31960	0.0 %	31960				
10.0	10.000	10.171	0.171	45046	0.0 %	45046				

LB86944 INSTRUMENT ID : CV1

Method: 7471A

Operator: Admin

Date of Analysis: 18 Apr 2017 12:03:30

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	SO	113	-	0.0000	7471A	PPB	18 Apr 2017 12:05:12	S	Std
0.2 - 1	SO.2	1010	-	0.2000	7471A	PPB	18 Apr 2017 12:07:29	S	Std
2.5 - 1	SO.25	11201	-	2.5000	7471A	PPB	18 Apr 2017 12:09:47	S	Std
5.0 - 1	SO.5	22379	-	5.0000	7471A	PPB	18 Apr 2017 12:12:04	S	Std
7.5 - 1	SO.75	31960	-	7.5000	7471A	PPB	18 Apr 2017 12:14:21	S	Std
10.0 - 1	SO.10	45046	-	10.0000	7471A	PPB	18 Apr 2017 12:19:28	S	Std
ICV22 - 1	ICV22	16751	3.7781	-	7471A	PPB	18 Apr 2017 12:22:12	U	SMPL
ICB22 - 1	ICB22	49	0.0044	-	7471A	PPB	18 Apr 2017 12:24:27	U	SMPL
CCV33 - 1	CCV33	21516	4.8548	-	7471A	PPB	18 Apr 2017 12:26:43	U	SMPL
CCB33 - 1	CCB33	49	0.0044	-	7471A	PPB	18 Apr 2017 12:28:59	U	SMPL
CRA - 1	CRA	963	0.2109	-	7471A	PPB	18 Apr 2017 12:31:15	U	SMPL
HighStd - 1	HighStd	44570	10.0637	-	7471A	PPB	18 Apr 2017 12:33:30	U	SMPL
ChkStd - 1	ChkStd	31092	7.0184	-	7471A	PPB	18 Apr 2017 12:35:46	U	SMPL
PB98290BL - 1	PBS	-48	-0.0176	-	7471A	PPB	18 Apr 2017 12:38:02	U	SMPL
PB98290BS - 1	LCSS	15712	3.5434	-	7471A	PPB	18 Apr 2017 12:40:19	U	SMPL
I2695-02 - 1	49C-9-11	286	0.0579	-	7471A	PPB	18 Apr 2017 12:47:29	U	SMPL
I2695-02DUP - 1	49C-9-11DUP	270	0.0543	-	7471A	PPB	18 Apr 2017 12:49:46	U	SMPL
I2695-02MS - 1	49C-9-11MS	15824	3.5687	-	7471A	PPB	18 Apr 2017 12:52:04	U	SMPL
I2695-02MSD - 1	49C-9-11MSD	15536	3.5036	-	7471A	PPB	18 Apr 2017 12:54:22	U	SMPL
I2701-01 - 1	S8-9004	138	0.0245	-	7471A	PPB	18 Apr 2017 12:56:38	U	SMPL
CCV34 - 1	CCV34	22019	4.9684	-	7471A	PPB	18 Apr 2017 12:58:54	U	SMPL
CCB34 - 1	CCB34	89	0.0134	-	7471A	PPB	18 Apr 2017 13:01:10	U	SMPL
I2707-01 - 1	E2-X8-BASE	9920	2.2347	-	7471A	PPB	18 Apr 2017 13:03:26	U	SMPL
I2707-02 - 1	E2-X7-BASE	156176	35.2808	-	7471A	PPB	18 Apr 2017 13:05:42	U	SMPL
I2707-03 - 1	E2-Y7-BASE	47454	10.7154	-	7471A	PPB	18 Apr 2017 13:07:58	U	SMPL
I2707-04 - 1	E2-XY67-BASE	9618	2.1664	-	7471A	PPB	18 Apr 2017 13:10:16	U	SMPL
I2728-01 - 1	WC-AGG3-14	83	0.0120	-	7471A	PPB	18 Apr 2017 13:12:33	U	SMPL
I2732-01 - 1	EME-COMPOST-1	956	0.2093	-	7471A	PPB	18 Apr 2017 13:14:50	U	SMPL
I2735-01 - 1	EME-COMPOST-01	1048	0.2301	-	7471A	PPB	18 Apr 2017 13:17:07	U	SMPL
I2741-01 - 1	WDS-02	905	0.1978	-	7471A	PPB	18 Apr 2017 13:19:25	U	SMPL
I2741-03 - 1	WS-03	2197	0.4897	-	7471A	PPB	18 Apr 2017 13:21:43	U	SMPL
PB98291BL - 1	PBS	40	0.0023	-	7471A	PPB	18 Apr 2017 13:23:58	U	SMPL
CCV35 - 1	CCV35	21836	4.9271	-	7471A	PPB	18 Apr 2017 13:26:15	U	SMPL
CCB35 - 1	CCB35	87	0.0129	-	7471A	PPB	18 Apr 2017 13:28:31	U	SMPL
PB98291BS - 1	LCSS	15003	3.3832	-	7471A	PPB	18 Apr 2017 13:30:47	U	SMPL
I2708-01 - 1	E2-Z10-ESW	31811	7.1809	-	7471A	PPB	18 Apr 2017 13:33:04	U	SMPL
I2708-02 - 1	E2-Z10-BASE	3309	0.7409	-	7471A	PPB	18 Apr 2017 13:35:20	U	SMPL
I2708-03 - 1	E2-X8-BASE	9681	2.1807	-	7471A	PPB	18 Apr 2017 13:37:37	U	SMPL
I2708-03DUP - 1	E2-X8-BASEDUP	10846	2.4439	-	7471A	PPB	18 Apr 2017 13:42:32	U	SMPL
I2708-03MS - 1	E2-X8-BASEMS	25703	5.8008	-	7471A	PPB	18 Apr 2017 13:44:49	U	SMPL
I2708-03MSD - 1	E2-X8-BASEMSD	26118	5.8946	-	7471A	PPB	18 Apr 2017 13:47:06	U	SMPL
I2708-04 - 1	E2-Y8-NSW	13911	3.1364	-	7471A	PPB	18 Apr 2017 13:49:24	U	SMPL
I2708-05 - 1	E2-Y8-ESW	5357	1.2037	-	7471A	PPB	18 Apr 2017 13:51:41	U	SMPL
I2708-06 - 1	E2-Y8-WSW	28444	6.4201	-	7471A	PPB	18 Apr 2017 13:53:58	U	SMPL
CCV36 - 1	CCV36	21876	4.9361	-	7471A	PPB	18 Apr 2017 13:56:14	U	SMPL
CCB36 - 1	CCB36	34	0.0010	-	7471A	PPB	18 Apr 2017 13:58:30	U	SMPL
I2708-07 - 1	E2-Z9-BASE	37168	8.3913	-	7471A	PPB	18 Apr 2017 14:00:47	U	SMPL
I2708-08 - 1	E2-Y10-BASE	55659	12.5693	-	7471A	PPB	18 Apr 2017 14:03:03	U	SMPL
I2708-09 - 1	E2-Y10-ESW	14664	3.3066	-	7471A	PPB	18 Apr 2017 14:05:19	U	SMPL
I2708-10 - 1	E2-Y9-BASE	27947	6.3078	-	7471A	PPB	18 Apr 2017 14:07:35	U	SMPL
I2708-11 - 1	E2-XY9-BASE	95850	21.6503	-	7471A	PPB	18 Apr 2017 14:09:52	U	SMPL
I2708-12 - 1	E2-XY9-ESW	10537	2.3741	-	7471A	PPB	18 Apr 2017 14:12:09	U	SMPL
I2708-13 - 1	E2-XY9-SSW	32439	7.3228	-	7471A	PPB	18 Apr 2017 14:14:27	U	SMPL
I2708-14 - 1	E2-XY9-WSW	31591	7.1312	-	7471A	PPB	18 Apr 2017 14:16:45	U	SMPL
I2708-15 - 1	E2-XY9-NSW	115913	26.1835	-	7471A	PPB	18 Apr 2017 14:19:03	U	SMPL
I2708-16 - 1	E2-X10-ESW	352687	79.6818	-	7471A	PPB	18 Apr 2017 14:21:19	U	SMPL
CCV37 - 1	CCV37	21800	4.9189	-	7471A	PPB	18 Apr 2017 14:23:37	U	SMPL
CCB37 - 1	CCB37	-43	-0.0164	-	7471A	PPB	18 Apr 2017 14:25:57	U	SMPL
I2708-17 - 1	E2-X10-BASE	276989	62.5781	-	7471A	PPB	18 Apr 2017 14:28:13	U	SMPL
I2695-02LX5 - 1		64	0.0077	-	7471A	PPB	18 Apr 2017 14:33:09	U	SMPL
I2695-02A - 1		17515	3.9507	-	7471A	PPB	18 Apr 2017 14:35:25	U	SMPL
I2708-03LX5 - 1		2141	0.4770	-	7471A	PPB	18 Apr 2017 14:37:41	U	SMPL
I2708-03A - 1		26806	6.0500	-	7471A	PPB	18 Apr 2017 14:39:58	U	SMPL
I2707-02DLX5 - 1		32590	7.3569	-	7471A	PPB	18 Apr 2017 14:42:15	U	SMPL
I2707-03DLX2 - 1		24204	5.4621	-	7471A	PPB	18 Apr 2017 14:44:32	U	SMPL
I2708-08DLX5 - 1		10856	2.4462	-	7471A	PPB	18 Apr 2017 14:46:49	U	SMPL
I2708-11DLX5 - 1		18803	4.2418	-	7471A	PPB	18 Apr 2017 14:49:07	U	SMPL
I2708-15DLX5 - 1		22902	5.1679	-	7471A	PPB	18 Apr 2017 14:51:24	U	SMPL
CCV38 - 1	CCV38	22529	5.0836	-	7471A	PPB	18 Apr 2017 14:53:41	U	SMPL
CCB38 - 1	CCB38	39	0.0021	-	7471A	PPB	18 Apr 2017 14:55:57	U	SMPL
I2708-16DLX10 - 1		38031	8.5863	-	7471A	PPB	18 Apr 2017 14:58:14	U	SMPL
I2708-17DLX10 - 1		29185	6.5875	-	7471A	PPB	18 Apr 2017 15:00:30	U	SMPL
CCV39 - 1	CCV39	22153	4.9987	-	7471A	PPB	18 Apr 2017 15:02:47	U	SMPL
CCB39 - 1	CCB39	49	0.0044	-	7471A	PPB	18 Apr 2017 15:05:04	U	SMPL