


7470A

LB87126
INSTRUMENT ID: CV1

Linear

 μ Abs.:

35723

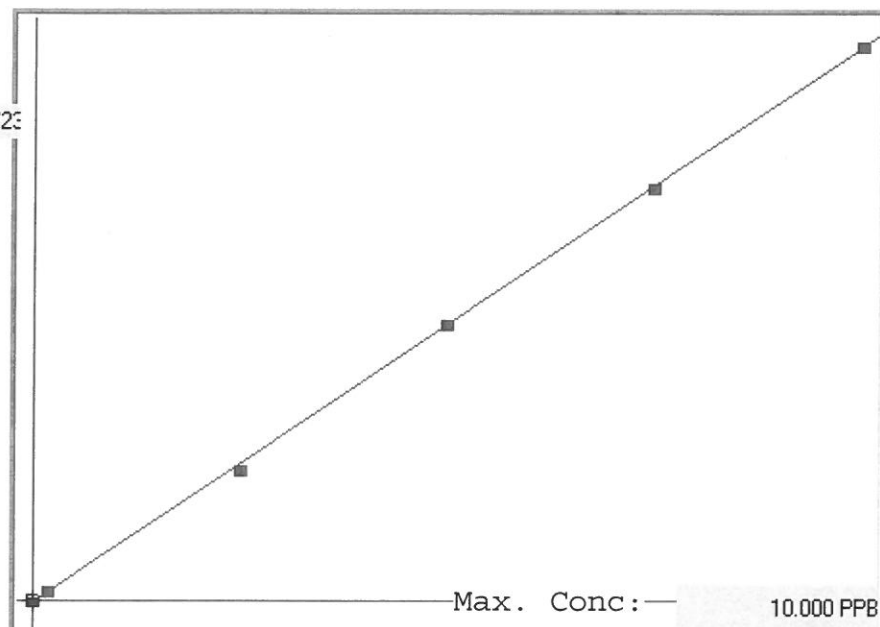

A= 0.0000e+000

B= 2.7955e-004

C= 3.6918e-002

Rho= 0.9999056

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.043	0.043	20	0.000	20				
0.2	0.200	0.235	0.035	710	0.0 %	710				
2.5	2.500	2.392	-0.108	8426	0.0 %	8426				
5.0	5.000	5.014	0.014	17803	0.0 %	17803				
7.5	7.500	7.493	-0.007	26670	0.0 %	26670				
10.0	10.000	10.023	0.023	35723	0.0 %	35723				

LB87126 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 28 Apr 2017 13:11:27

Sample ID	Extended ID	µ Abs.	Conc.	Std ConcMethod	Units	Date	Type	Type
0.0 - 1	50	20	-	0.00007470A	PPB	28 Apr 2017 13:56:16	S	Std
0.2 - 1	50.2	710	-	0.20007470A	PPB	28 Apr 2017 13:58:24	S	Std
2.5 - 1	52.5	8426	-	2.50007470A	PPB	28 Apr 2017 14:00:32	S	Std
5.0 - 1	55	17803	-	5.00007470A	PPB	28 Apr 2017 14:02:40	S	Std
7.5 - 1	57.5	26670	-	7.50007470A	PPB	28 Apr 2017 14:04:48	S	Std
10.0 - 1	57.5	35723	-	10.00007470A	PPB	28 Apr 2017 14:09:22	S	Std
ICV35 - 1	ICV35	14408	4.0647	-7470A	PPB	28 Apr 2017 14:11:59	U	SMPL
ICB35 - 1	ICB35	-95	0.0104	-7470A	PPB	28 Apr 2017 14:14:05	U	SMPL
CCV92 - 1	CCV92	18092	5.0946	-7470A	PPB	28 Apr 2017 14:16:12	U	SMPL
CCB92 - 1	CCB92	-111	0.0059	-7470A	PPB	28 Apr 2017 14:18:19	U	SMPL
CRA - 1	CRA	688	0.2292	-7470A	PPB	28 Apr 2017 14:20:25	U	SMPL
HighStd - 1	HighStd	35469	9.9523	-7470A	PPB	28 Apr 2017 14:22:32	U	SMPL
ChkStd - 1	ChkStd	25552	7.1800	-7470A	PPB	28 Apr 2017 14:24:39	U	SMPL
PB98525BL - 1	PBW	-130	0.0006	-7470A	PPB	28 Apr 2017 14:26:46	U	SMPL
PB98525BS - 1	LCSW	13835	3.9045	-7470A	PPB	28 Apr 2017 14:28:54	U	SMPL
PB98525TB - 1	PB98509TB	-71	0.0171	-7470A	PPB	28 Apr 2017 14:31:01	U	SMPL
I2855-01 - 1	OWS-2	437	0.1591	-7470A	PPB	28 Apr 2017 14:33:09	U	SMPL
I2855-02 - 1	OWS-1	440	0.1599	-7470A	PPB	28 Apr 2017 14:35:17	U	SMPL
I2869-05 - 1	KEARNY-GEN-STA-SP-(0-2)	-17	0.0322	-7470A	PPB	28 Apr 2017 14:37:26	U	SMPL
I2870-02 - 1	SOIL-CUTTINGS-DRUMS(COMP)	51	0.0512	-7470A	PPB	28 Apr 2017 14:39:33	U	SMPL
CCV93 - 1	CCV93	17811	5.0160	-7470A	PPB	28 Apr 2017 14:41:40	U	SMPL
CCB93 - 1	CCB93	-54	0.0218	-7470A	PPB	28 Apr 2017 14:43:46	U	SMPL
I2870-02DUP - 1	SOIL-CUTTINGS-DRUMS(COMP)DUP	81	0.0596	-7470A	PPB	28 Apr 2017 14:45:53	U	SMPL
I2870-02MS - 1	SOIL-CUTTINGS-DRUMS(COMP)MS	13426	3.7902	-7470A	PPB	28 Apr 2017 14:48:00	U	SMPL
I2870-02MSD - 1	SOIL-CUTTINGS-DRUMS(COMP)MSD	13313	3.7586	-7470A	PPB	28 Apr 2017 14:50:07	U	SMPL
I2870-08 - 1	PURGE-WATER-DRUMS(COMP)	-48	0.0235	-7470A	PPB	28 Apr 2017 14:52:14	U	SMPL
PB98526BL - 1	PBW	-40	0.0257	-7470A	PPB	28 Apr 2017 14:54:22	U	SMPL
PB98526BS - 1	LCSW	13138	3.7097	-7470A	PPB	28 Apr 2017 14:56:29	U	SMPL
I2859-05 - 1	UT-W	37214	10.4402	-7470A	PPB	28 Apr 2017 14:58:38	U	SMPL
I2870-07 - 1	PURGE-WATER-DRUMS(COMP)	4844	1.3911	-7470A	PPB	28 Apr 2017 15:00:45	U	SMPL
I2870-07DUP - 1	PURGE-WATER-DRUMS(COMP)DUP	5096	1.4615	-7470A	PPB	28 Apr 2017 15:02:54	U	SMPL
I2870-07MS - 1	PURGE-WATER-DRUMS(COMP)MS	20707	5.8256	-7470A	PPB	28 Apr 2017 15:05:01	U	SMPL
CCV94 - 1	CCV94	17924	5.0476	-7470A	PPB	28 Apr 2017 15:07:08	U	SMPL
CCB94 - 1	CCB94	-56	0.0213	-7470A	PPB	28 Apr 2017 15:09:15	U	SMPL
I2870-07MSD - 1	PURGE-WATER-DRUMS(COMP)MSD	22189	6.2399	-7470A	PPB	28 Apr 2017 15:11:22	U	SMPL
I2873-08 - 1	FRAC-TANK-A1841DW	-17	0.0322	-7470A	PPB	28 Apr 2017 15:13:28	U	SMPL
I2870-02LX5 - 1		-1	0.0366	-7470A	PPB	28 Apr 2017 15:15:35	U	SMPL
I2870-02A - 1		14252	4.0211	-7470A	PPB	28 Apr 2017 15:17:42	U	SMPL
I2870-07LX5 - 1		891	0.2860	-7470A	PPB	28 Apr 2017 15:19:50	U	SMPL
I2870-07A - 1		22662	6.3721	-7470A	PPB	28 Apr 2017 15:21:57	U	SMPL
I2859-05DLX2 - 1		18602	5.2371	-7470A	PPB	28 Apr 2017 15:26:22	U	SMPL
CCV95 - 1	CCV95	18178	5.1186	-7470A	PPB	28 Apr 2017 15:28:30	U	SMPL
CCB95 - 1	CCB95	-52	0.0224	-7470A	PPB	28 Apr 2017 15:30:39	U	SMPL