

7470A


LB87270

INSTRUMENT ID: CVd

Linear

 μ Abs.:

36240

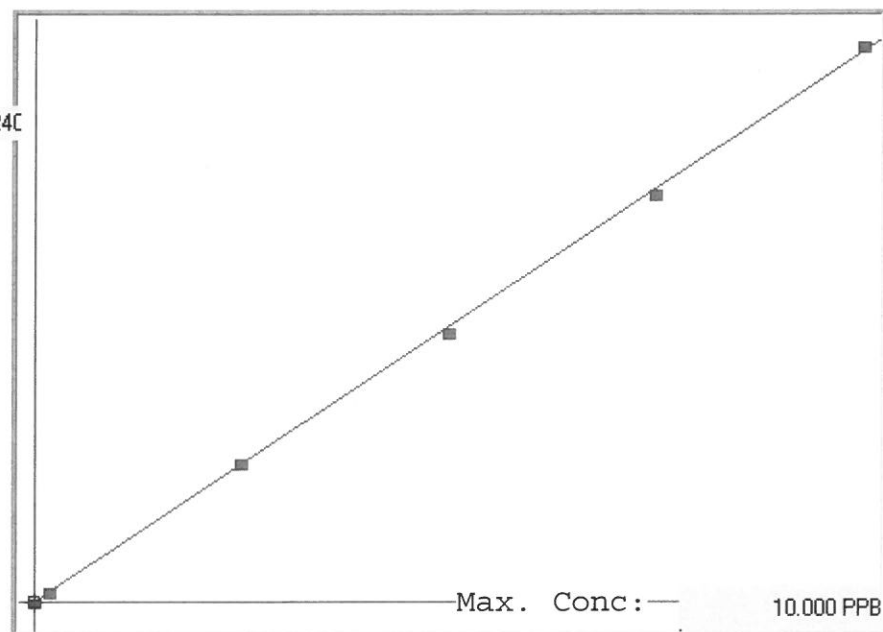

A= 0.0000e+000

B= 2.7817e-004

C= 8.3395e-003

Rho= 0.9998508

Accept=Accepted

Std ID	Conc.	Calc.	Dev.	Mean	SD or %RSD	Rep 1	Rep 2	Rep 3	Rep 4	Rep 5
0.0	0.000	0.014	0.014	22	0.000	22				
0.2	0.200	0.213	0.013	737	0.0 %	737				
2.5	2.500	2.548	0.048	9131	0.0 %	9131				
5.0	5.000	4.920	-0.080	17657	0.0 %	17657				
7.5	7.500	7.415	-0.085	26625	0.0 %	26625				
10.0	10.000	10.089	0.089	36240	0.0 %	36240				

LB87270 INSTRUMENT ID : CV1

Method: 7470A

Operator: Admin

Date of Analysis: 05 May 2017 09:04:32

Sample ID	Extended ID	μ Abs.	Conc.	Std Conc	Method	Units	Date	Type	Type
0.0 - 1	50	22	-	0.0000	7470A	PPB	05 May 2017 09:17:02	S	Std
0.2 - 1	50.2	737	-	0.2000	7470A	PPB	05 May 2017 09:19:11	S	Std
2.5 - 1	52.5	9131	-	2.5000	7470A	PPB	05 May 2017 09:21:19	S	Std
5.0 - 1	55	17657	-	5.0000	7470A	PPB	05 May 2017 09:23:27	S	Std
7.5 - 1	57.5	26625	-	7.5000	7470A	PPB	05 May 2017 09:28:03	S	Std
10.0 - 1	510	36240	-	10.0000	7470A	PPB	05 May 2017 09:30:10	S	Std
ICV44 - 1	ICV44	14257	3.9742	-	7470A	PPB	05 May 2017 09:32:44	U	SMPL
ICB44 - 1	ICB44	-89	-0.0164	-	7470A	PPB	05 May 2017 09:34:50	U	SMPL
CCV43 - 1	CCV43	17712	4.9353	-	7470A	PPB	05 May 2017 09:36:57	U	SMPL
CCB43 - 1	CCB43	-87	-0.0159	-	7470A	PPB	05 May 2017 09:39:03	U	SMPL
CRA - 1	CRA	710	0.2058	-	7470A	PPB	05 May 2017 09:41:10	U	SMPL
HighStd - 1	HighStd	35907	9.9966	-	7470A	PPB	05 May 2017 09:43:17	U	SMPL
ChkStd - 1	ChkStd	24820	6.9125	-	7470A	PPB	05 May 2017 09:45:24	U	SMPL
PB98710BL - 1	PBW	-140	-0.0306	-	7470A	PPB	05 May 2017 09:47:32	U	SMPL
PB98710BS - 1	LCSW	13940	3.8860	-	7470A	PPB	05 May 2017 09:49:40	U	SMPL
PB98710TB - 1	PB98683TB	-98	-0.0189	-	7470A	PPB	05 May 2017 09:51:47	U	SMPL
I2947-21 - 1	SB-01-COMP	6	0.0100	-	7470A	PPB	05 May 2017 09:53:56	U	SMPL
I2947-22 - 1	SB-02-COMP	-39	-0.0025	-	7470A	PPB	05 May 2017 09:56:04	U	SMPL
I2947-23 - 1	SB-03-COMP	158	0.0523	-	7470A	PPB	05 May 2017 09:58:12	U	SMPL
I2947-24 - 1	SB-04-COMP	-51	-0.0058	-	7470A	PPB	05 May 2017 10:00:19	U	SMPL
CCV44 - 1	CCV44	17427	4.8560	-	7470A	PPB	05 May 2017 10:02:25	U	SMPL
CCB44 - 1	CCB44	-64	-0.0095	-	7470A	PPB	05 May 2017 10:04:32	U	SMPL
I2947-25 - 1	SB-05-COMP	-15	0.0042	-	7470A	PPB	05 May 2017 10:06:39	U	SMPL
I2947-26 - 1	SB-06-COMP	-20	0.0028	-	7470A	PPB	05 May 2017 10:08:46	U	SMPL
I2949-03 - 1	SB-07-COMP	-22	0.0022	-	7470A	PPB	05 May 2017 10:10:52	U	SMPL
I2953-04 - 1	TP7-8-COMP	141	0.0476	-	7470A	PPB	05 May 2017 10:12:59	U	SMPL
I2956-03 - 1	IP-TP(0-5)	-13	0.0047	-	7470A	PPB	05 May 2017 10:15:07	U	SMPL
I2956-06 - 1	CHERRY-ST-TP(0-5)	15	0.0125	-	7470A	PPB	05 May 2017 10:17:15	U	SMPL
I2957-03 - 1	RT-3025	19	0.0136	-	7470A	PPB	05 May 2017 10:19:23	U	SMPL
I2957-06 - 1	RT-2342	1	0.0086	-	7470A	PPB	05 May 2017 10:21:31	U	SMPL
I2969-02 - 1	TP4-5-COMP	7	0.0103	-	7470A	PPB	05 May 2017 10:23:40	U	SMPL
I2969-12 - 1	TP1-COMP	29	0.0164	-	7470A	PPB	05 May 2017 10:25:47	U	SMPL
CCV45 - 1	CCV45	17953	5.0023	-	7470A	PPB	05 May 2017 10:27:54	U	SMPL
CCB45 - 1	CCB45	-55	-0.0070	-	7470A	PPB	05 May 2017 10:30:00	U	SMPL
I2969-12DUP - 1	TP1-COMP-DUP	59	0.0248	-	7470A	PPB	05 May 2017 10:32:07	U	SMPL
I2969-12MS - 1	TP1-COMPMS	12780	3.5634	-	7470A	PPB	05 May 2017 10:34:14	U	SMPL
I2969-12MSD - 1	TP1-COMPMSD	12967	3.6154	-	7470A	PPB	05 May 2017 10:36:21	U	SMPL
PB98711BL - 1	PBW	16	0.0128	-	7470A	PPB	05 May 2017 10:38:28	U	SMPL
PB98711BS - 1	LCSW	13304	3.7091	-	7470A	PPB	05 May 2017 10:40:36	U	SMPL
I2942-01 - 1	MW-4	160	0.0528	-	7470A	PPB	05 May 2017 10:47:25	U	SMPL
I2942-01DUP - 1	MW-4DUP	129	0.0442	-	7470A	PPB	05 May 2017 10:49:33	U	SMPL
I2942-01MS - 1	MW-4MS	15959	4.4477	-	7470A	PPB	05 May 2017 10:51:41	U	SMPL
I2942-01MSD - 1	MW-4MSD	16136	4.4969	-	7470A	PPB	05 May 2017 10:53:50	U	SMPL
I2942-02 - 1	MW-5	185	0.0598	-	7470A	PPB	05 May 2017 10:55:57	U	SMPL
CCV46 - 1	CCV46	17927	4.9951	-	7470A	PPB	05 May 2017 10:58:04	U	SMPL
CCB46 - 1	CCB46	-55	-0.0070	-	7470A	PPB	05 May 2017 11:00:11	U	SMPL
I2943-01 - 1	MW-1	110	0.0389	-	7470A	PPB	05 May 2017 11:02:18	U	SMPL
I2943-02 - 1	MW-2	54	0.0234	-	7470A	PPB	05 May 2017 11:04:25	U	SMPL
I2943-03 - 1	SW-1	4173	1.1691	-	7470A	PPB	05 May 2017 11:06:32	U	SMPL
I2944-01 - 1	SW-2	3529	0.9900	-	7470A	PPB	05 May 2017 11:08:40	U	SMPL
I2944-02 - 1	MW-3	138	0.0467	-	7470A	PPB	05 May 2017 11:10:47	U	SMPL
I2949-05 - 1	TWP-07	124	0.0428	-	7470A	PPB	05 May 2017 11:12:55	U	SMPL
I2949-06 - 1	TWP-07	201	0.0643	-	7470A	PPB	05 May 2017 11:15:03	U	SMPL
I2949-08 - 1	TWP-07-DUP	159	0.0526	-	7470A	PPB	05 May 2017 11:17:11	U	SMPL
I2949-09 - 1	TWP-07-DUP	284	0.0873	-	7470A	PPB	05 May 2017 11:19:20	U	SMPL
I2949-10 - 1	FIELD BLANK	18	0.0133	-	7470A	PPB	05 May 2017 11:21:27	U	SMPL
CCV47 - 1	CCV47	16867	4.7002	-	7470A	PPB	05 May 2017 11:23:34	U	SMPL
CCB47 - 1	CCB47	-27	0.0008	-	7470A	PPB	05 May 2017 11:25:42	U	SMPL
I2949-11 - 1	FIELD BLANK	212	0.0673	-	7470A	PPB	05 May 2017 11:27:49	U	SMPL
I2952-01 - 1	MW-1	155	0.0515	-	7470A	PPB	05 May 2017 11:29:56	U	SMPL
I2969-12LX5 - 1		13	0.0120	-	7470A	PPB	05 May 2017 11:32:03	U	SMPL
I2969-12A - 1		14131	3.9392	-	7470A	PPB	05 May 2017 11:34:10	U	SMPL
I2942-01LX5 - 1		-1	0.0081	-	7470A	PPB	05 May 2017 11:36:18	U	SMPL
I2942-01A - 1		14373	4.0065	-	7470A	PPB	05 May 2017 11:38:25	U	SMPL
CCV48 - 1	CCV48	18163	5.0608	-	7470A	PPB	05 May 2017 11:40:33	U	SMPL
CCB48 - 1	CCB48	-69	-0.0109	-	7470A	PPB	05 May 2017 11:42:41	U	SMPL